
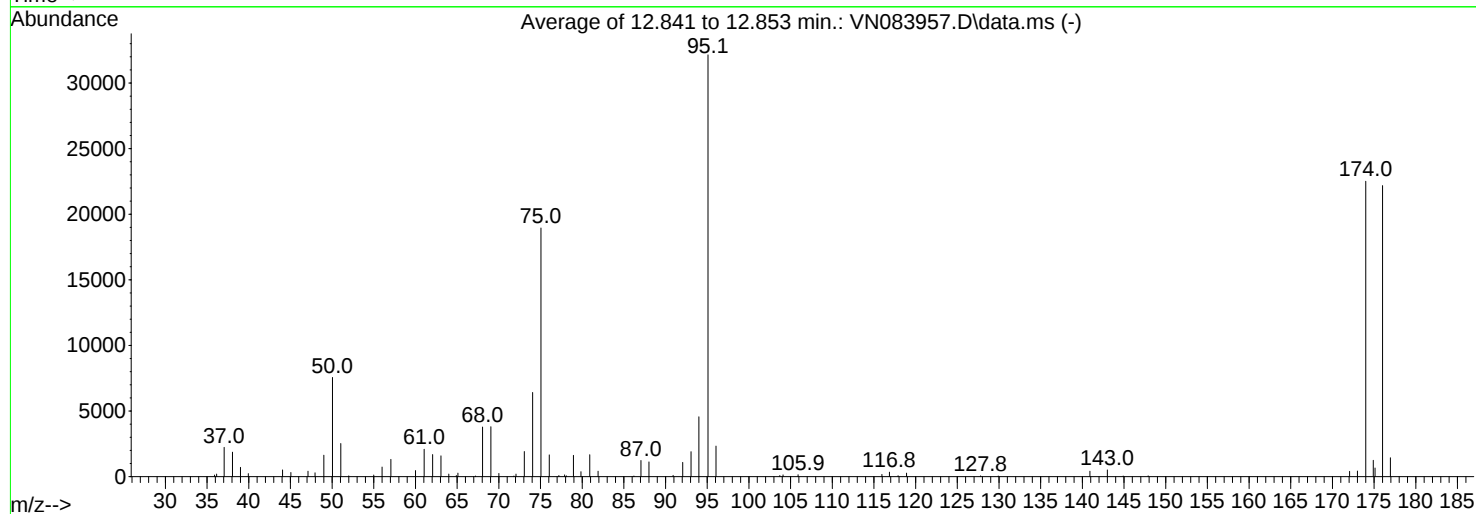


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091724\
Data File : VN083957.D
Acq On : 18 Sep 2024 02:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

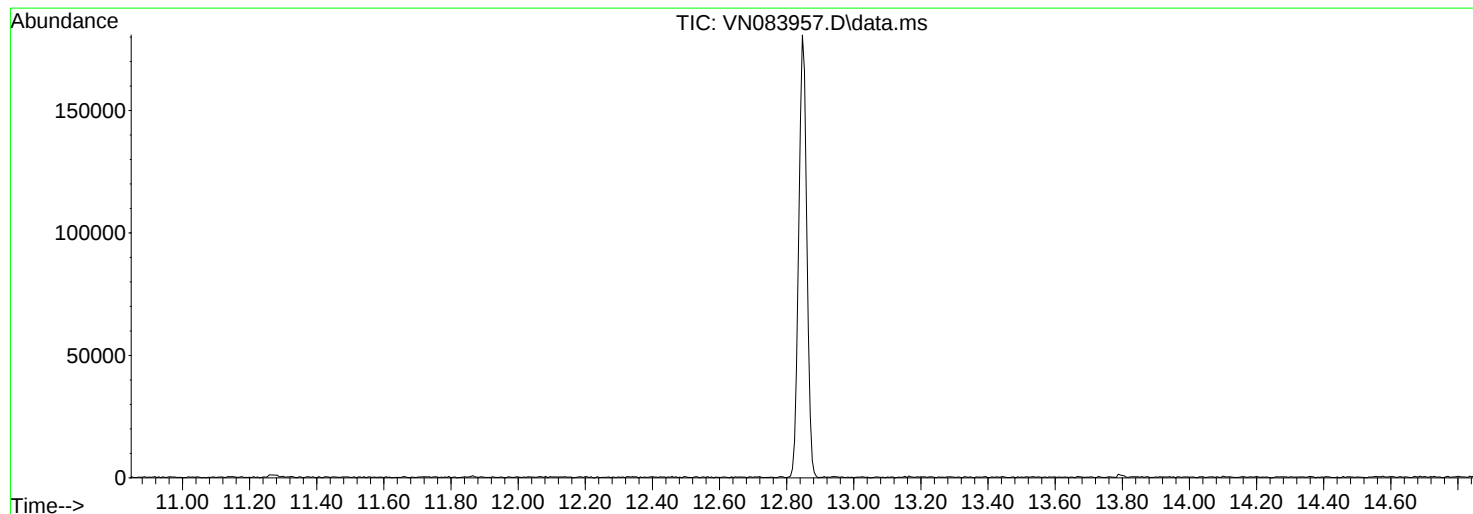

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.5	7560	PASS
75	95	30	60	58.9	18947	PASS
95	95	100	100	100.0	32147	PASS
96	95	5	9	7.2	2326	PASS
173	174	0.00	2	1.9	433	PASS
174	95	50	100	70.0	22517	PASS
175	174	5	9	5.6	1250	PASS
176	174	95	101	98.5	22181	PASS
177	176	5	9	6.5	1442	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	124	50.05	7560	64.90	89	76.05	1654
36.15	193	51.05	2521	65.10	274	77.20	80
37.05	2226	52.00	59	67.20	55	77.90	132
38.05	1864	55.00	120	68.05	3780	78.10	61
39.00	713	56.00	726	69.05	3809	78.95	1628
39.95	228	57.05	1319	70.00	247	79.85	374
44.05	515	60.00	461	71.80	53	80.90	1673
45.05	322	61.05	2082	72.05	200	81.90	412
47.10	421	62.05	1685	73.05	1916	86.20	51
47.95	289	63.05	1585	74.05	6420	87.05	1232
49.00	1632	64.00	198	75.05	18947	88.00	1128

Average of 12.841 to 12.853 min.: VN083957.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.90	105	117.90	78	174.90	1250		
92.05	1081	118.90	266	175.10	663		
93.05	1904	127.80	58	176.00	22181		
94.00	4559	129.90	52	176.95	1442		
95.10	32147	140.90	417				
96.05	2326	143.00	514				
103.70	87	144.90	54				
104.10	130	147.90	66				
105.90	153	172.05	402				
115.95	170	173.00	433				
116.85	340	174.00	22517				

Instrument :

MSVOA_N

ClientSampleId :

BFB