


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091818\
 Data File : VN051284.D
 Acq On : 18 Sep 2018 7:32
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091718W.M
 Title : SW846 8260
 Last Update : Tue Sep 18 06:04:06 2018

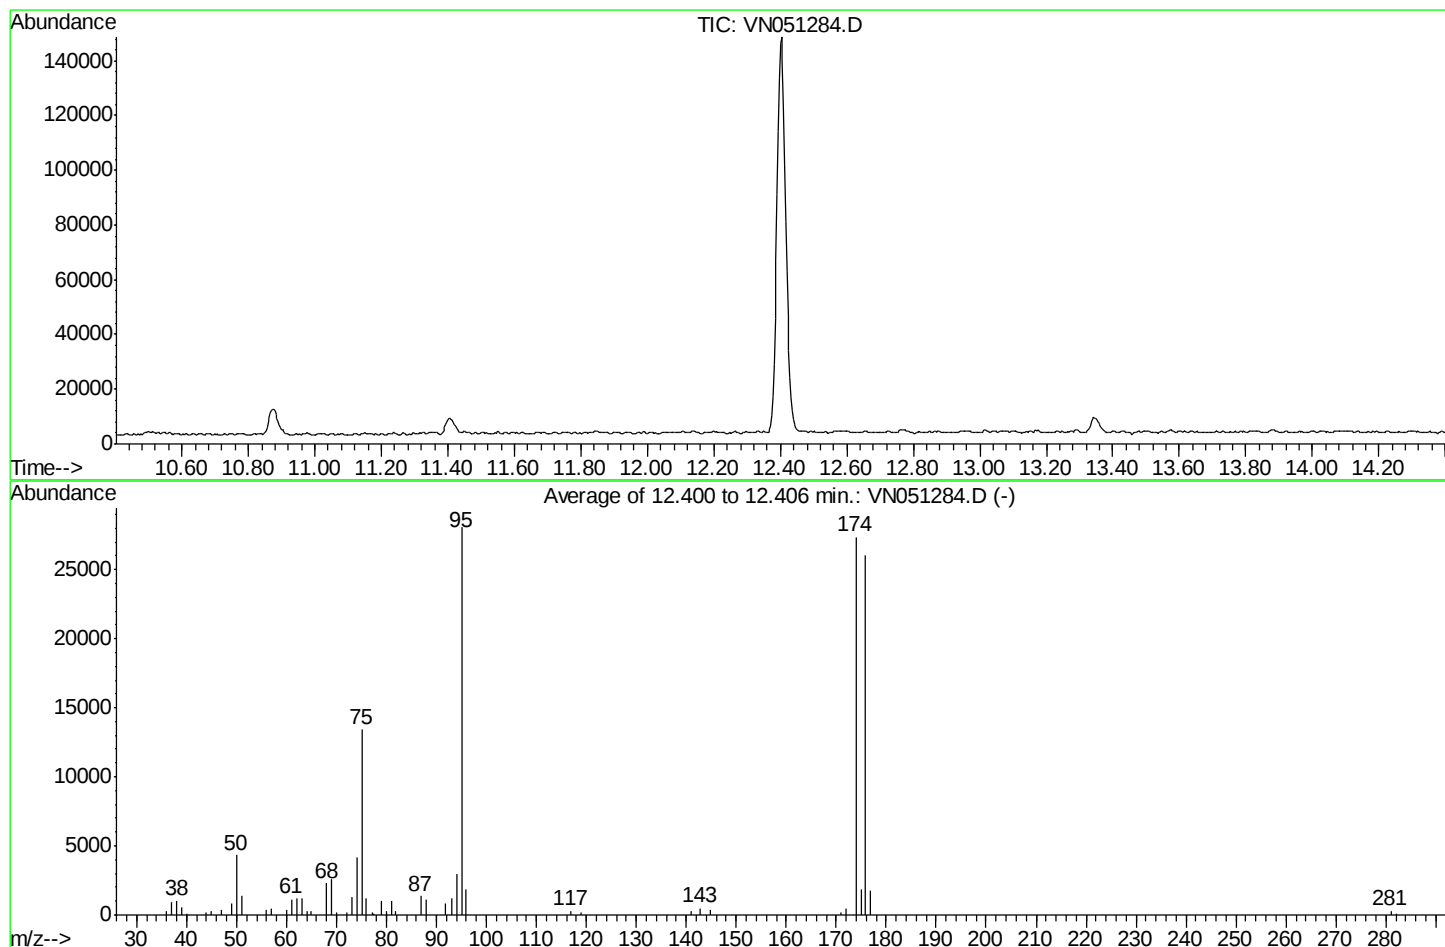

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	4350	PASS
75	95	30	60	47.8	13404	PASS
95	95	100	100	100.0	28056	PASS
96	95	5	9	6.5	1829	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	97.5	27346	PASS
175	174	5	9	6.8	1872	PASS
176	174	95	101	95.1	26008	PASS
177	176	5	9	6.9	1790	PASS