
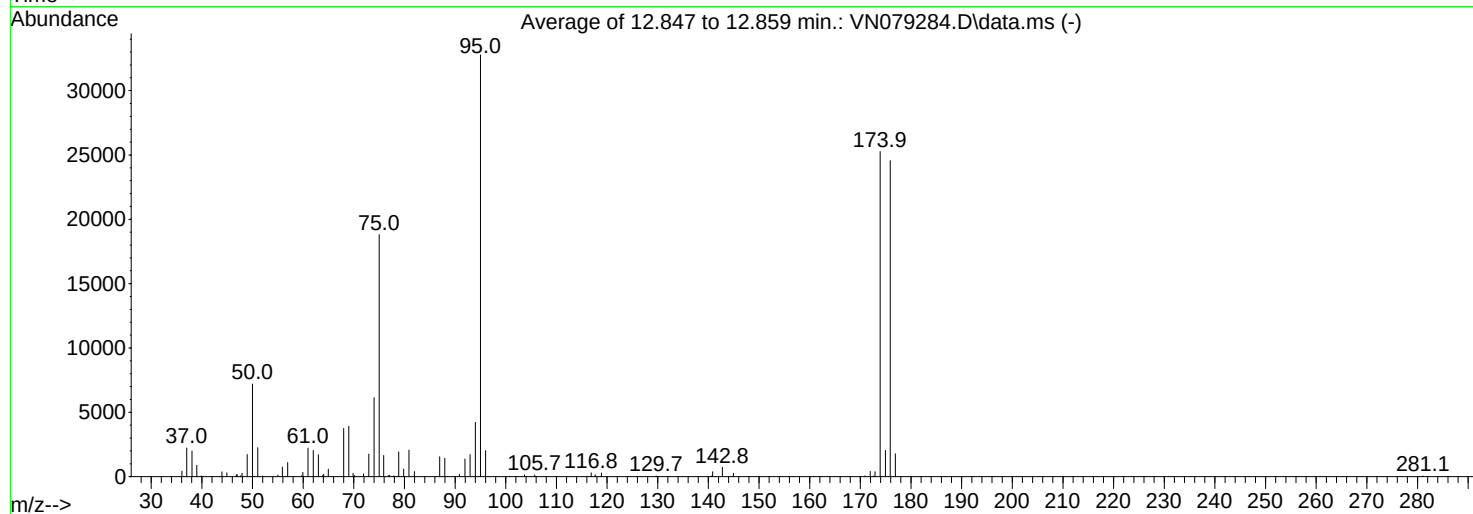


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091823\
Data File : VN079284.D
Acq On : 18 Sep 2023 11:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 05:05:24 2023

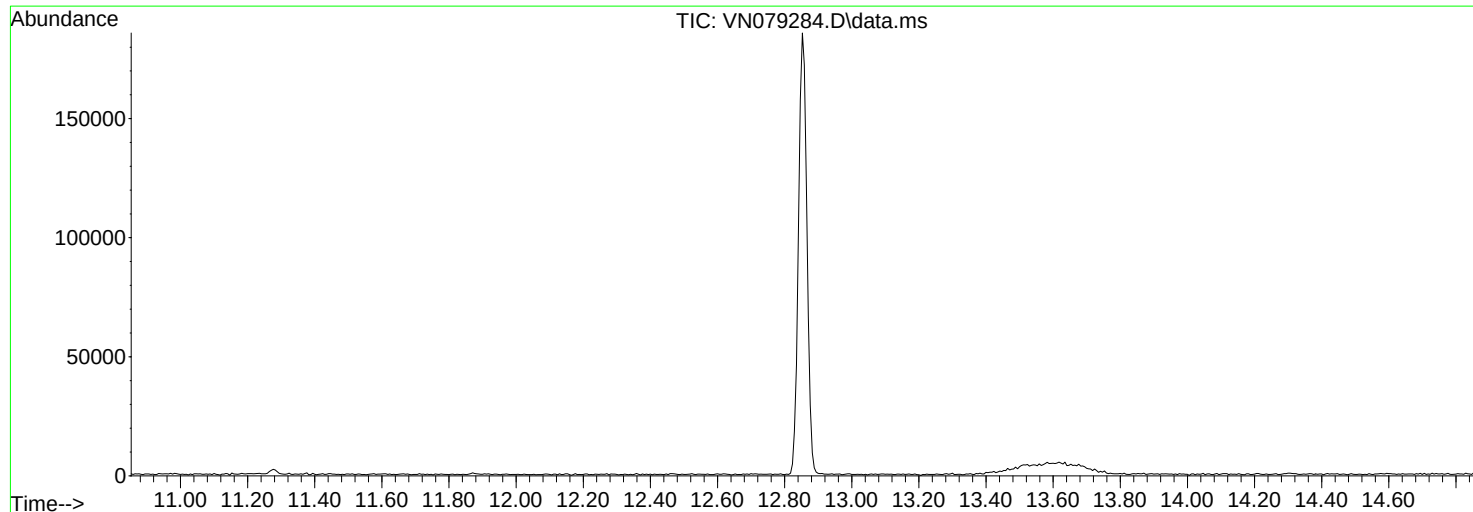

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	7205	PASS
75	95	30	60	57.4	18813	PASS
95	95	100	100	100.0	32781	PASS
96	95	5	9	6.2	2031	PASS
173	174	0.00	2	1.5	380	PASS
174	95	50	100	77.1	25269	PASS
175	174	5	9	8.1	2049	PASS
176	174	95	101	97.2	24563	PASS
177	176	5	9	7.2	1777	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	439	48.95	1717	63.00	1705	75.00	1881
37.00	2224	50.00	7205	63.80	88	75.90	1641
38.05	1987	51.05	2251	64.05	184	76.80	8
39.00	887	52.00	57	64.95	588	77.05	11
39.90	62	55.00	121	68.00	3739	77.90	65
43.95	378	55.90	747	69.00	3913	78.85	1924
44.95	305	56.95	1098	69.85	258	79.85	584
46.80	142	59.70	78	70.10	87	80.90	2060
46.95	173	59.95	338	71.90	209	81.95	401
47.70	78	60.95	2213	72.95	1749	86.95	1544
47.95	264	62.00	2035	74.00	6148	87.95	1436

Average of 12.847 to 12.859 min.: VN079284.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.85	189	129.70	55	175.90	24563		
91.95	1383	140.60	52	176.90	1777		
92.95	1721	140.85	385	281.10	53		
94.00	4216	142.75	716				
95.00	32781	144.95	260				
96.00	2031	170.90	63				
103.70	139	171.95	417				
105.70	121	172.60	57				
116.85	296	172.90	380				
117.65	155	173.90	25269				
118.90	293	174.95	2049				

Instrument :

MSVOA_N

ClientSampleId :

BFB