

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091824\
 Data File : VN084006.D
 Acq On : 19 Sep 2024 02:58
 Operator : JC\MD
 Sample : VN0918MBL02
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0918MBL02

Quant Time: Sep 19 05:45:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 11 15:18:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	172858	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	296194	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	249652	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	109909	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	132782	50.944	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	101.880%
35) Dibromofluoromethane	8.165	113	94447	49.809	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.620%
50) Toluene-d8	10.565	98	350325	53.442	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	106.880%
62) 4-Bromofluorobenzene	12.847	95	134867	49.867	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	99.740%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091824\
Data File : VN084006.D
Acq On : 19 Sep 2024 02:58
Operator : JC\MD
Sample : VN0918MBL02
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0918MBL02

Quant Time: Sep 19 05:45:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 11 15:18:56 2024
Response via : Initial Calibration




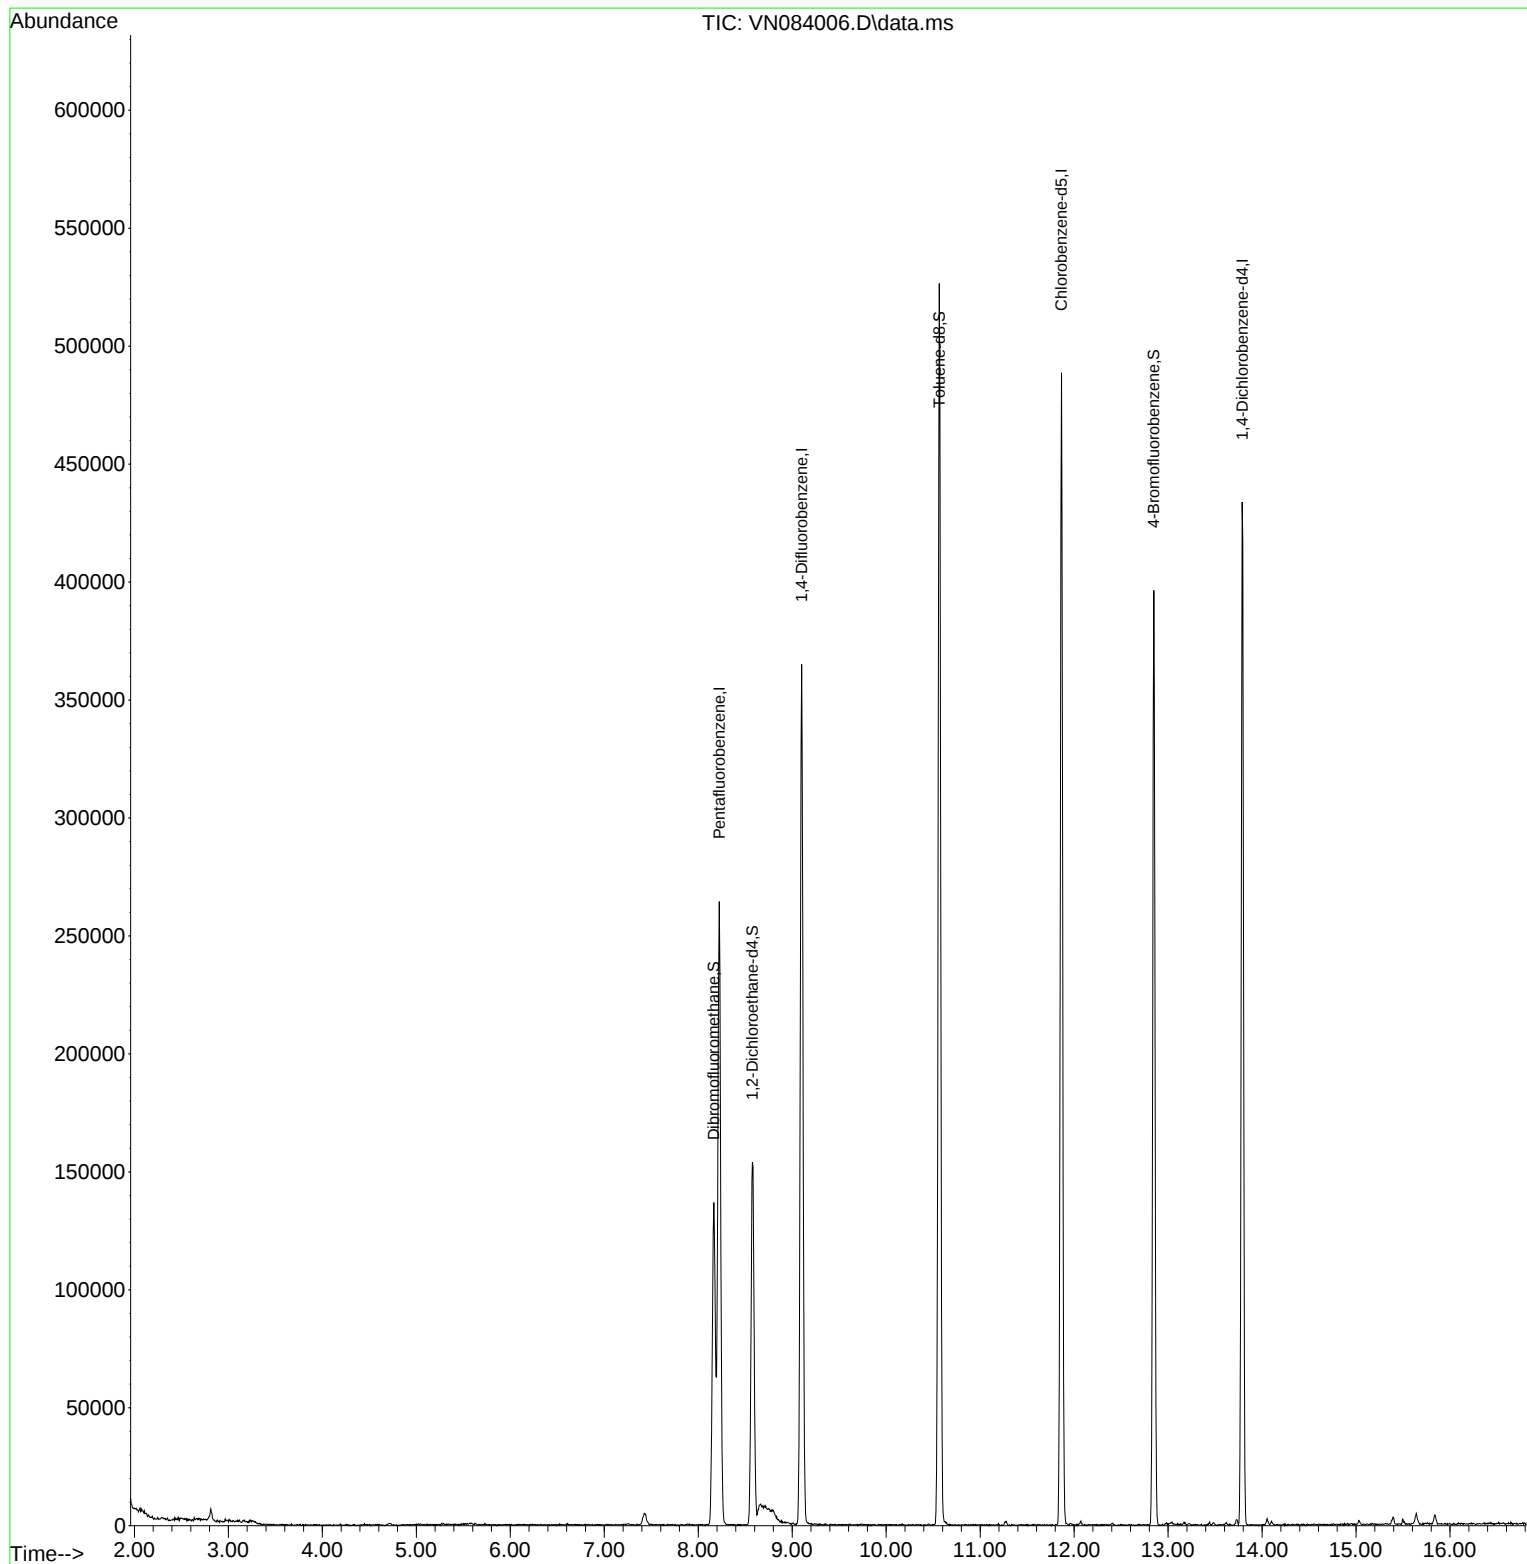


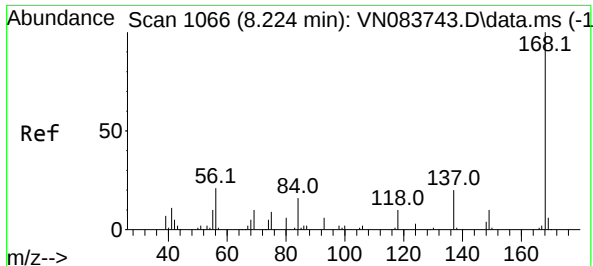

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN084006.D
Acq: 19 Sep 2024 02:58




Instrument :
MSVOA_N
ClientSampleId :
VN0918MBL02

Tgt Ion:168 Resp: 172858
Ion Ratio Lower Upper
168 100
99 70.5 54.2 81.2

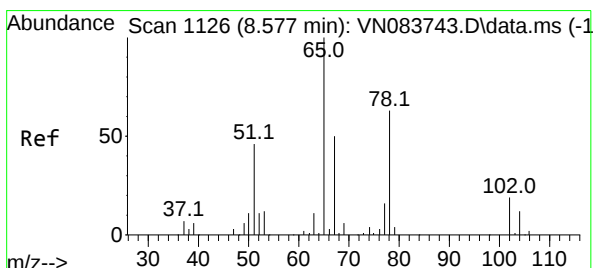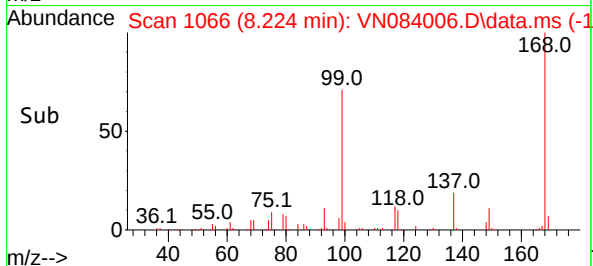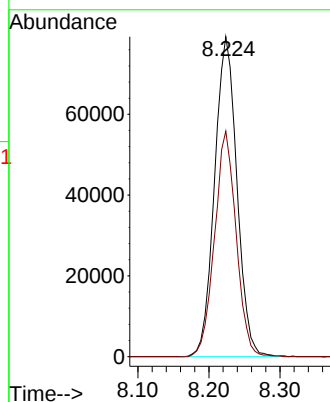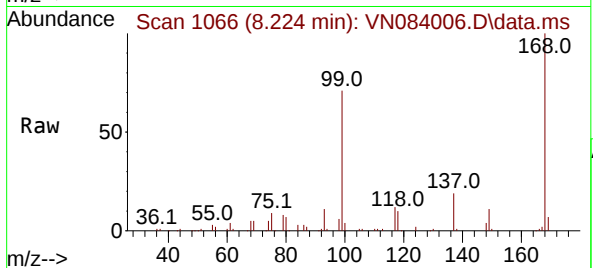

#33
1,2-Dichloroethane-d4
Concen: 50.944 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN084006.D
Acq: 19 Sep 2024 02:58

Tgt Ion: 65 Resp: 132782
Ion Ratio Lower Upper
65 100
67 49.7 0.0 100.8

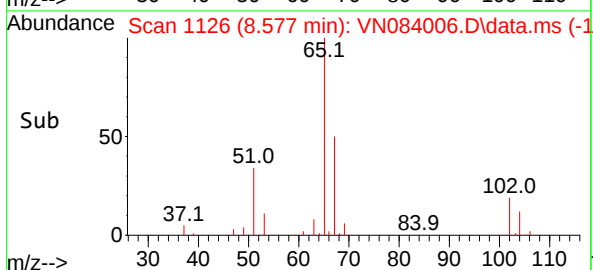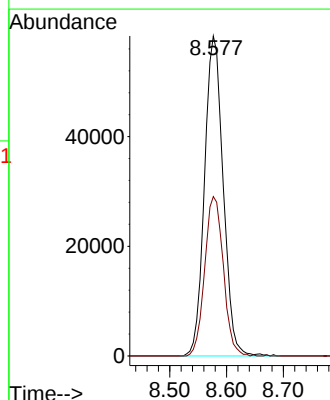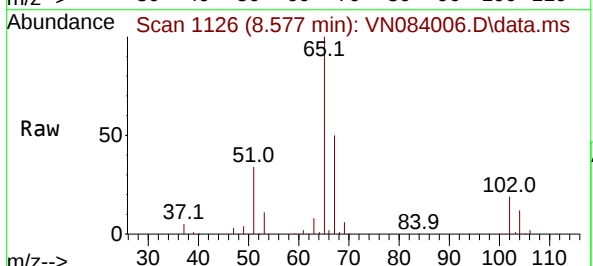



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. 0.000 min

Lab File: VN084006.D

Acq: 19 Sep 2024 02:58

Instrument :

MSVOA_N

ClientSampleId :

VN0918MBL02




Tgt Ion:114 Resp: 296194

Ion Ratio Lower Upper

114 100

63 21.8 0.0 43.4

88 18.1 0.0 32.6

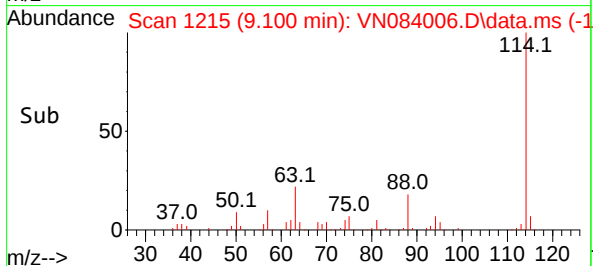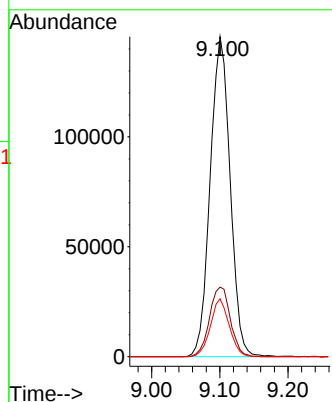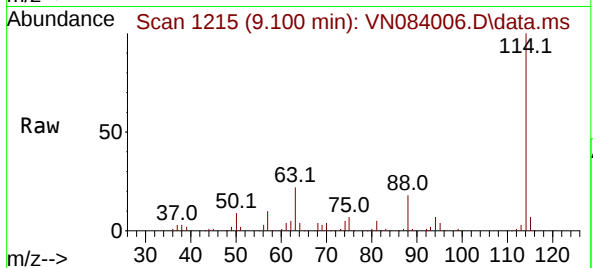

#35

Dibromofluoromethane

Concen: 49.809 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN084006.D

Acq: 19 Sep 2024 02:58




Tgt Ion:113 Resp: 94447


Ion Ratio Lower Upper

113 100

111 104.0 82.6 124.0

192 16.7 14.3 21.5


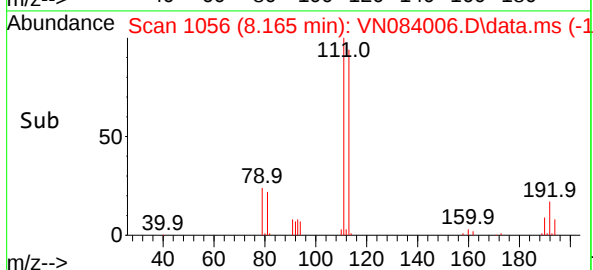
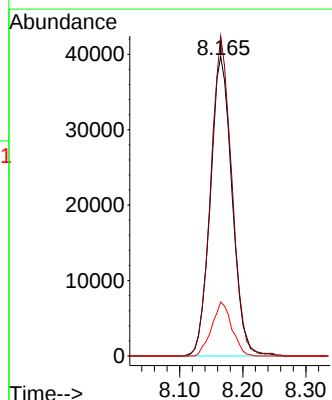
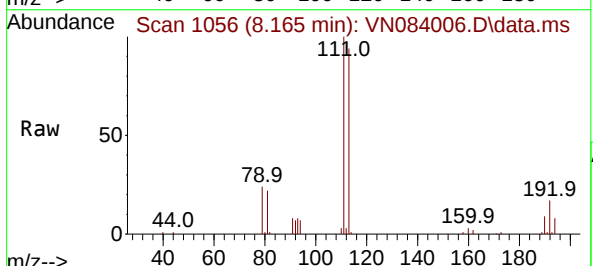


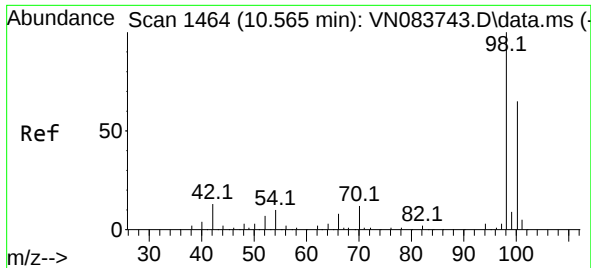

#50
Toluene-d8
Concen: 53.442 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN084006.D
Acq: 19 Sep 2024 02:58




Instrument :
MSVOA_N
ClientSampleId :
VN0918MBL02


Tgt Ion: 98 Resp: 350325
Ion Ratio Lower Upper
98 100
100 64.8 52.0 78.0

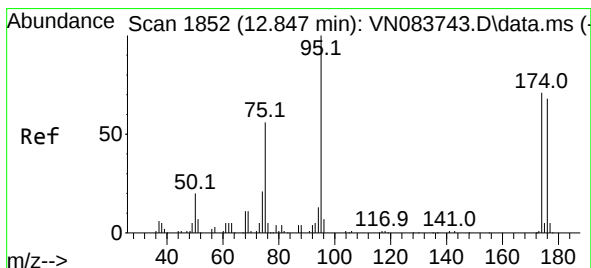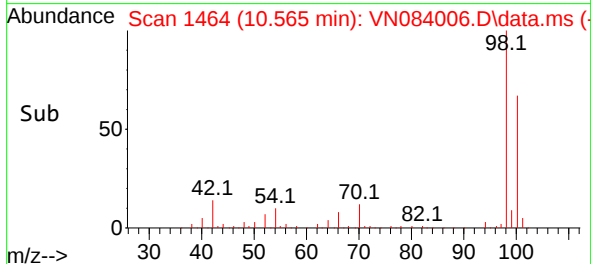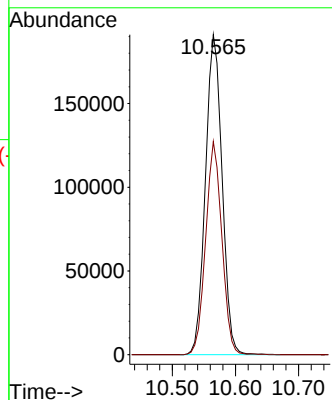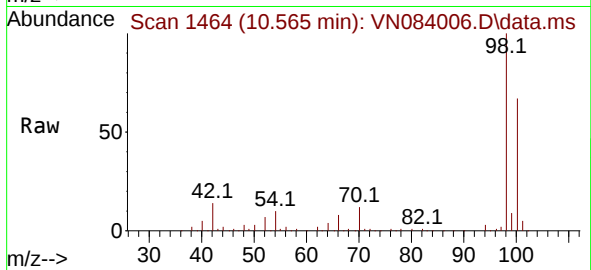

#62
4-Bromofluorobenzene
Concen: 49.867 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN084006.D
Acq: 19 Sep 2024 02:58

Tgt Ion: 95 Resp: 134867
Ion Ratio Lower Upper
95 100
174 69.5 0.0 139.8
176 66.1 0.0 131.4


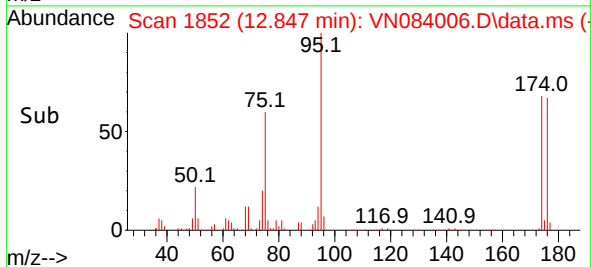
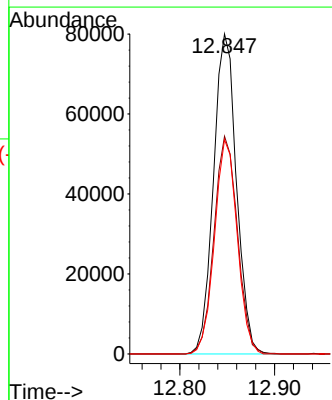
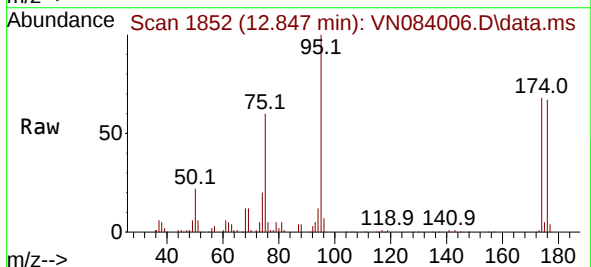


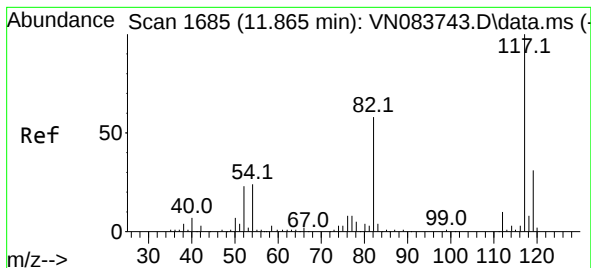

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN084006.D
Acq: 19 Sep 2024 02:58

Instrument :
MSVOA_N
ClientSampleId :
VN0918MBL02

Tgt Ion:117 Resp: 249652
Ion Ratio Lower Upper
117 100
82 62.0 47.4 71.0
119 33.2 26.3 39.5

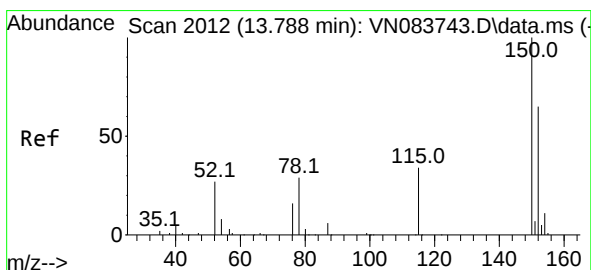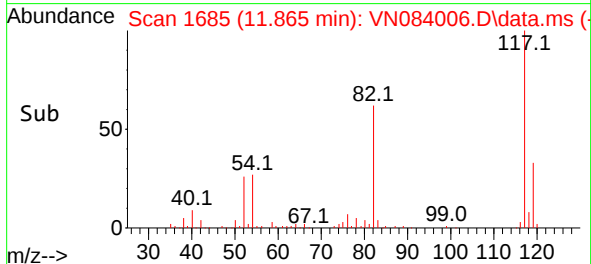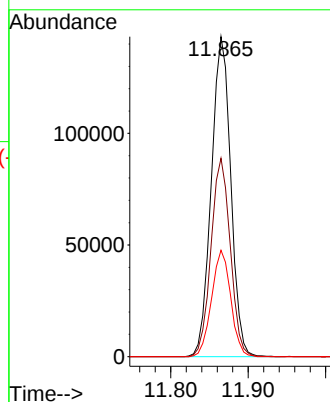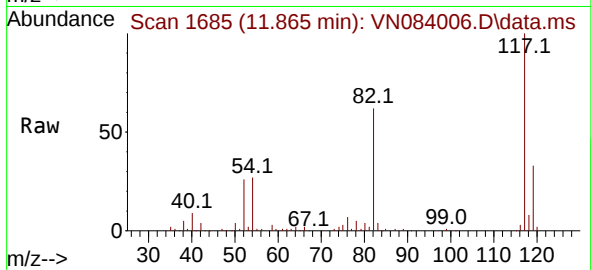

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. 0.000 min
Lab File: VN084006.D
Acq: 19 Sep 2024 02:58

Tgt Ion:152 Resp: 109909
Ion Ratio Lower Upper
152 100
115 63.6 32.2 96.6
150 157.9 0.0 348.6

