
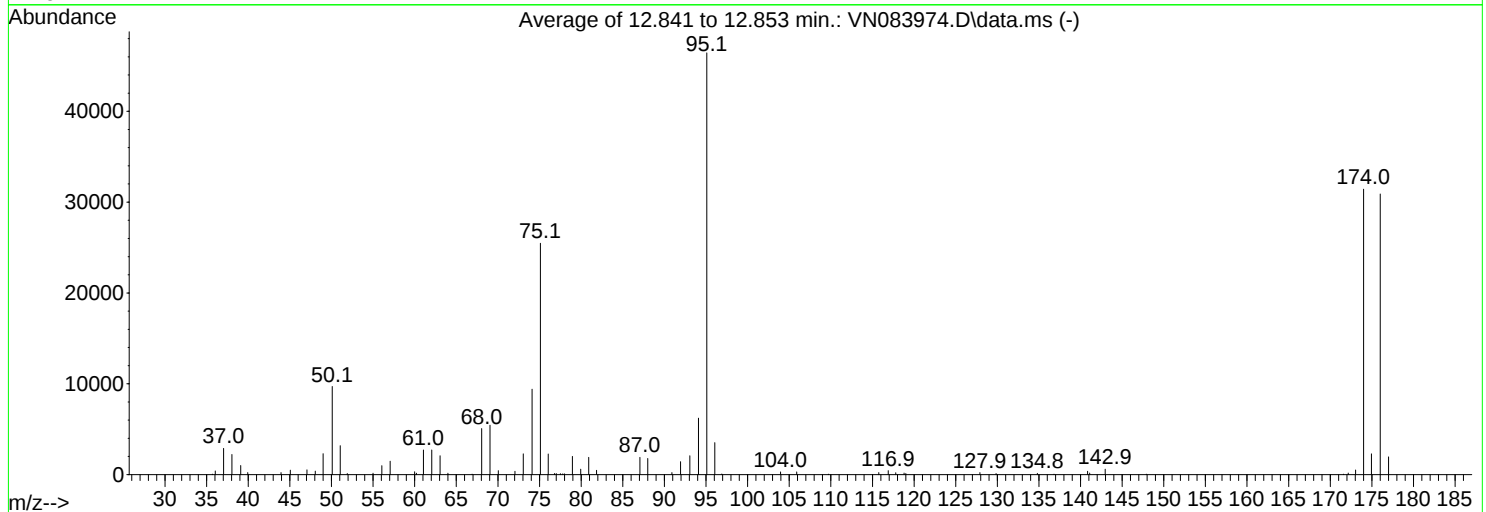


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091824\
Data File : VN083974.D
Acq On : 18 Sep 2024 11:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

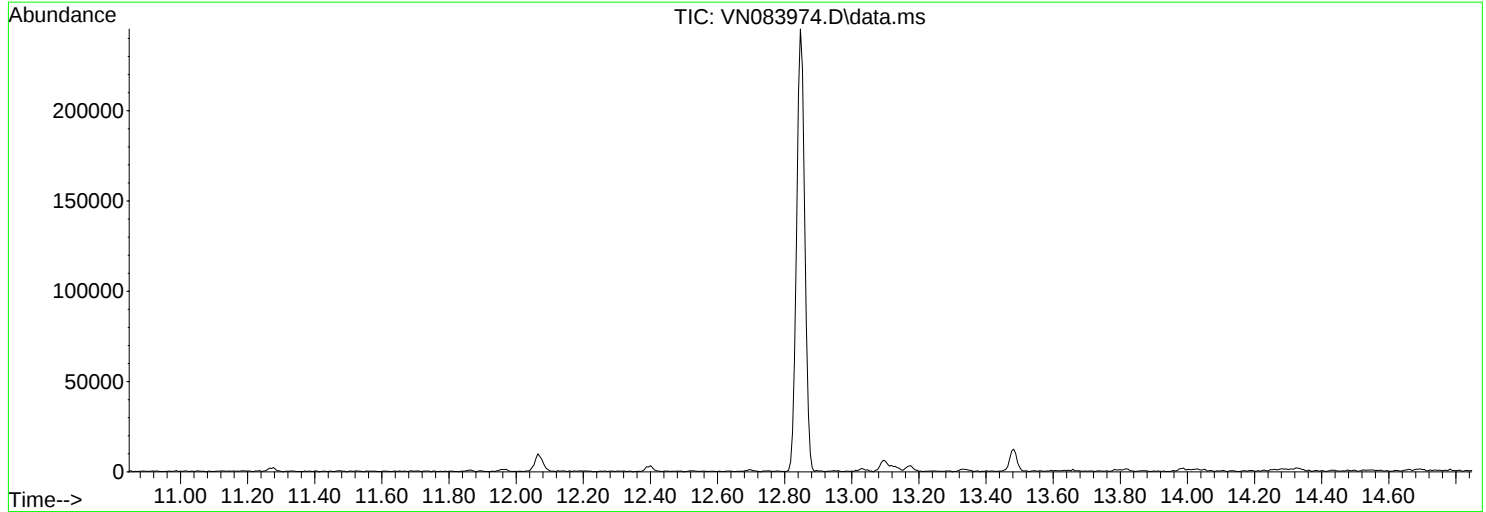

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	9712	PASS
75	95	30	60	54.9	25475	PASS
95	95	100	100	100.0	46437	PASS
96	95	5	9	7.6	3533	PASS
173	174	0.00	2	1.6	506	PASS
174	95	50	100	67.7	31429	PASS
175	174	5	9	7.3	2291	PASS
176	174	95	101	98.3	30904	PASS
177	176	5	9	6.4	1964	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.70	60	50.10	9712	64.00	154	77.00	121
36.05	402	51.05	3195	66.90	56	77.50	101
37.05	2898	51.90	121	68.05	5069	77.80	8
38.05	2220	55.00	156	69.05	5449	78.00	8
39.10	1013	56.05	992	70.05	447	78.95	2012
39.95	223	57.05	1479	72.05	378	79.95	609
43.95	237	60.00	312	73.05	2289	80.90	1908
45.05	501	60.20	164	74.10	9408	81.85	472
47.05	537	61.05	2723	75.10	25475	87.05	1907
48.05	382	62.05	2710	76.05	2279	88.00	1775
49.00	2301	63.05	2079	76.80	129	90.90	238

Average of 12.841 to 12.853 min.: VN083974.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.95	1420	117.80	216	171.60	60		
93.05	2087	118.80	175	172.15	173		
94.10	6222	119.00	124	173.05	506		
95.10	46437	127.90	229	174.00	31429		
96.05	3533	129.85	118	174.95	2291		
96.90	73	134.80	147	176.00	30904		
103.95	309	136.80	55	177.00	1964		
105.90	305	140.85	372				
109.70	62	141.10	176				
115.75	228	142.95	600				
116.90	441	147.90	51				

Instrument :

MSVOA_N

ClientSampleId :

BFB