
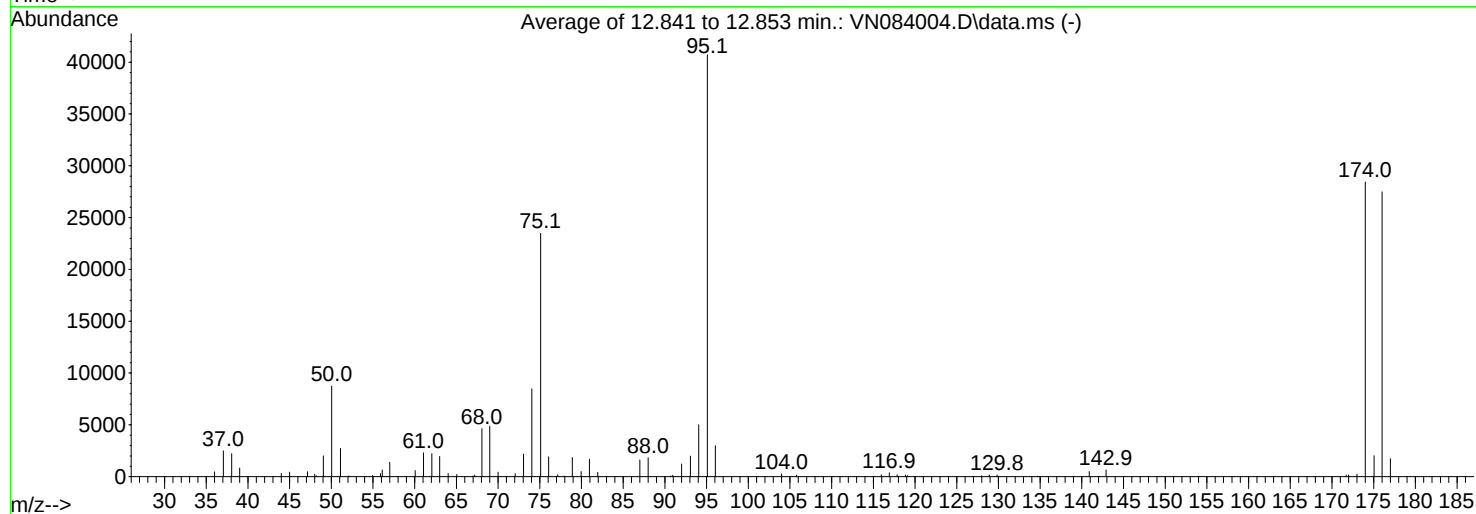


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091824\
Data File : VN084004.D
Acq On : 19 Sep 2024 01:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

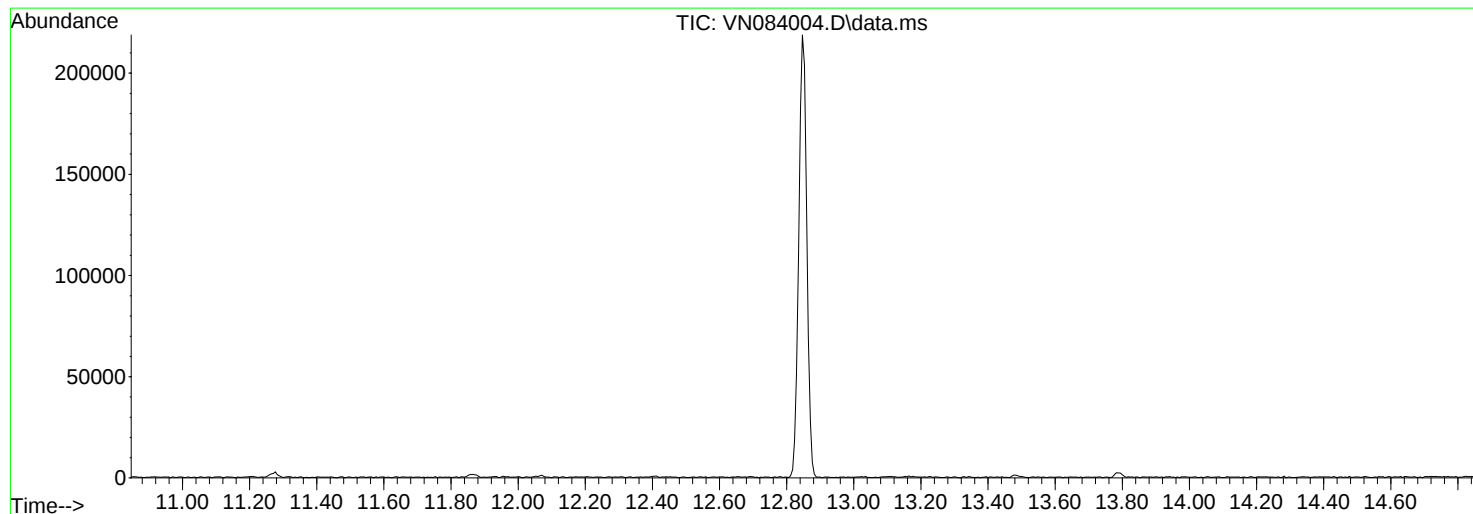

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	8740	PASS
75	95	30	60	57.7	23483	PASS
95	95	100	100	100.0	40707	PASS
96	95	5	9	7.3	2980	PASS
173	174	0.00	2	0.9	252	PASS
174	95	50	100	69.8	28427	PASS
175	174	5	9	7.1	2024	PASS
176	174	95	101	96.7	27491	PASS
177	176	5	9	6.3	1733	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	460	51.10	2713	65.05	224	77.15	191
37.05	2482	52.10	75	67.00	56	77.90	60
38.05	2213	54.95	111	67.20	143	78.90	183
39.00	834	55.90	288	68.05	4633	79.95	50
44.00	315	56.10	644	69.00	4869	80.95	1690
45.00	438	57.00	1368	70.00	434	81.95	412
47.15	476	60.05	584	72.05	297	87.00	1603
48.00	234	61.05	2295	73.05	2180	88.00	1828
48.20	73	62.05	2221	74.05	8483	90.70	59
49.05	2007	63.00	1952	75.10	23483	90.95	139
50.05	8740	64.00	307	76.05	1912	92.00	1218

Average of 12.841 to 12.853 min.: VN084004.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.05	1977	128.00	81	176.00	27491		
94.05	5000	128.90	156	177.00	1733		
95.10	40707	129.85	173				
96.05	2980	134.70	52				
104.00	258	140.90	502				
105.80	147	142.90	648				
115.95	190	171.70	150				
116.90	368	172.00	177				
117.85	190	173.00	252				
118.85	162	174.00	28427				
119.10	94	175.05	2024				

Instrument :

MSVOA_N

ClientSampleId :

BFB