
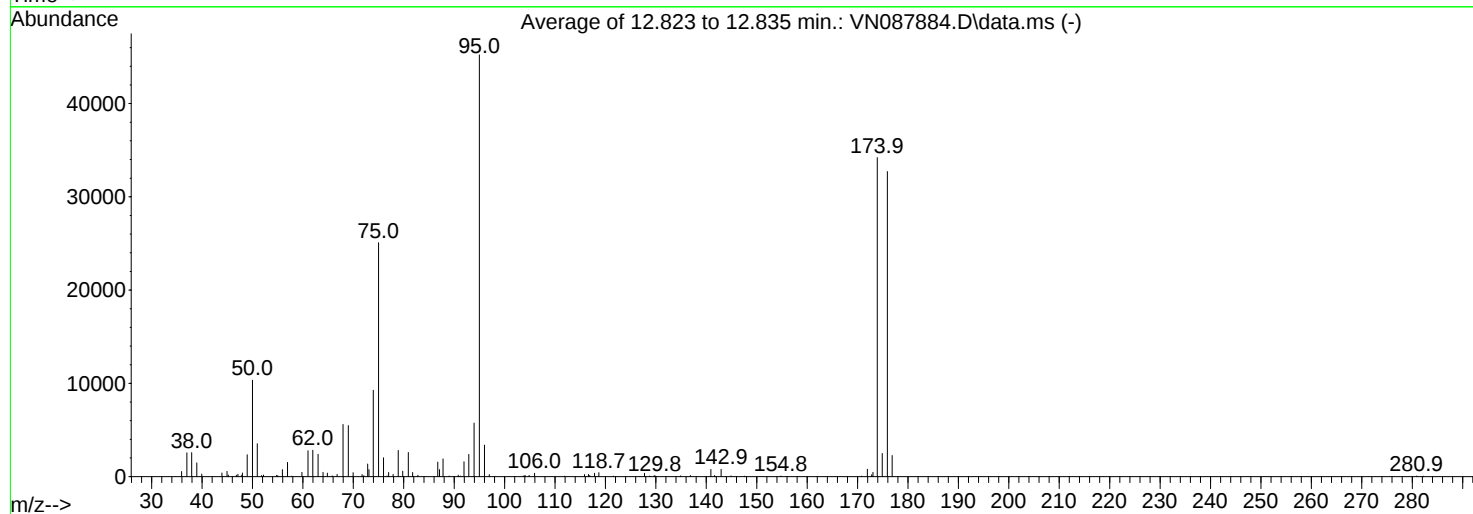


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN091825\  
Data File : VN087884.D  
Acq On : 18 Sep 2025 08:48  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N082125W.M  
Title : SW846 8260  
Last Update : Fri Aug 22 02:55:42 2025

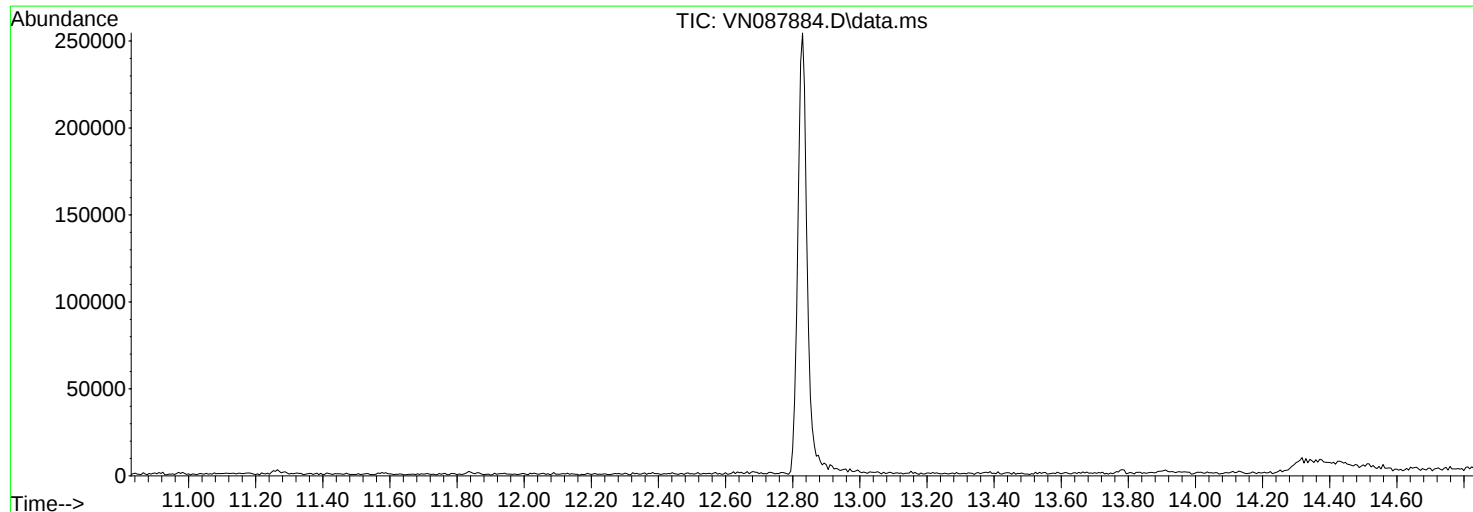

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1839

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 22.9  | 10345 | PASS      |
| 75     | 95      | 30     | 60     | 55.5  | 25088 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 45224 | PASS      |
| 96     | 95      | 5      | 9      | 7.5   | 3377  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.3   | 459   | PASS      |
| 174    | 95      | 50     | 100    | 75.7  | 34213 | PASS      |
| 175    | 174     | 5      | 9      | 7.3   | 2491  | PASS      |
| 176    | 174     | 95     | 101    | 95.6  | 32717 | PASS      |
| 177    | 176     | 5      | 9      | 6.9   | 2267  | PASS      |

Average of 12.823 to 12.835 min.: VN087884.D\data.ms

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 35.95 | 554    | 48.00 | 398    | 59.80 | 457    | 71.75 | 221    |
| 37.00 | 2553   | 48.95 | 2347   | 61.00 | 2772   | 72.10 | 107    |
| 37.95 | 2573   | 50.00 | 10345  | 61.95 | 2826   | 72.85 | 135    |
| 38.95 | 1473   | 50.95 | 3527   | 63.00 | 2407   | 73.10 | 75     |
| 39.95 | 281    | 51.80 | 125    | 64.00 | 468    | 73.95 | 9264   |
| 43.95 | 397    | 52.20 | 180    | 64.85 | 377    | 75.00 | 25088  |
| 44.95 | 571    | 54.80 | 147    | 65.80 | 79     | 76.00 | 2032   |
| 45.20 | 178    | 55.00 | 98     | 66.80 | 241    | 76.70 | 75     |
| 46.80 | 157    | 55.95 | 753    | 67.95 | 5589   | 77.00 | 439    |
| 47.10 | 265    | 56.95 | 1523   | 69.00 | 5467   | 77.90 | 234    |
| 47.80 | 120    | 57.80 | 58     | 69.95 | 431    | 78.90 | 2822   |

Average of 12.823 to 12.835 min.: VN087884.D\data.ms

BFB

Modified:subtracted

| m/z   | abund. | m/z    | abund. | m/z    | abund. | m/z    | abund. |
|-------|--------|--------|--------|--------|--------|--------|--------|
| 79.80 | 584    | 92.90  | 2384   | 115.85 | 233    | 136.85 | 127    |
| 80.90 | 2585   | 93.95  | 5755   | 116.65 | 239    | 140.90 | 774    |
| 81.75 | 450    | 95.00  | 45224  | 116.90 | 119    | 141.65 | 127    |
| 82.80 | 160    | 96.00  | 3377   | 117.85 | 364    | 142.95 | 791    |
| 86.75 | 1564   | 96.95  | 225    | 118.70 | 437    | 144.90 | 90     |
| 87.10 | 754    | 103.70 | 62     | 121.60 | 53     | 147.60 | 58     |
| 87.80 | 1906   | 103.90 | 99     | 127.75 | 355    | 154.80 | 65     |
| 89.00 | 65     | 104.10 | 103    | 128.80 | 73     | 170.80 | 52     |
| 90.80 | 158    | 104.85 | 132    | 129.60 | 71     | 171.95 | 799    |
| 91.20 | 76     | 105.95 | 365    | 129.80 | 124    | 172.80 | 211    |
| 91.95 | 1591   | 111.90 | 56     | 134.90 | 79     | 173.05 | 459    |

Average of 12.823 to 12.835 min.: VN087884.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z | abund. | m/z | abund. | m/z | abund. |
|--------|--------|-----|--------|-----|--------|-----|--------|
| 173.90 | 34213  |     |        |     |        |     |        |
| 174.90 | 2491   |     |        |     |        |     |        |
| 175.90 | 32717  |     |        |     |        |     |        |
| 176.85 | 2267   |     |        |     |        |     |        |
| 280.90 | 74     |     |        |     |        |     |        |
| 282.20 | 51     |     |        |     |        |     |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB