


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091919\
 Data File : VN058205.D
 Acq On : 19 Sep 2019 15:15
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091819W.M
 Title : SW846 8260
 Last Update : Thu Sep 19 09:27:53 2019

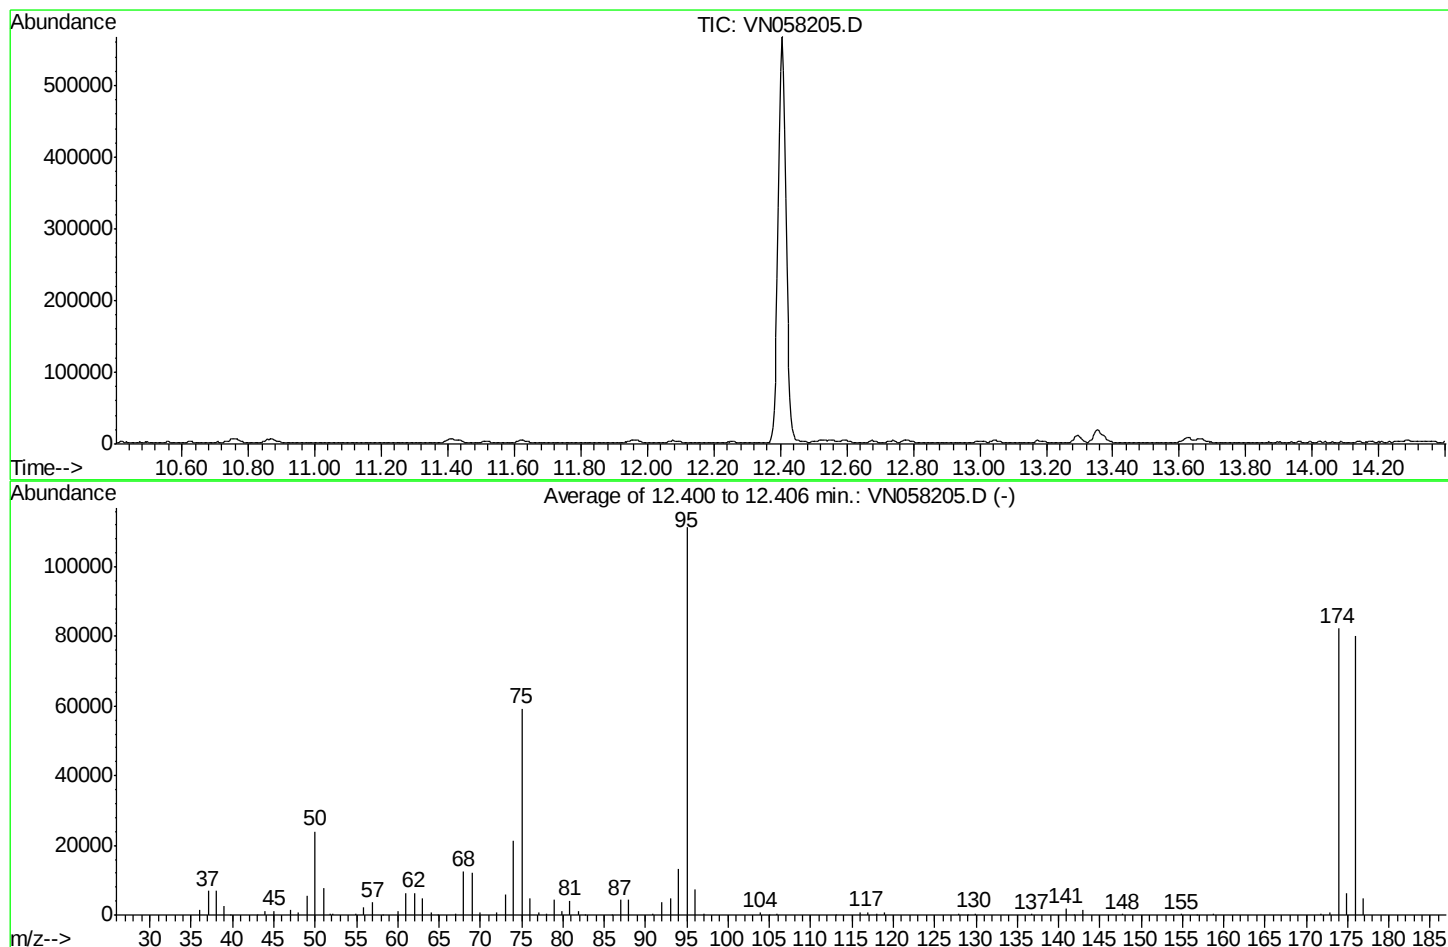

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	23928	PASS
75	95	30	60	53.2	59216	PASS
95	95	100	100	100.0	111370	PASS
96	95	5	9	6.6	7394	PASS
173	174	0.00	2	0.8	638	PASS
174	95	50	100	73.9	82330	PASS
175	174	5	9	7.7	6378	PASS
176	174	95	101	97.3	80138	PASS
177	176	5	9	6.2	4948	PASS