
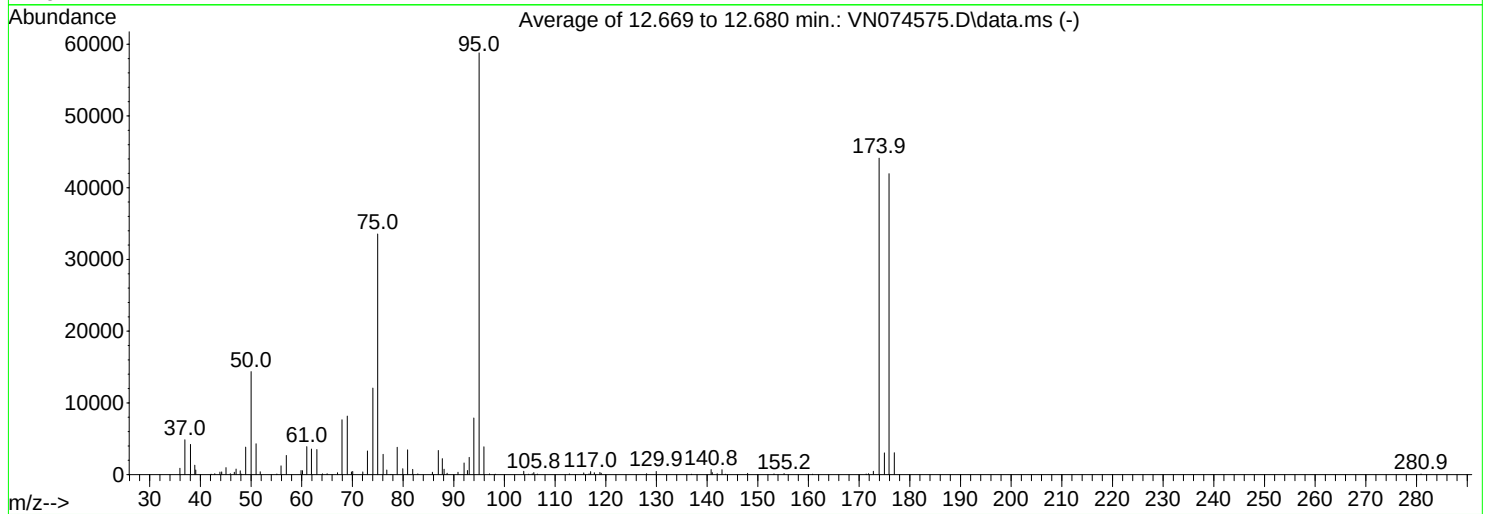


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091922\
Data File : VN074575.D
Acq On : 19 Sep 2022 09:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091522W.M
Title : SW846 8260
Last Update : Thu Sep 15 19:20:33 2022

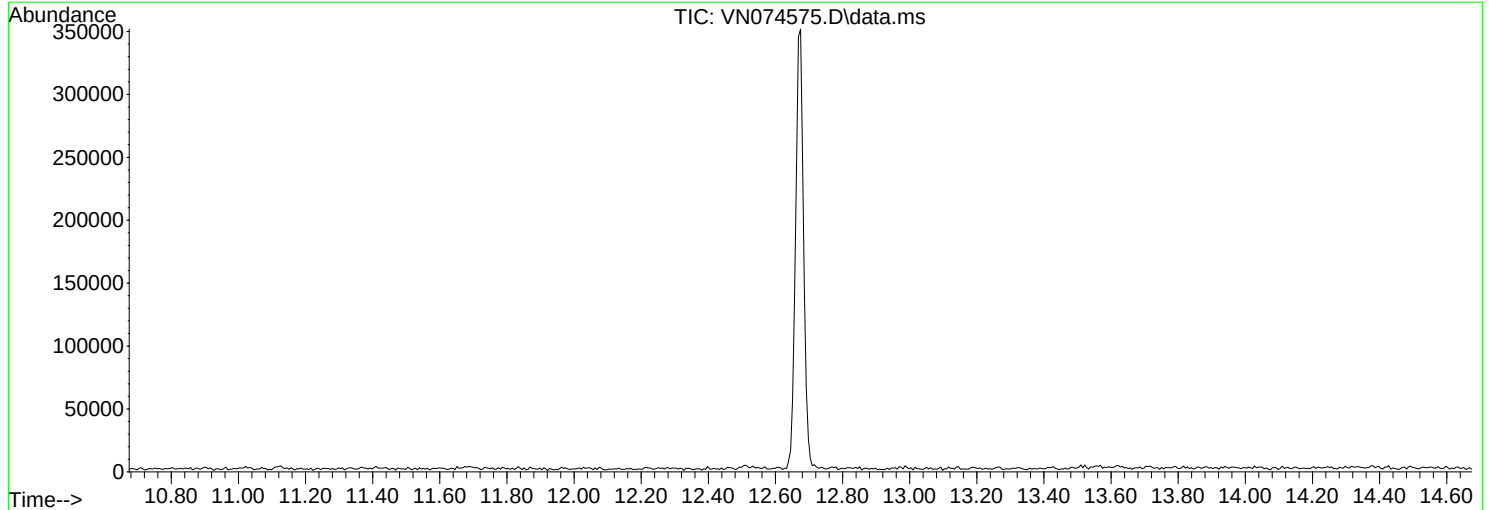

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.4	14374	PASS
75	95	30	60	57.1	33557	PASS
95	95	100	100	100.0	58797	PASS
96	95	5	9	6.6	3891	PASS
173	174	0.00	2	1.1	469	PASS
174	95	50	100	75.0	44117	PASS
175	174	5	9	6.9	3037	PASS
176	174	95	101	95.1	41947	PASS
177	176	5	9	7.3	3056	PASS