
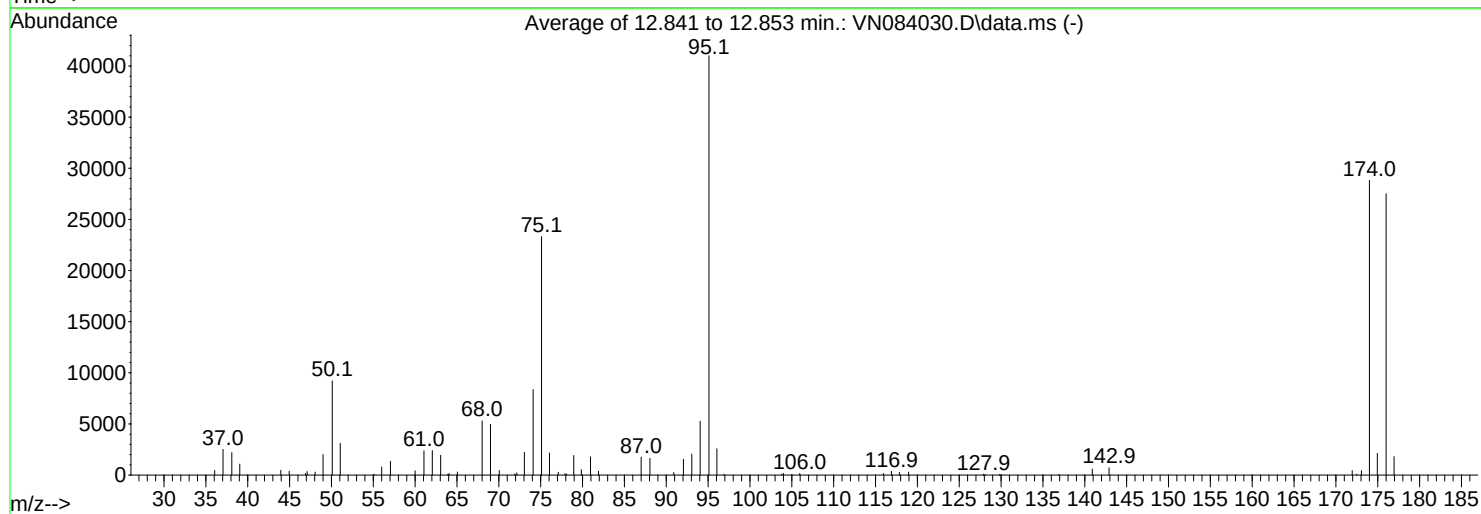


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091924\
Data File : VN084030.D
Acq On : 19 Sep 2024 12:56
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

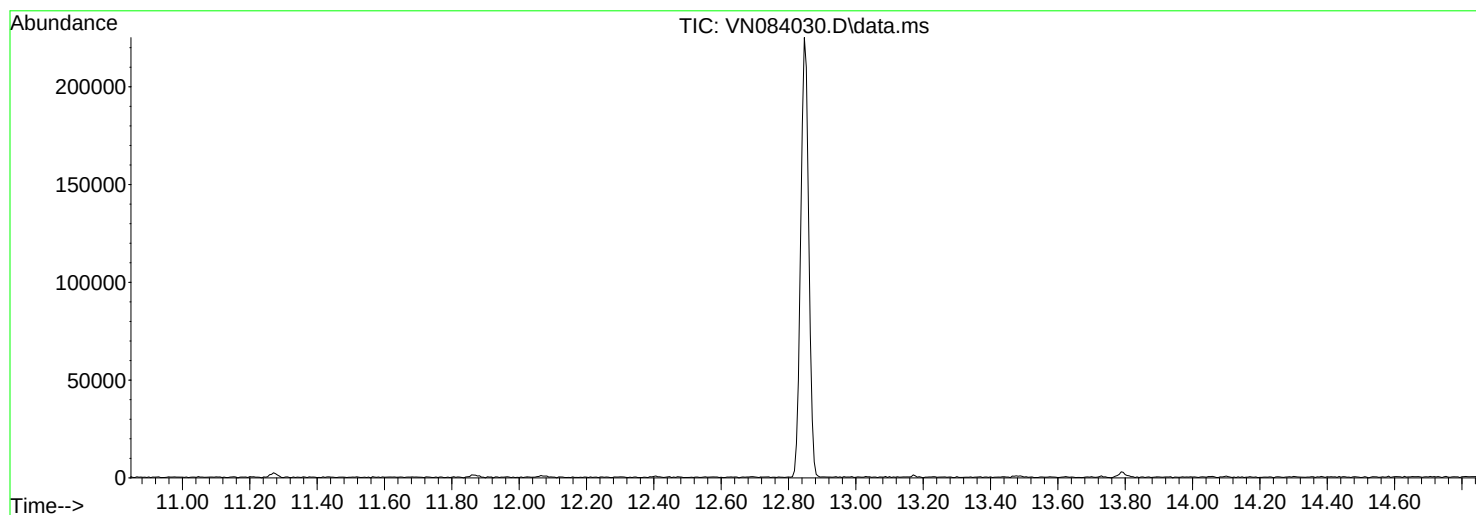

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	9209	PASS
75	95	30	60	56.9	23320	PASS
95	95	100	100	100.0	41005	PASS
96	95	5	9	6.3	2575	PASS
173	174	0.00	2	1.5	431	PASS
174	95	50	100	70.3	28816	PASS
175	174	5	9	7.4	2119	PASS
176	174	95	101	95.5	27512	PASS
177	176	5	9	6.6	1815	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	456	50.10	9209	65.05	303	77.90	140
37.05	2513	51.05	3097	68.00	5294	78.10	100
38.10	2199	55.10	90	69.00	4953	78.95	1915
39.05	1072	56.00	800	70.05	454	79.85	524
39.90	5	57.05	1354	71.90	108	80.95	1783
43.95	471	60.00	420	72.15	214	81.90	375
44.95	388	61.05	2380	73.05	2227	87.00	1751
46.90	174	62.05	2393	74.10	8367	88.05	1632
47.10	348	63.05	1928	75.10	23320	90.90	249
48.05	296	63.90	84	76.05	2164	92.05	1549
49.00	2009	64.05	154	77.10	273	93.05	2056

Average of 12.841 to 12.853 min.: VN084030.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	5260	118.95	287	174.00	28816		
95.10	41005	127.90	87	174.95	2119		
96.05	2575	128.10	58	176.00	27512		
96.90	78	129.80	70	176.95	1815		
103.80	91	130.00	66				
104.00	154	136.90	53				
105.00	56	140.90	591				
105.95	160	142.90	717				
115.95	155	171.95	437				
116.90	372	172.50	105				
117.85	257	173.05	431				

Instrument :

MSVOA_N

ClientSampleId :

BFB