



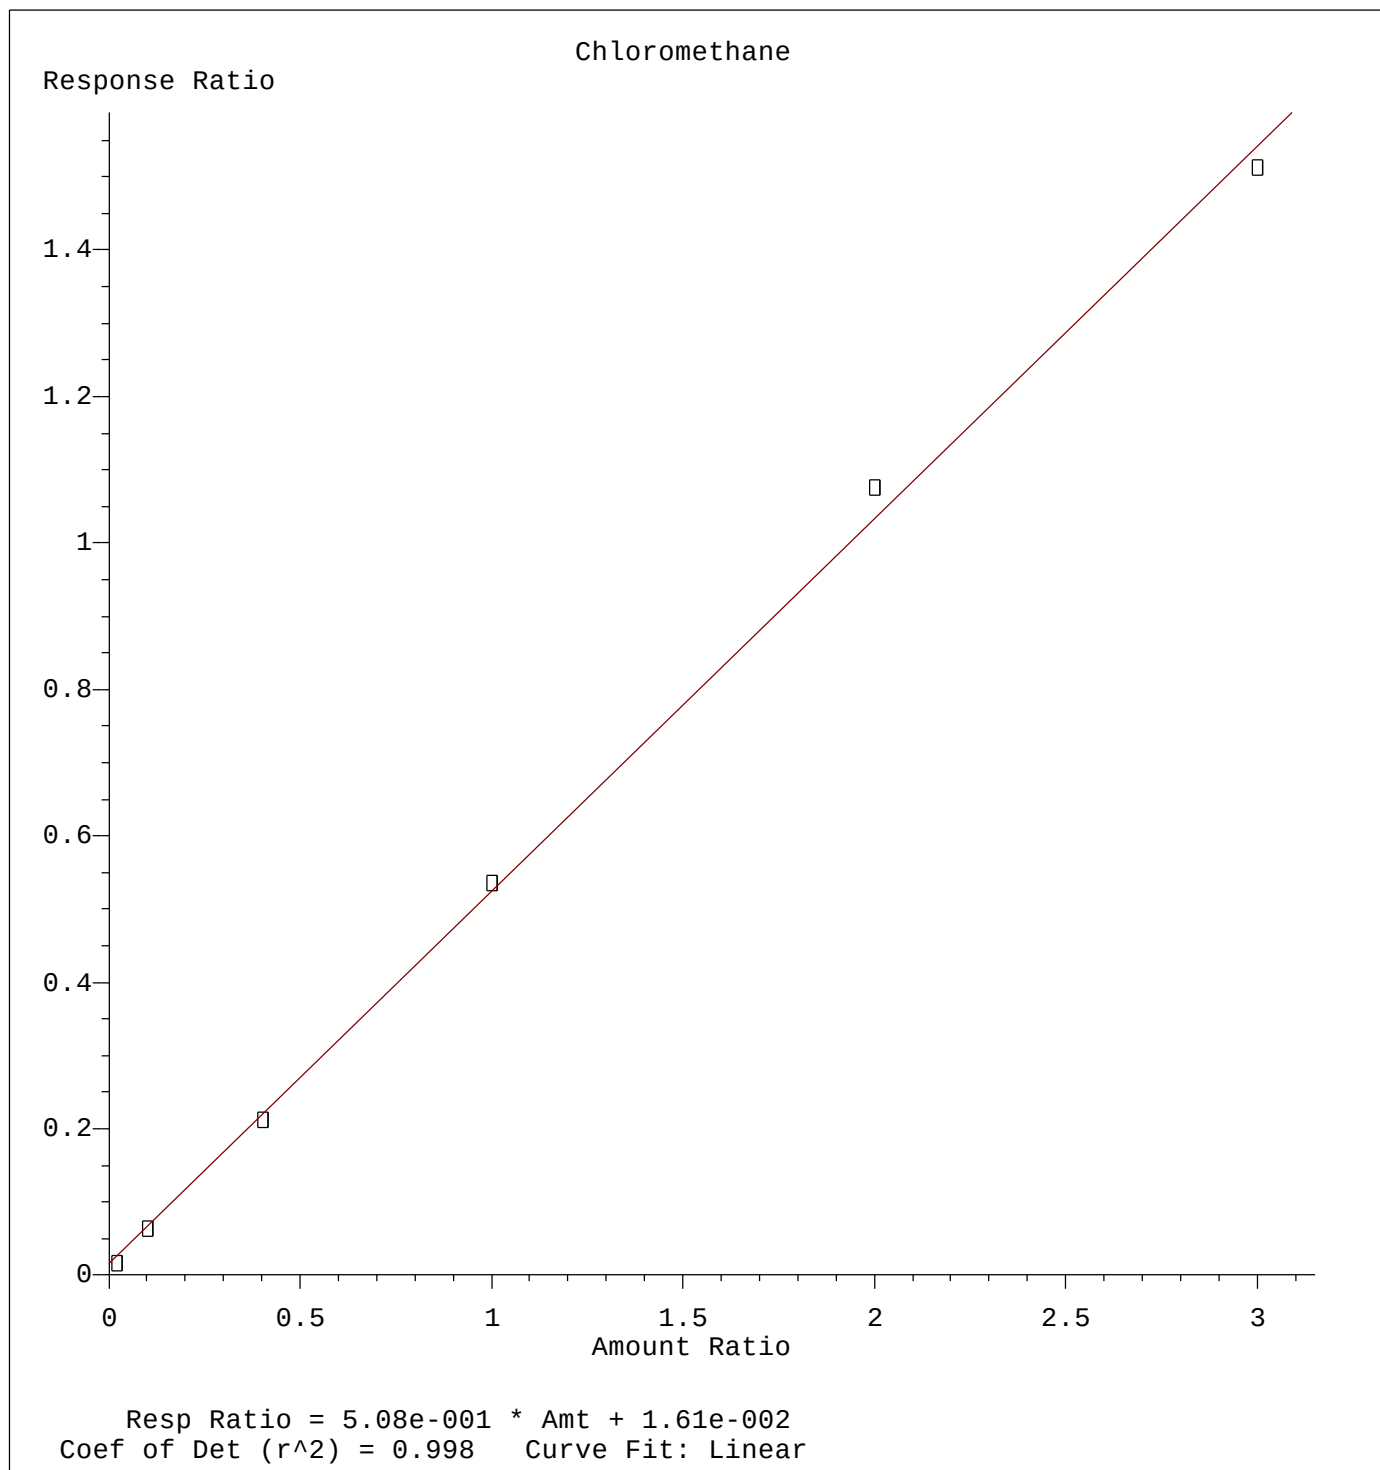

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018


1,2,3-Trichlorobenzene

Response Ratio

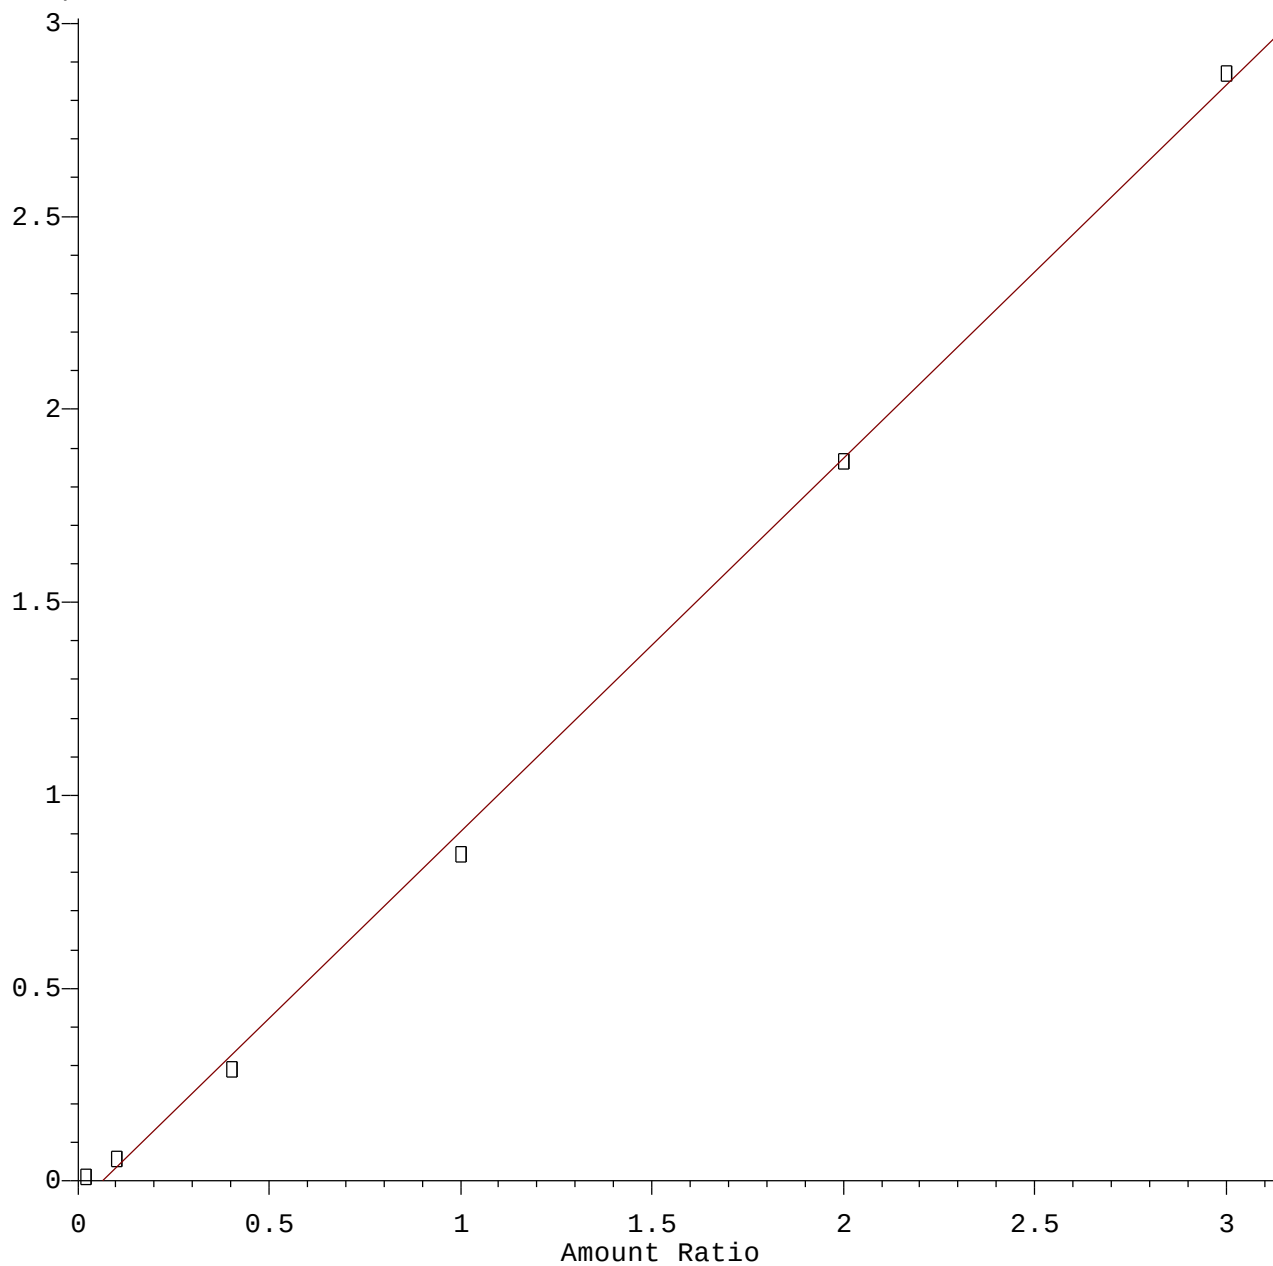

Resp Ratio = $9.67 \times 10^{-1} \times \text{Amt} - 6.28 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018

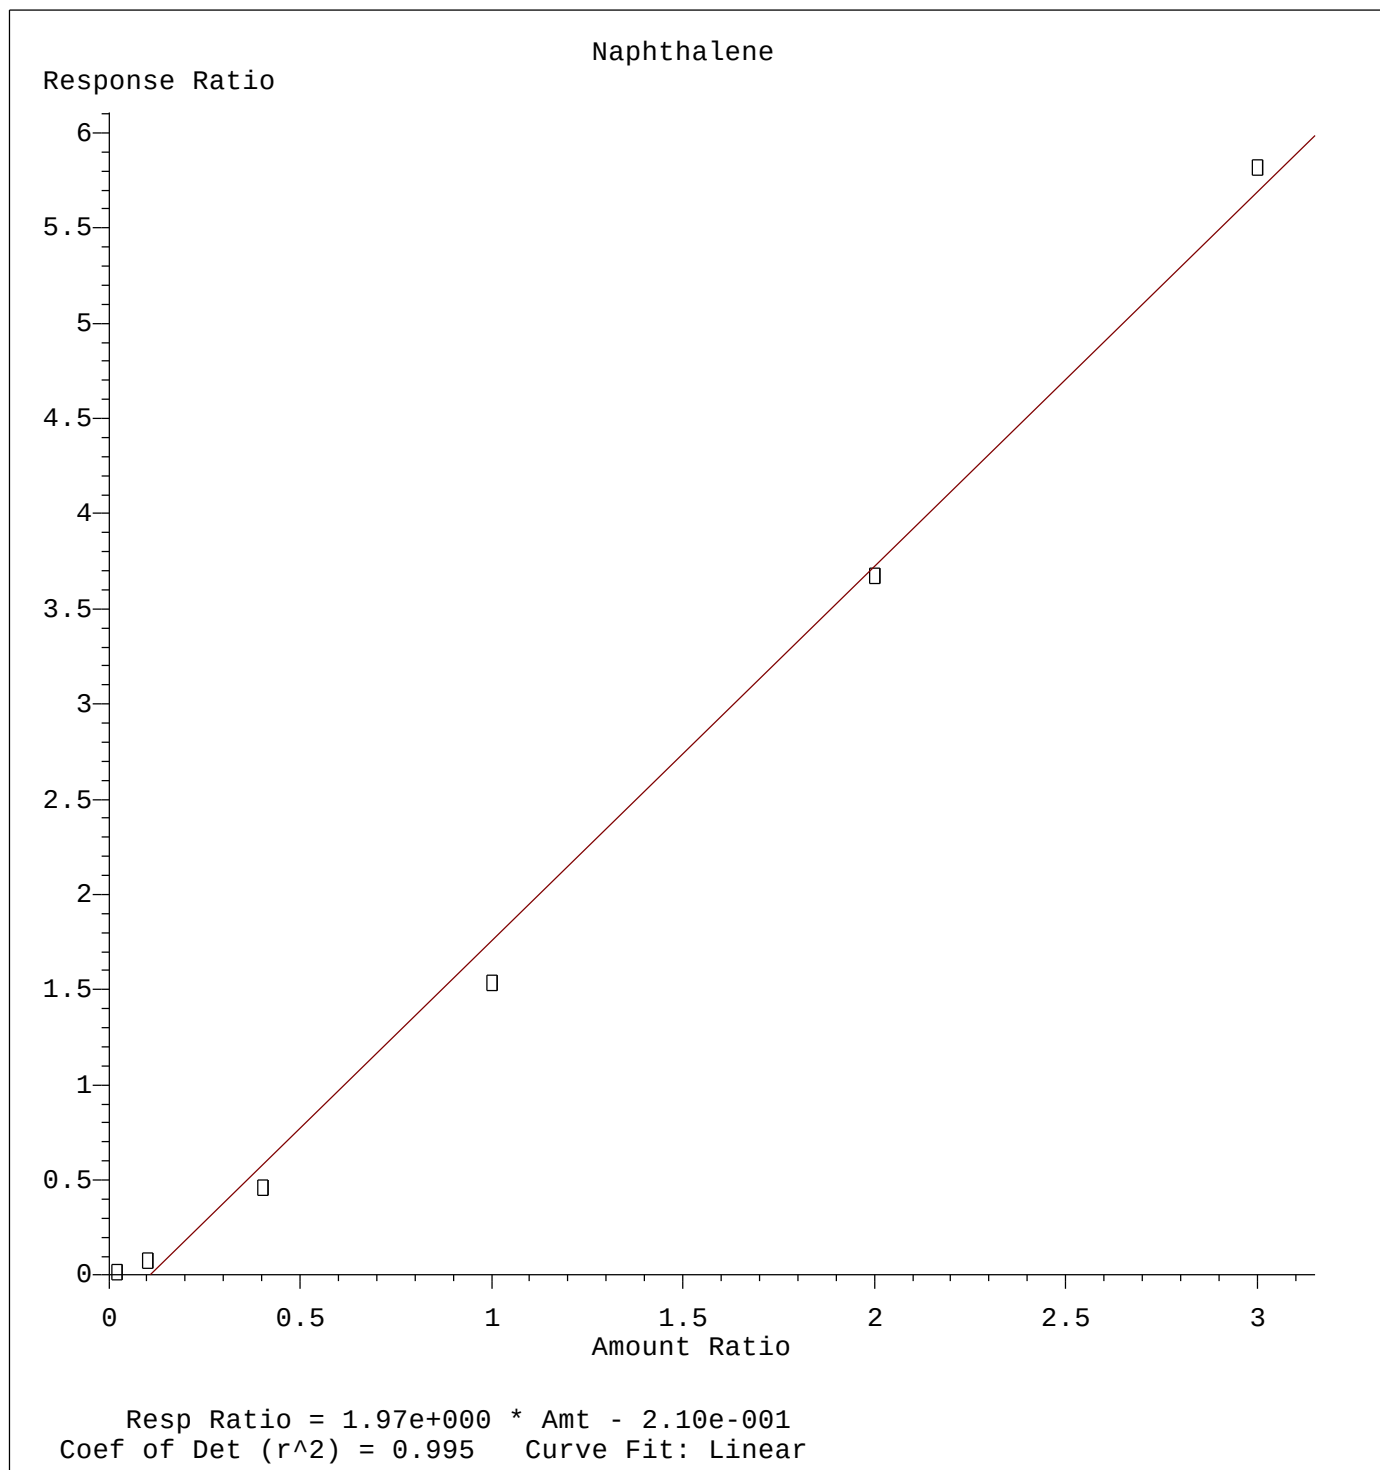

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018


1,2,4-Trichlorobenzene

Response Ratio

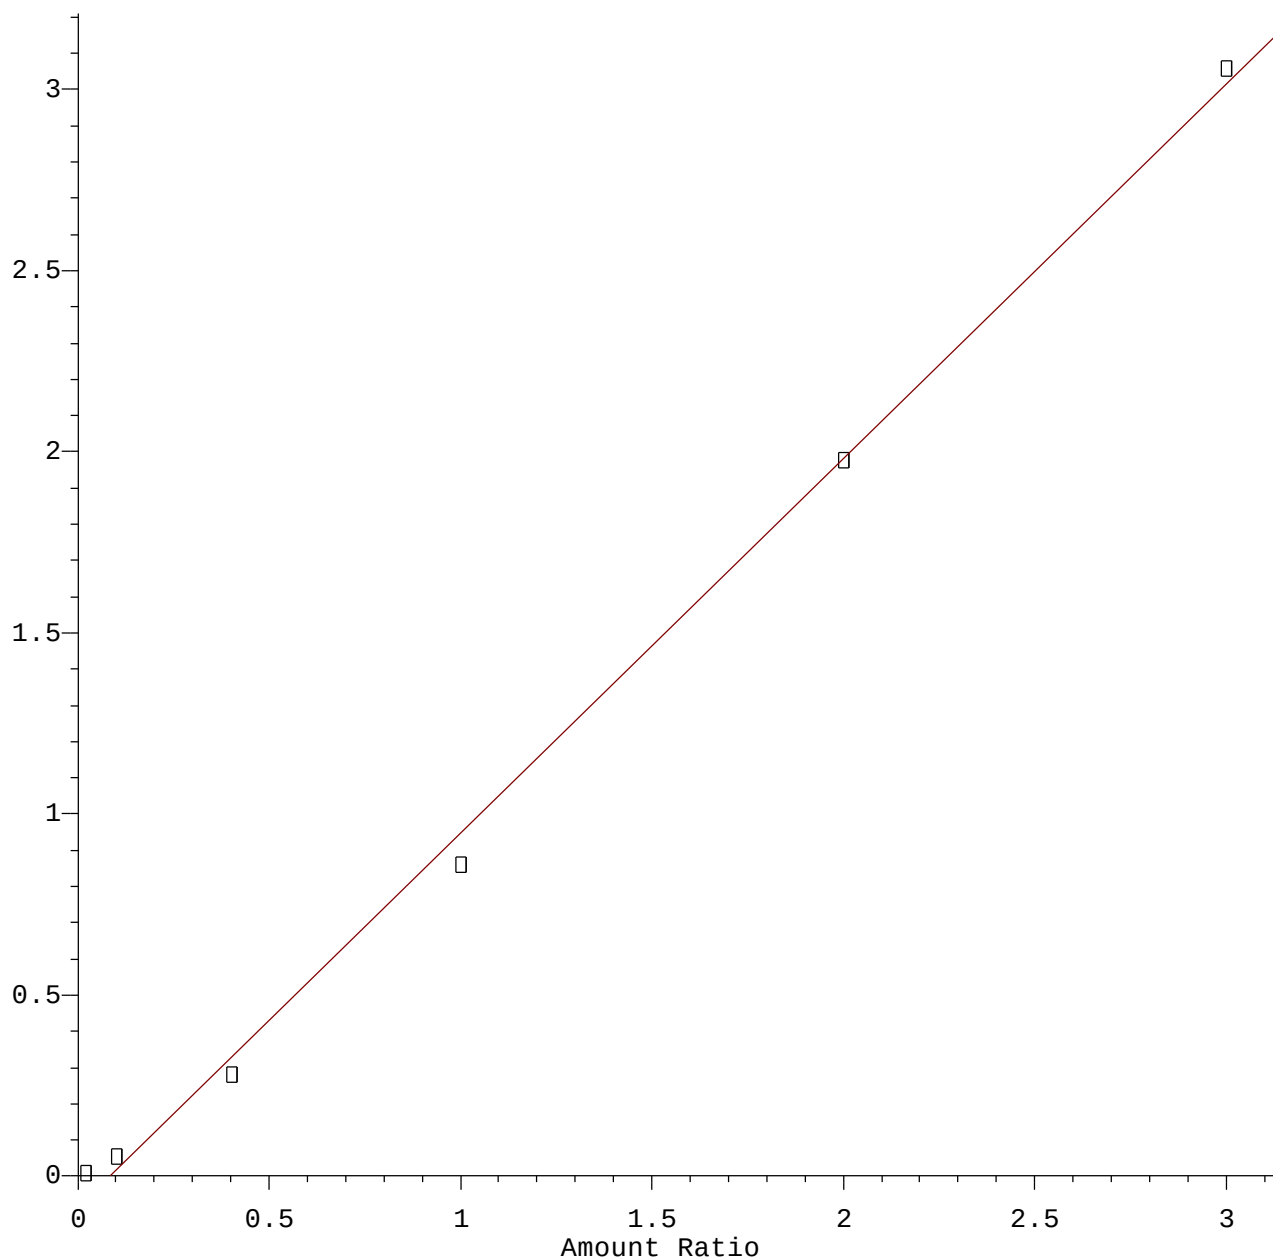

Resp Ratio = $1.03 \times 10^0 \times \text{Amt} - 8.47 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018

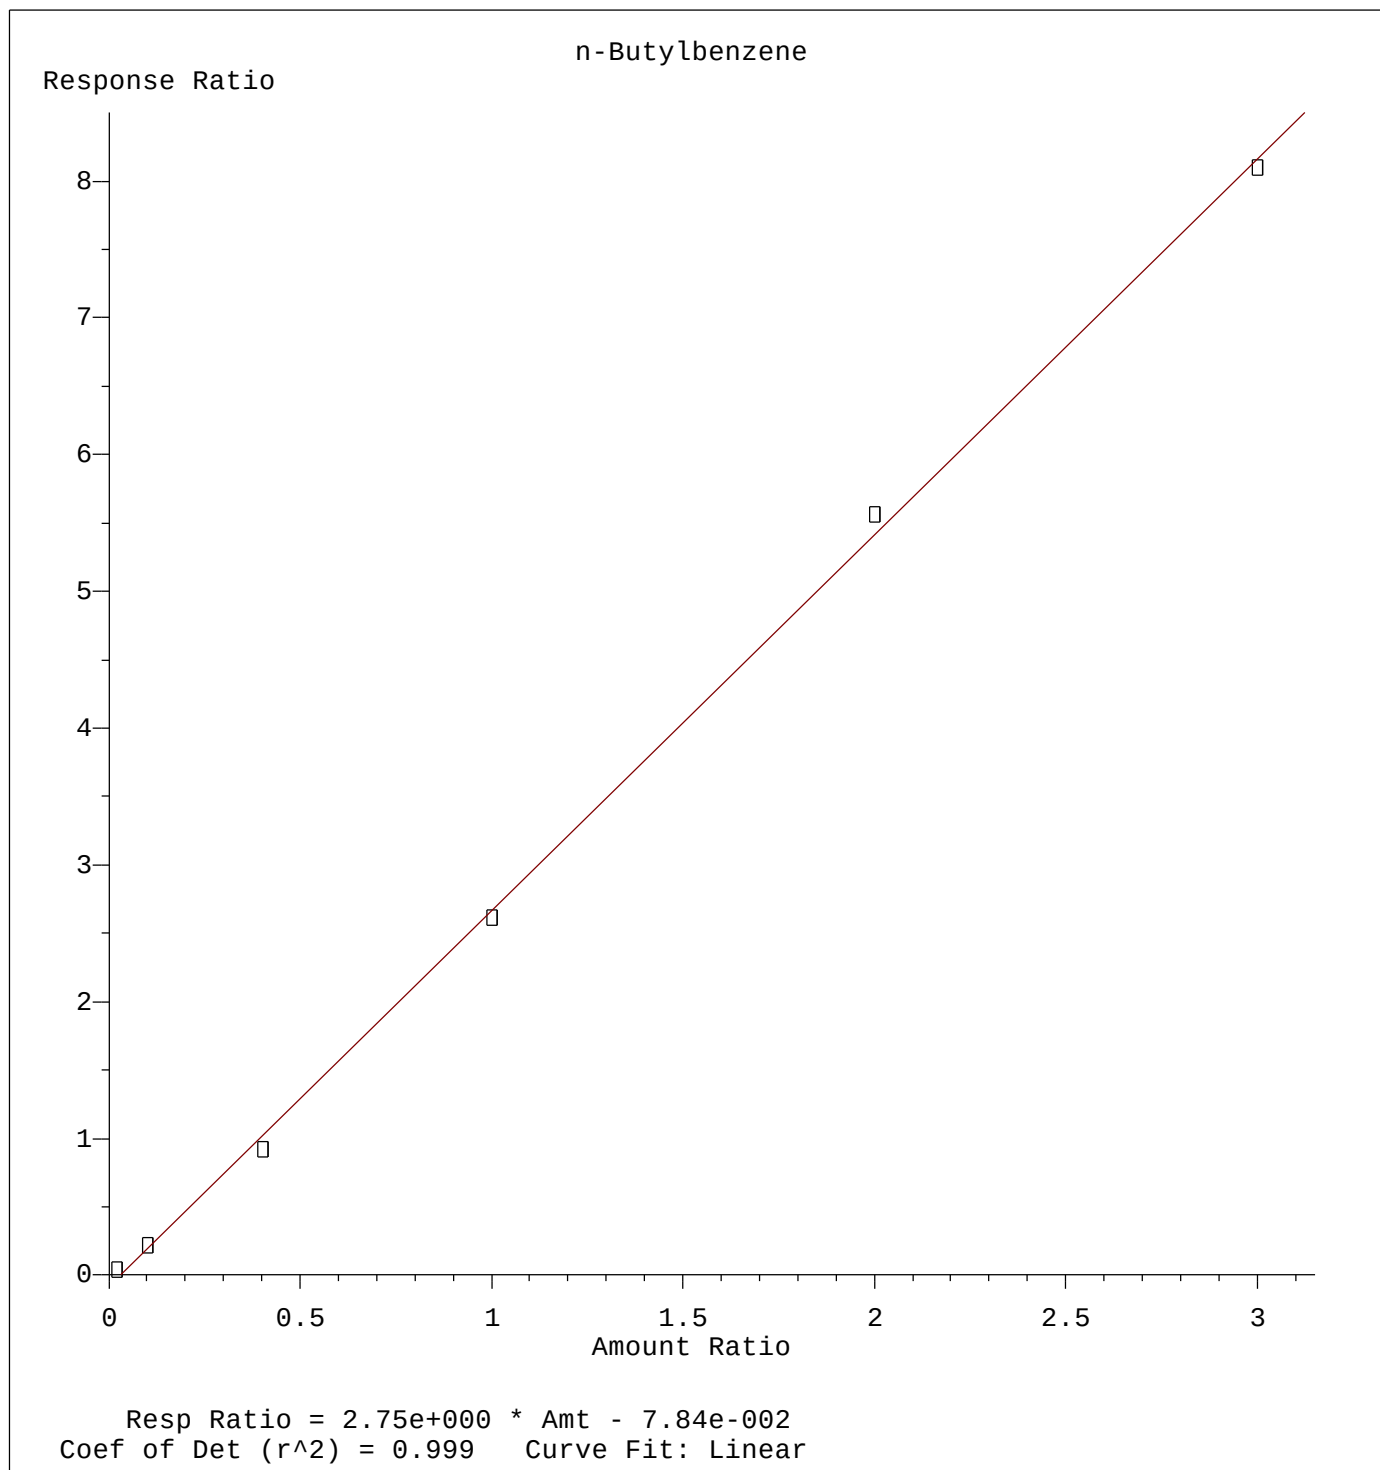

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018

1,2,3-Trichloropropane

Response Ratio

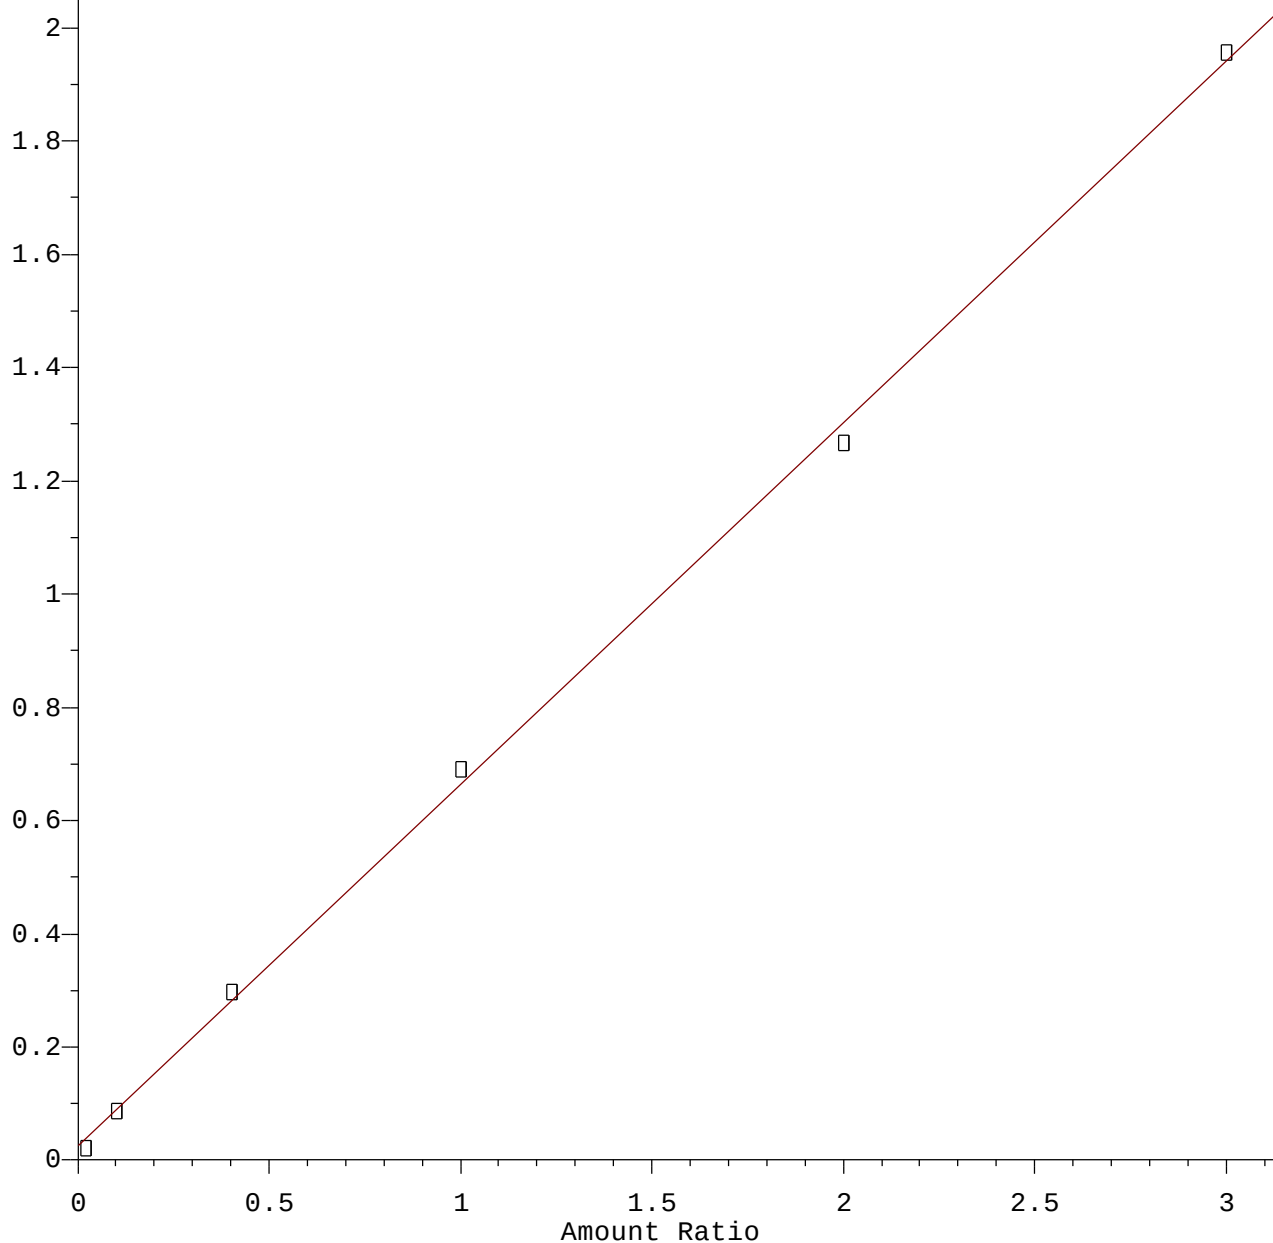


Resp Ratio = $6.39 \times 10^{-1} \times \text{Amt} + 2.40 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018


1,1,2,2-Tetrachloroethane

Response Ratio

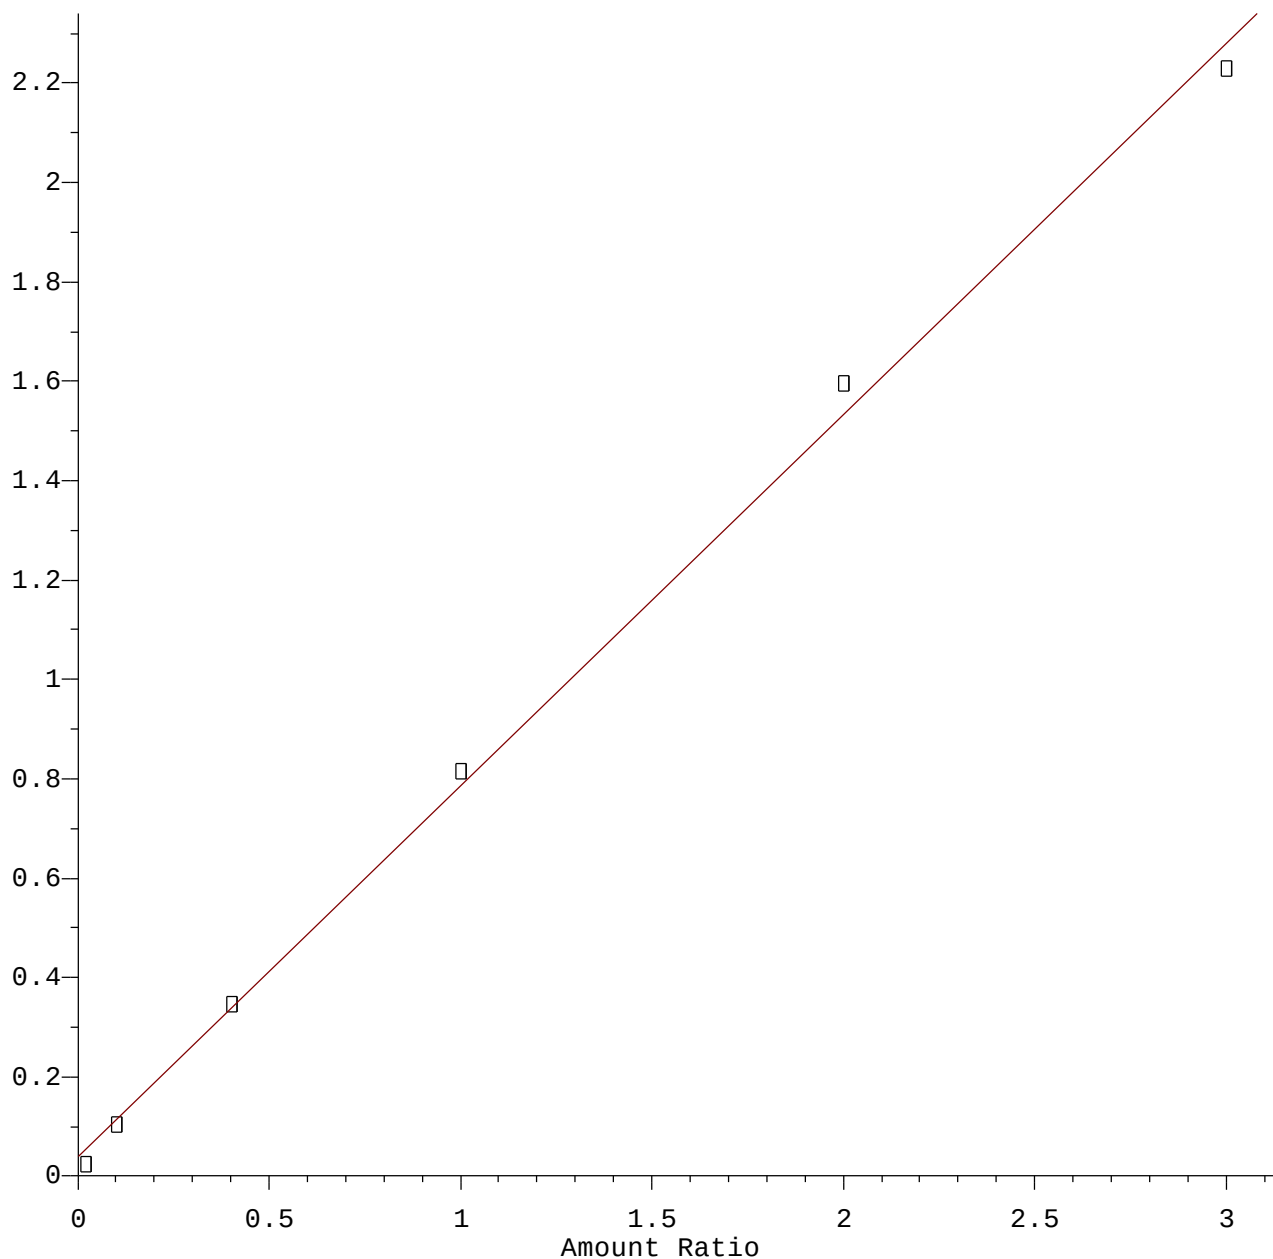

Resp Ratio = $7.46 \times 10^{-1} \times \text{Amt} + 4.03 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018

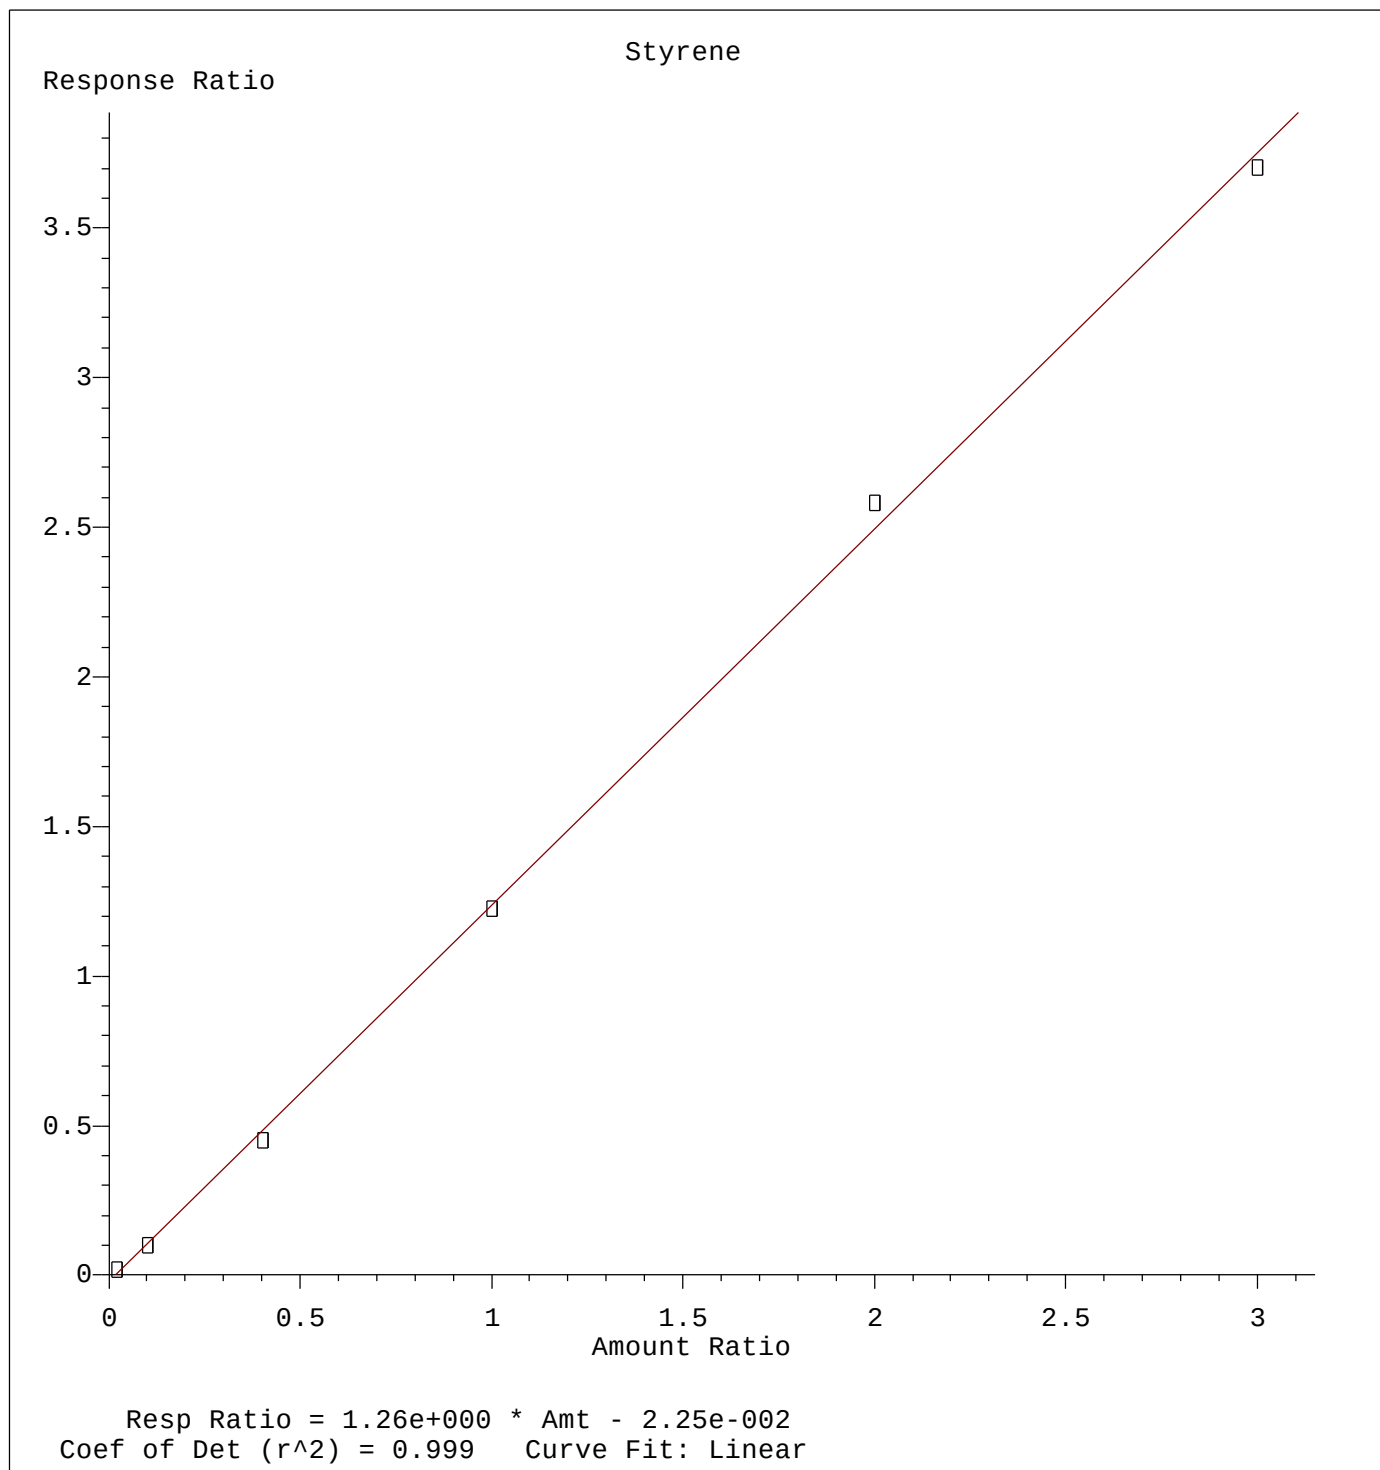

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018


2-Chloroethyl Vinyl ether

Response Ratio

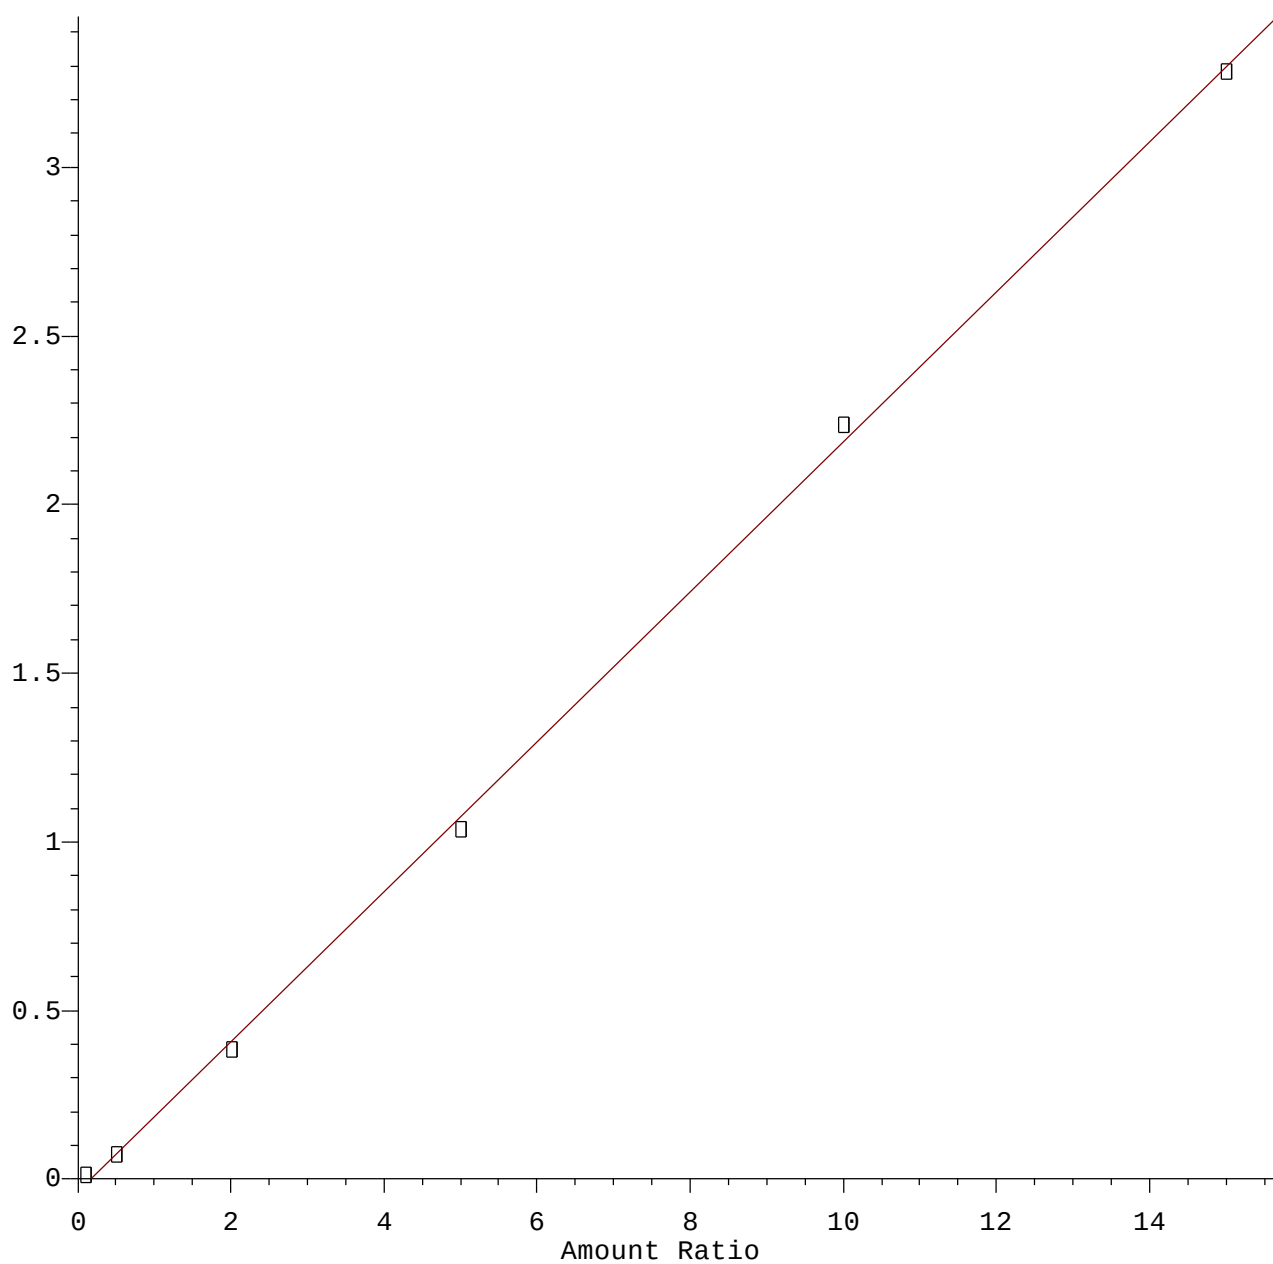


Resp Ratio = $2.22 \times 10^{-1} \times \text{Amt} - 3.81 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018

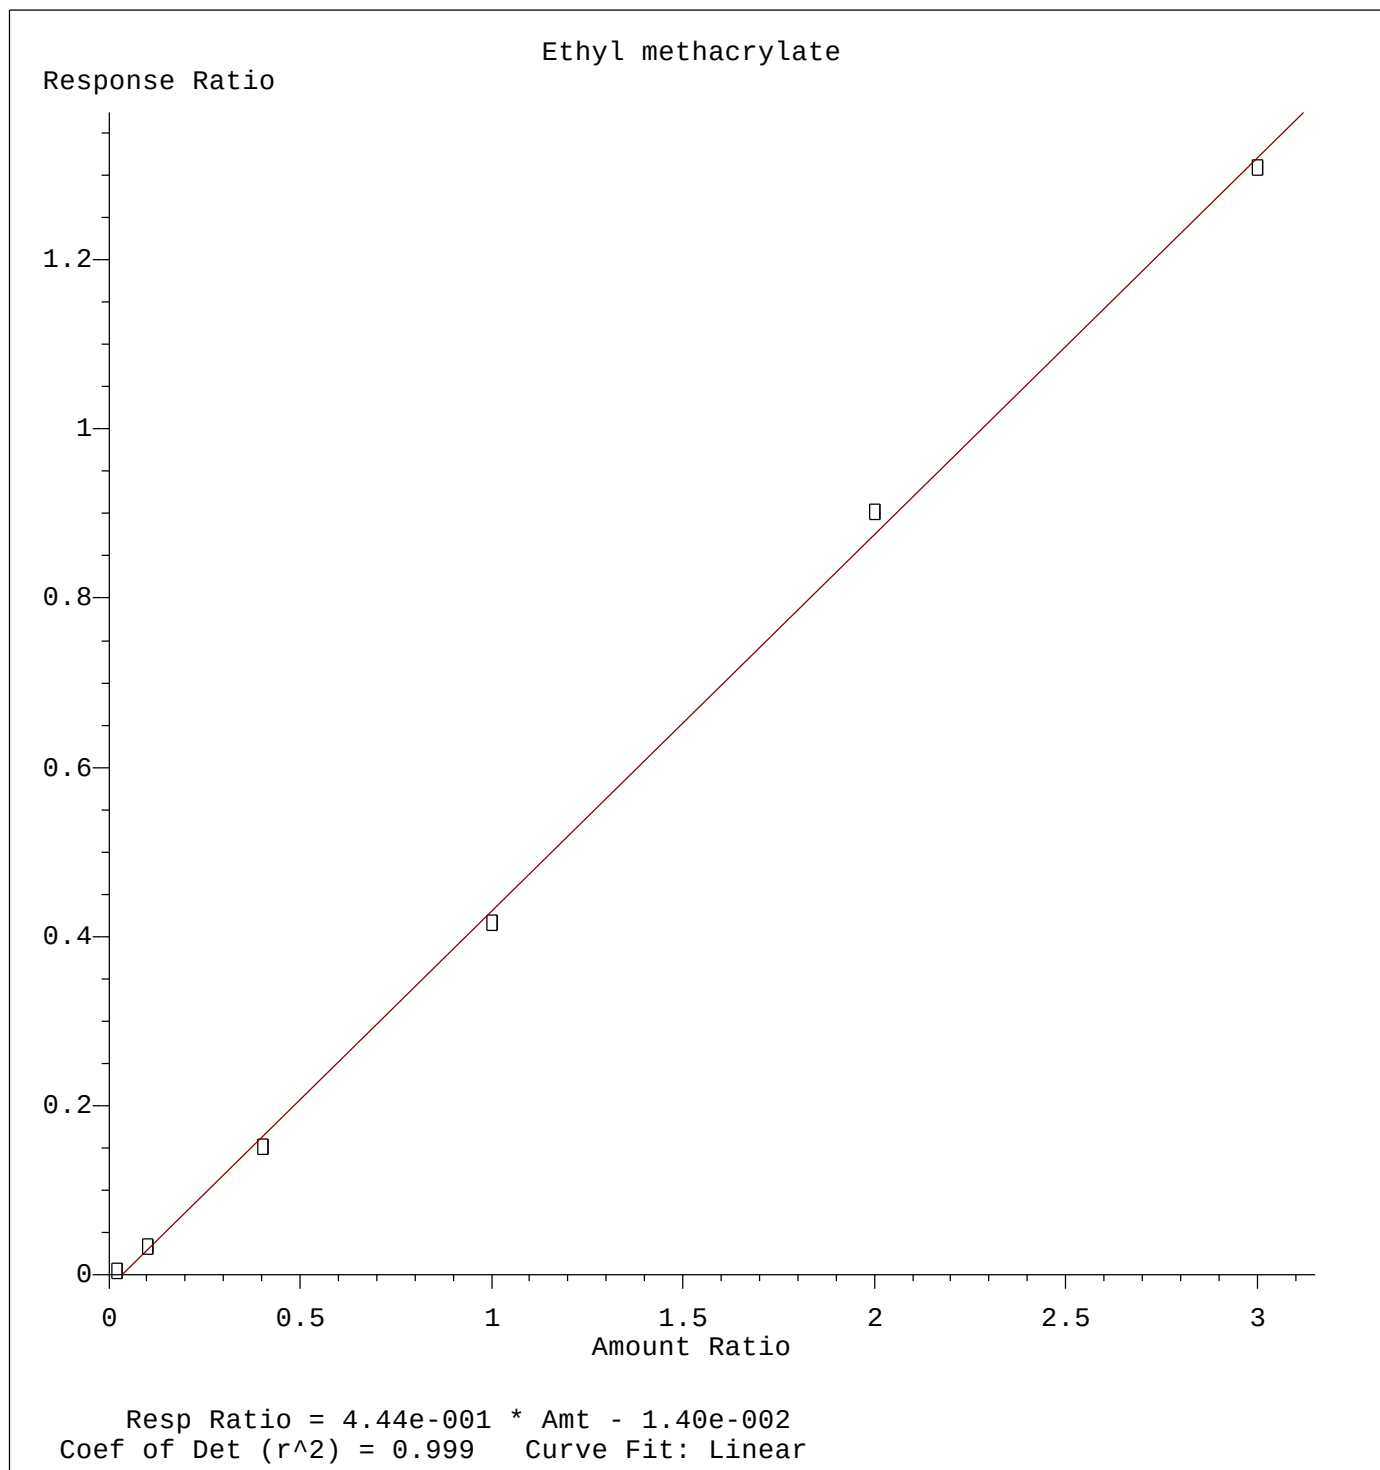


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018

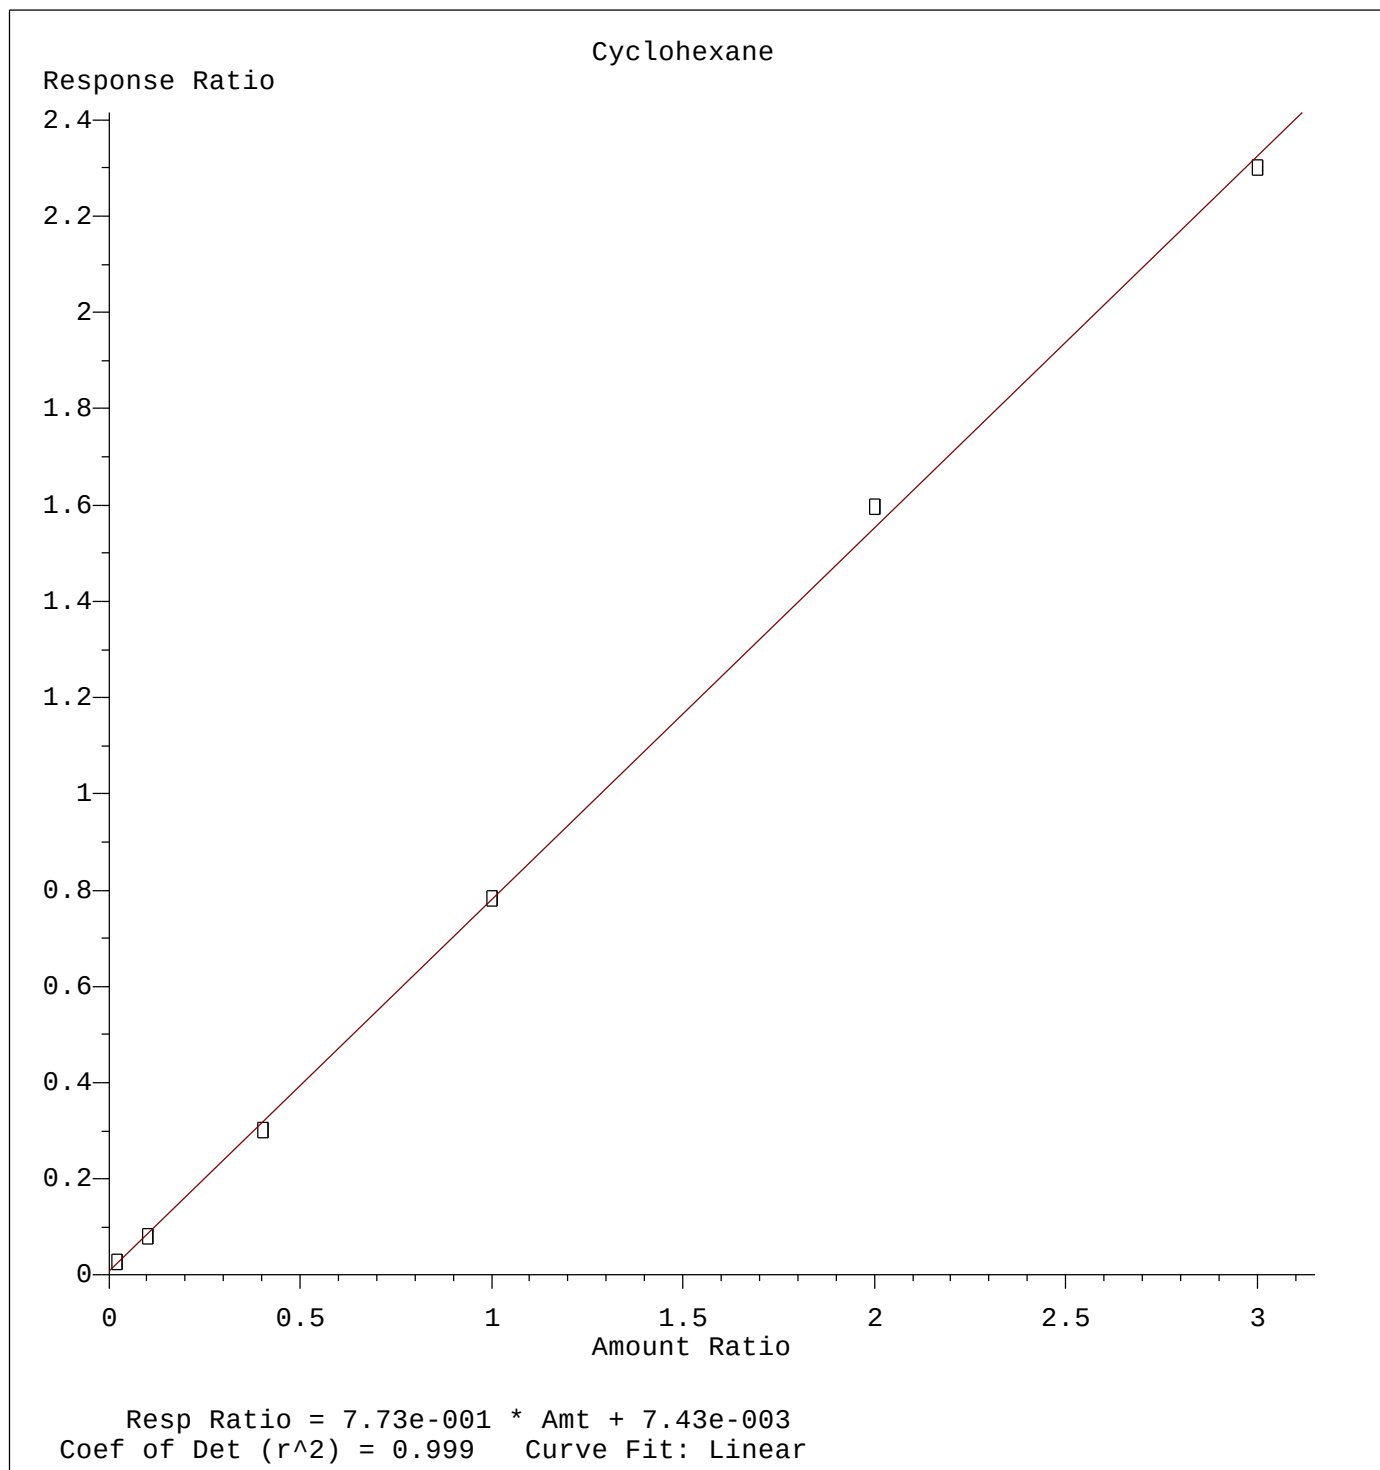


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018

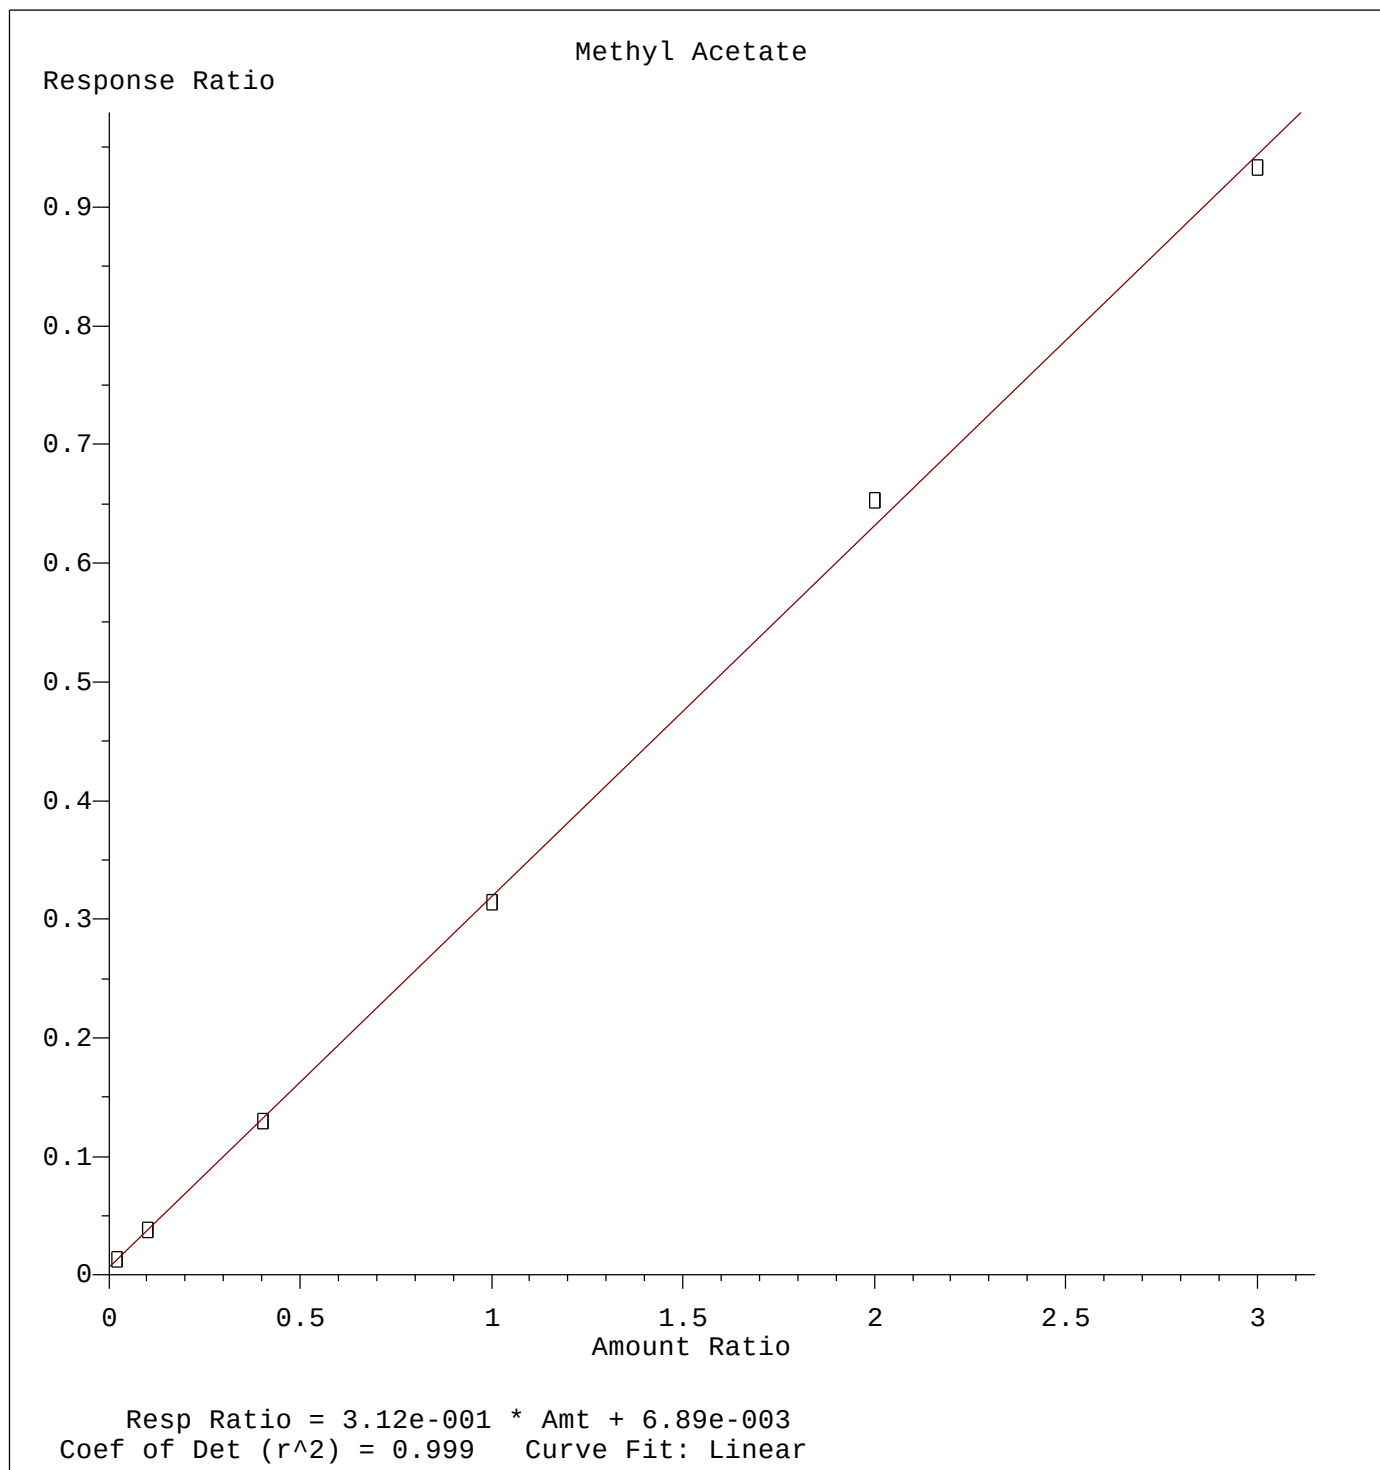

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018

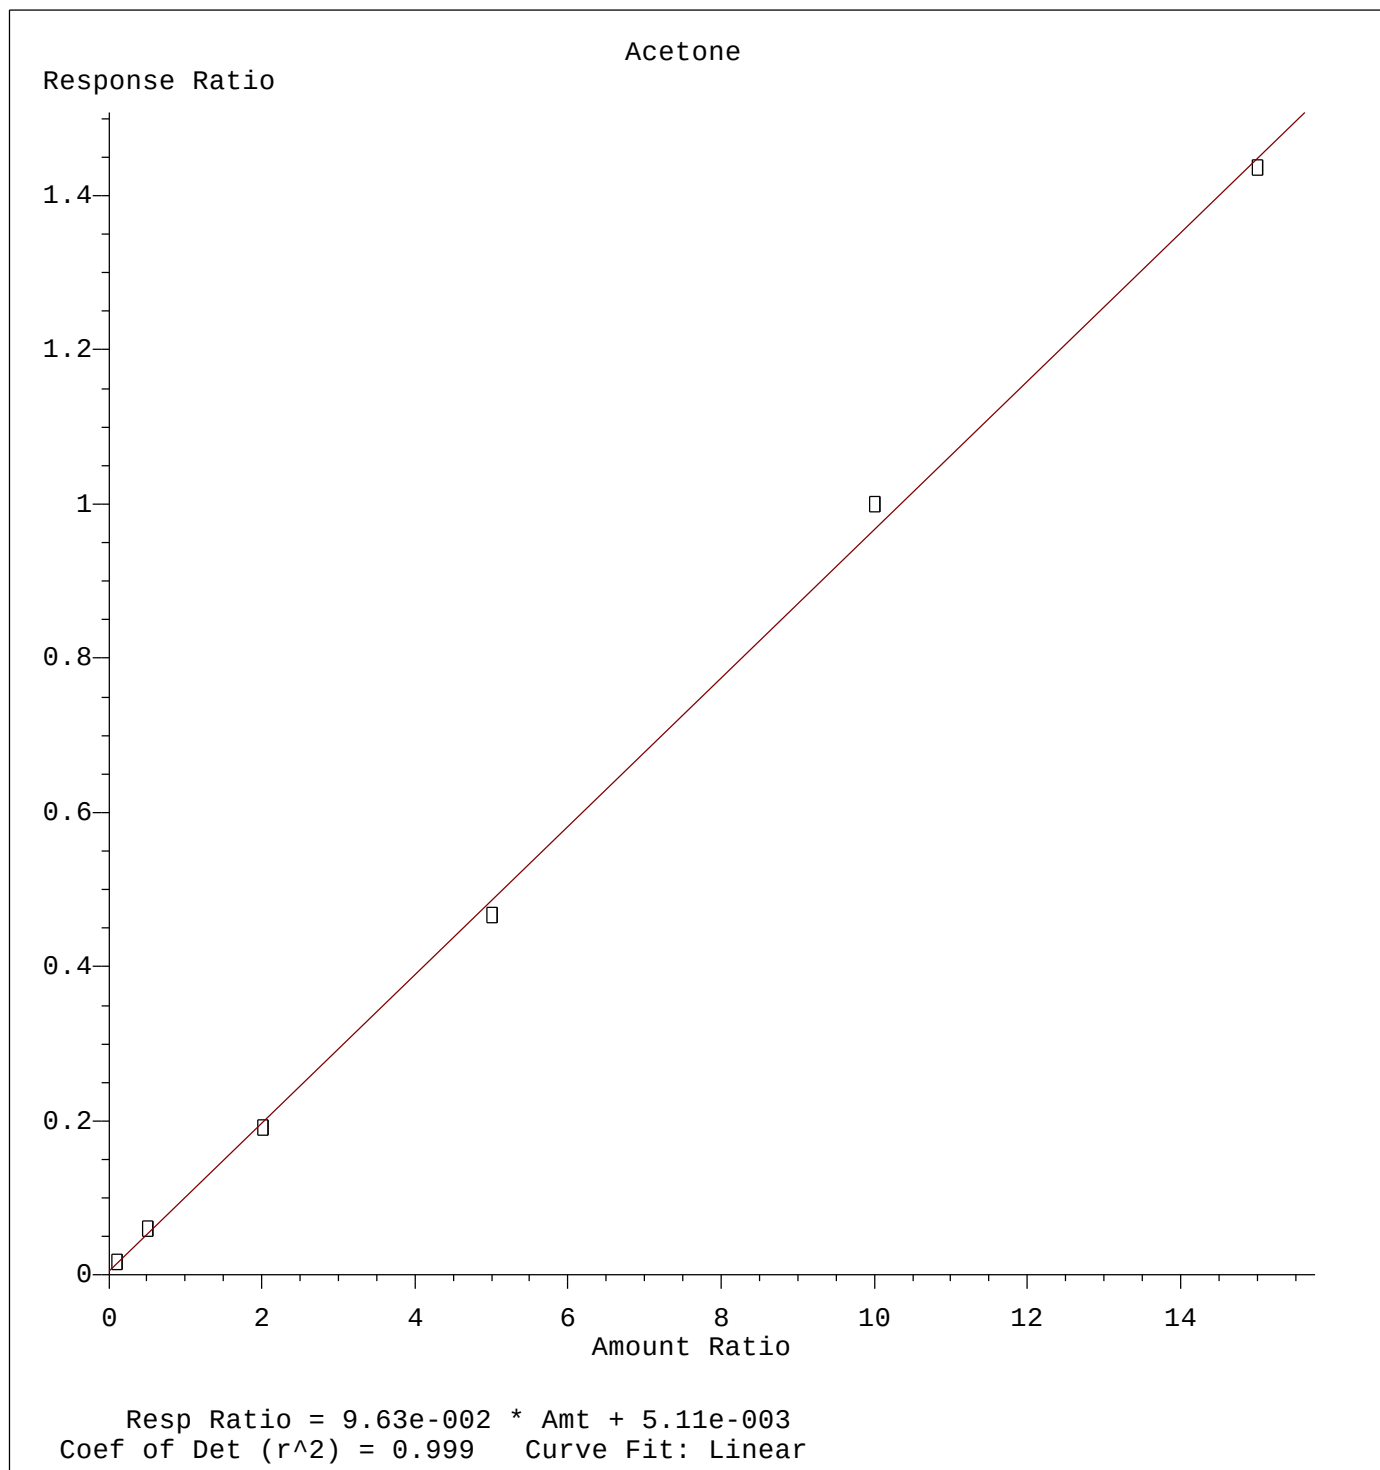

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018

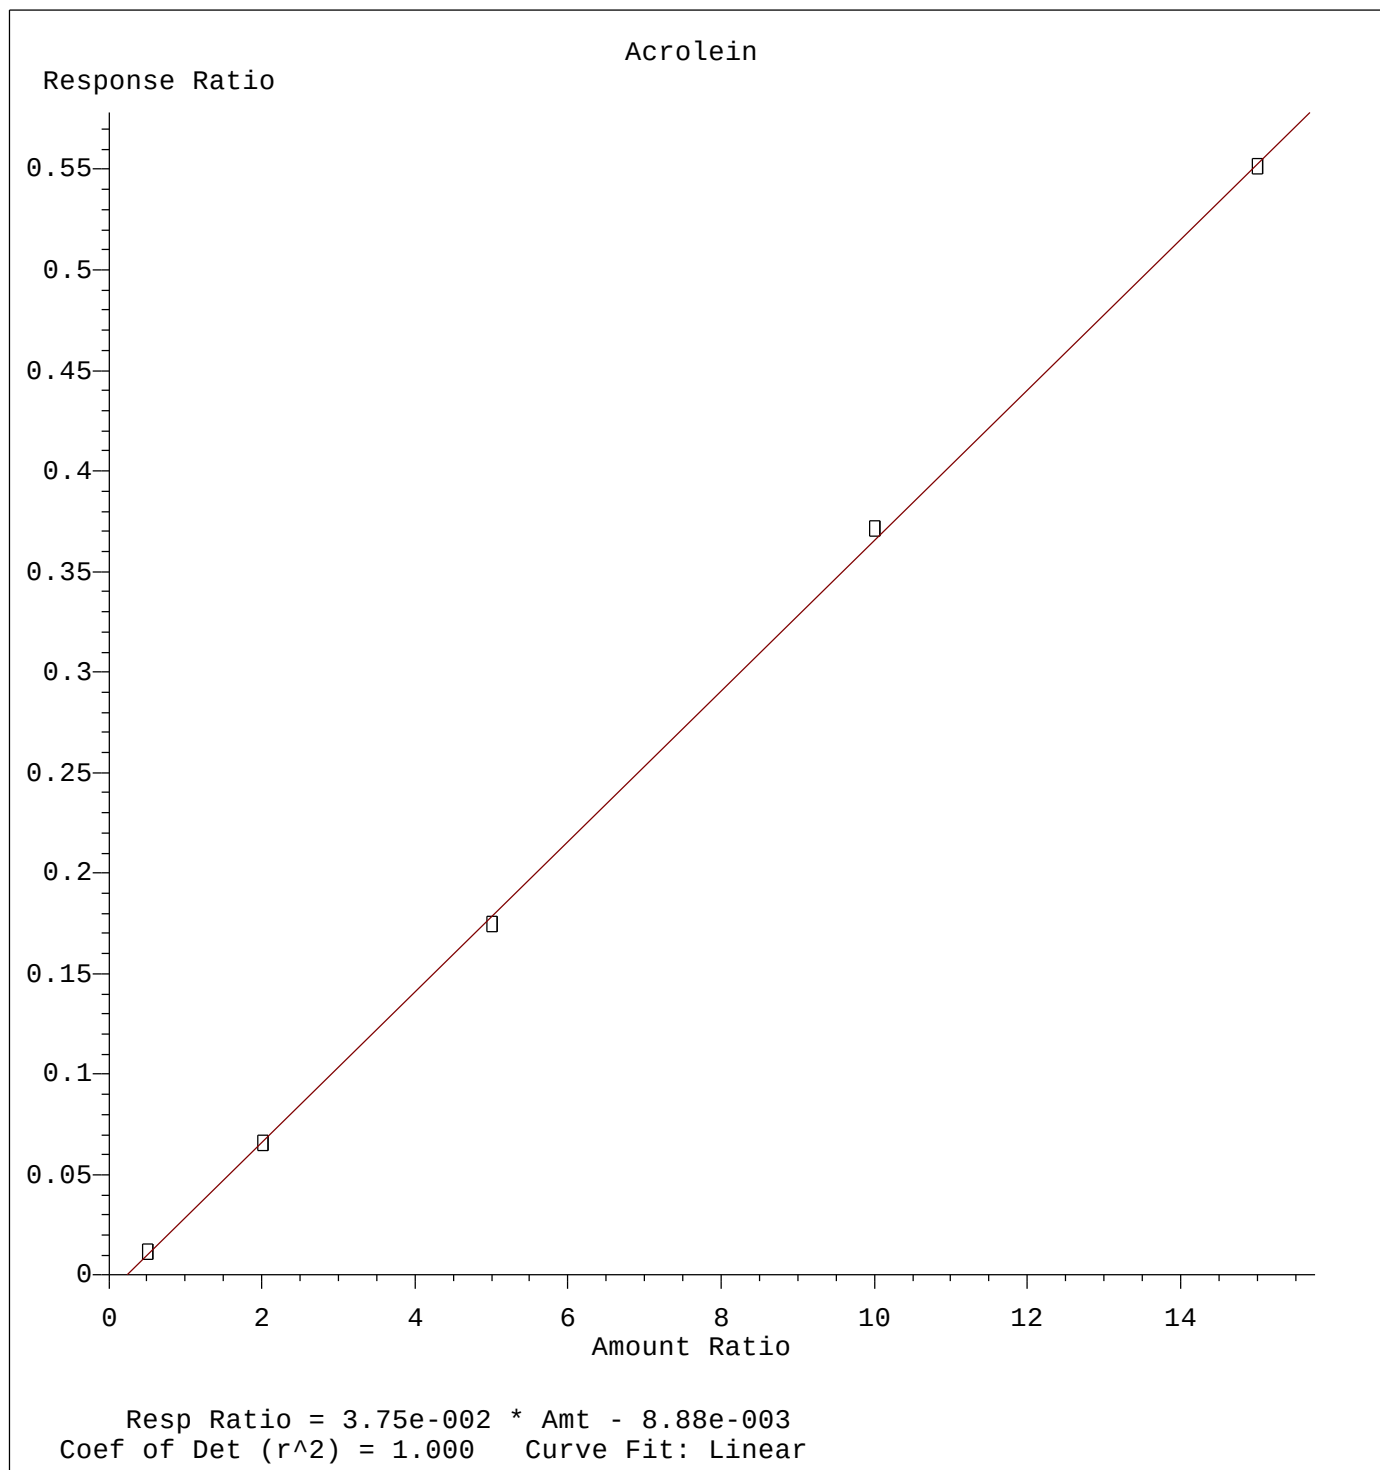

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Calibration Table Last Updated: Fri Sep 21 04:23:57 2018