


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN092018\
Data File : VN051335.D
Acq On : 20 Sep 2018 12:29
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092018W.M
Title : SW846 8260
Last Update : Fri Sep 21 04:23:57 2018

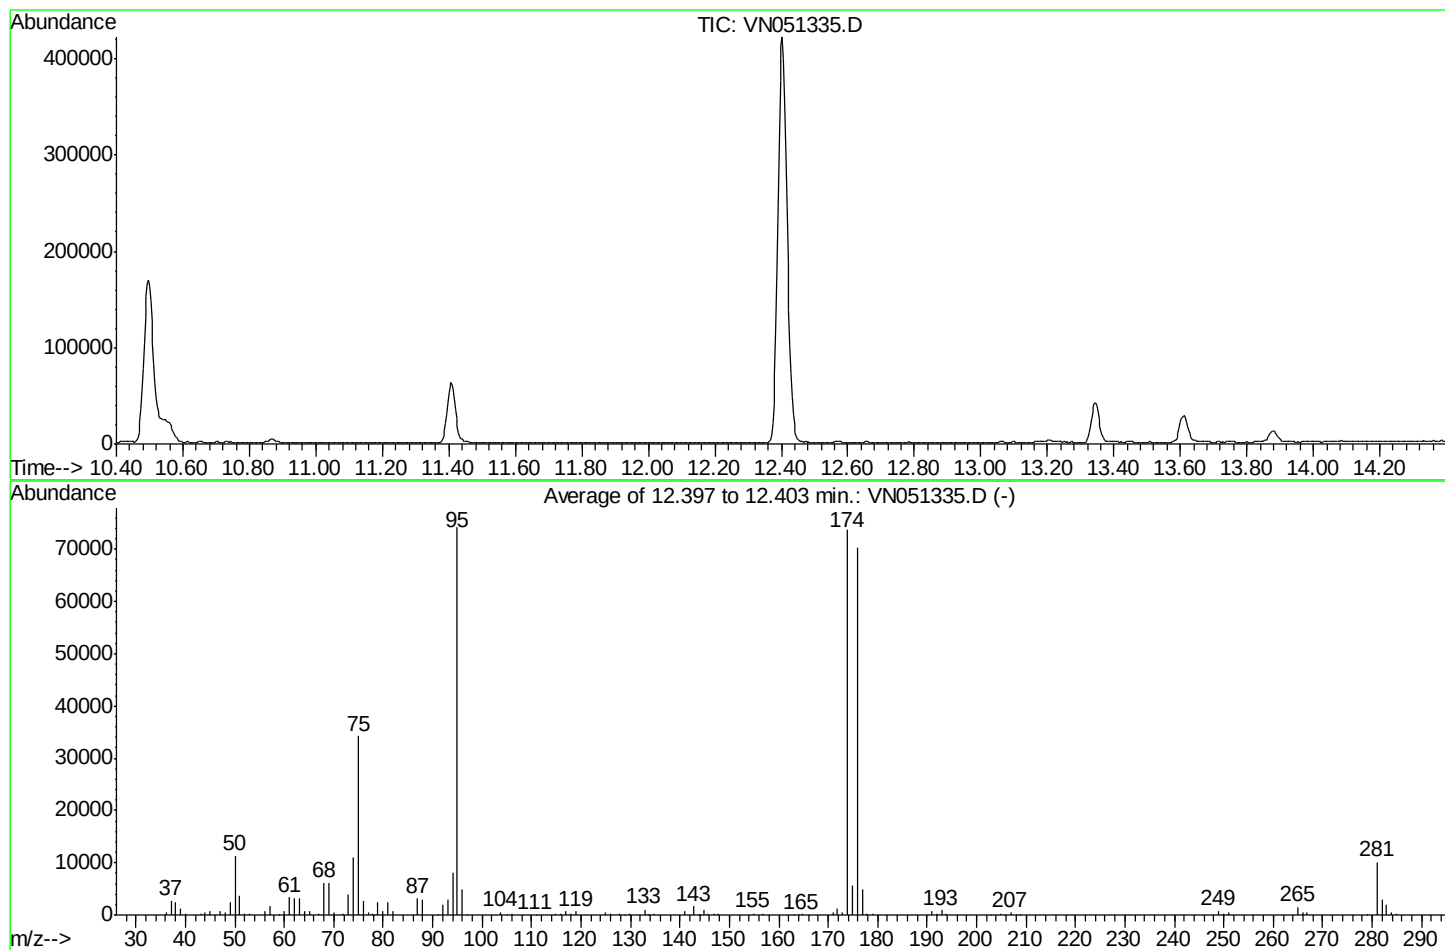

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	11298	PASS
75	95	30	60	46.1	34178	PASS
95	95	100	100	100.0	74173	PASS
96	95	5	9	6.5	4853	PASS
173	174	0.00	2	0.5	396	PASS
174	95	50	100	99.3	73629	PASS
175	174	5	9	7.6	5562	PASS
176	174	95	101	95.3	70186	PASS
177	176	5	9	6.8	4788	PASS