


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN092019\  
Data File : VN058233.D  
Acq On : 20 Sep 2019 8:12  
Operator : JC/SP  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\624N090919W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Mon Sep 09 12:14:07 2019

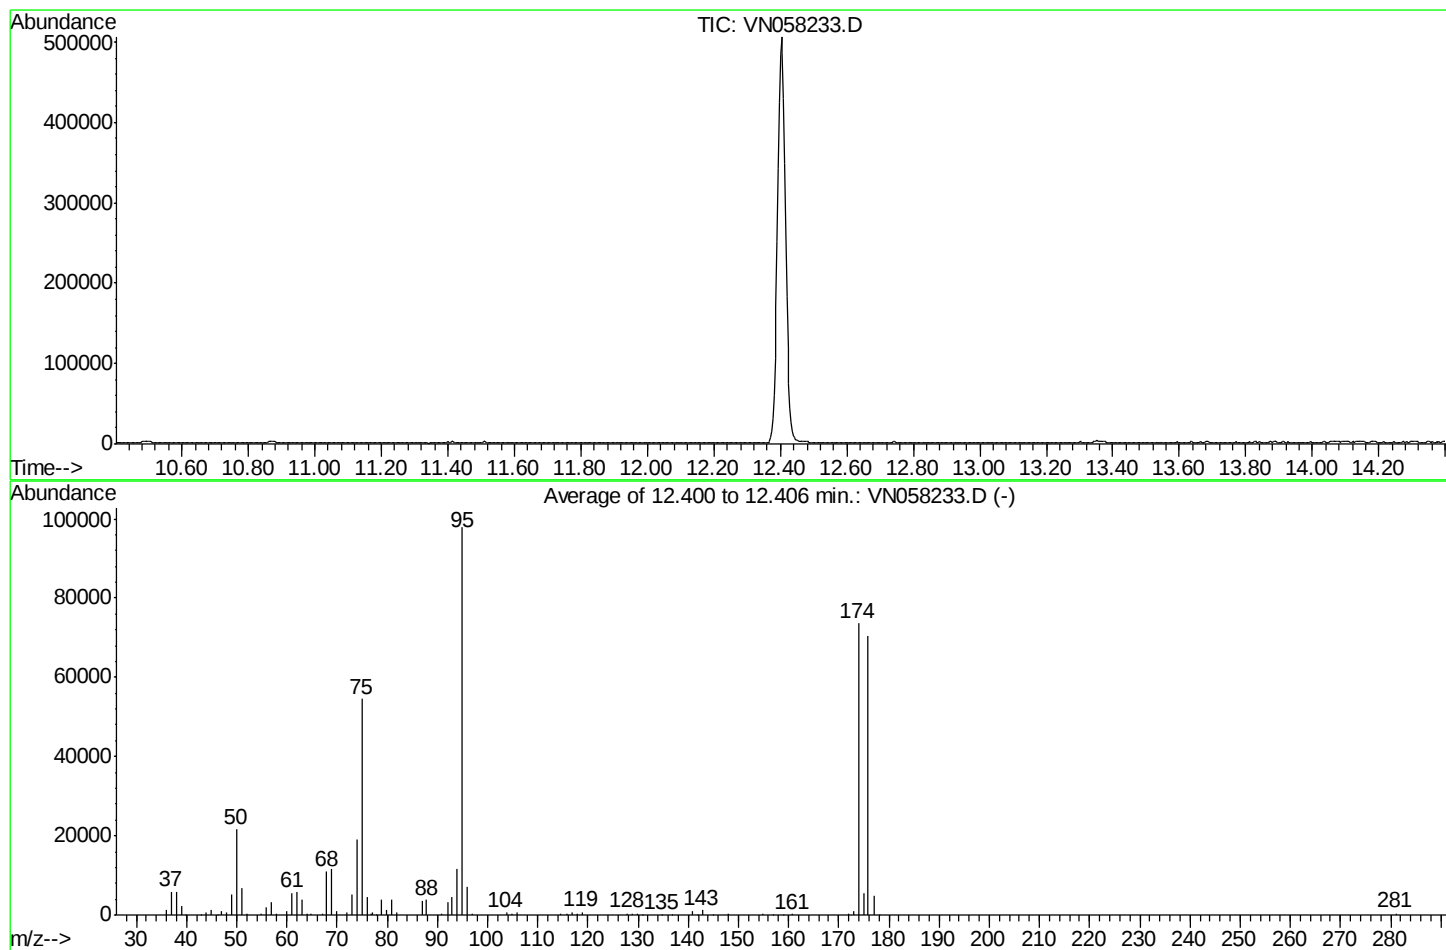

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 22.1      | 21648   | PASS             |
| 75          | 95           | 30           | 60           | 55.7      | 54469   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 97858   | PASS             |
| 96          | 95           | 5            | 9            | 7.2       | 7094    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.3       | 974     | PASS             |
| 174         | 95           | 50           | 100          | 75.1      | 73533   | PASS             |
| 175         | 174          | 5            | 9            | 7.6       | 5564    | PASS             |
| 176         | 174          | 95           | 101          | 95.6      | 70298   | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 4727    | PASS             |