


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN092019\
Data File : VN058242.D
Acq On : 20 Sep 2019 12:04
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091819W.M
Title : SW846 8260
Last Update : Thu Sep 19 09:27:53 2019

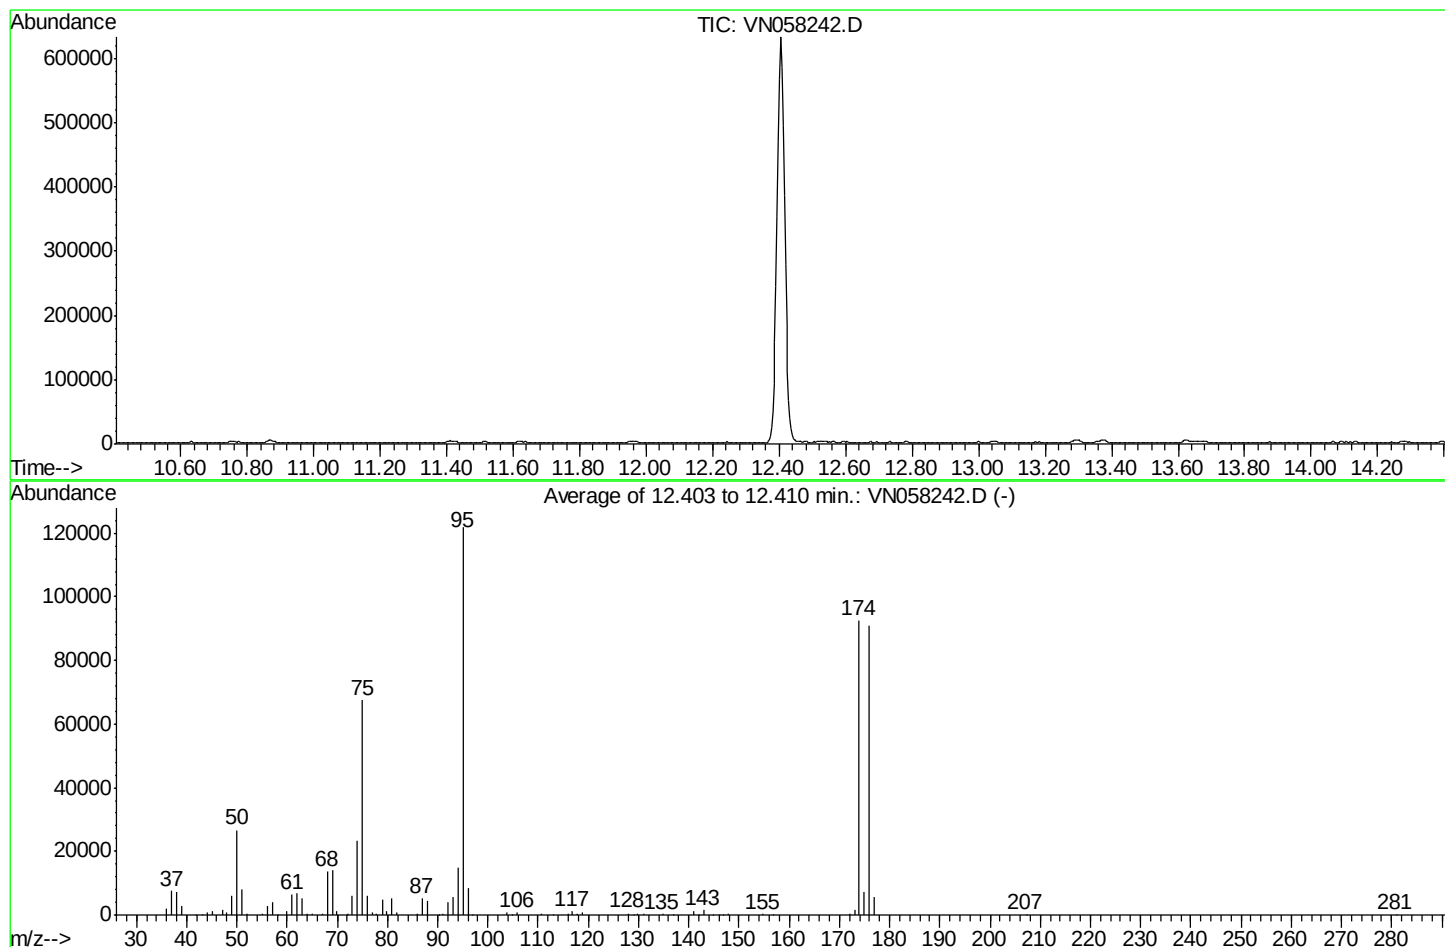

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	26709	PASS
75	95	30	60	55.3	67408	PASS
95	95	100	100	100.0	121853	PASS
96	95	5	9	6.8	8305	PASS
173	174	0.00	2	1.6	1453	PASS
174	95	50	100	75.9	92485	PASS
175	174	5	9	7.8	7251	PASS
176	174	95	101	98.3	90896	PASS
177	176	5	9	6.1	5552	PASS