


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092021\
 Data File : VN068558.D
 Acq On : 20 Sep 2021 13:05
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Title : SW846 8260
 Last Update : Fri Sep 17 11:02:11 2021

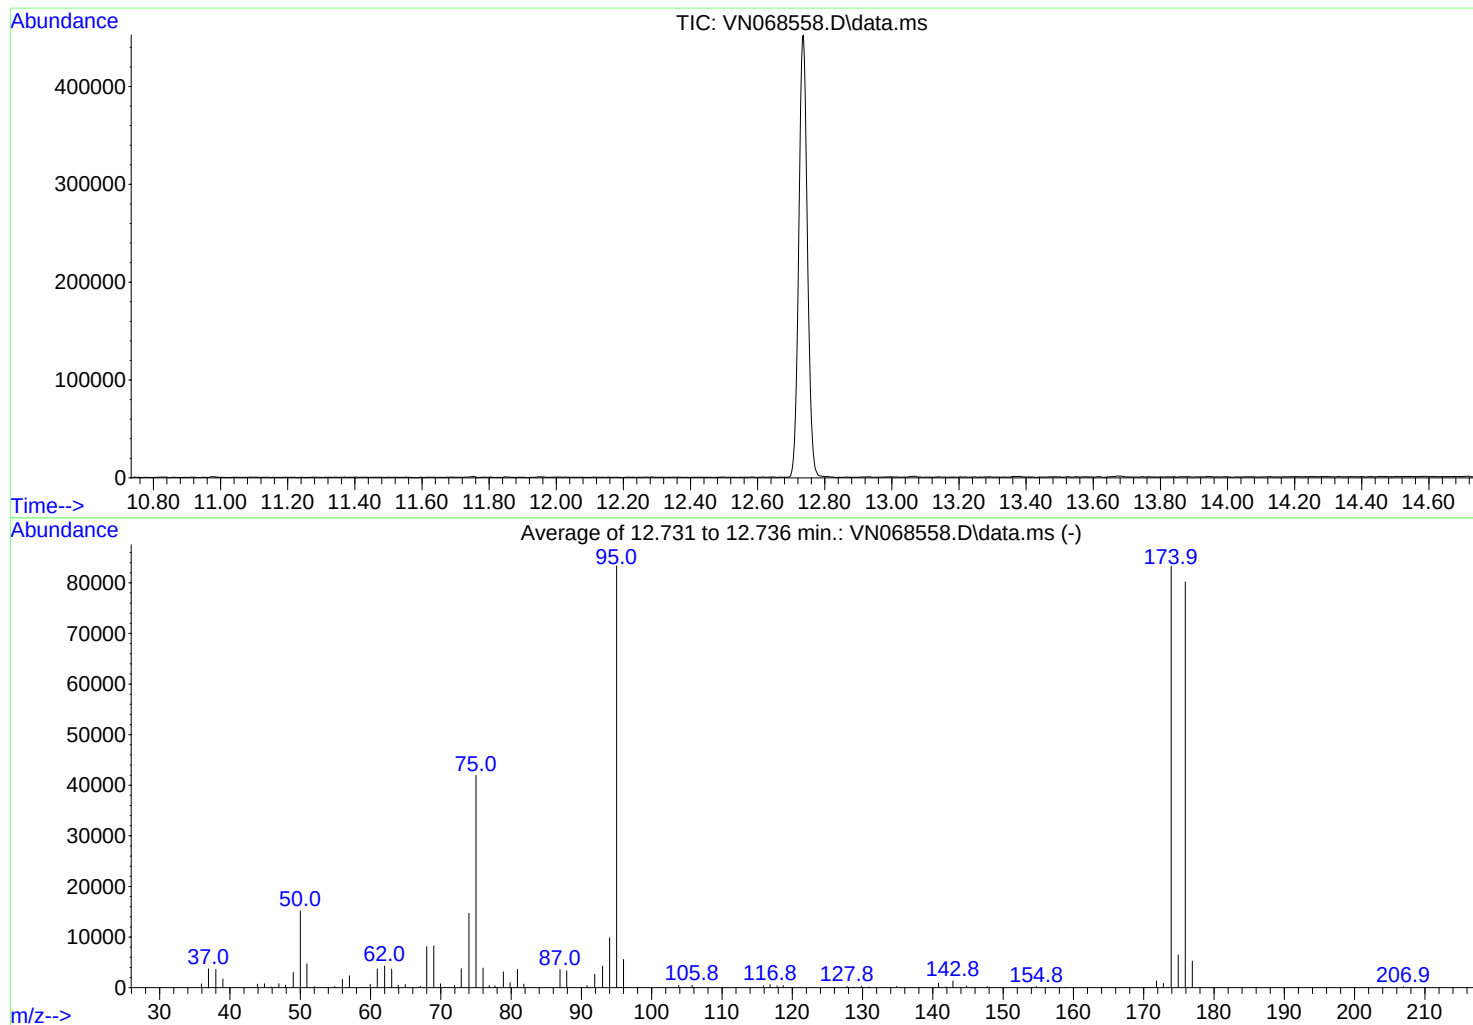

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	15164	PASS
75	95	30	60	50.3	41936	PASS
95	95	100	100	100.0	83360	PASS
96	95	5	9	6.7	5570	PASS
173	174	0.00	2	1.0	828	PASS
174	95	50	100	99.9	83309	PASS
175	174	5	9	7.7	6443	PASS
176	174	95	101	96.3	80208	PASS
177	176	5	9	6.5	5236	PASS