

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092023\
 Data File : VN079307.D
 Acq On : 20 Sep 2023 10:34
 Operator : JC\MD
 Sample : VN0920MBL01
 Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0920MBL01

Quant Time: Sep 21 01:54:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 12 05:05:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.229	168	168894	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	310804	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	266239	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	73473	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	126232	55.367	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	110.740%
35) Dibromofluoromethane	8.171	113	95415	46.152	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.300%
50) Toluene-d8	10.570	98	322439	42.475	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	84.960%#
62) 4-Bromofluorobenzene	12.853	95	93535	38.628	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	77.260%#


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092023\
Data File : VN079307.D
Acq On : 20 Sep 2023 10:34
Operator : JC\MD
Sample : VN0920MBL01
Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0920MBL01


Quant Time: Sep 21 01:54:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 12 05:05:24 2023
Response via : Initial Calibration

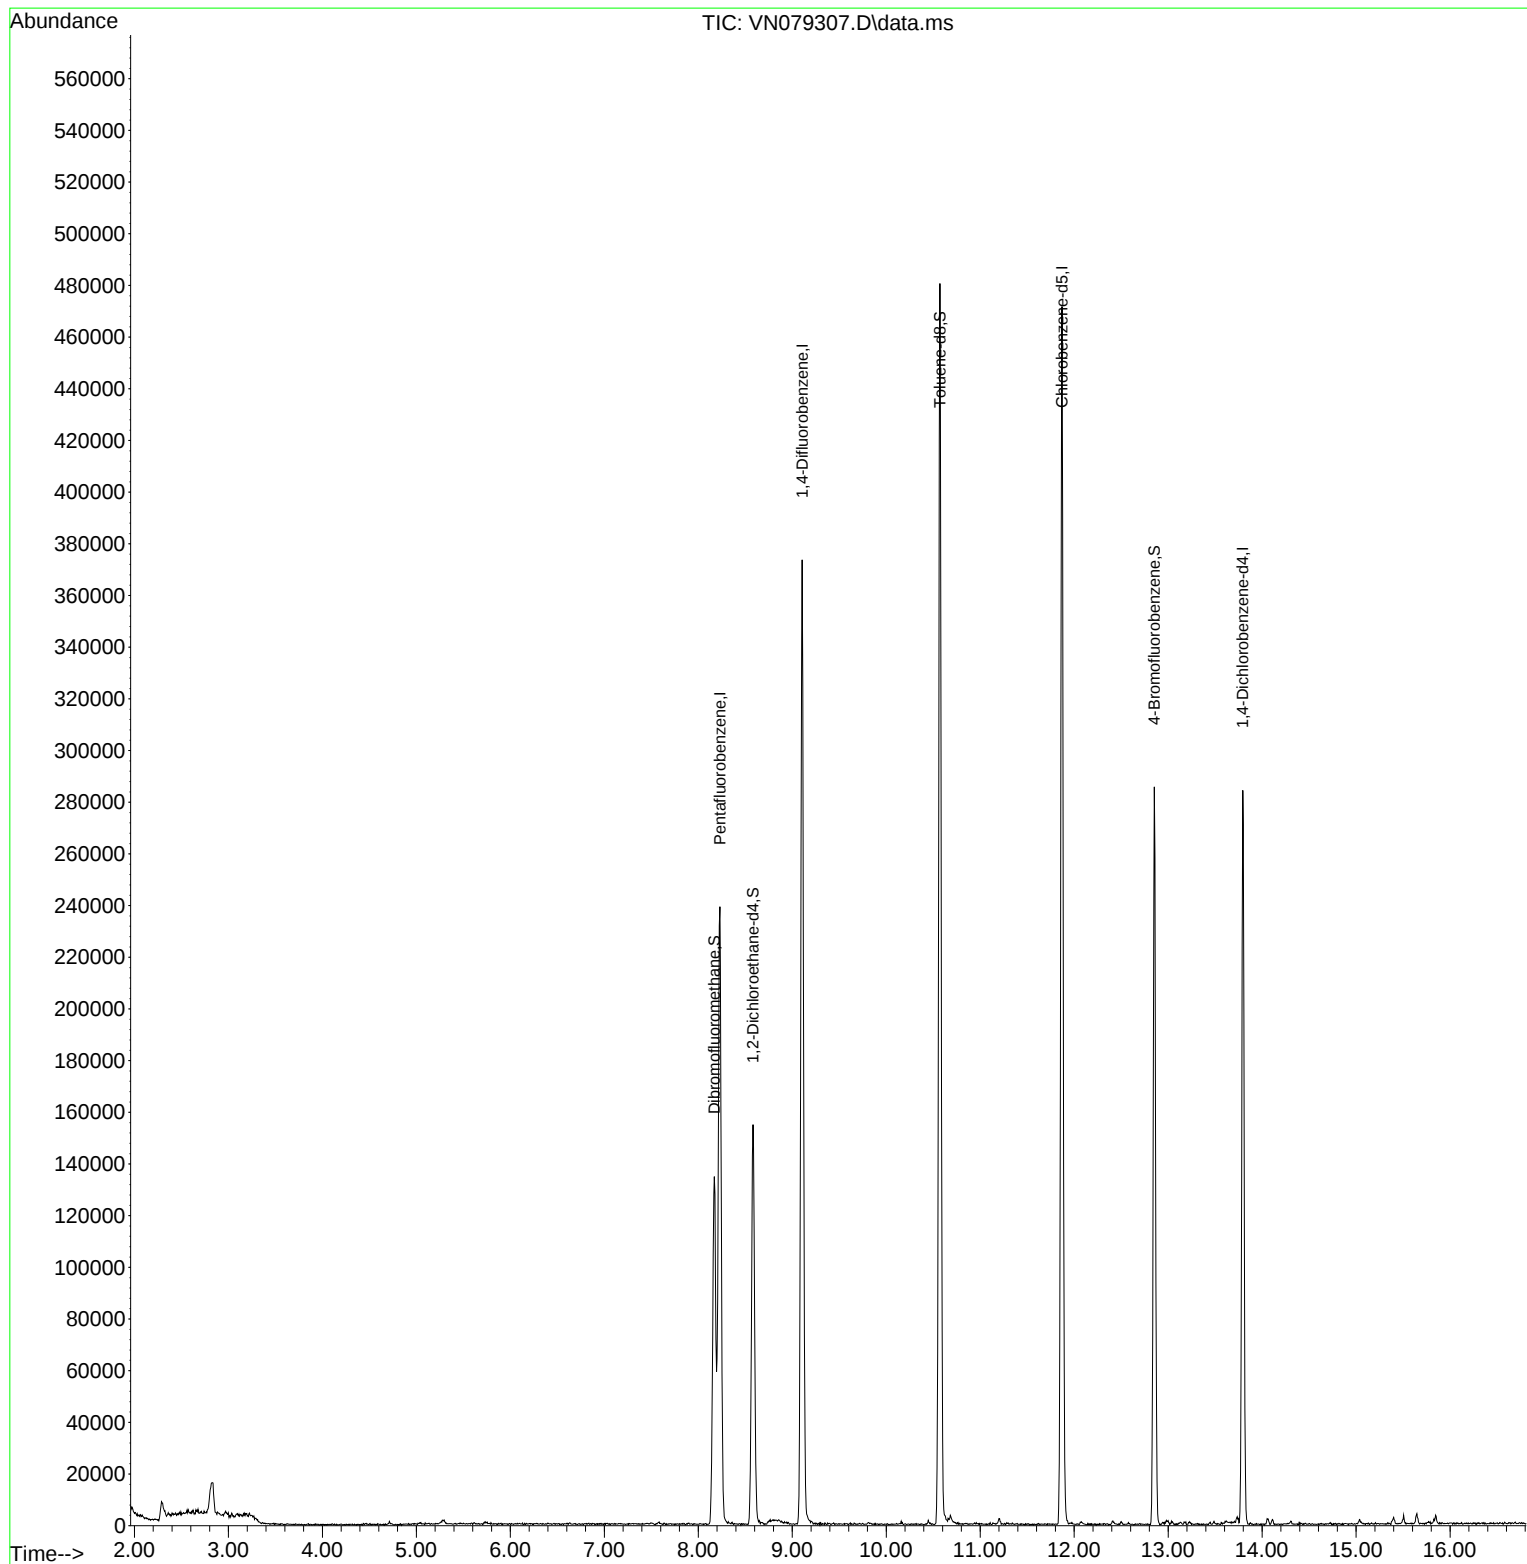



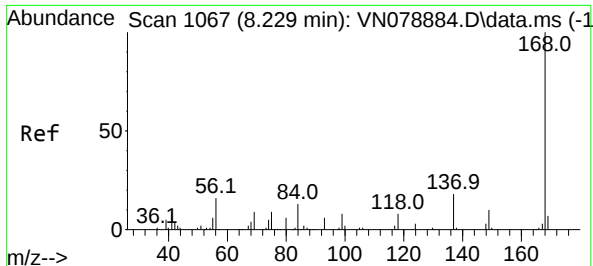


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.001 min
Lab File: VN079307.D
Acq: 20 Sep 2023 10:34

Instrument :
MSVOA_N
ClientSampleId :
VN0920MBL01



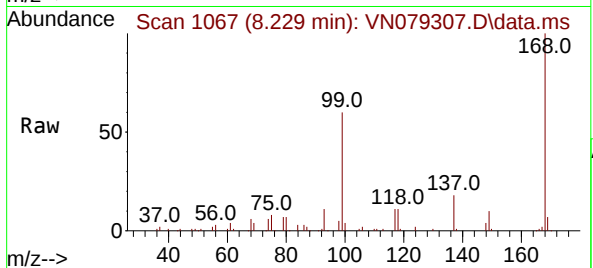



Tgt Ion:168 Resp: 168894
Ion Ratio Lower Upper
168 100
99 60.2 53.0 79.6

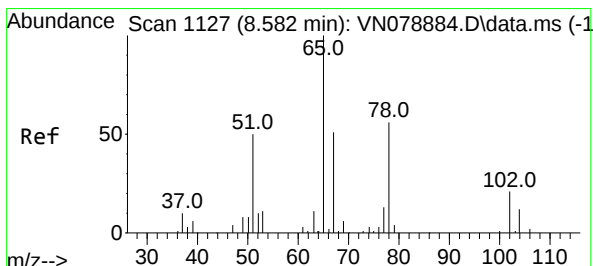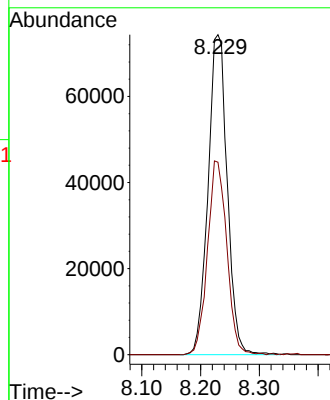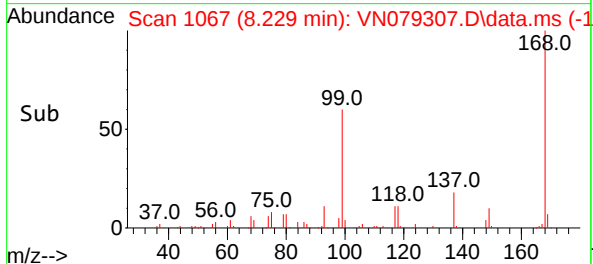

#33
1,2-Dichloroethane-d4
Concen: 55.367 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.001 min
Lab File: VN079307.D
Acq: 20 Sep 2023 10:34

Tgt Ion: 65 Resp: 126232
Ion Ratio Lower Upper
65 100
67 50.7 0.0 106.6

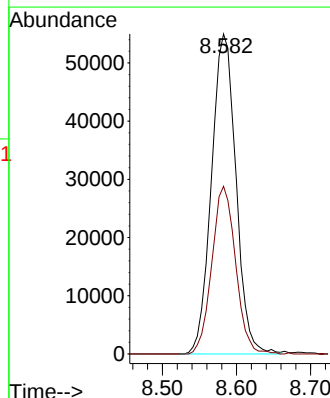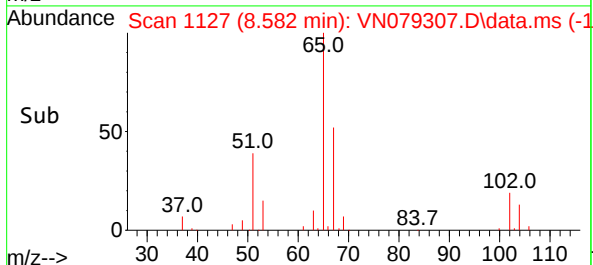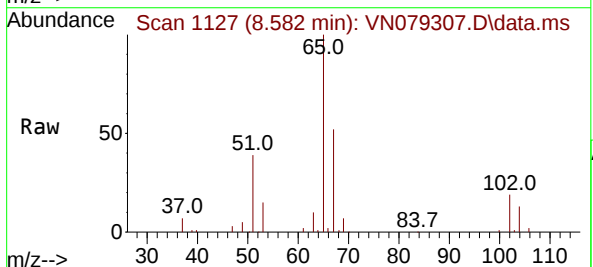

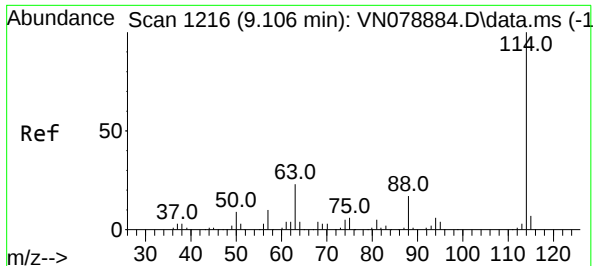

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.006 min

Lab File: VN079307.D

Acq: 20 Sep 2023 10:34

Instrument :

MSVOA_N

ClientSampleId :

VN0920MBL01





Tgt Ion:114 Resp: 310804

Ion Ratio Lower Upper

114 100

63 22.6 0.0 36.4

88 15.6 0.0 30.6

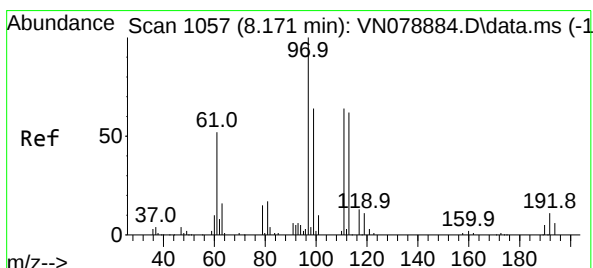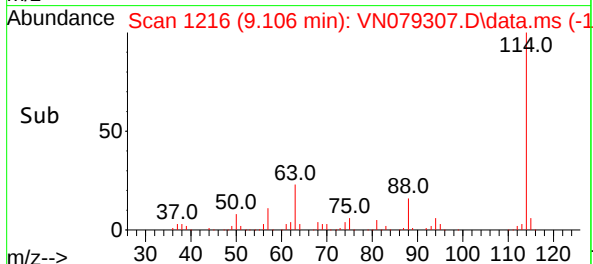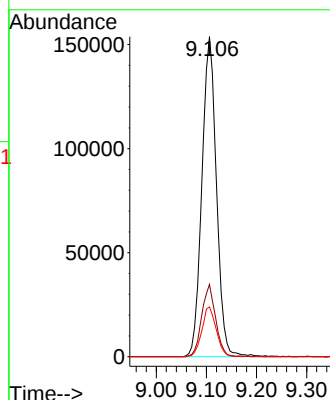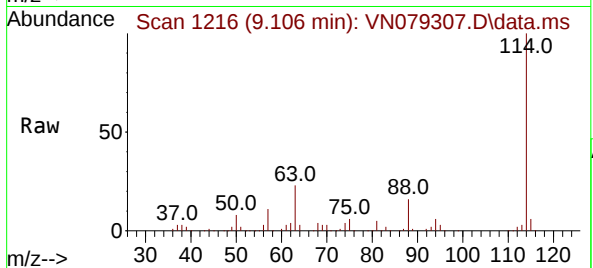

#35

Dibromofluoromethane

Concen: 46.152 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN079307.D

Acq: 20 Sep 2023 10:34




Tgt Ion:113 Resp: 95415


Ion Ratio Lower Upper

113 100

111 104.7 82.6 123.8

192 17.1 12.7 19.1


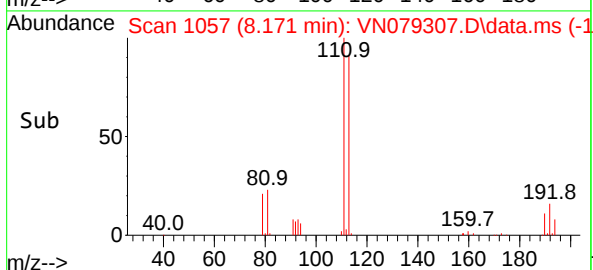
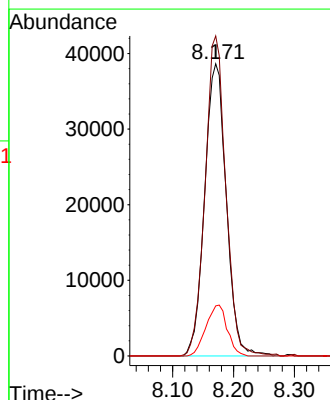
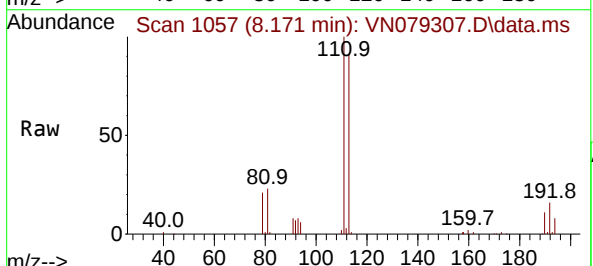


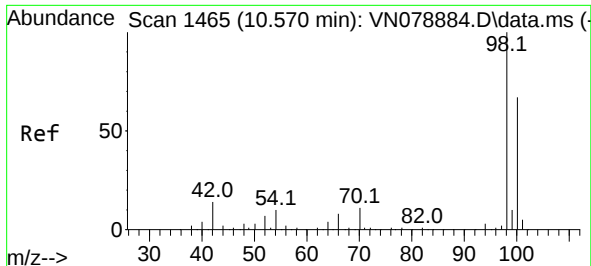

#50
Toluene-d8
Concen: 42.475 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.001 min
Lab File: VN079307.D
Acq: 20 Sep 2023 10:34




Instrument :
MSVOA_N
ClientSampleId :
VN0920MBL01


Tgt Ion: 98 Resp: 322439
Ion Ratio Lower Upper
98 100
100 63.5 52.0 78.0

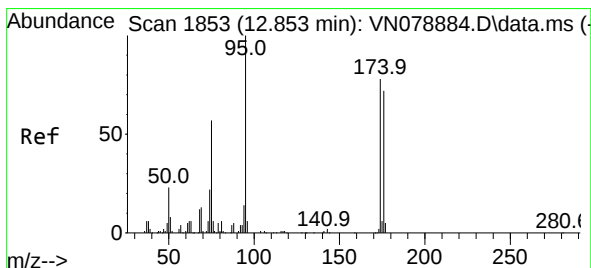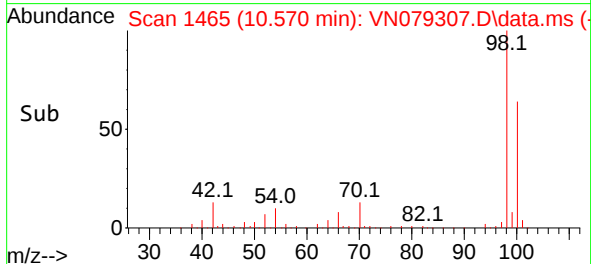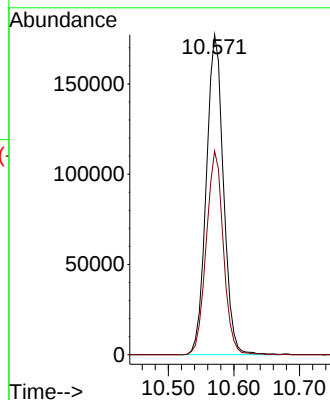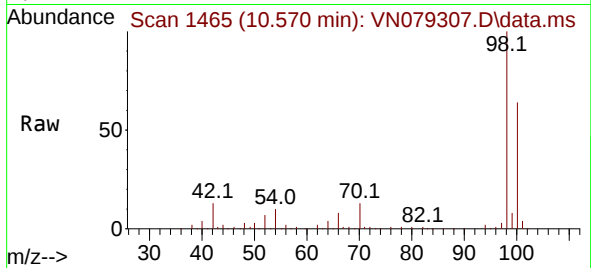

#62
4-Bromofluorobenzene
Concen: 38.628 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079307.D
Acq: 20 Sep 2023 10:34

Tgt Ion: 95 Resp: 93535
Ion Ratio Lower Upper
95 100
174 76.0 0.0 143.8
176 73.6 0.0 135.8


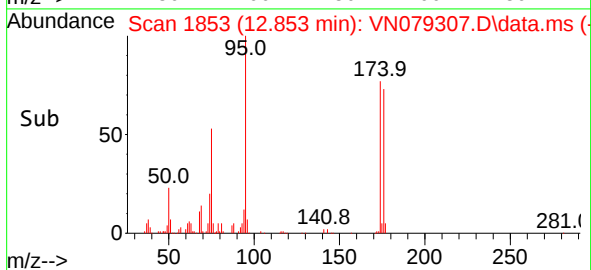
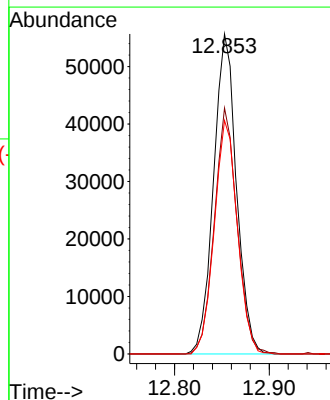
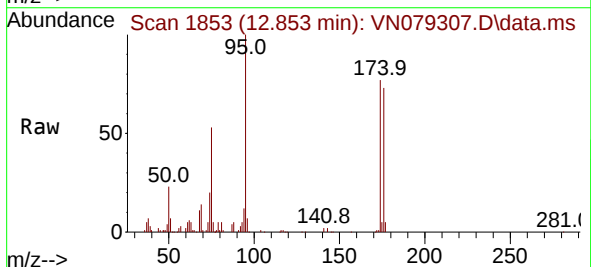


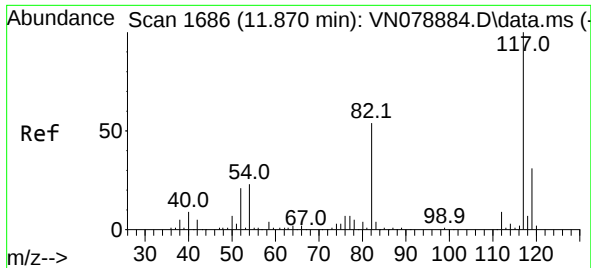

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1
Delta R.T. -0.001 min
Lab File: VN079307.D
Acq: 20 Sep 2023 10:34

Instrument :
MSVOA_N
ClientSampleId :
VN0920MBL01

Tgt Ion:117 Resp: 266239
Ion Ratio Lower Upper
117 100
82 54.6 44.0 66.0
119 31.4 25.6 38.4

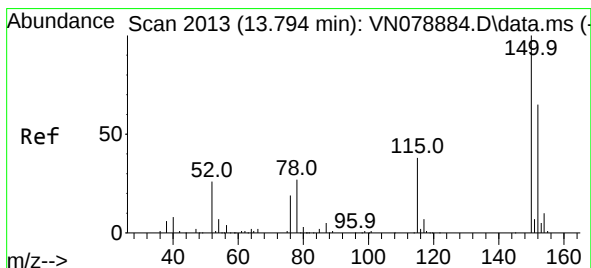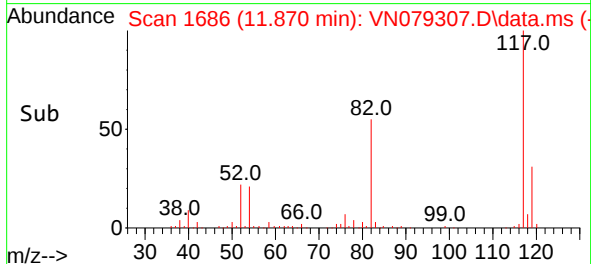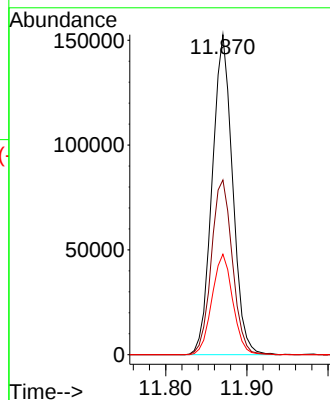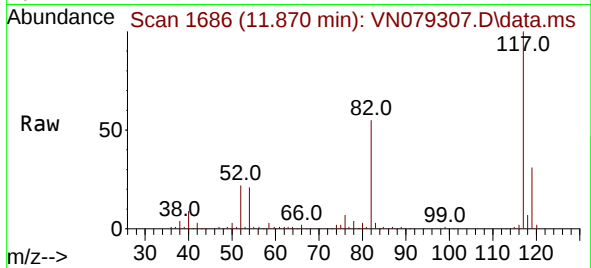

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN079307.D
Acq: 20 Sep 2023 10:34

Tgt Ion:152 Resp: 73473
Ion Ratio Lower Upper
152 100
115 62.3 32.3 96.8
150 156.7 0.0 355.8

