
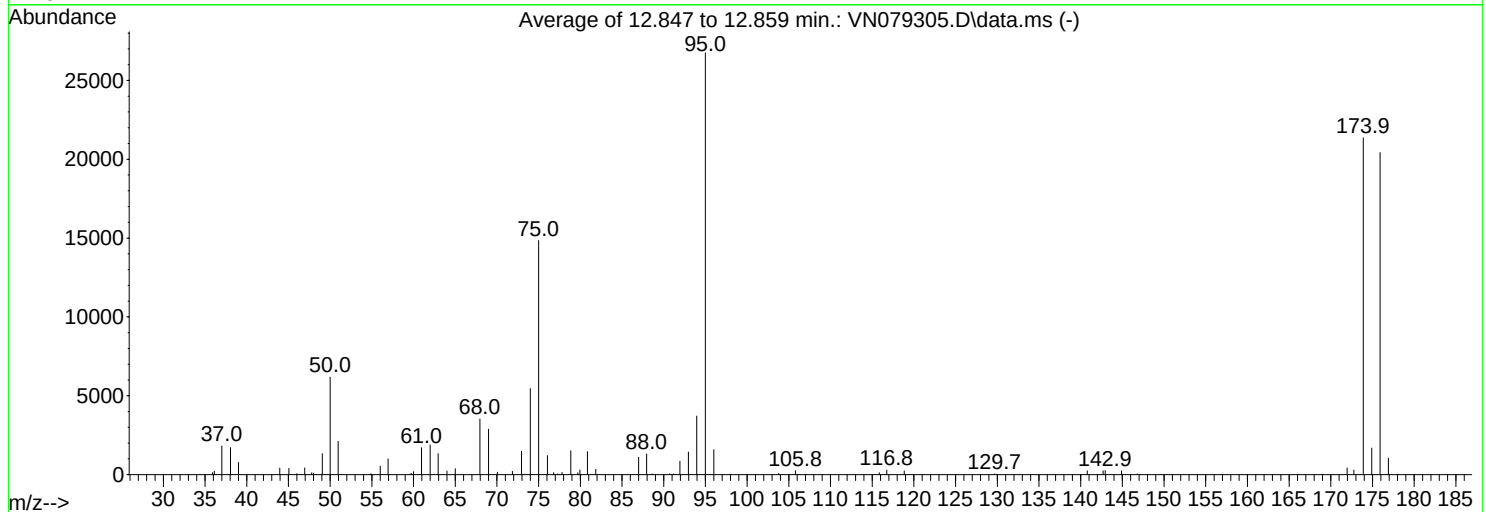


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092023\
Data File : VN079305.D
Acq On : 20 Sep 2023 09:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 05:05:24 2023

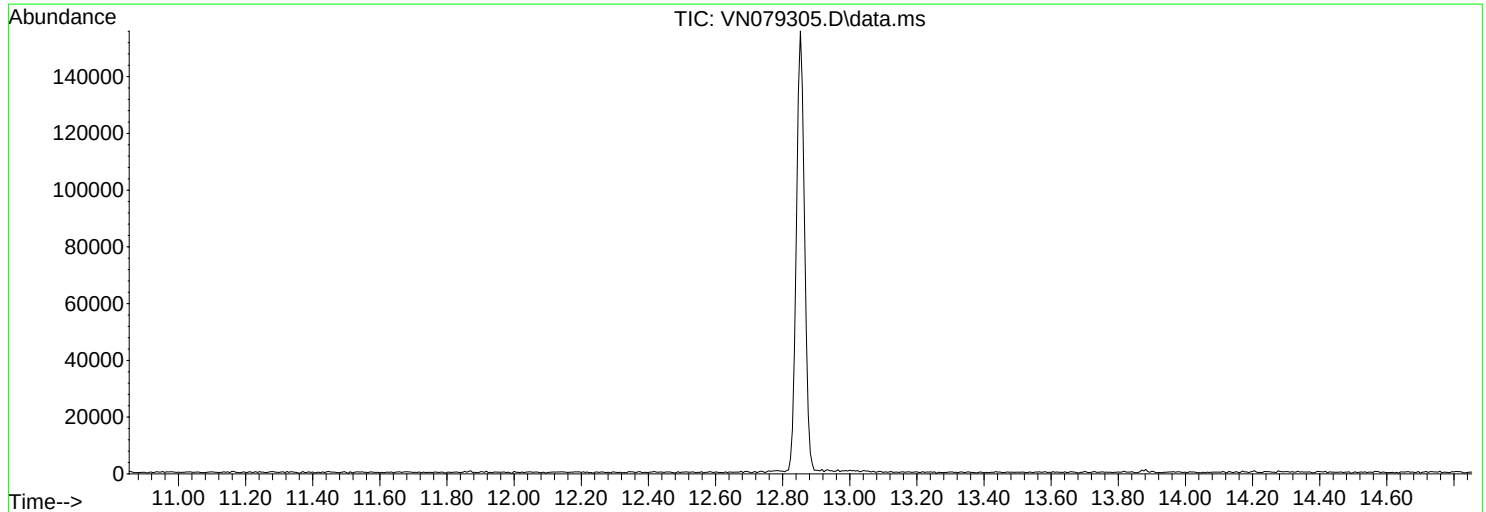

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.1	6178	PASS
75	95	30	60	55.5	14841	PASS
95	95	100	100	100.0	26749	PASS
96	95	5	9	5.9	1586	PASS
173	174	0.00	2	1.4	297	PASS
174	95	50	100	79.9	21363	PASS
175	174	5	9	7.9	1684	PASS
176	174	95	101	95.6	20421	PASS
177	176	5	9	5.1	1046	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	131	48.00	99	62.95	1329	76.80	131
36.10	214	49.05	1334	64.00	228	77.30	51
37.00	1814	50.00	6178	65.00	377	77.80	14
38.05	1718	50.95	2110	67.95	3528	78.85	151
39.00	770	54.90	64	69.00	2884	79.70	126
39.95	6	56.00	541	70.05	153	79.95	294
43.95	413	56.95	1003	71.85	212	80.85	1465
45.05	398	59.70	90	72.95	1485	81.85	332
46.00	58	60.00	189	74.00	5464	87.00	1110
46.95	424	60.95	1701	75.00	14841	87.95	1312
47.80	122	62.00	1891	76.05	1207	88.60	52

Average of 12.847 to 12.859 min.: VN079305.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.70	55	118.85	237	175.90	20421		
91.20	53	129.70	56	176.90	1046		
91.95	850	140.80	244				
92.95	1433	142.70	248				
93.95	3712	142.95	268				
95.00	26749	144.90	241				
96.00	1586	146.80	55				
103.80	74	171.95	431				
105.80	249	172.75	297				
115.85	122	173.90	21363				
116.75	293	174.90	1684				

Instrument :

MSVOA_N

ClientSampleId :

BFB