


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092118\
 Data File : VN051358.D
 Acq On : 21 Sep 2018 9:40
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N082818W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Aug 29 01:38:44 2018

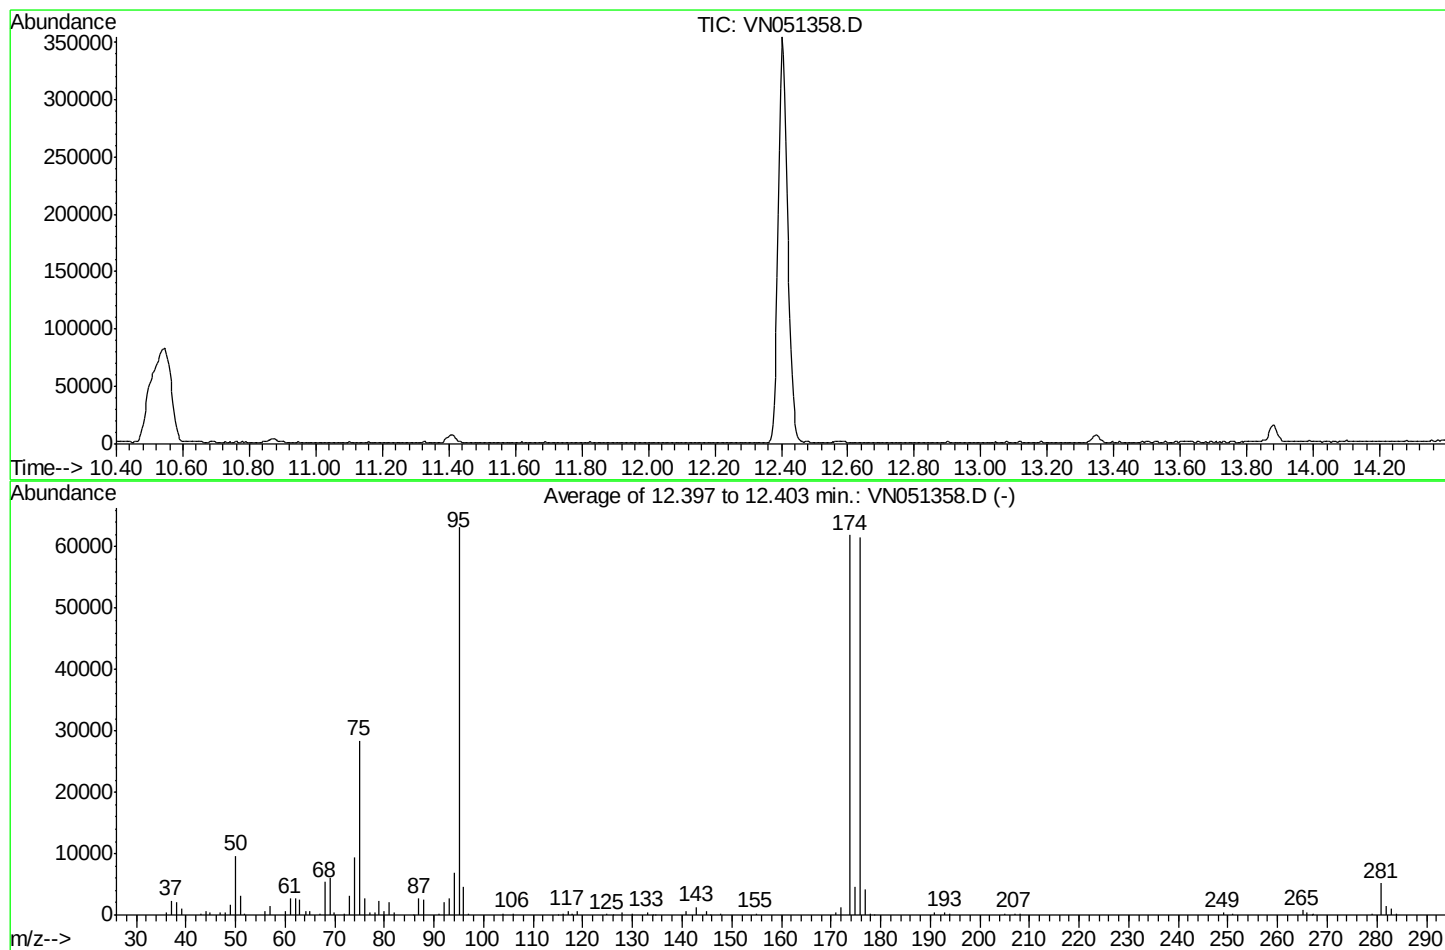

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	9671	PASS
75	95	30	60	45.0	28461	PASS
95	95	100	100	100.0	63189	PASS
96	95	5	9	7.4	4696	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	98.0	61898	PASS
175	174	5	9	7.6	4700	PASS
176	174	95	101	99.5	61597	PASS
177	176	5	9	6.7	4099	PASS