


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN092120\
 Data File : VN063474.D
 Acq On : 21 Sep 2020 9:27
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091620W.M
 Title : SW846 8260
 Last Update : Wed Sep 16 13:05:20 2020

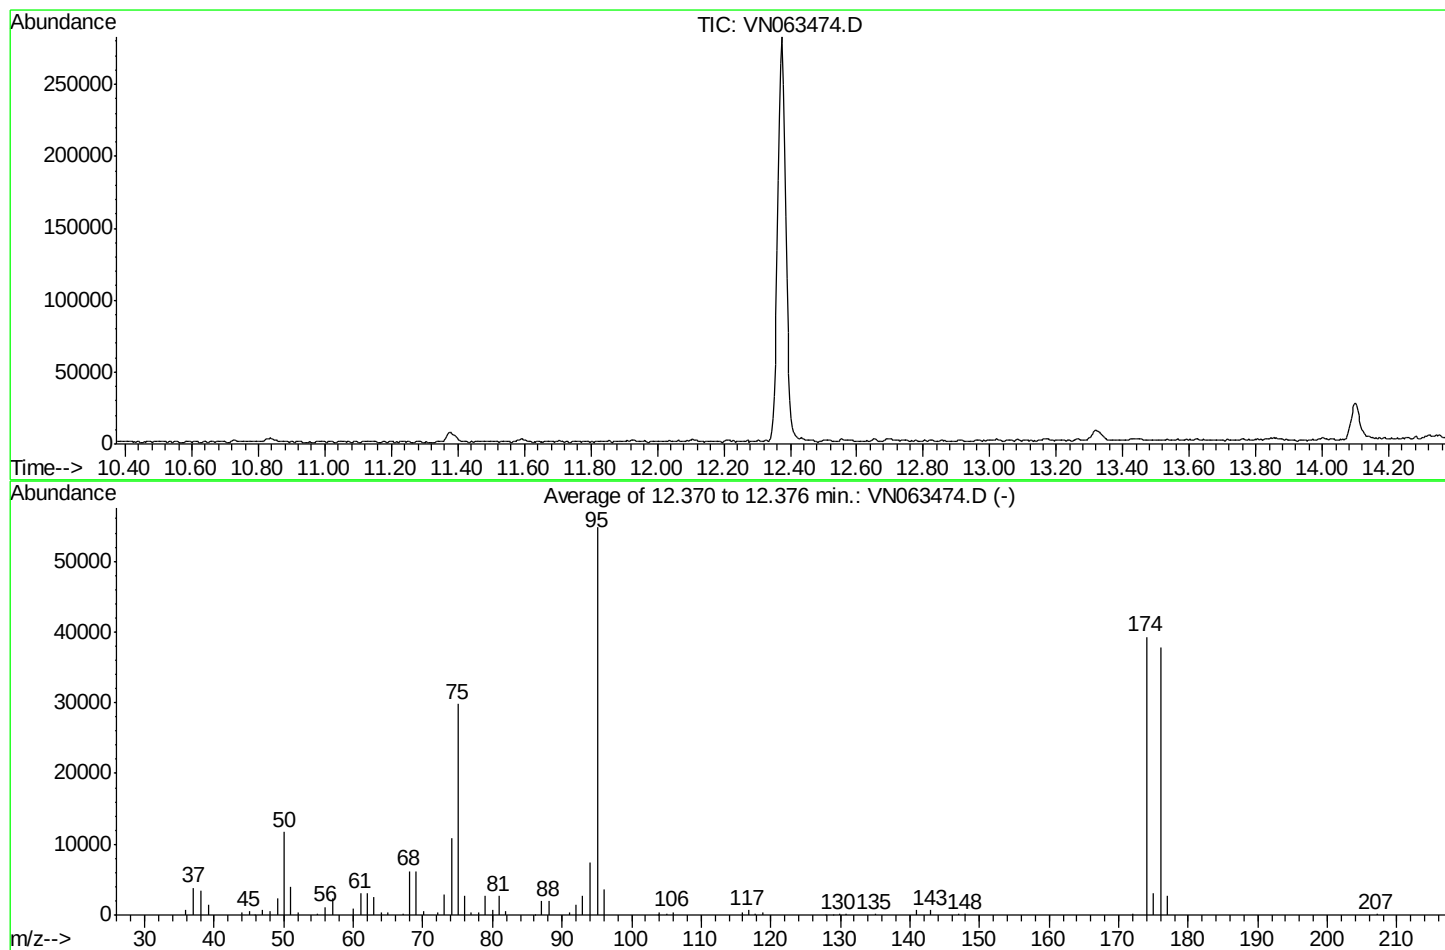

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	11742	PASS
75	95	30	60	54.4	29834	PASS
95	95	100	100	100.0	54792	PASS
96	95	5	9	6.6	3623	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.7	39261	PASS
175	174	5	9	8.0	3134	PASS
176	174	95	101	96.3	37810	PASS
177	176	5	9	7.0	2634	PASS