

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092121\
 Data File : VN068590.D
 Acq On : 21 Sep 2021 18:33
 Operator : JC/MD
 Sample : PB139153TB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB139153TB

Quant Time: Sep 22 03:42:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 17 11:02:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.091	168	618353	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	966105	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	944871	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	357497	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.442	65	331144	58.381	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 116.760%			
35) Dibromofluoromethane	8.027	113	293809	50.423	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 100.840%			
50) Toluene-d8	10.446	98	1186130	49.659	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 99.320%			
62) 4-Bromofluorobenzene	12.734	95	430516	54.265	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 108.520%			
Target Compounds					Qvalue	
3) Chloromethane	2.303	50	618	Below Cal	#	42
5) Bromomethane	2.850	94	202	Below Cal	#	69
11) Tert butyl alcohol	5.380	59	96	Below Cal	#	84
16) Acetone	4.293	43	14308	Below Cal		96
18) Methyl Acetate	4.862	43	1161	Below Cal	#	45
20) Methylene Chloride	5.106	84	25309	3.499	ug/l	98
25) 2-Butanone	7.345	43	14606	5.299	ug/l	95
29) Tetrahydrofuran	7.697	42	1164	0.647	ug/l #	50
31) Cyclohexane	8.091	56	11268	1.311	ug/l #	32
36) 1,1-Dichloropropene	8.088	75	42082	5.225	ug/l #	46
37) Ethyl Acetate	7.345	43	14606	2.384	ug/l #	66
38) Carbon Tetrachloride	8.088	117	59341	6.150	ug/l #	17
43) Isopropyl Acetate	8.563	43	42404	3.923	ug/l #	87
45) 1,2-Dichloropropane	9.620	63	2661	0.468	ug/l #	44
48) Methyl methacrylate	9.550	41	9942	2.203	ug/l #	6
49) 1,4-Dioxane	9.628	88	540	5.215	ug/l #	1
51) 4-Methyl-2-Pentanone	10.333	43	6650	1.078	ug/l	96
52) Toluene	10.508	92	4912	0.311	ug/l	98
54) cis-1,3-Dichloropropene	10.245	75	76367	8.367	ug/l #	66
57) 1,3-Dichloropropane	11.092	76	47092	4.868	ug/l #	42
59) 2-Hexanone	11.092	43	601932	145.657	ug/l #	47
60) Dibromochloromethane	11.489	129	545	1.864	ug/l #	11
70) Styrene	12.294	104	199	1.762	ug/l #	56
71) Bromoform	12.717	173	547	2.598	ug/l #	29
74) N-amyl acetate	12.361	43	3156	0.556	ug/l #	38
76) 1,2,3-Trichloropropane	12.734	75	226820	46.051	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.058	105	4457	0.216	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.734	75	226820	140.610	ug/l #	13
93) 1,2,4-Trichlorobenzene	15.260	180	109	2.974	ug/l #	12
95) Naphthalene	15.501	128	496	3.529	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.697	180	155	2.997	ug/l #	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092121\
Data File : VN068590.D
Acq On : 21 Sep 2021 18:33
Operator : JC/MD
Sample : PB139153TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB139153TB

Quant Time: Sep 22 03:42:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 17 11:02:11 2021
Response via : Initial Calibration




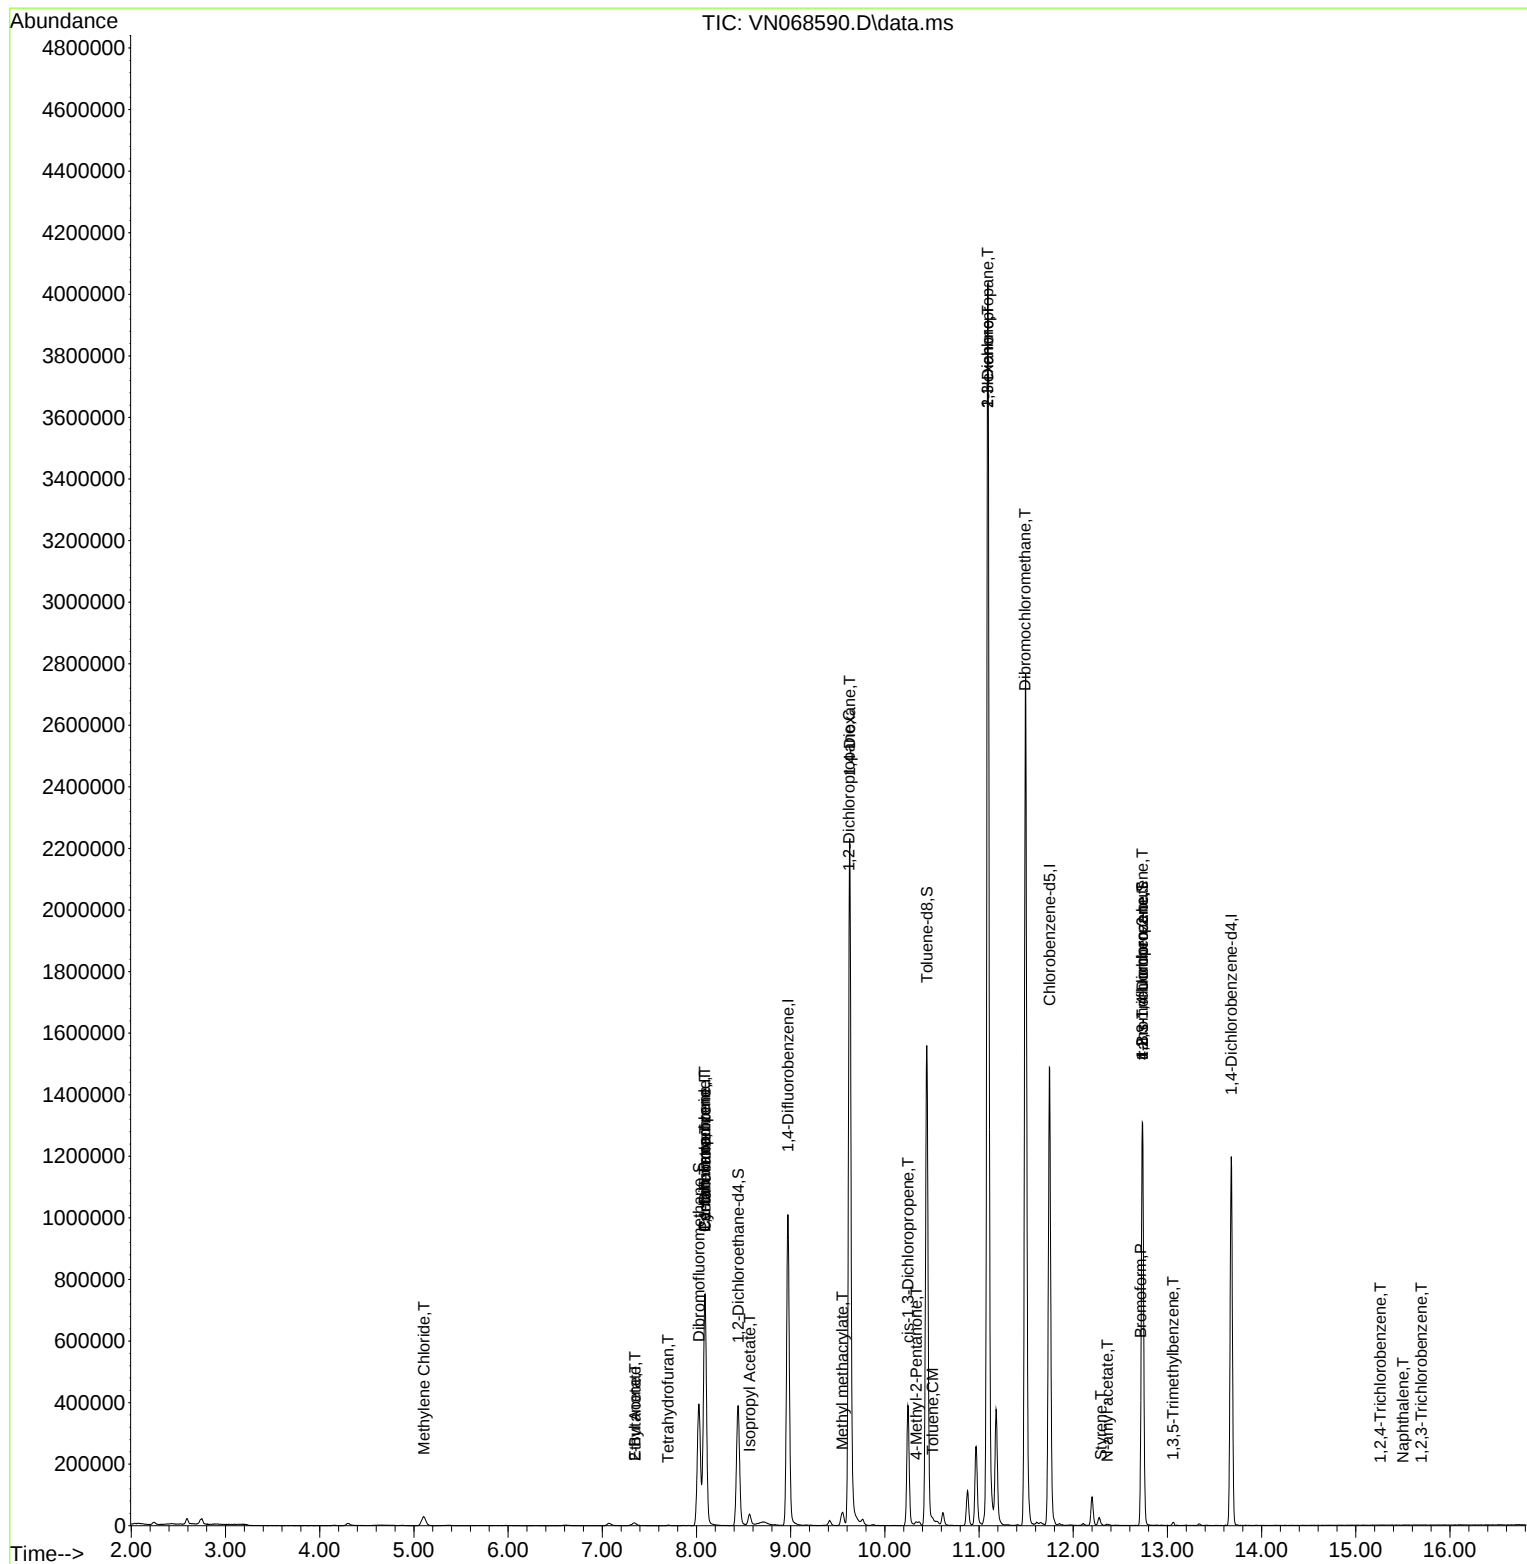




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. 0.000 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampled :
PB139153TB


Tgt Ion:168 Resp: 618353
Ion Ratio Lower Upper
168 100
99 51.8 38.2 57.4



#3
Chloromethane
Concen: Below Cal
RT: 2.303 min Scan# 117
Delta R.T. -0.006 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33


Tgt Ion: 50 Resp: 618
Ion Ratio Lower Upper
50 100
52 0.0 25.8 38.6#








#5
Bromomethane
Concen: Below Cal
RT: 2.850 min Scan# 321
Delta R.T. 0.010 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Instrument :
MSVOA_N
ClientSampleId :
PB139153TB







Tgt Ion: 94 Resp: 202
Ion Ratio Lower Upper
94 100
96 64.6 75.4 113.0#



#11
Tert butyl alcohol
Concen: Below Cal
RT: 5.380 min Scan# 1264
Delta R.T. 0.006 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion: 59 Resp: 96
Ion Ratio Lower Upper
59 100
57 0.0 4.3 6.5#









#16
Acetone
Concen: Below Cal
RT: 4.293 min Scan# 859
Delta R.T. 0.002 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampled :
PB139153TB


Tgt Ion: 43 Resp: 14308
Ion Ratio Lower Upper
43 100
58 31.4 27.0 40.6



#18
Methyl Acetate
Concen: Below Cal
RT: 4.862 min Scan# 1071
Delta R.T. 0.006 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion: 43 Resp: 1161
Ion Ratio Lower Upper
43 100
74 0.0 23.5 35.3#

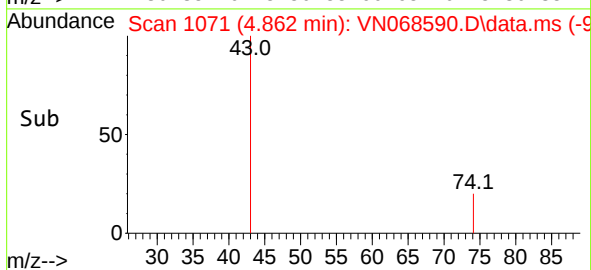

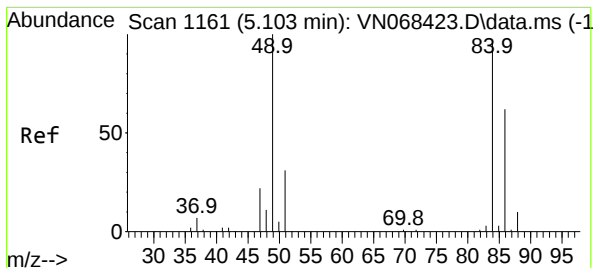

#20

Methylene Chloride

Concen: 3.499 ug/l

RT: 5.106 min Scan# 1162

Delta R.T. 0.003 min

Lab File: VN068590.D

Acq: 21 Sep 2021 18:33

Instrument :

MSVOA_N

ClientSampled :

PB139153TB

Tgt Ion: 84 Resp: 25309





Ion Ratio Lower Upper

84 100

49 102.0 83.0 124.6

51 29.6 25.4 38.0

86 65.2 51.3 76.9

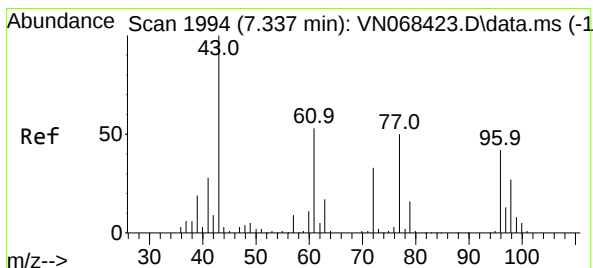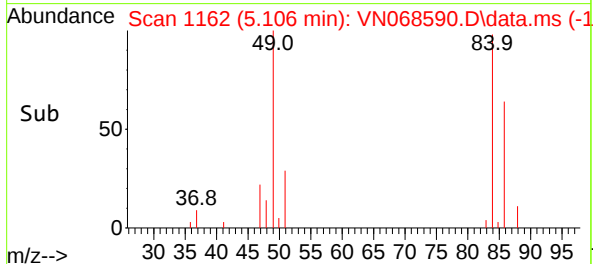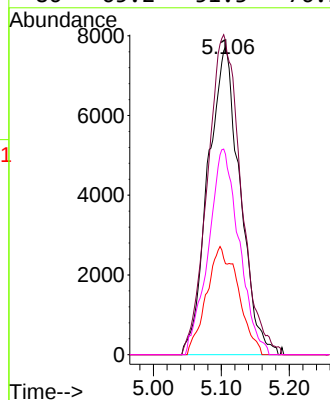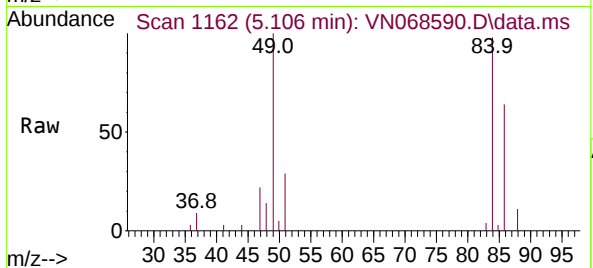

#25

2-Butanone

Concen: 5.299 ug/l

RT: 7.345 min Scan# 1997

Delta R.T. 0.008 min

Lab File: VN068590.D




Acq: 21 Sep 2021 18:33


Tgt Ion: 43 Resp: 14606

Ion Ratio Lower Upper

43 100

72 30.7 26.7 40.1

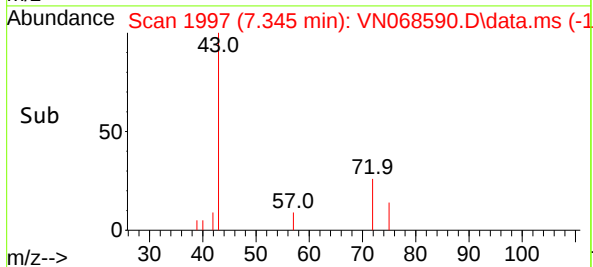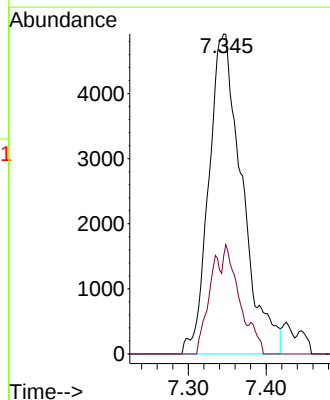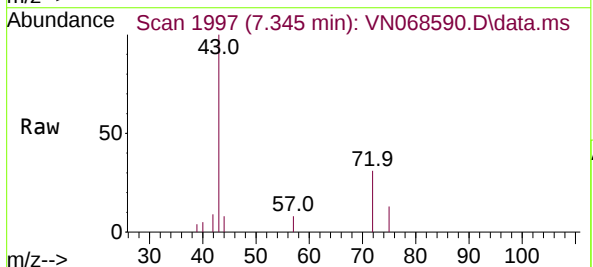



#29

Tetrahydrofuran

Concen: 0.647 ug/l

RT: 7.697 min Scan# 2128





Delta R.T. 0.011 min

Lab File: VN068590.D

Acq: 21 Sep 2021 18:33

Tgt Ion:	42	Resp:	1164
Ion	Ratio	Lower	Upper
42	100		
72	24.7	44.4	66.6#
71	11.1	42.3	63.5#

Instrument :
MSVOA_N
ClientSampleId :
PB139153TB



#31

Cyclohexane

Concen: 1.311 ug/l




RT: 8.091 min Scan# 2275


Delta R.T. -0.008 min

Lab File: VN068590.D

Acq: 21 Sep 2021 18:33

Tgt Ion:	56	Resp:	11268
Ion	Ratio	Lower	Upper
56	100		
69	149.0	29.4	44.0#
84	130.6	83.6	125.4#

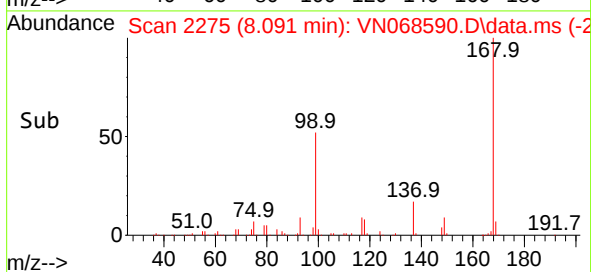







#33

1,2-Dichloroethane-d4
Concen: 58.381 ug/l
RT: 8.442 min Scan# 2406
Delta R.T. 0.002 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Instrument :
MSVOA_N
ClientSampled :
PB139153TB




Tgt Ion: 65 Resp: 331144
Ion Ratio Lower Upper
65 100
67 51.9 0.0 104.0




#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. -0.000 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion: 114 Resp: 966105
Ion Ratio Lower Upper
114 100
63 17.3 0.0 33.2
88 14.1 0.0 28.4









#35
Dibromofluoromethane
Concen: 50.423 ug/l
RT: 8.027 min Scan# 2251
Delta R.T. 0.003 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampled :
PB139153TB


Tgt Ion:113 Resp: 293809
Ion Ratio Lower Upper
113 100
111 101.7 81.1 121.7
192 20.2 17.7 26.5

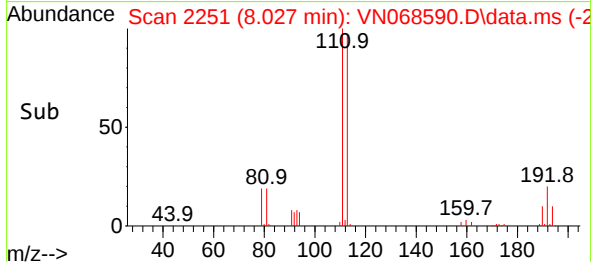

#36
1,1-Dichloropropene
Concen: 5.225 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.137 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion: 75 Resp: 42082
Ion Ratio Lower Upper
75 100
110 9.5 20.8 62.5#
77 0.0 25.0 37.6#

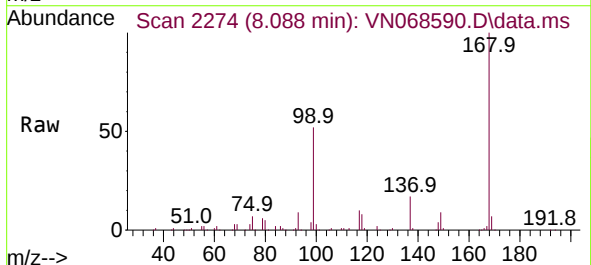



#37

Ethyl Acetate

Concen: 2.384 ug/l

RT: 7.345 min Scan# 1997

Delta R.T. -0.070 min

Lab File: VN068590.D

Acq: 21 Sep 2021 18:33





Instrument :

MSVOA_N

ClientSampled :

PB139153TB

Tgt Ion:	43	Resp:	14606
Ion	Ratio	Lower	Upper
43	100		
61	0.0	12.4	18.6#
70	0.0	9.6	14.4#

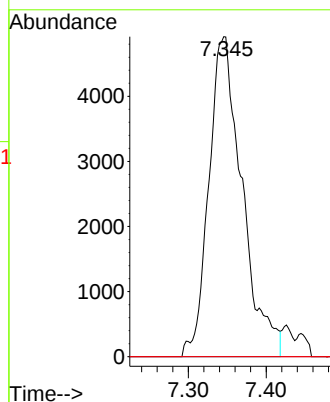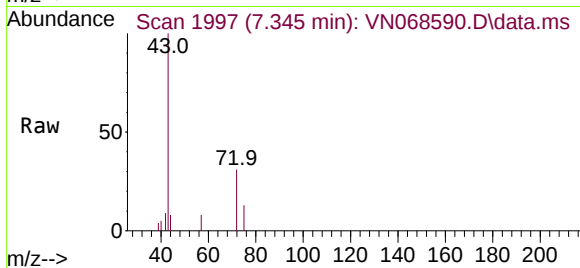

#38

Carbon Tetrachloride

Concen: 6.150 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.121 min

Lab File: VN068590.D

Acq: 21 Sep 2021 18:33


Tgt Ion:	117	Resp:	59341
Ion	Ratio	Lower	Upper
117	100		
119	6.0	76.6	114.8#
121	0.0	24.5	36.7#

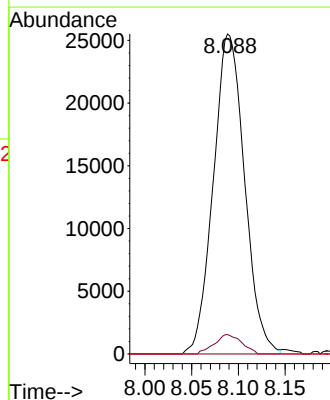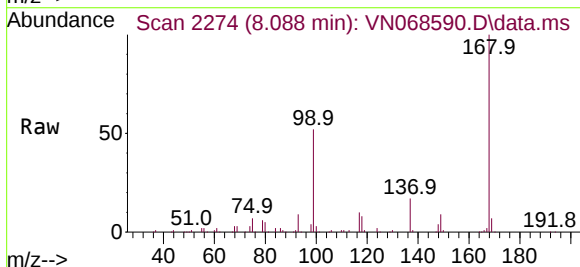






#43
Isopropyl Acetate
Concen: 3.923 ug/l
RT: 8.563 min Scan# 2451
Delta R.T. 0.000 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Instrument :
MSVOA_N
ClientSampled :
PB139153TB







Tgt Ion	Ratio	Lower	Upper
43	100		
61	19.6	23.3	34.9#
87	15.1	13.8	20.6



#45
1,2-Dichloropropane
Concen: 0.468 ug/l
RT: 9.620 min Scan# 2845
Delta R.T. 0.126 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion	Ratio	Lower	Upper
63	100		
65	0.0	24.8	37.2#


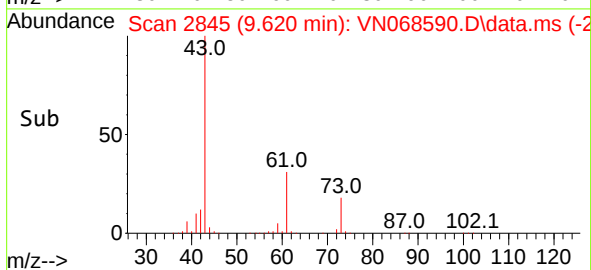






#48
Methyl methacrylate
Concen: 2.203 ug/l
RT: 9.550 min Scan# 2819
Delta R.T. -0.011 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampled :
PB139153TB


Tgt Ion: 41 Resp: 9942
Ion Ratio Lower Upper
41 100
69 0.0 82.9 124.3#
39 0.0 50.3 75.5#

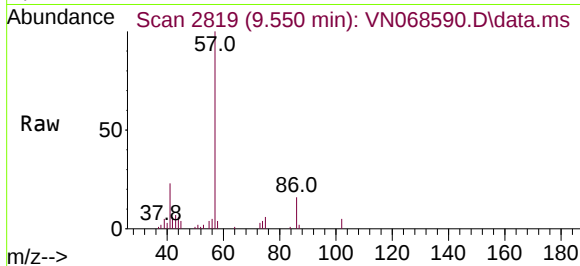

#49
1,4-Dioxane
Concen: 5.215 ug/l
RT: 9.628 min Scan# 2848
Delta R.T. 0.057 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion: 88 Resp: 540
Ion Ratio Lower Upper
88 100
43 410595.0 18.9 28.3#
58 1896.9 46.6 69.8#




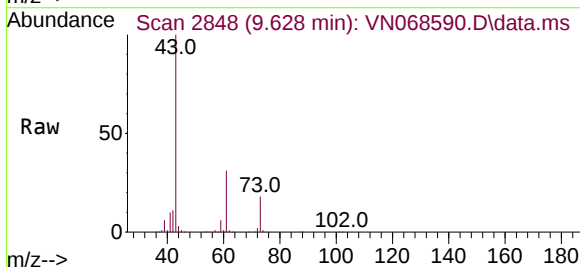




#50
Toluene-d8
Concen: 49.659 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampleId :
PB139153TB


Tgt Ion: 98 Resp: 1186130
Ion Ratio Lower Upper
98 100
100 64.4 51.0 76.6



#51
4-Methyl-2-Pentanone
Concen: 1.078 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.000 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion: 43 Resp: 6650
Ion Ratio Lower Upper
43 100
58 45.2 34.3 51.5


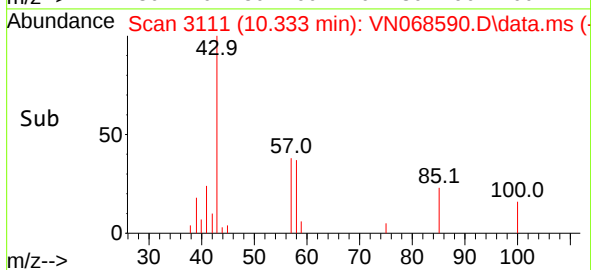






#52
Toluene
Concen: 0.311 ug/l
RT: 10.508 min Scan# 3176
Delta R.T. 0.001 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampled :
PB139153TB


Tgt Ion: 92 Resp: 4912
Ion Ratio Lower Upper
92 100
91 176.4 139.4 209.0

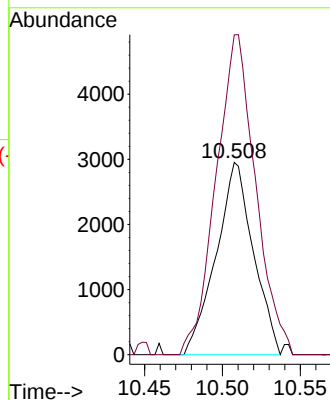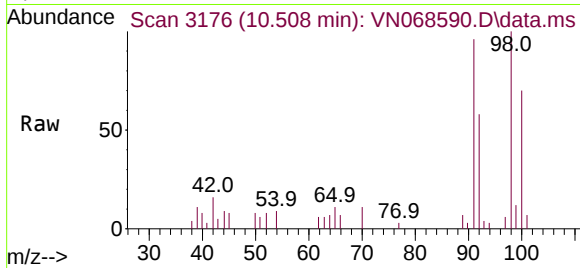

#54
cis-1,3-Dichloropropene
Concen: 8.367 ug/l
RT: 10.245 min Scan# 3078
Delta R.T. 0.054 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion: 75 Resp: 76367
Ion Ratio Lower Upper
75 100
77 0.5 25.3 37.9#
39 32.2 34.6 52.0#


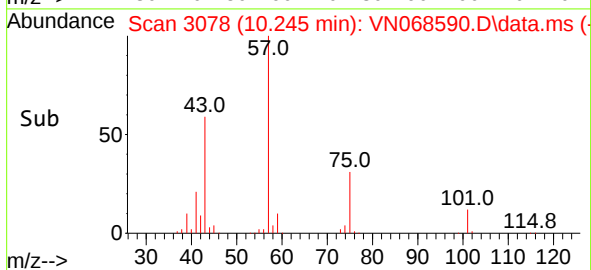
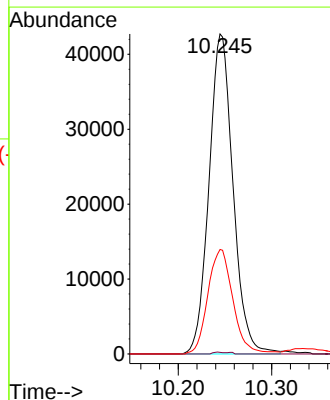
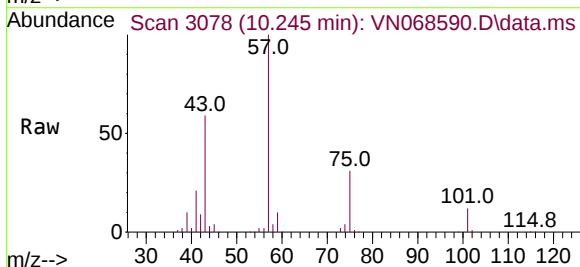


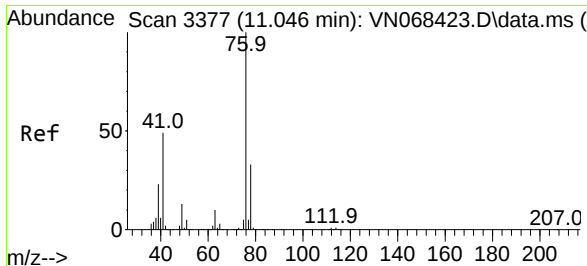

#57
1,3-Dichloropropane
Concen: 4.868 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.046 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampled :
PB139153TB


Tgt Ion: 76 Resp: 47092
Ion Ratio Lower Upper
76 100
78 0.1 25.9 38.9#

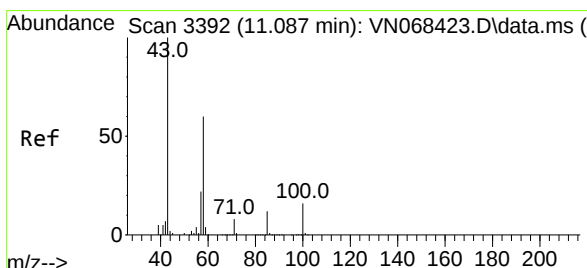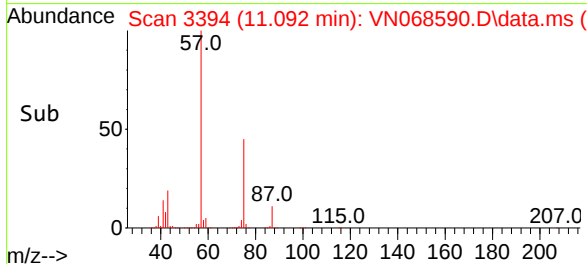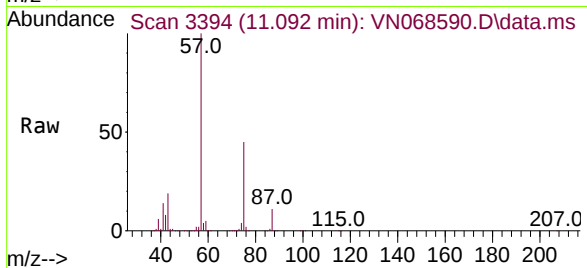

#59
2-Hexanone
Concen: 145.657 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.005 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion: 43 Resp: 601932
Ion Ratio Lower Upper
43 100
58 19.9 30.0 90.1#


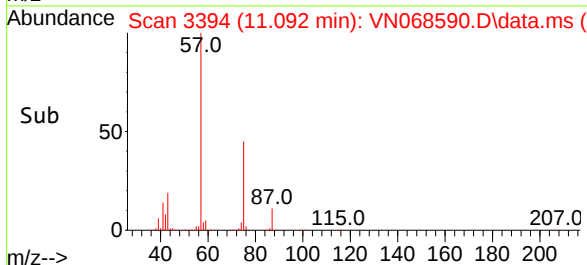

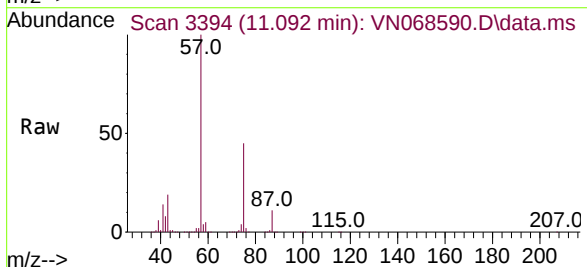




#60
Dibromochloromethane
Concen: 1.864 ug/l
RT: 11.489 min Scan# 3542
Delta R.T. 0.249 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampleId :
PB139153TB


Tgt Ion:129 Resp: 545
Ion Ratio Lower Upper
129 100
127 0.0 38.5 115.3#

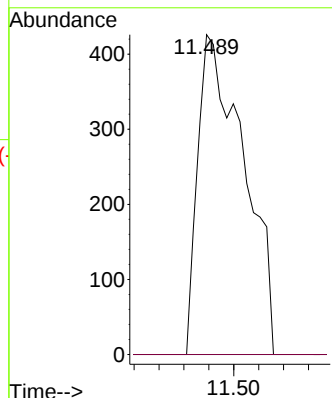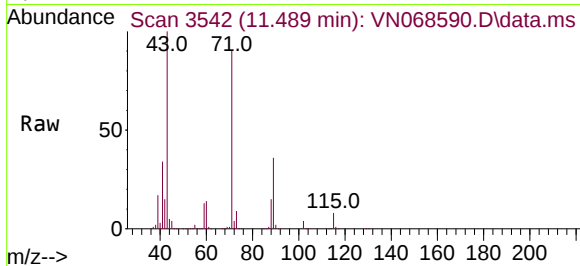

#62
4-Bromofluorobenzene
Concen: 54.265 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion: 95 Resp: 430516
Ion Ratio Lower Upper
95 100
174 94.2 0.0 214.0
176 90.0 0.0 205.4


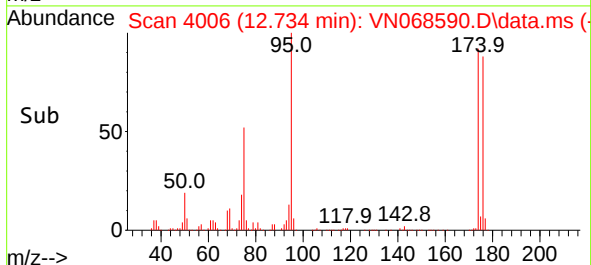
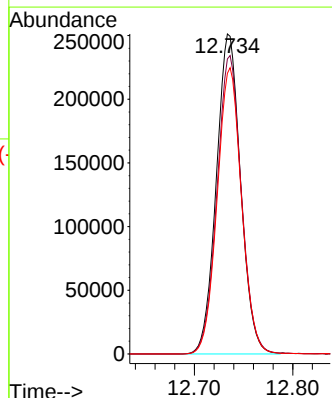
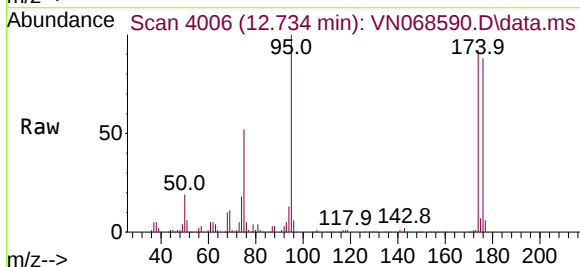




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampleId :
PB139153TB


Tgt Ion:117 Resp: 944871
Ion Ratio Lower Upper
117 100
82 49.6 38.7 58.1
119 32.2 25.5 38.3

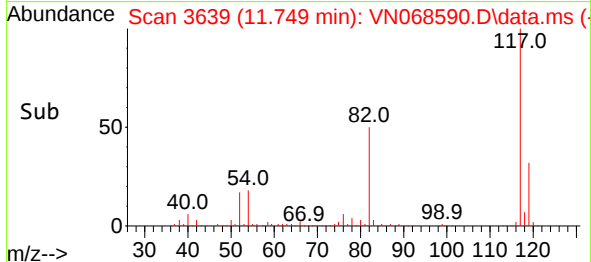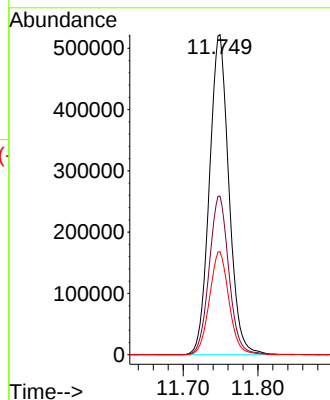

#70
Styrene
Concen: 1.762 ug/l
RT: 12.294 min Scan# 3842
Delta R.T. -0.002 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion:104 Resp: 199
Ion Ratio Lower Upper
104 100
78 28.1 36.2 54.2#
103 12.6 44.4 66.6#



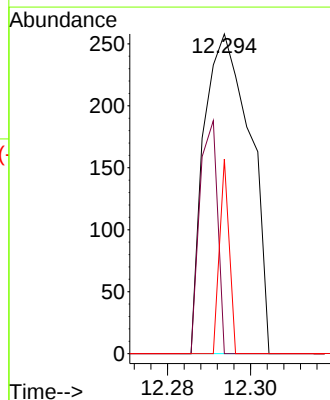
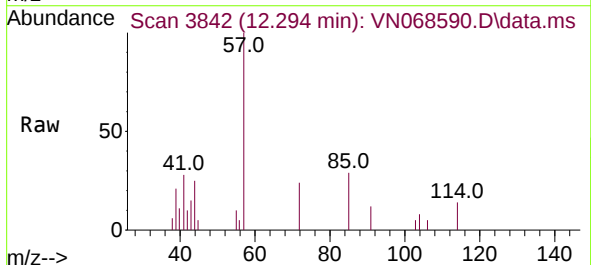


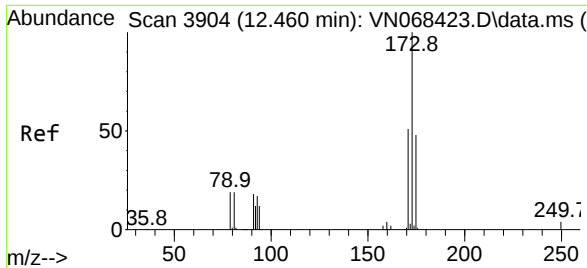

#71
Bromoform
Concen: 2.598 ug/l
RT: 12.717 min Scan# 4000
Delta R.T. 0.257 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampleId :
PB139153TB


Tgt Ion:173 Resp: 547
Ion Ratio Lower Upper
173 100
175 0.0 24.1 72.3#
254 0.0 0.0 0.0

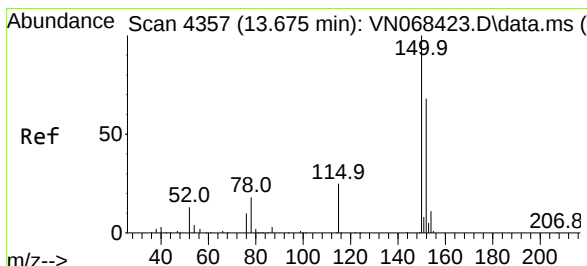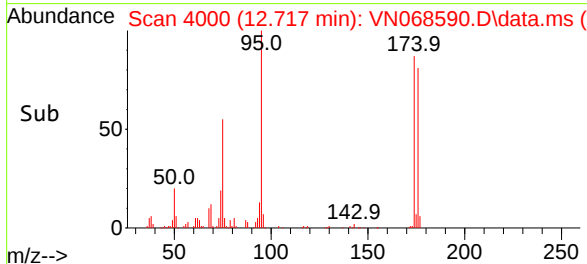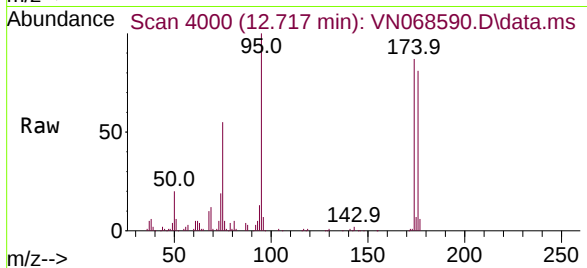

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33


Tgt Ion:152 Resp: 357497
Ion Ratio Lower Upper
152 100
115 53.3 25.6 76.6
150 156.3 0.0 346.8

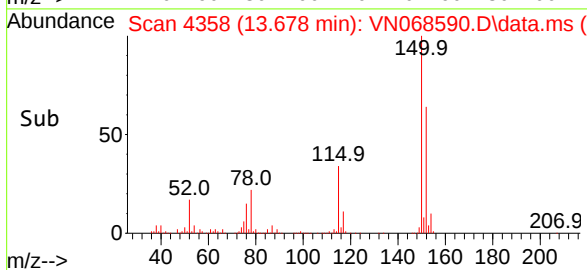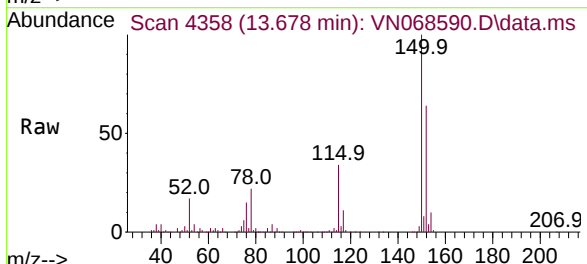






#74
N-amy1 acetate
Concen: 0.556 ug/l
RT: 12.361 min Scan# 3867
Delta R.T. -0.029 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Instrument :
MSVOA_N
ClientSampleId :
PB139153TB







Tgt Ion:	43	Resp:	3156
Ion	Ratio	Lower	Upper
43	100		
70	0.0	40.0	60.0#
55	0.0	21.1	31.7#
61	0.0	21.2	31.8#



#76
1,2,3-Trichloropropane
Concen: 46.051 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.147 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion:	75	Resp:	226820
Ion	Ratio	Lower	Upper
75	100		
77	1.2	100.9	302.7#







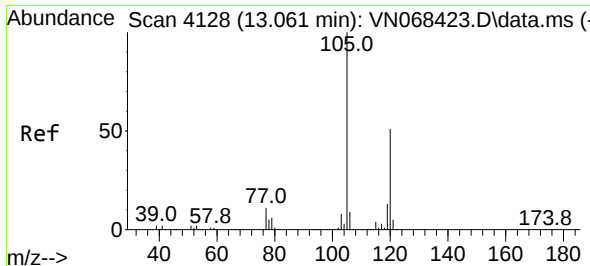

#80
1,3,5-Trimethylbenzene
Concen: 0.216 ug/l
RT: 13.058 min Scan# 4127
Delta R.T. -0.003 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampled :
PB139153TB


Tgt Ion:105 Resp: 4457
Ion Ratio Lower Upper
105 100
120 49.7 25.7 77.1

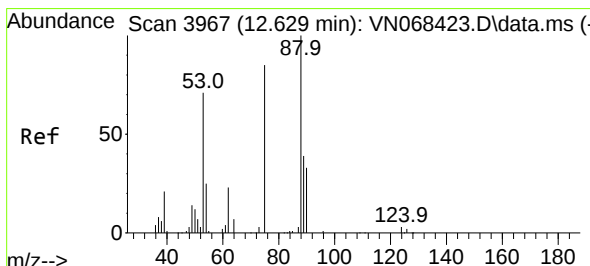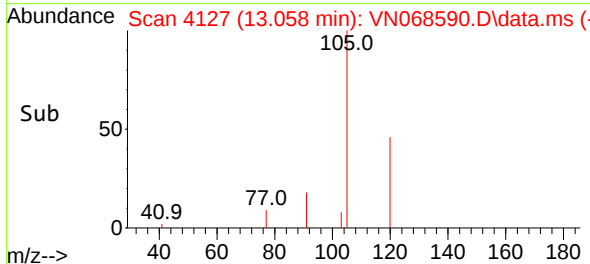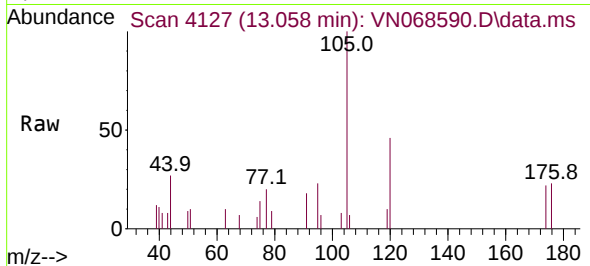

#81
trans-1,4-Dichloro-2-butene
Concen: 140.610 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion: 75 Resp: 226820
Ion Ratio Lower Upper
75 100
53 0.1 70.6 105.8#
89 0.0 39.5 59.3#


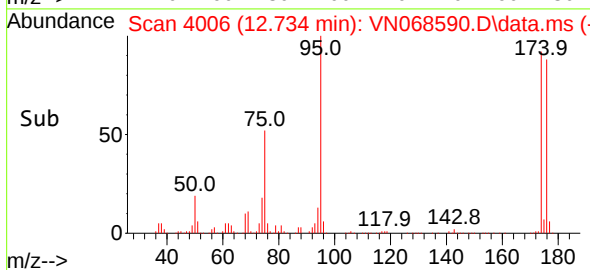

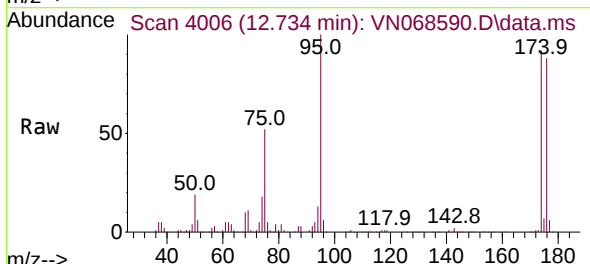




#93
1,2,4-Trichlorobenzene
Concen: 2.974 ug/l
RT: 15.260 min Scan# 4948
Delta R.T. -0.005 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33




Instrument :
MSVOA_N
ClientSampleId :
PB139153TB


Tgt Ion:180 Resp: 109
Ion Ratio Lower Upper
180 100
182 0.0 47.5 142.6#
145 0.0 14.1 42.4#

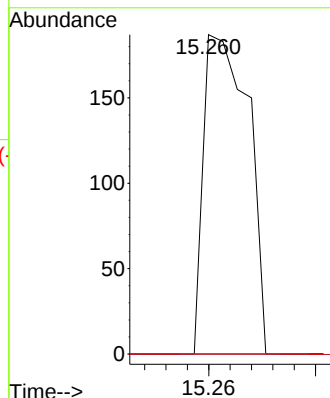

#95
Naphthalene
Concen: 3.529 ug/l
RT: 15.501 min Scan# 5038
Delta R.T. -0.006 min
Lab File: VN068590.D
Acq: 21 Sep 2021 18:33

Tgt Ion:128 Resp: 496
Ion Ratio Lower Upper
128 100
127 0.0 10.6 15.8#
129 0.0 8.6 13.0#

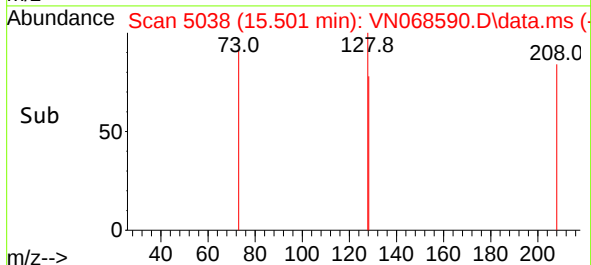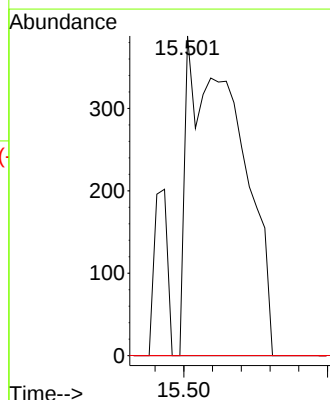



#96
 1,2,3-Trichlorobenzene
 Concen: 2.997 ug/l
 RT: 15.697 min Scan# 5111
 Delta R.T. -0.005 min
 Lab File: VN068590.D
 Acq: 21 Sep 2021 18:33

Instrument :
 MSVOA_N
 ClientSampleId :
 PB139153TB

Tgt Ion:	180	Resp:	155
Ion	Ratio	Lower	Upper
180	100		
182	33.5	47.9	143.6#
145	0.0	15.2	45.5#

