

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092121\
 Data File : VN068592.D
 Acq On : 21 Sep 2021 19:23
 Operator : JC/MD
 Sample : PB139153ZHE#02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB139153ZHE#02

Quant Time: Sep 22 03:43:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 17 11:02:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.091	168	775393	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	1029625	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	946358	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	372499	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	404638	56.890	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 113.780%			
35) Dibromofluoromethane	8.027	113	357512	57.571	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 115.140%			
50) Toluene-d8	10.443	98	1202033	47.395	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 94.800%			
62) 4-Bromofluorobenzene	12.733	95	411895	49.140	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 98.280%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.295	50	231	Below Cal	#	42
5) Bromomethane	2.799	94	151	Below Cal	#	3
11) Tert butyl alcohol	5.361	59	51	Below Cal	#	84
16) Acetone	4.293	43	46213	14.555	ug/l	94
18) Methyl Acetate	4.867	43	2334	Below Cal	#	61
20) Methylene Chloride	5.103	84	29698	3.183	ug/l	96
25) 2-Butanone	7.340	43	4513	1.306	ug/l	96
29) Tetrahydrofuran	7.697	42	2633	1.167	ug/l #	51
31) Cyclohexane	8.086	56	14119	1.310	ug/l #	28
36) 1,1-Dichloropropene	8.091	75	50960	5.937	ug/l #	47
37) Ethyl Acetate	7.340	43	4513	0.691	ug/l #	66
38) Carbon Tetrachloride	8.088	117	71522	6.955	ug/l #	16
41) Methacrylonitrile	7.691	41	903	0.281	ug/l #	29
43) Isopropyl Acetate	8.563	43	60276	5.232	ug/l #	83
45) 1,2-Dichloropropane	9.622	63	3225	0.532	ug/l #	44
48) Methyl methacrylate	9.545	41	10414	2.165	ug/l #	6
49) 1,4-Dioxane	9.620	88	284	2.573	ug/l #	1
51) 4-Methyl-2-Pentanone	10.336	43	8944	1.360	ug/l	91
54) cis-1,3-Dichloropropene	10.245	75	84150	8.651	ug/l #	65
57) 1,3-Dichloropropane	11.092	76	47995	4.655	ug/l #	42
59) 2-Hexanone	11.095	43	631170	143.310	ug/l #	46
60) Dibromochloromethane	11.502	129	498	1.855	ug/l #	11
70) Styrene	12.286	104	24	1.755	ug/l #	27
71) Bromoform	12.728	173	1183	2.682	ug/l #	1
74) N-amyl acetate	12.200	43	26448	4.475	ug/l #	48
76) 1,2,3-Trichloropropane	12.733	75	216097	42.011	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.733	75	216097	128.568	ug/l #	13
93) 1,2,4-Trichlorobenzene	15.271	180	160	2.981	ug/l #	12
95) Naphthalene	15.509	128	691	3.540	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.716	180	25	2.978	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092121\
Data File : VN068592.D
Acq On : 21 Sep 2021 19:23
Operator : JC/MD
Sample : PB139153ZHE#02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02

Quant Time: Sep 22 03:43:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 17 11:02:11 2021
Response via : Initial Calibration




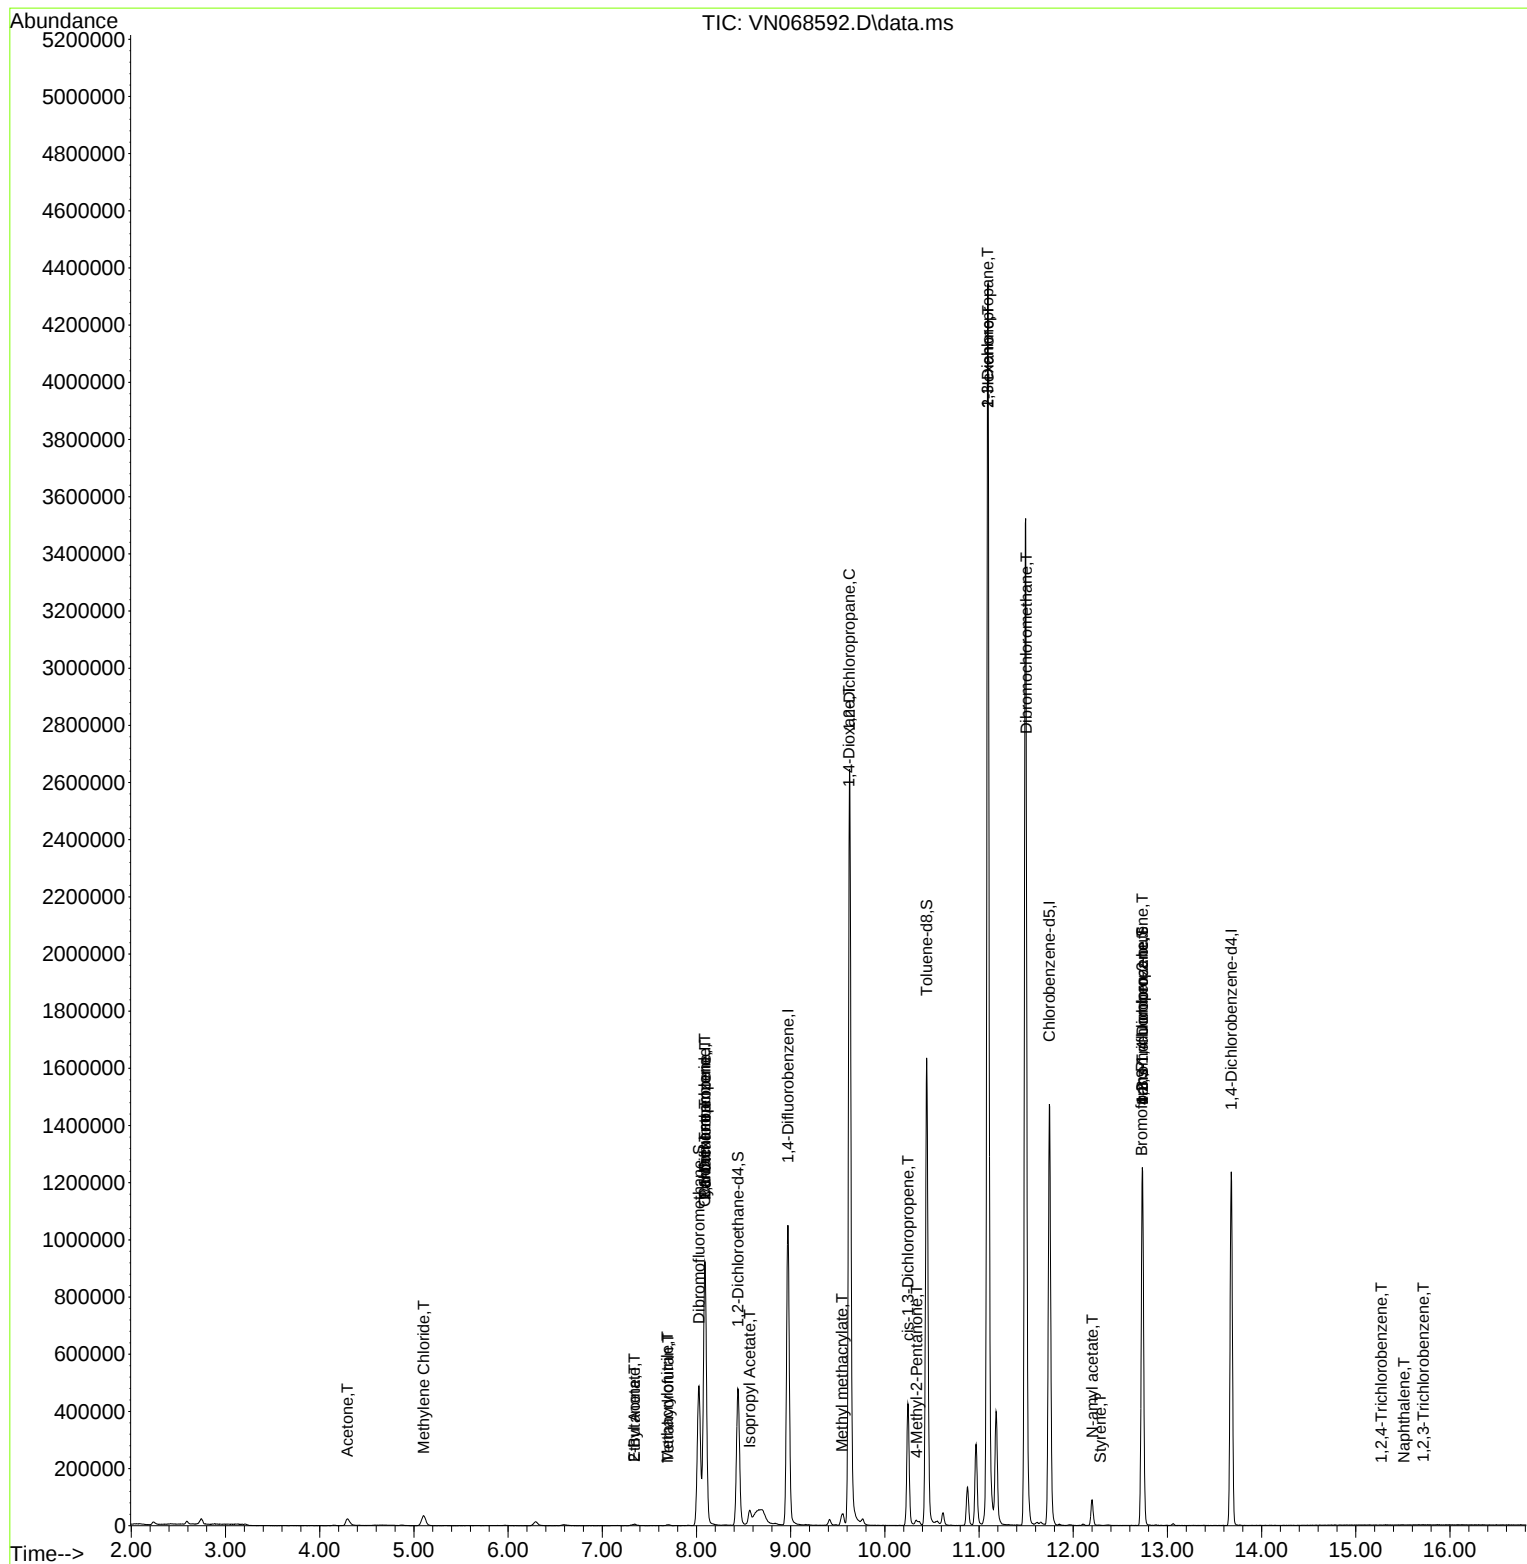




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. 0.000 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23




Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02


Tgt Ion:168 Resp: 775393
Ion Ratio Lower Upper
168 100
99 50.5 38.2 57.4



#3
Chloromethane
Concen: Below Cal
RT: 2.295 min Scan# 114
Delta R.T. -0.014 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion: 50 Resp: 231
Ion Ratio Lower Upper
50 100
52 0.0 25.8 38.6#


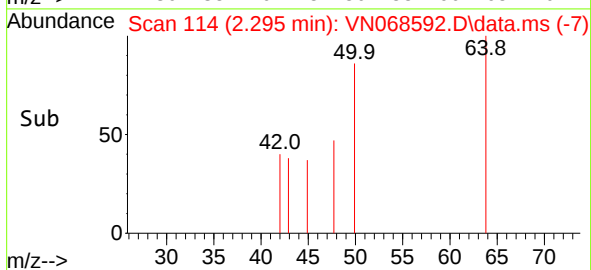






#5
Bromomethane
Concen: Below Cal
RT: 2.799 min Scan# 302
Delta R.T. -0.041 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23




Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02


Tgt Ion: 94 Resp: 151
Ion Ratio Lower Upper
94 100
96 0.0 75.4 113.0#



#11
Tert butyl alcohol
Concen: Below Cal
RT: 5.361 min Scan# 1257
Delta R.T. -0.013 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion: 59 Resp: 51
Ion Ratio Lower Upper
59 100
57 0.0 4.3 6.5#


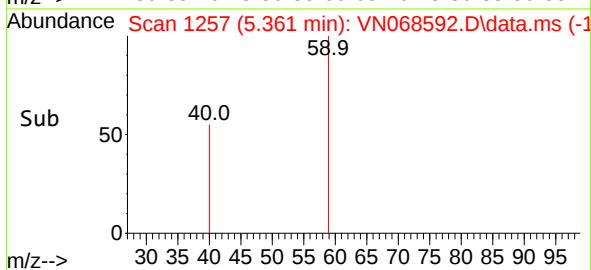






#16
Acetone
Concen: 14.555 ug/l
RT: 4.293 min Scan# 859
Delta R.T. 0.002 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23




Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02


Tgt Ion: 43 Resp: 46213
Ion Ratio Lower Upper
43 100
58 30.5 27.0 40.6



#18
Methyl Acetate
Concen: Below Cal
RT: 4.867 min Scan# 1073
Delta R.T. 0.011 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23


Tgt Ion: 43 Resp: 2334
Ion Ratio Lower Upper
43 100
74 8.4 23.5 35.3#

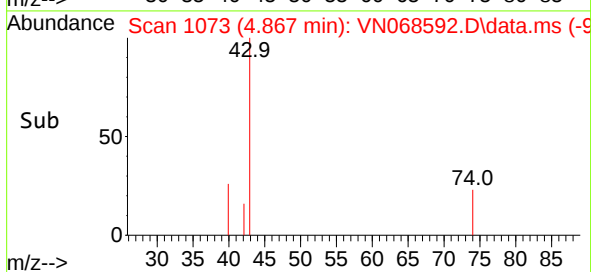



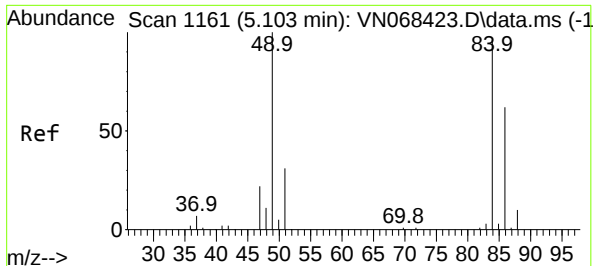


#20
Methylene Chloride
Concen: 3.183 ug/l
RT: 5.103 min Scan# 1161
Delta R.T. 0.000 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02







Tgt Ion:	84	Resp:	29698
Ion	Ratio	Lower	Upper
84	100		
49	101.6	83.0	124.6
51	37.1	25.4	38.0
86	66.2	51.3	76.9

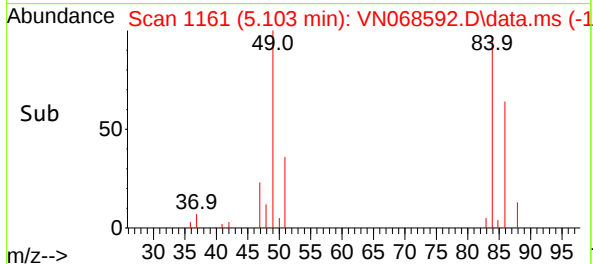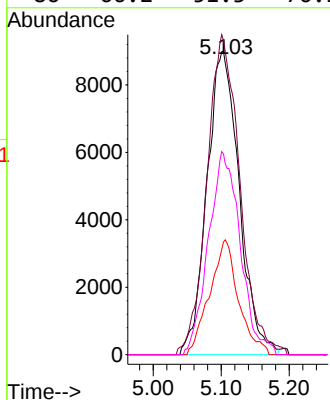

#25
2-Butanone
Concen: 1.306 ug/l
RT: 7.340 min Scan# 1995
Delta R.T. 0.003 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion:	43	Resp:	4513
Ion	Ratio	Lower	Upper
43	100		
72	31.3	26.7	40.1

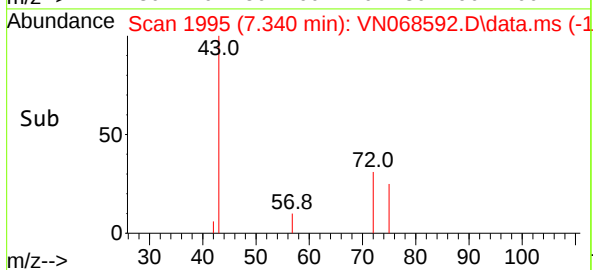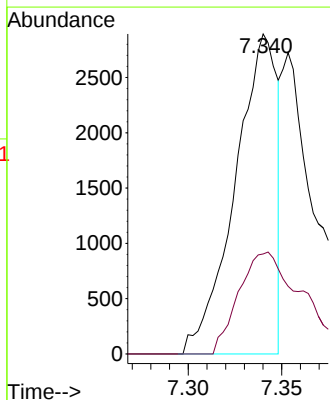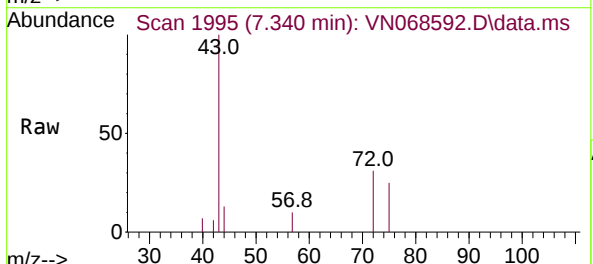

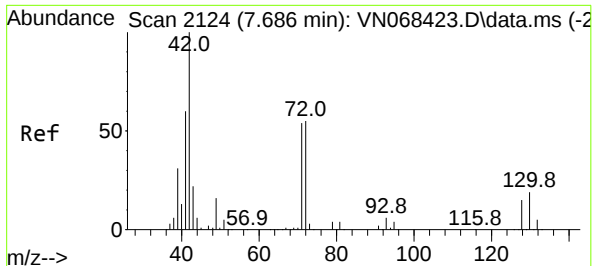

#29

Tetrahydrofuran

Concen: 1.167 ug/l

RT: 7.697 min Scan# 2128





Delta R.T. 0.011 min

Lab File: VN068592.D

Acq: 21 Sep 2021 19:23

Tgt Ion:	42	Resp:	2633
Ion	Ratio	Lower	Upper
42	100		
72	5.5	44.4	66.6#
71	32.5	42.3	63.5#

Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02

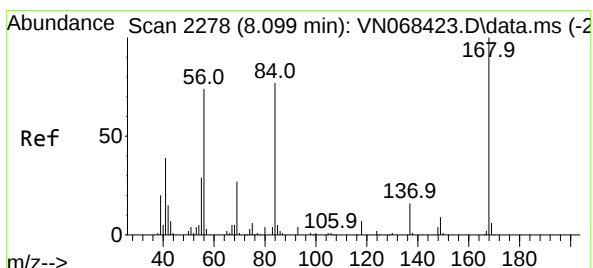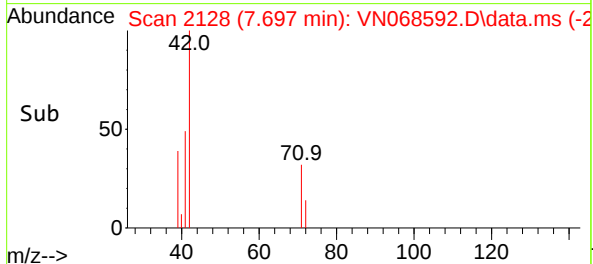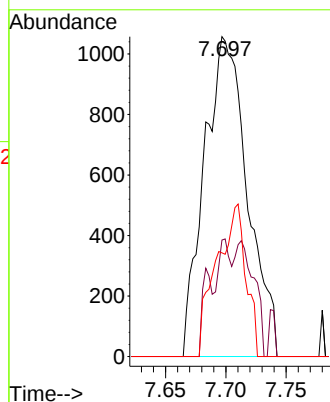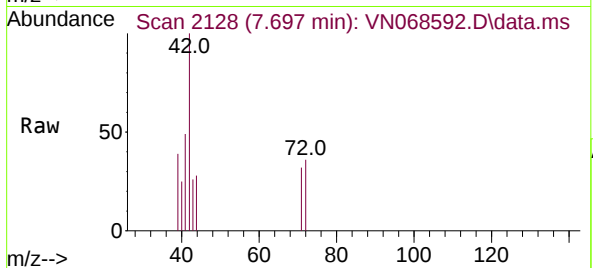

#31

Cyclohexane

Concen: 1.310 ug/l




RT: 8.086 min Scan# 2273


Delta R.T. -0.013 min

Lab File: VN068592.D

Acq: 21 Sep 2021 19:23

Tgt Ion:	56	Resp:	14119
Ion	Ratio	Lower	Upper
56	100		
69	159.4	29.4	44.0#
84	130.0	83.6	125.4#

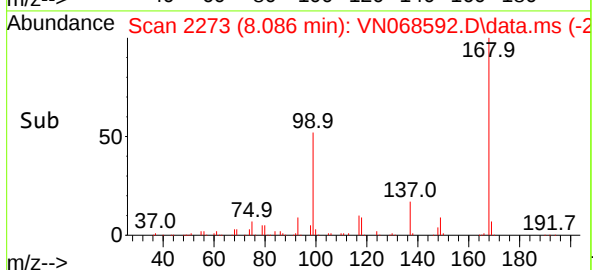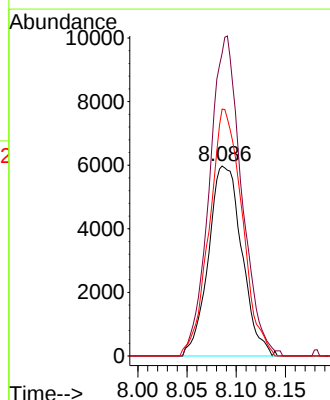







#33

1,2-Dichloroethane-d4
Concen: 56.890 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02




Tgt Ion: 65 Resp: 404638
Ion Ratio Lower Upper
65 100
67 51.8 0.0 104.0

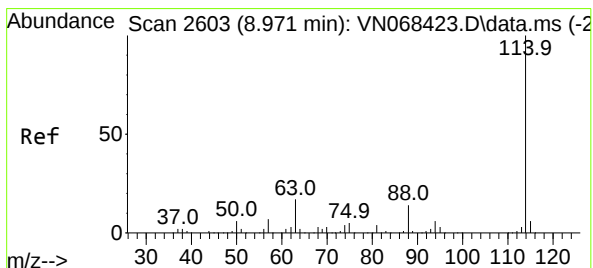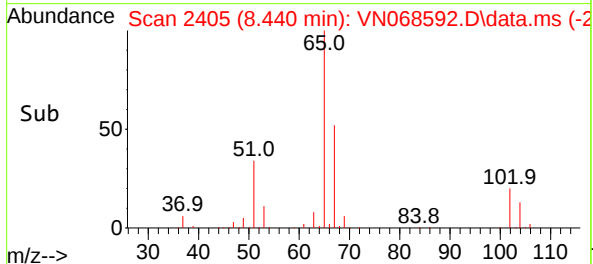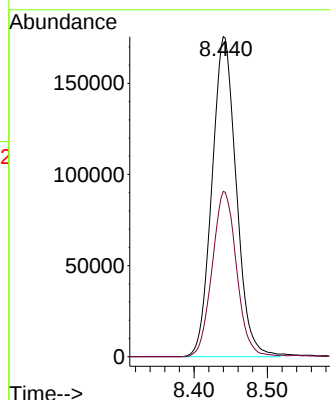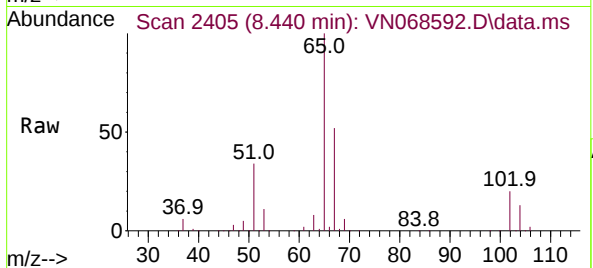


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. -0.000 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion: 114 Resp: 1029625
Ion Ratio Lower Upper
114 100
63 17.0 0.0 33.2
88 14.0 0.0 28.4

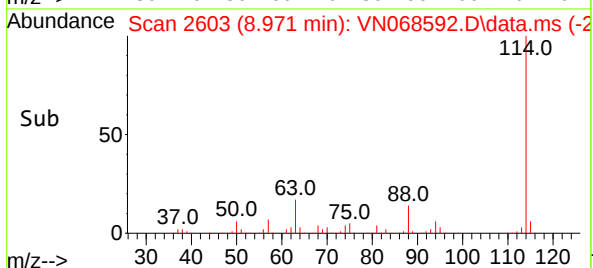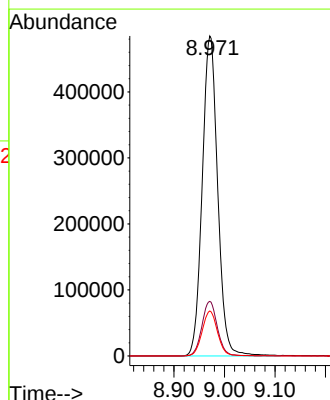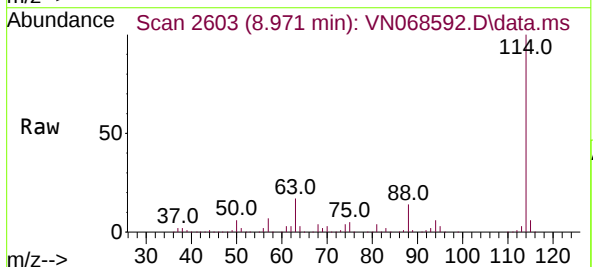



#35

Dibromofluoromethane

Concen: 57.571 ug/l

RT: 8.027 min Scan# 2251

Delta R.T. 0.003 min

Lab File: VN068592.D

Acq: 21 Sep 2021 19:23





Tgt Ion: 113 Resp: 357512

Ion Ratio Lower Upper

113 100

111 102.3 81.1 121.7

192 21.4 17.7 26.5

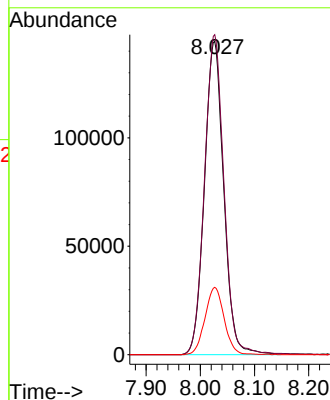

#36

1,1-Dichloropropene

Concen: 5.937 ug/l

RT: 8.091 min Scan# 2275

Delta R.T. -0.134 min

Lab File: VN068592.D

Acq: 21 Sep 2021 19:23




Tgt Ion: 75 Resp: 50960


Ion Ratio Lower Upper

75 100

110 10.1 20.8 62.5#

77 0.0 25.0 37.6#

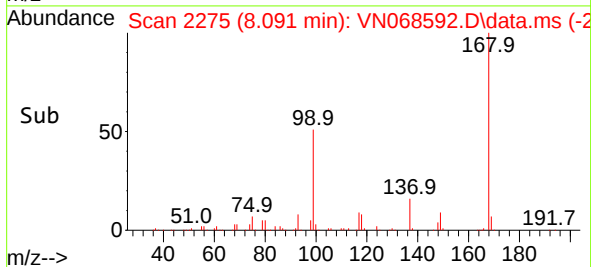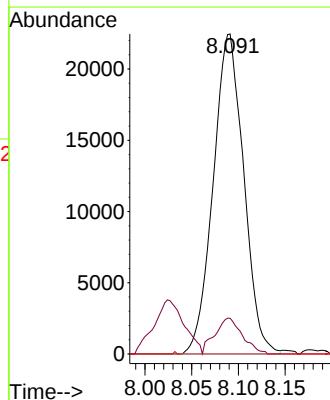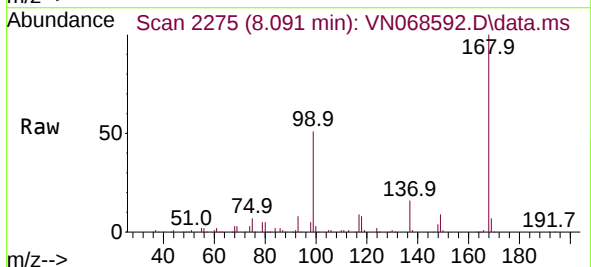



#37

Ethyl Acetate

Concen: 0.691 ug/l

RT: 7.340 min Scan# 1995

Delta R.T. -0.075 min

Lab File: VN068592.D


Acq: 21 Sep 2021 19:23

Instrument :




MSVOA_N

ClientSampleId :

PB139153ZHE#02



Tgt Ion:	43	Resp:	4513
Ion	Ratio	Lower	Upper
43	100		
61	0.0	12.4	18.6#
70	0.0	9.6	14.4#



#38

Carbon Tetrachloride

Concen: 6.955 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.121 min

Lab File: VN068592.D

Acq: 21 Sep 2021 19:23

Tgt Ion:	117	Resp:	71522
Ion	Ratio	Lower	Upper
117	100		
119	5.1	76.6	114.8#
121	0.0	24.5	36.7#

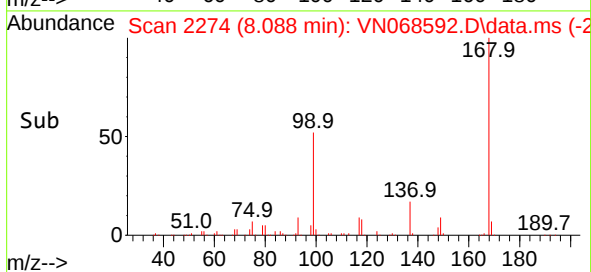







#41
Methacrylonitrile
Concen: 0.281 ug/l
RT: 7.691 min Scan# 2126
Delta R.T. 0.053 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02

Tgt Ion: 41 Resp: 903




Ion	Ratio	Lower	Upper
41	100		
39	35.1	45.4	68.2#
67	0.0	78.7	118.1#
52	0.0	29.0	43.6#

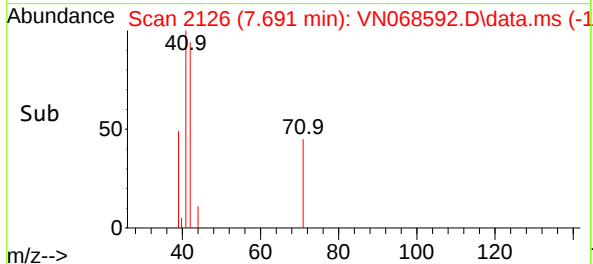


#43
Isopropyl Acetate
Concen: 5.232 ug/l
RT: 8.563 min Scan# 2451
Delta R.T. 0.000 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion: 43 Resp: 60276

Ion	Ratio	Lower	Upper
43	100		
61	17.4	23.3	34.9#
87	13.1	13.8	20.6#

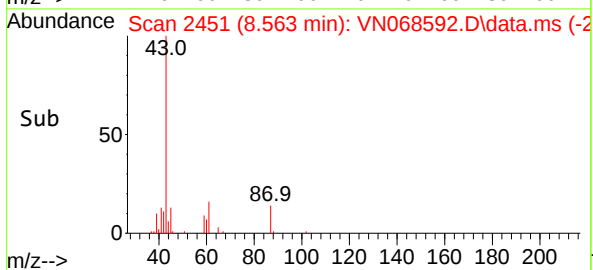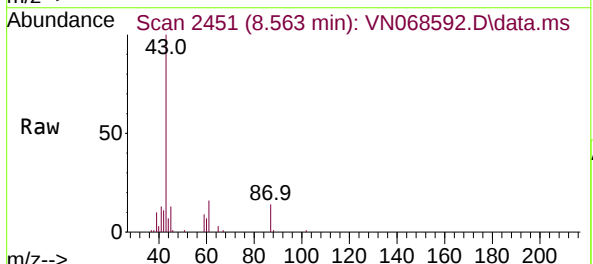







#45

1,2-Dichloropropane
Concen: 0.532 ug/l
RT: 9.622 min Scan# 2846
Delta R.T. 0.128 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02




Tgt Ion: 63 Resp: 3225
Ion Ratio Lower Upper
63 100
65 0.0 24.8 37.2#

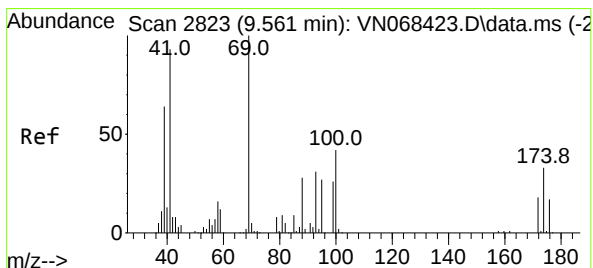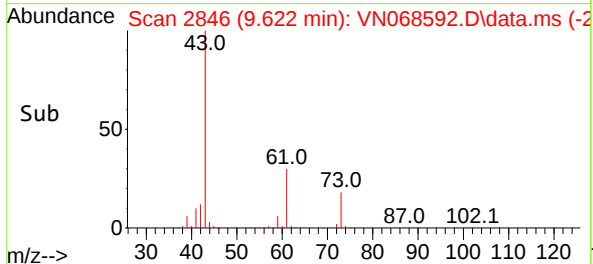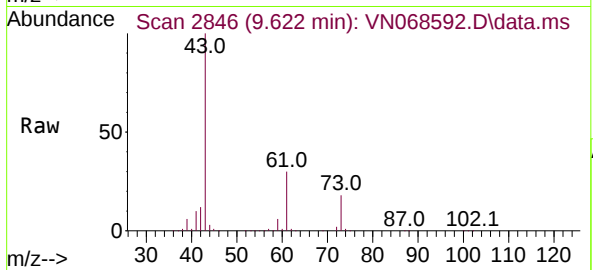


#48

Methyl methacrylate
Concen: 2.165 ug/l
RT: 9.545 min Scan# 2817
Delta R.T. -0.016 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion: 41 Resp: 10414
Ion Ratio Lower Upper
41 100
69 0.0 82.9 124.3#
39 0.0 50.3 75.5#

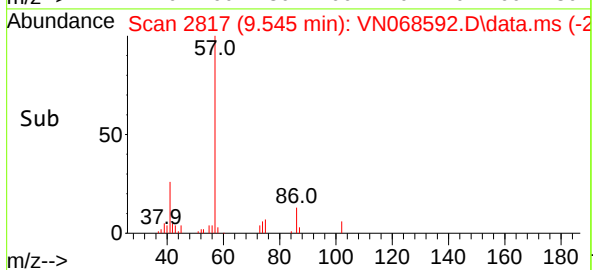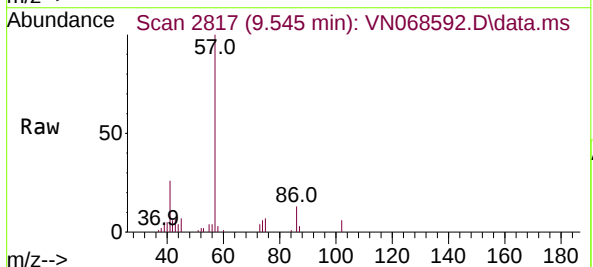



#49

1,4-Dioxane

Concen: 2.573 ug/l

RT: 9.620 min Scan# 2845

Delta R.T. 0.049 min

Lab File: VN068592.D

Acq: 21 Sep 2021 19:23

Instrument :

MSVOA_N

ClientSampleId :

PB139153ZHE#02





Tgt Ion: 88 Resp: 284

Ion Ratio Lower Upper

88 100

43 912614.4 18.9 28.3#

58 4541.9 46.6 69.8#

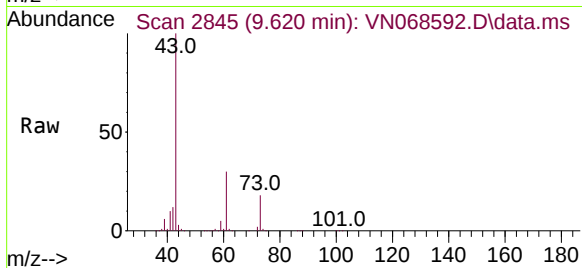

#50

Toluene-d8

Concen: 47.395 ug/l

RT: 10.443 min Scan# 3152

Delta R.T. 0.000 min

Lab File: VN068592.D




Acq: 21 Sep 2021 19:23


Tgt Ion: 98 Resp: 1202033

Ion Ratio Lower Upper

98 100

100 64.1 51.0 76.6


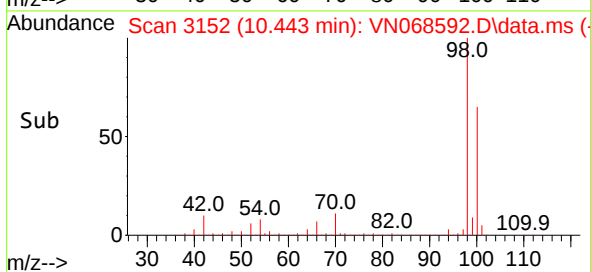

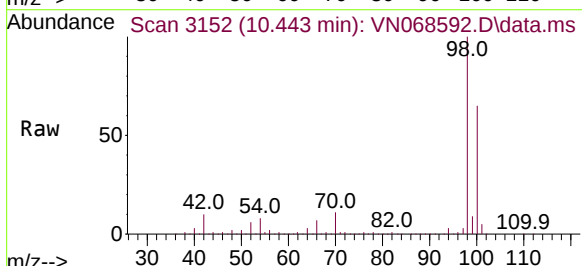




#51
4-Methyl-2-Pentanone
Concen: 1.360 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23




Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02


Tgt Ion: 43 Resp: 8944
Ion Ratio Lower Upper
43 100
58 48.9 34.3 51.5



#54
cis-1,3-Dichloropropene
Concen: 8.651 ug/l
RT: 10.245 min Scan# 3078
Delta R.T. 0.054 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion: 75 Resp: 84150
Ion Ratio Lower Upper
75 100
77 0.3 25.3 37.9#
39 31.4 34.6 52.0#


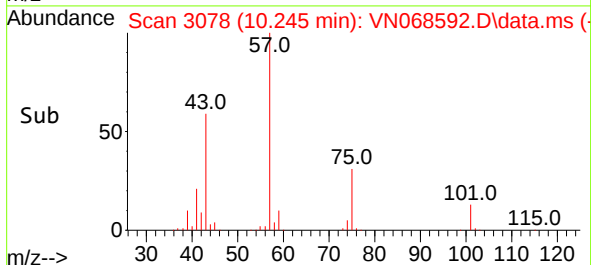

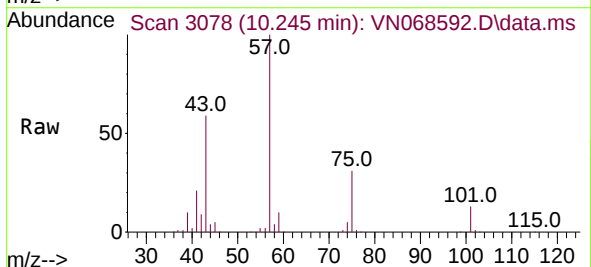


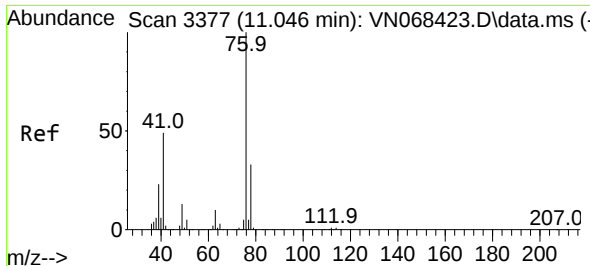

#57
1,3-Dichloropropane
Concen: 4.655 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.046 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23




Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02


Tgt Ion: 76 Resp: 47995
Ion Ratio Lower Upper
76 100
78 0.1 25.9 38.9#

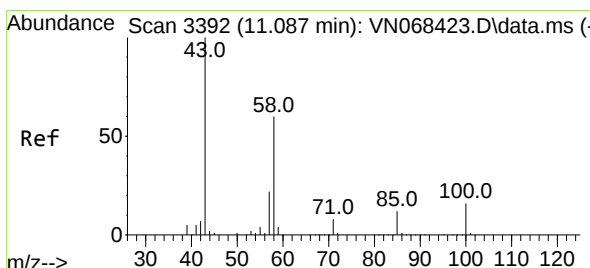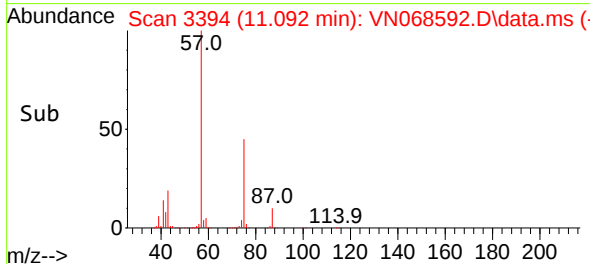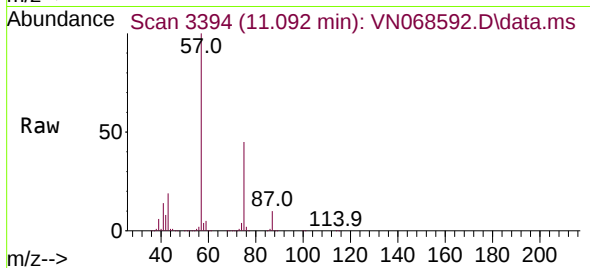

#59
2-Hexanone
Concen: 143.310 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion: 43 Resp: 631170
Ion Ratio Lower Upper
43 100
58 19.6 30.0 90.1#


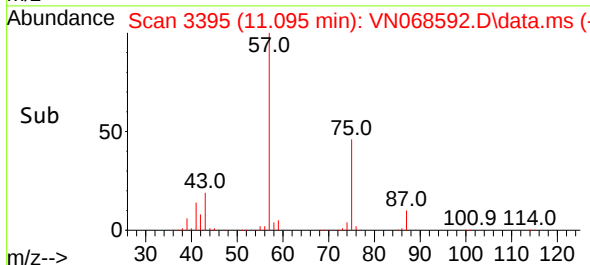

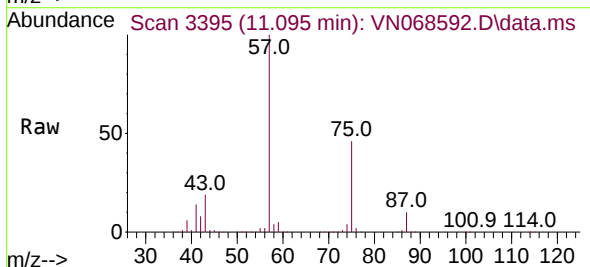




#60
Dibromochloromethane
Concen: 1.855 ug/l
RT: 11.502 min Scan# 3547
Delta R.T. 0.262 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23




Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02


Tgt Ion:129 Resp: 498
Ion Ratio Lower Upper
129 100
127 0.0 38.5 115.3#



#62
4-Bromofluorobenzene
Concen: 49.140 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion: 95 Resp: 411895
Ion Ratio Lower Upper
95 100
174 95.5 0.0 214.0
176 90.9 0.0 205.4


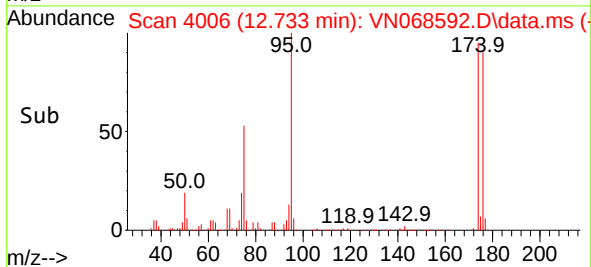

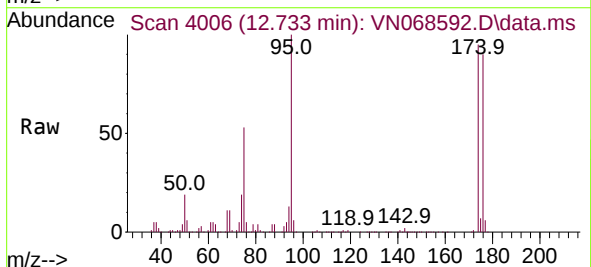




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.001 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23




Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02


Tgt Ion:117 Resp: 946358
Ion Ratio Lower Upper
117 100
82 50.3 38.7 58.1
119 31.9 25.5 38.3

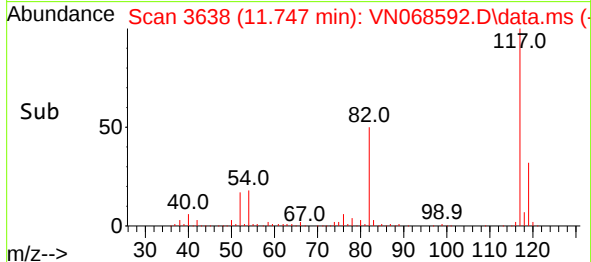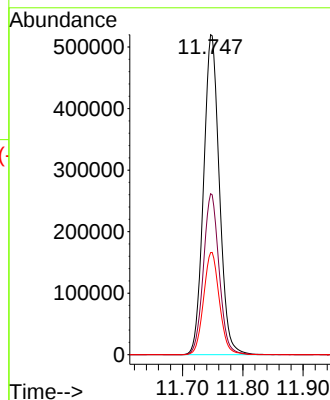

#70
Styrene
Concen: 1.755 ug/l
RT: 12.286 min Scan# 3839
Delta R.T. -0.010 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion:104 Resp: 24
Ion Ratio Lower Upper
104 100
78 0.0 36.2 54.2#
103 0.0 44.4 66.6#


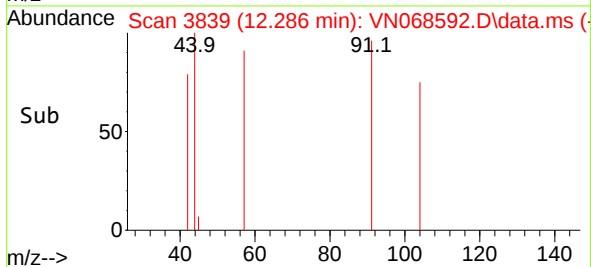
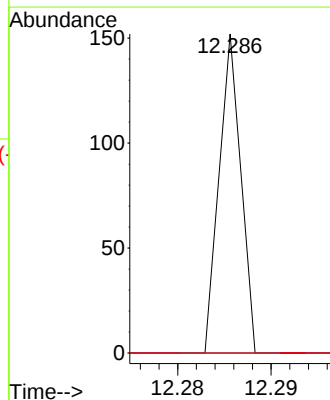
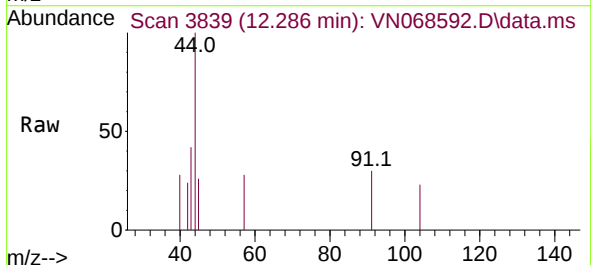


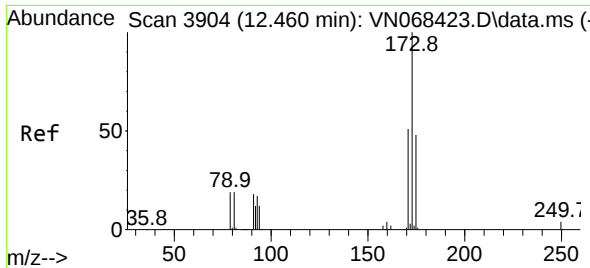

#71
Bromoform
Concen: 2.682 ug/l
RT: 12.728 min Scan# 4004
Delta R.T. 0.268 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23




Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02


Tgt Ion:173 Resp: 1183
Ion Ratio Lower Upper
173 100
175 2317.6 24.1 72.3#
254 0.0 0.0 0.0

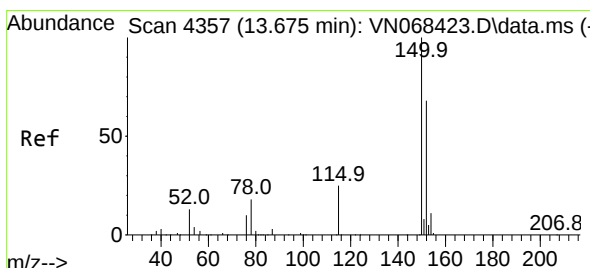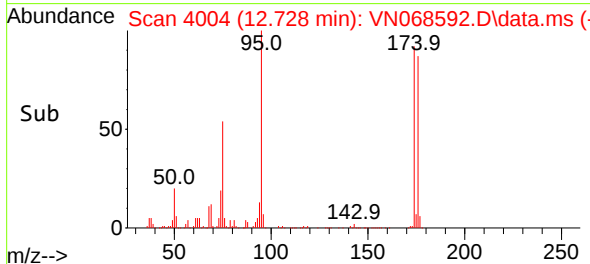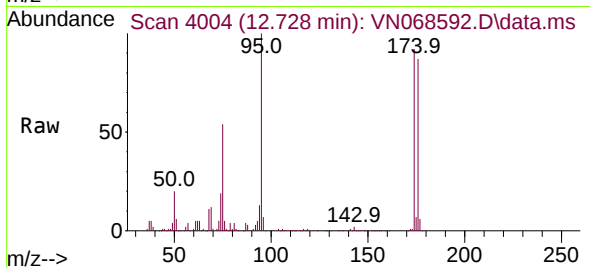

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23


Tgt Ion:152 Resp: 372499
Ion Ratio Lower Upper
152 100
115 54.2 25.6 76.6
150 157.7 0.0 346.8

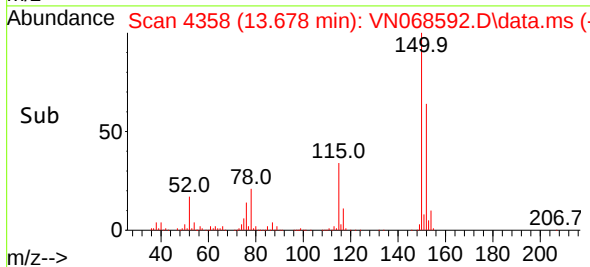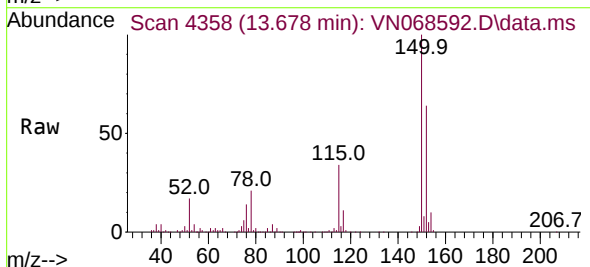






#74
N-amy1 acetate
Concen: 4.475 ug/l
RT: 12.200 min Scan# 3807
Delta R.T. -0.190 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02



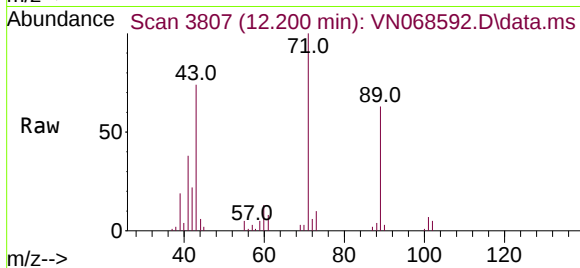



Tgt Ion:	43	Resp:	26448
Ion Ratio	100	Lower	Upper
70	2.3	40.0	60.0#
55	6.1	21.1	31.7#
61	9.9	21.2	31.8#



#76
1,2,3-Trichloropropane
Concen: 42.011 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.148 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion:	75	Resp:	216097
Ion Ratio	100	Lower	Upper
77	1.0	100.9	302.7#


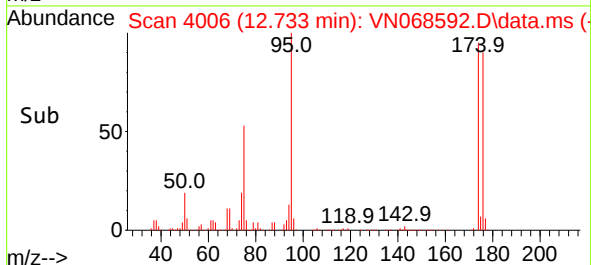

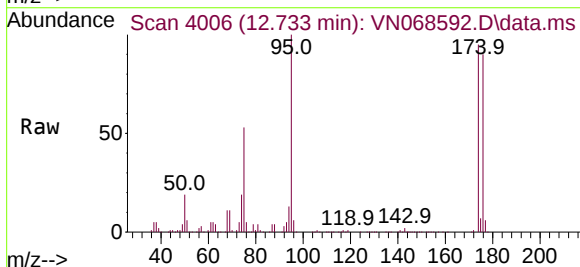




#81
trans-1,4-Dichloro-2-butene
Concen: 128.568 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23




Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02


Tgt Ion: 75 Resp: 216097
Ion Ratio Lower Upper
75 100
53 0.1 70.6 105.8#
89 0.0 39.5 59.3#

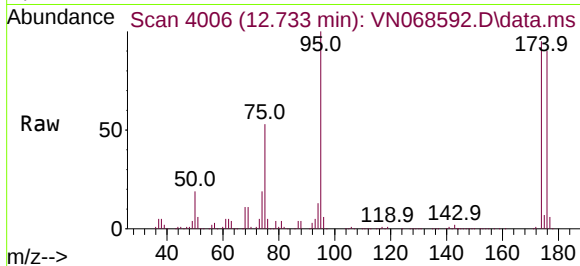

#93
1,2,4-Trichlorobenzene
Concen: 2.981 ug/l
RT: 15.271 min Scan# 4952
Delta R.T. 0.006 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion:180 Resp: 160
Ion Ratio Lower Upper
180 100
182 0.0 47.5 142.6#
145 0.0 14.1 42.4#


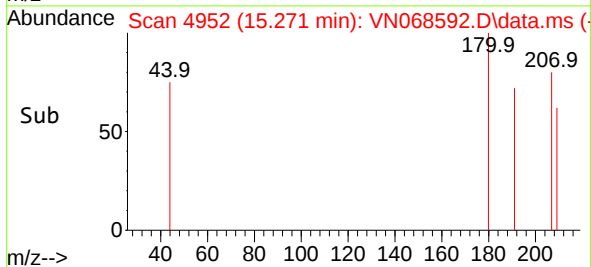

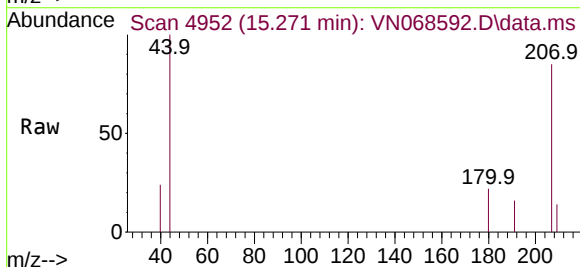




#95
Naphthalene
Concen: 3.540 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Instrument :
MSVOA_N
ClientSampleId :
PB139153ZHE#02

Tgt Ion:128 Resp: 691
Ion Ratio Lower Upper
128 100
127 0.0 10.6 15.8#
129 0.0 8.6 13.0#

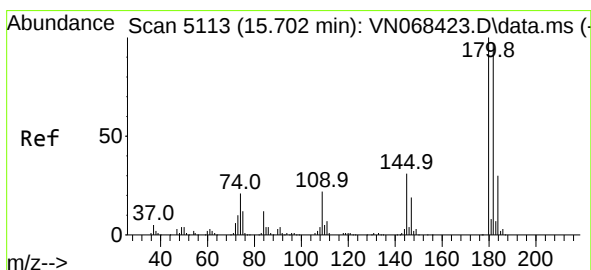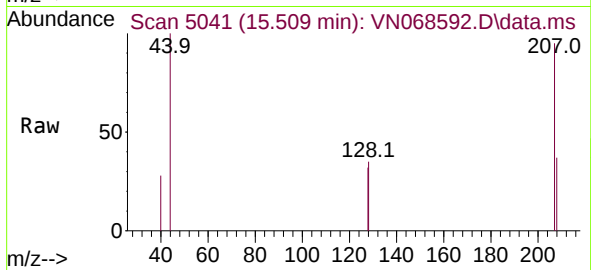

#96
1,2,3-Trichlorobenzene
Concen: 2.978 ug/l
RT: 15.716 min Scan# 5118
Delta R.T. 0.014 min
Lab File: VN068592.D
Acq: 21 Sep 2021 19:23

Tgt Ion:180 Resp: 25
Ion Ratio Lower Upper
180 100
182 332.0 47.9 143.6#
145 0.0 15.2 45.5#

