

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN092121\  
 Data File : VN068595.D  
 Acq On : 21 Sep 2021 20:38  
 Operator : JC/MD  
 Sample : PB139153ZHE#05  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :

Quant Time: Sep 22 03:43:49 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N090721W.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Sep 17 11:02:11 2021  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response            | Conc      | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|-----------|--------|----------|
| -----                         |                |      |                     |           |        |          |
| Internal Standards            |                |      |                     |           |        |          |
| 1) Pentafluorobenzene         | 8.091          | 168  | 827018              | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 8.971          | 114  | 1257347             | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.747         | 117  | 1182438             | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.678         | 152  | 456493              | 50.000    | ug/l   | 0.00     |
|                               |                |      |                     |           |        |          |
| System Monitoring Compounds   |                |      |                     |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.440          | 65   | 457642              | 60.325    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 61 - 141 |      | Recovery = 120.660% |           |        |          |
| 35) Dibromofluoromethane      | 8.024          | 113  | 382276              | 50.409    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 69 - 133 |      | Recovery = 100.820% |           |        |          |
| 50) Toluene-d8                | 10.446         | 98   | 1500998             | 48.384    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 65 - 126 |      | Recovery = 96.760%  |           |        |          |
| 62) 4-Bromofluorobenzene      | 12.734         | 95   | 464897              | 45.732    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 58 - 135 |      | Recovery = 91.460%  |           |        |          |
|                               |                |      |                     |           |        |          |
| Target Compounds              |                |      |                     |           |        |          |
|                               |                |      |                     |           | Qvalue |          |
| 3) Chloromethane              | 2.306          | 50   | 717                 | Below Cal | #      | 78       |
| 5) Bromomethane               | 2.832          | 94   | 28                  | Below Cal | #      | 3        |
| 11) Tert butyl alcohol        | 5.369          | 59   | 845                 | Below Cal | #      | 84       |
| 16) Acetone                   | 4.296          | 43   | 59770               | 19.740    | ug/l   | 93       |
| 18) Methyl Acetate            | 4.867          | 43   | 5863                | Below Cal |        | 96       |
| 20) Methylene Chloride        | 5.103          | 84   | 44611               | 5.062     | ug/l   | 93       |
| 25) 2-Butanone                | 7.345          | 43   | 12689               | 3.442     | ug/l   | 96       |
| 29) Tetrahydrofuran           | 7.699          | 42   | 2493                | 1.036     | ug/l # | 63       |
| 31) Cyclohexane               | 8.088          | 56   | 15292               | 1.330     | ug/l # | 29       |
| 36) 1,1-Dichloropropene       | 8.088          | 75   | 55057               | 5.252     | ug/l # | 47       |
| 37) Ethyl Acetate             | 7.345          | 43   | 12689               | 1.591     | ug/l # | 66       |
| 38) Carbon Tetrachloride      | 8.091          | 117  | 78312               | 6.236     | ug/l # | 16       |
| 43) Isopropyl Acetate         | 8.566          | 43   | 81843               | 5.818     | ug/l # | 78       |
| 45) 1,2-Dichloropropane       | 9.625          | 63   | 4217                | 0.569     | ug/l # | 44       |
| 48) Methyl methacrylate       | 9.545          | 41   | 13316               | 2.267     | ug/l # | 6        |
| 49) 1,4-Dioxane               | 9.628          | 88   | 486                 | 3.606     | ug/l # | 1        |
| 51) 4-Methyl-2-Pentanone      | 10.336         | 43   | 10963               | 1.365     | ug/l   | 89       |
| 54) cis-1,3-Dichloropropene   | 10.245         | 75   | 104074              | 8.761     | ug/l # | 68       |
| 57) 1,3-Dichloropropane       | 11.092         | 76   | 63959               | 5.080     | ug/l # | 43       |
| 59) 2-Hexanone                | 11.092         | 43   | 871662              | 162.069   | ug/l # | 45       |
| 60) Dibromochloromethane      | 11.494         | 129  | 747                 | 1.867     | ug/l # | 11       |
| 71) Bromoform                 | 12.723         | 173  | 893                 | 2.620     | ug/l # | 29       |
| 76) 1,2,3-Trichloropropane    | 12.734         | 75   | 244222              | 38.655    | ug/l # | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.734         | 75   | 244222              | 118.566   | ug/l # | 13       |
| 93) 1,2,4-Trichlorobenzene    | 15.263         | 180  | 167                 | 2.978     | ug/l # | 12       |
| 95) Naphthalene               | 15.501         | 128  | 251                 | 3.509     | ug/l # | 69       |
| 96) 1,2,3-Trichlorobenzene    | 15.705         | 180  | 83                  | 2.984     | ug/l # | 85       |
| -----                         |                |      |                     |           |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN092121\  
Data File : VN068595.D  
Acq On : 21 Sep 2021 20:38  
Operator : JC/MD  
Sample : PB139153ZHE#05  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :

Quant Time: Sep 22 03:43:49 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N090721W.M  
Quant Title : SW846 8260  
QLast Update : Fri Sep 17 11:02:11 2021  
Response via : Initial Calibration




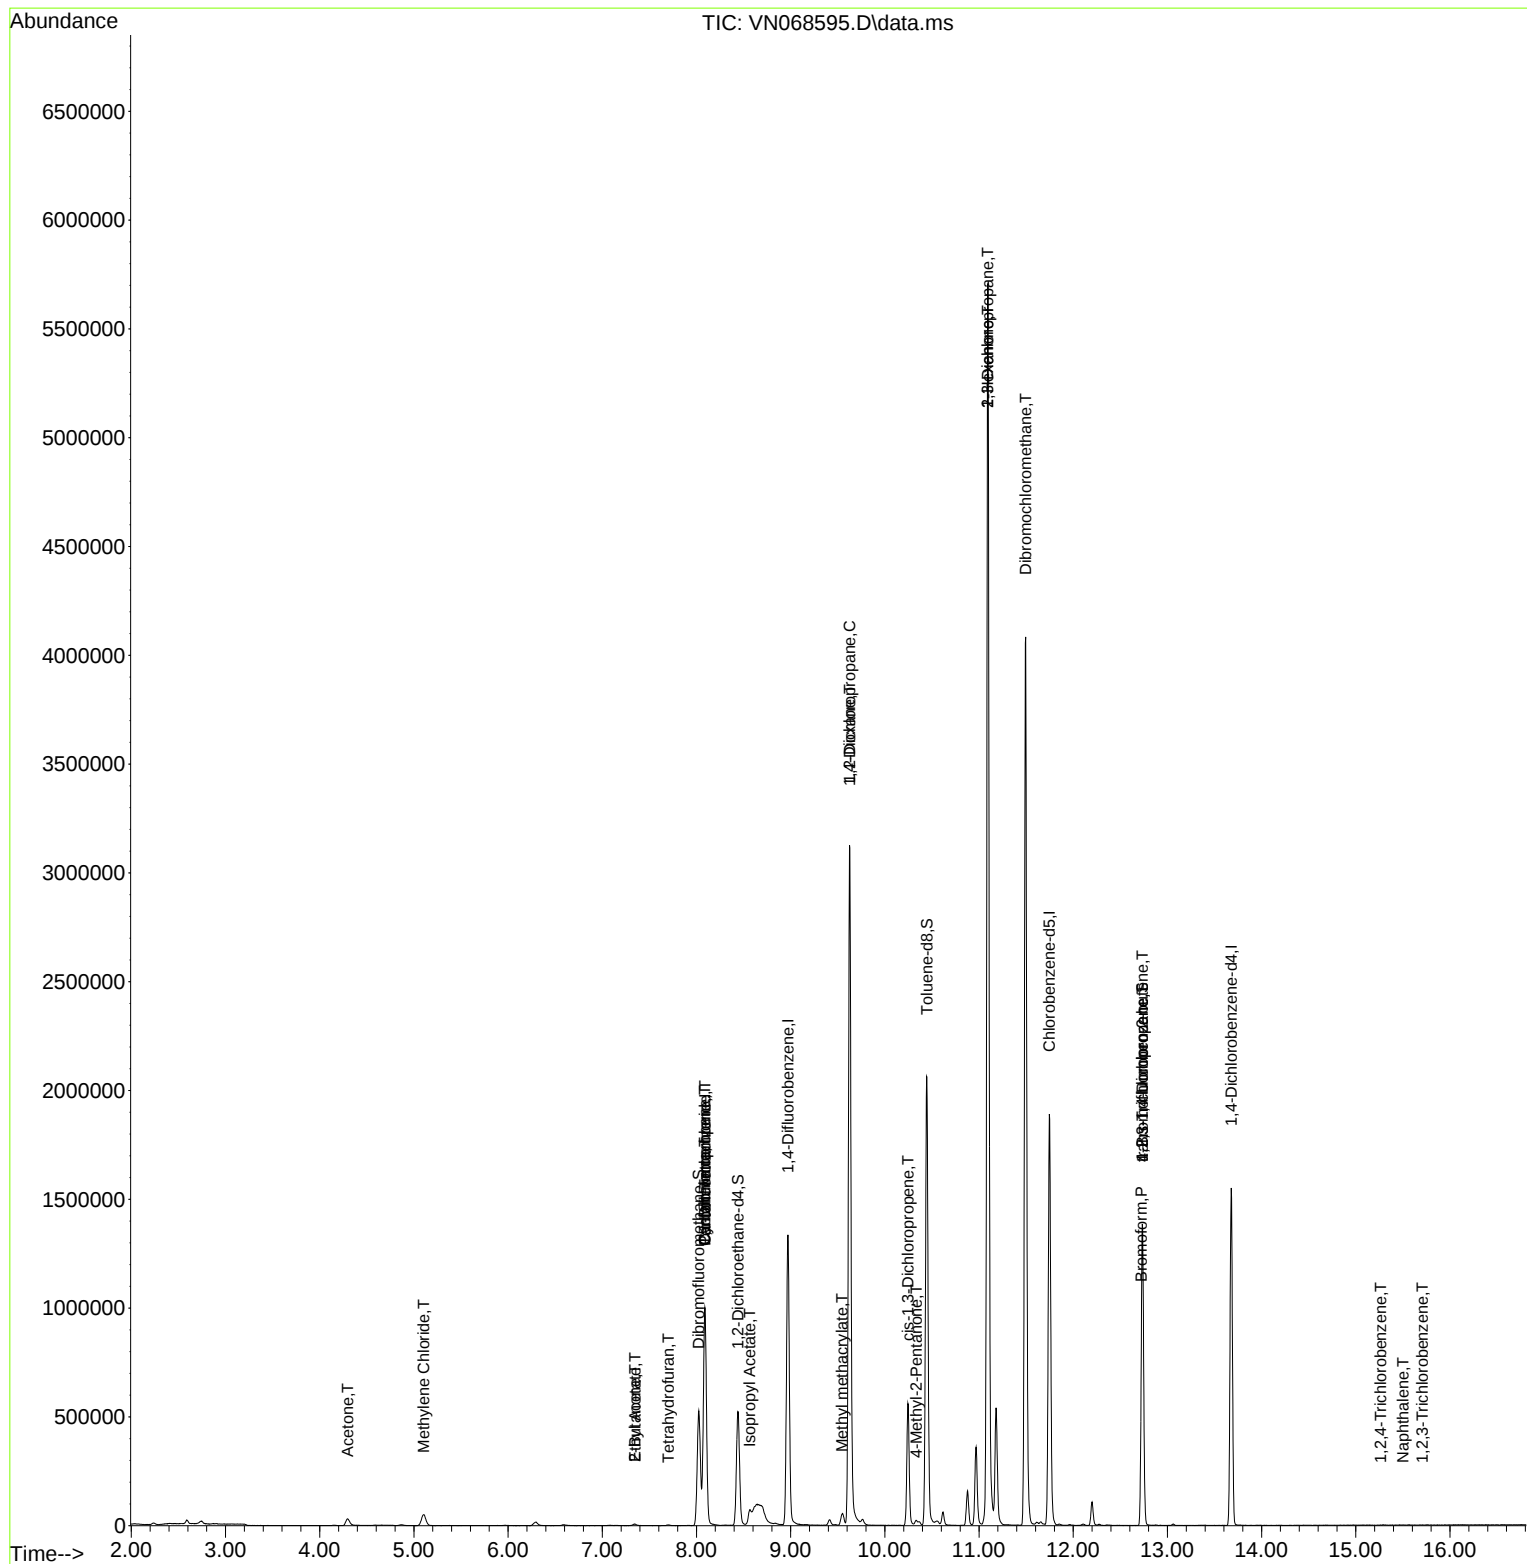


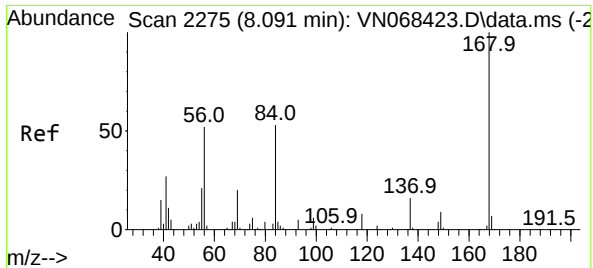

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.091 min Scan# 2275  
Delta R.T. 0.000 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion:168 Resp: 827018  
Ion Ratio Lower Upper  
168 100  
99 51.6 38.2 57.4

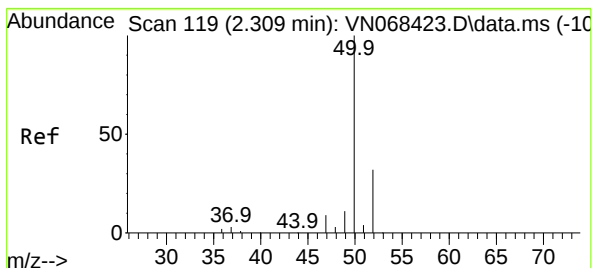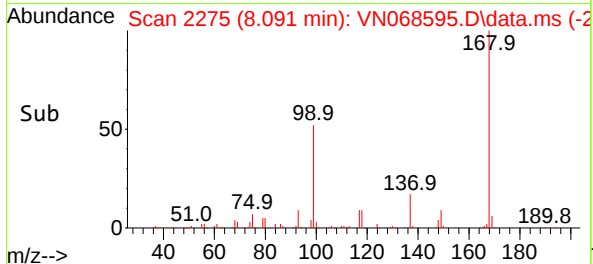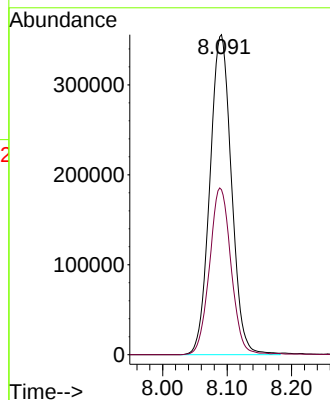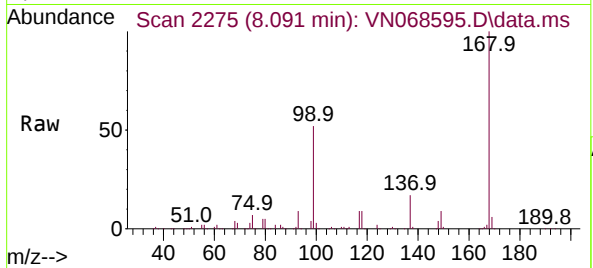

#3  
Chloromethane  
Concen: Below Cal  
RT: 2.306 min Scan# 118  
Delta R.T. -0.003 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Tgt Ion: 50 Resp: 717  
Ion Ratio Lower Upper  
50 100  
52 44.5 25.8 38.6#


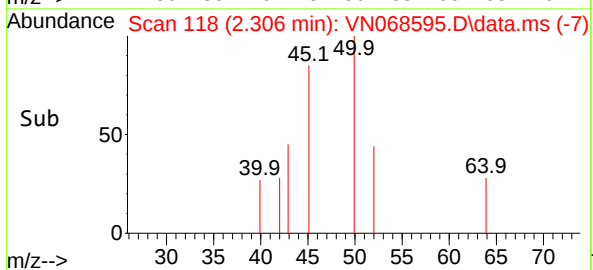
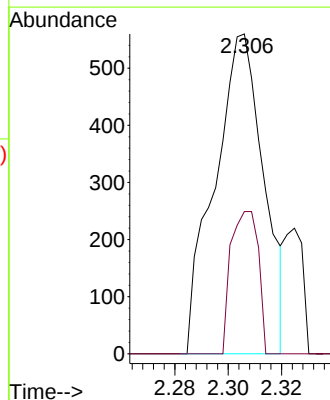
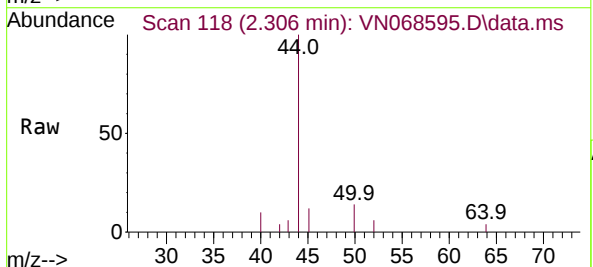




#5  
Bromomethane  
Concen: Below Cal  
RT: 2.832 min Scan# 314  
Delta R.T. -0.008 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 94 Resp: 28  
Ion Ratio Lower Upper  
94 100  
96 0.0 75.4 113.0#

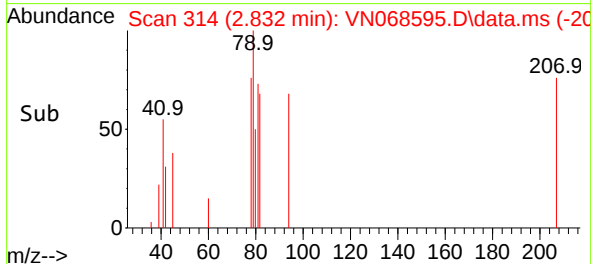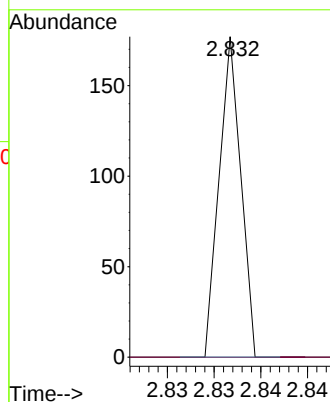

#11  
Tert butyl alcohol  
Concen: Below Cal  
RT: 5.369 min Scan# 1260  
Delta R.T. -0.005 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Tgt Ion: 59 Resp: 845  
Ion Ratio Lower Upper  
59 100  
57 0.0 4.3 6.5#



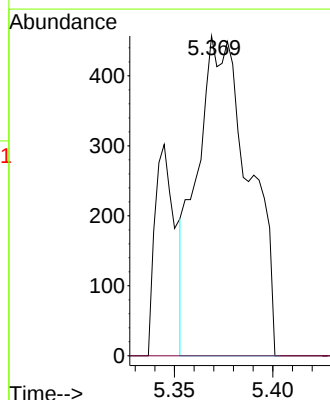
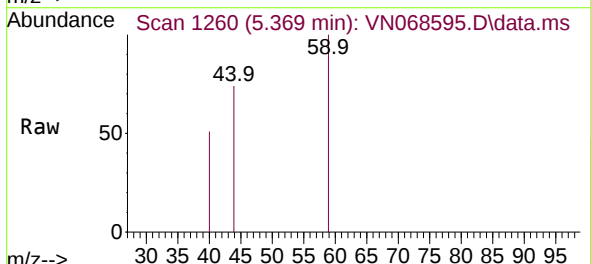




#16  
Acetone  
Concen: 19.740 ug/l  
RT: 4.296 min Scan# 860  
Delta R.T. 0.005 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 43 Resp: 59770  
Ion Ratio Lower Upper  
43 100  
58 29.7 27.0 40.6

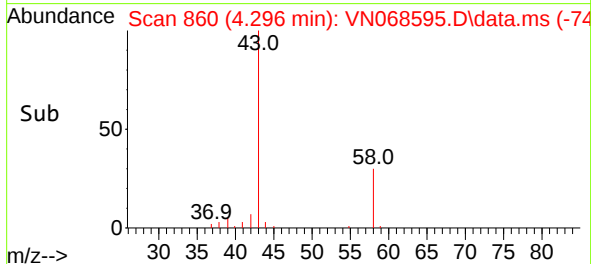

#18  
Methyl Acetate  
Concen: Below Cal  
RT: 4.867 min Scan# 1073  
Delta R.T. 0.011 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38


Tgt Ion: 43 Resp: 5863  
Ion Ratio Lower Upper  
43 100  
74 31.4 23.5 35.3

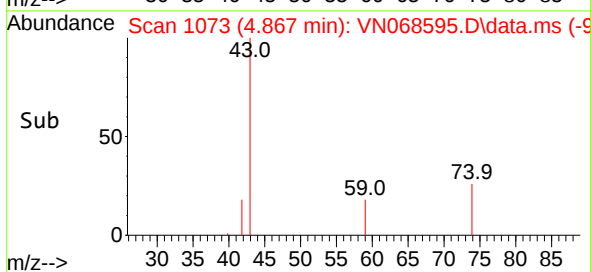



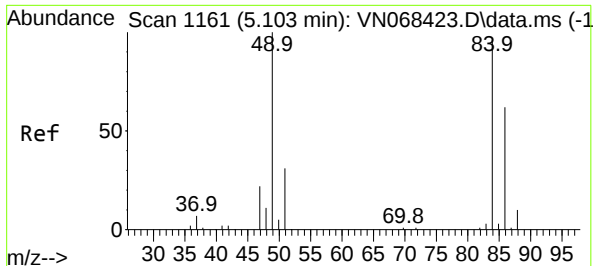


#20  
Methylene Chloride  
Concen: 5.062 ug/l  
RT: 5.103 min Scan# 1161  
Delta R.T. 0.000 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Instrument :  
MSVOA\_N  
ClientSampled :



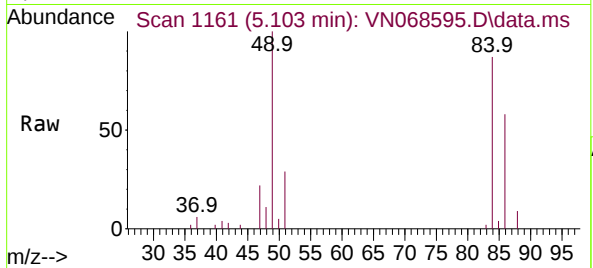



|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 84    | Resp: | 44611 |
| Ion      | Ratio | Lower | Upper |
| 84       | 100   |       |       |
| 49       | 115.3 | 83.0  | 124.6 |
| 51       | 33.6  | 25.4  | 38.0  |
| 86       | 66.7  | 51.3  | 76.9  |

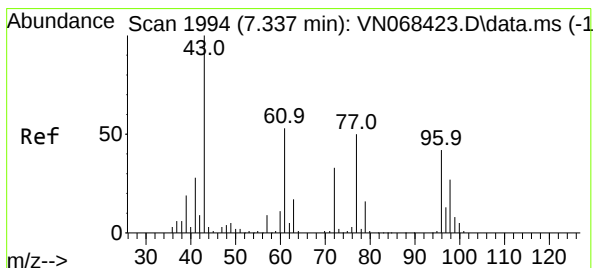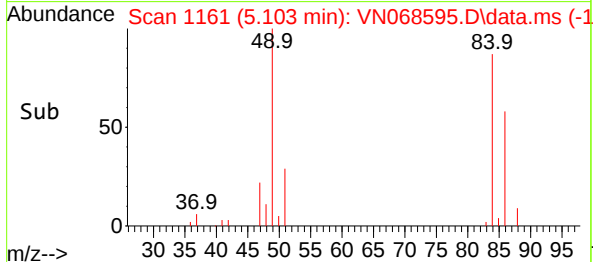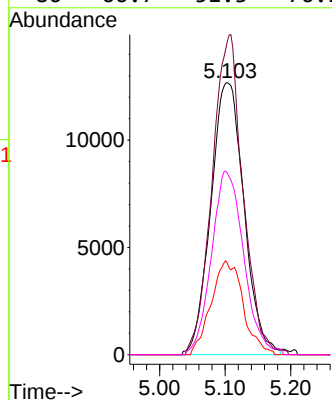

#25  
2-Butanone  
Concen: 3.442 ug/l  
RT: 7.345 min Scan# 1997  
Delta R.T. 0.008 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 43    | Resp: | 12689 |
| Ion      | Ratio | Lower | Upper |
| 43       | 100   |       |       |
| 72       | 31.0  | 26.7  | 40.1  |

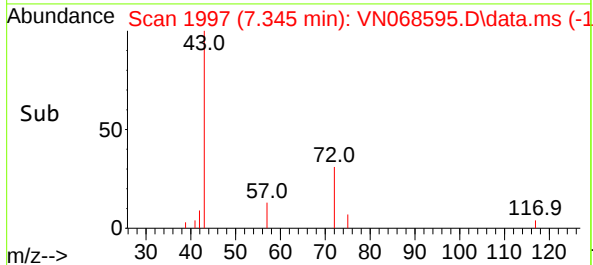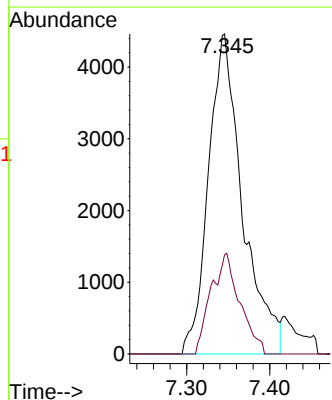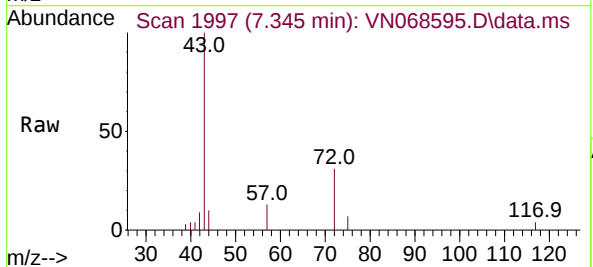

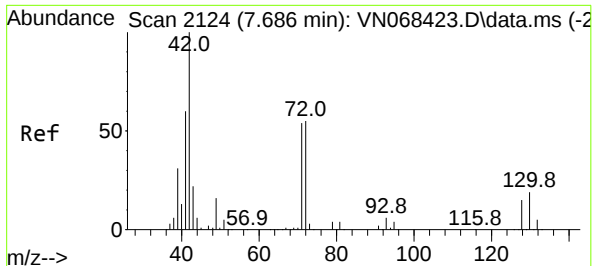

#29

Tetrahydrofuran

Concen: 1.036 ug/l

RT: 7.699 min Scan# 2129





Delta R.T. 0.013 min

Lab File: VN068595.D

Acq: 21 Sep 2021 20:38

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 42    | Resp: | 2493  |
| Ion      | Ratio | Lower | Upper |
| 42       | 100   |       |       |
| 72       | 9.9   | 44.4  | 66.6# |
| 71       | 46.5  | 42.3  | 63.5  |

Instrument :  
MSVOA\_N  
ClientSampled :

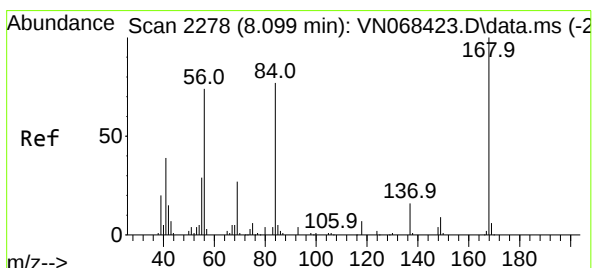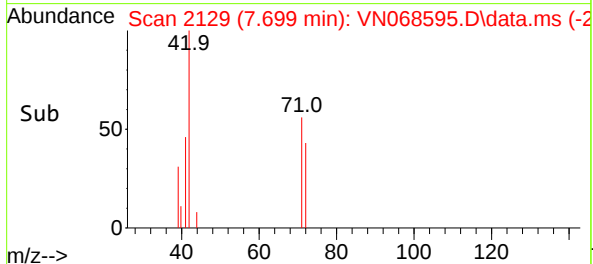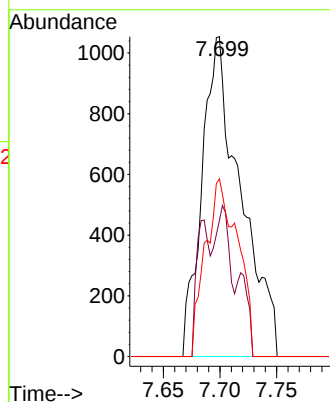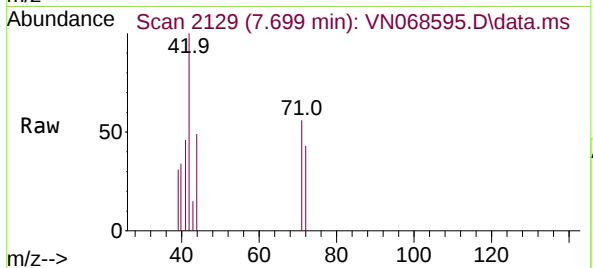

#31

Cyclohexane

Concen: 1.330 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.011 min

Lab File: VN068595.D

Acq: 21 Sep 2021 20:38

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 56    | Resp: | 15292 |
| Ion      | Ratio | Lower | Upper |
| 56       | 100   |       |       |
| 69       | 168.4 | 29.4  | 44.0# |
| 84       | 122.5 | 83.6  | 125.4 |

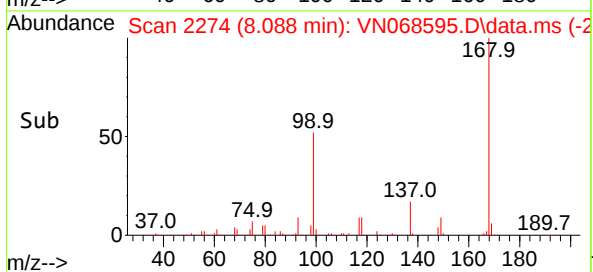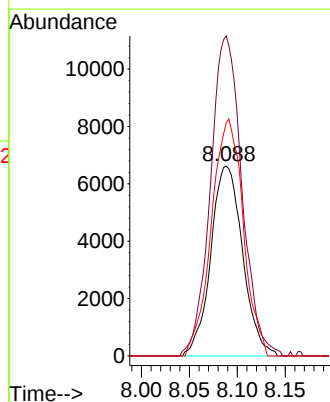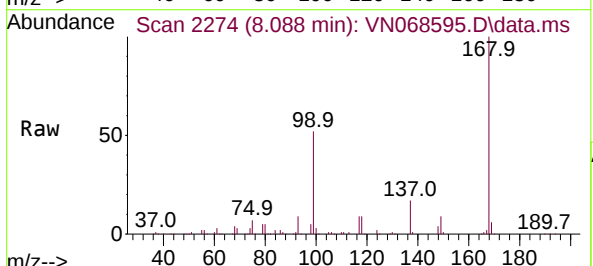




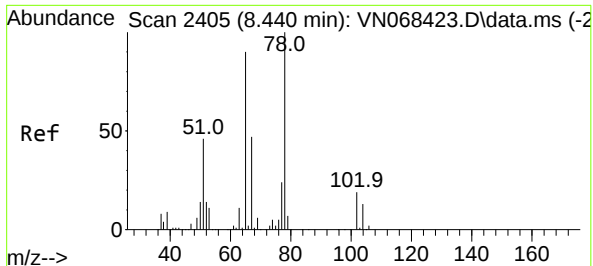


#33

1,2-Dichloroethane-d4  
Concen: 60.325 ug/l  
RT: 8.440 min Scan# 2405  
Delta R.T. -0.000 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Instrument :  
MSVOA\_N  
ClientSampled :




Tgt Ion: 65 Resp: 457642  
Ion Ratio Lower Upper  
65 100  
67 51.2 0.0 104.0

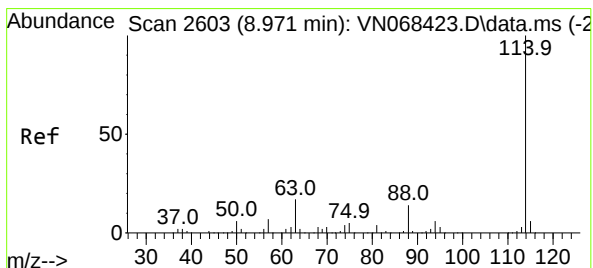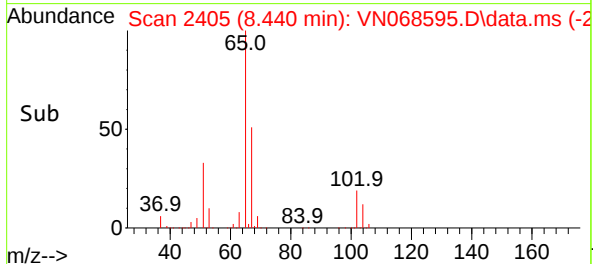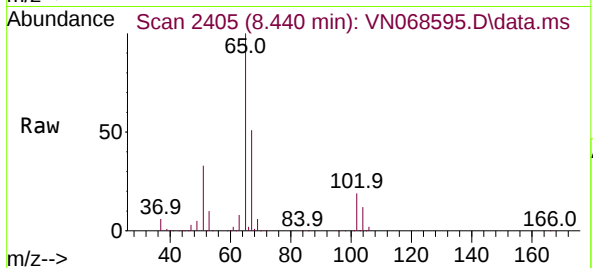


#34

1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 8.971 min Scan# 2603  
Delta R.T. -0.000 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Tgt Ion: 114 Resp: 1257347  
Ion Ratio Lower Upper  
114 100  
63 17.9 0.0 33.2  
88 14.8 0.0 28.4


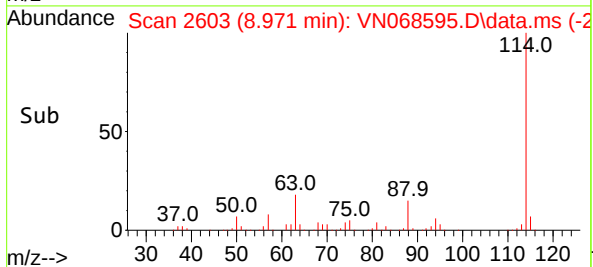

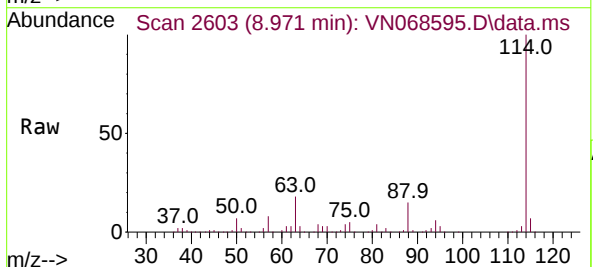




#35  
Dibromofluoromethane  
Concen: 50.409 ug/l  
RT: 8.024 min Scan# 2250  
Delta R.T. 0.000 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion:113 Resp: 382276  
Ion Ratio Lower Upper  
113 100  
111 102.4 81.1 121.7  
192 22.0 17.7 26.5

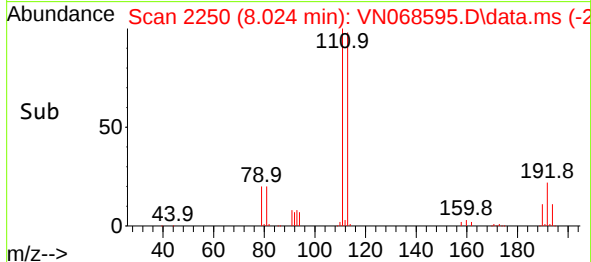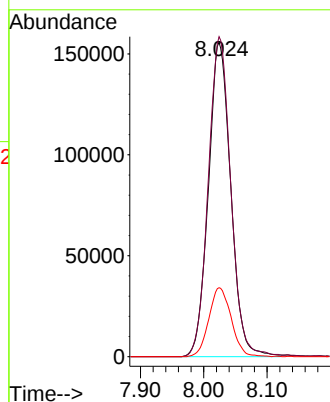

#36  
1,1-Dichloropropene  
Concen: 5.252 ug/l  
RT: 8.088 min Scan# 2274  
Delta R.T. -0.137 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38


Tgt Ion: 75 Resp: 55057  
Ion Ratio Lower Upper  
75 100  
110 10.5 20.8 62.5#  
77 0.0 25.0 37.6#

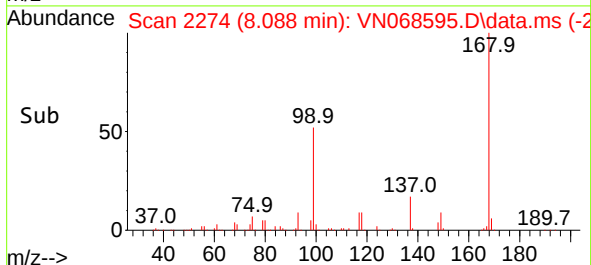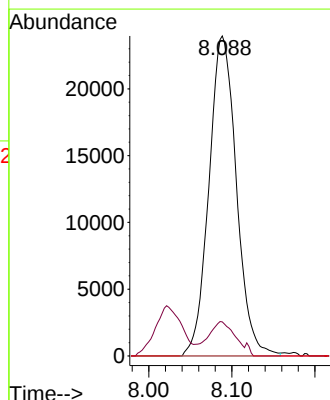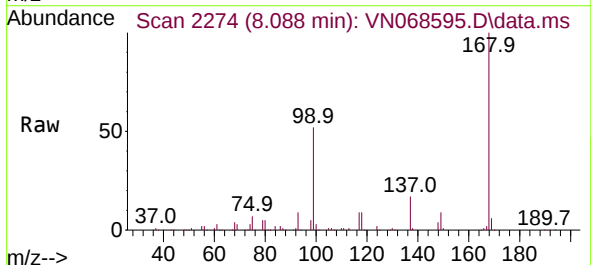






#37  
Ethyl Acetate  
Concen: 1.591 ug/l  
RT: 7.345 min Scan# 1997  
Delta R.T. -0.070 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Instrument :  
MSVOA\_N  
ClientSampled :







Tgt Ion: 43 Resp: 12689  
Ion Ratio Lower Upper  
43 100  
61 0.0 12.4 18.6#  
70 0.0 9.6 14.4#

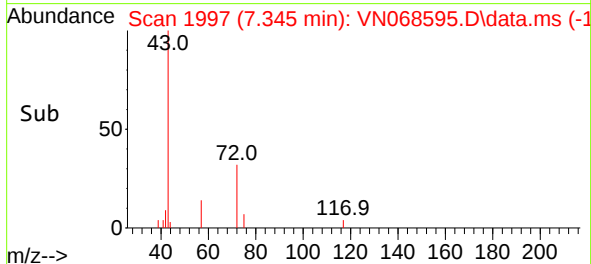

#38  
Carbon Tetrachloride  
Concen: 6.236 ug/l  
RT: 8.091 min Scan# 2275  
Delta R.T. -0.118 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38


Tgt Ion: 117 Resp: 78312  
Ion Ratio Lower Upper  
117 100  
119 4.9 76.6 114.8#  
121 0.0 24.5 36.7#

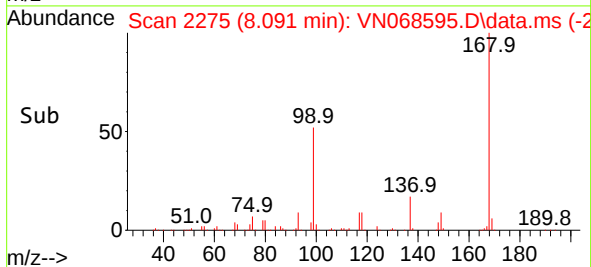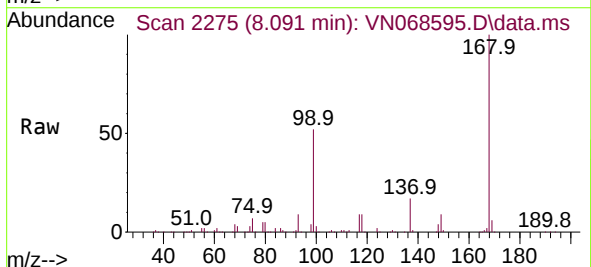






#43  
Isopropyl Acetate  
Concen: 5.818 ug/l  
RT: 8.566 min Scan# 2452  
Delta R.T. 0.003 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Instrument :  
MSVOA\_N  
ClientSampled :







Tgt Ion: 43 Resp: 81843  
Ion Ratio Lower Upper  
43 100  
61 14.5 23.3 34.9#  
87 10.9 13.8 20.6#

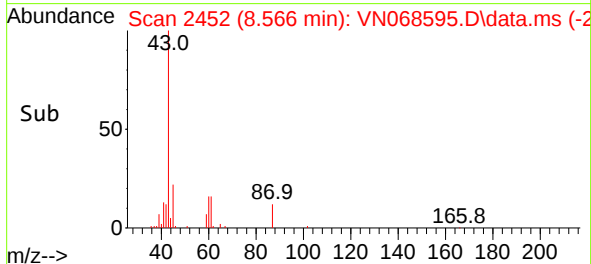

#45  
1,2-Dichloropropane  
Concen: 0.569 ug/l  
RT: 9.625 min Scan# 2847  
Delta R.T. 0.131 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Tgt Ion: 63 Resp: 4217  
Ion Ratio Lower Upper  
63 100  
65 0.0 24.8 37.2#



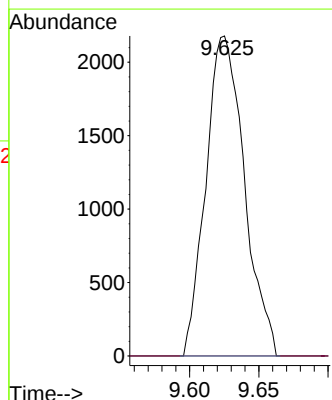
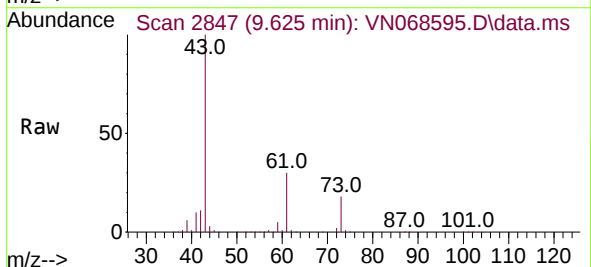




#48  
Methyl methacrylate  
Concen: 2.267 ug/l  
RT: 9.545 min Scan# 2817  
Delta R.T. -0.016 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 41 Resp: 13316  
Ion Ratio Lower Upper  
41 100  
69 0.0 82.9 124.3#  
39 0.0 50.3 75.5#

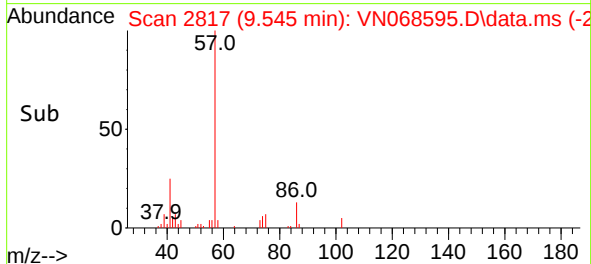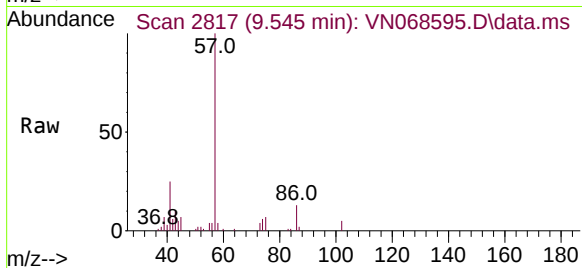

#49  
1,4-Dioxane  
Concen: 3.606 ug/l  
RT: 9.628 min Scan# 2848  
Delta R.T. 0.057 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Tgt Ion: 88 Resp: 486  
Ion Ratio Lower Upper  
88 100  
43 628912.6 18.9 28.3#  
58 3009.5 46.6 69.8#


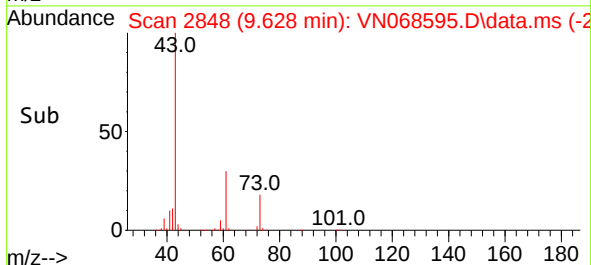
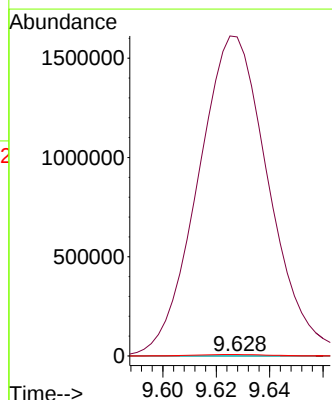
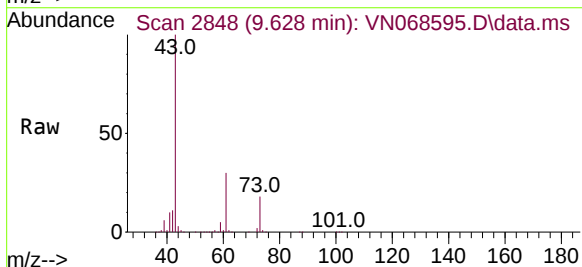




#50  
Toluene-d8  
Concen: 48.384 ug/l  
RT: 10.446 min Scan# 3153  
Delta R.T. 0.003 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 98 Resp: 1500998  
Ion Ratio Lower Upper  
98 100  
100 64.2 51.0 76.6

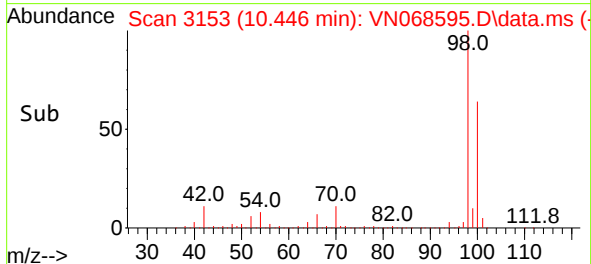

#51  
4-Methyl-2-Pentanone  
Concen: 1.365 ug/l  
RT: 10.336 min Scan# 3112  
Delta R.T. 0.003 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Tgt Ion: 43 Resp: 10963  
Ion Ratio Lower Upper  
43 100  
58 50.2 34.3 51.5


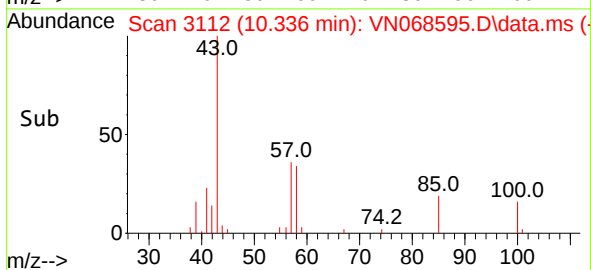

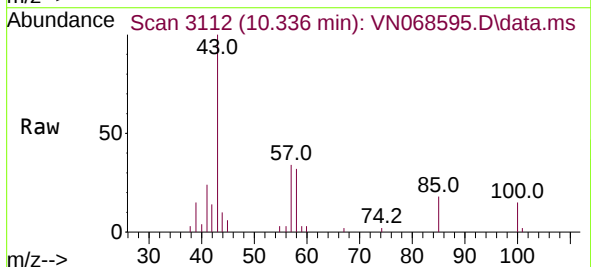


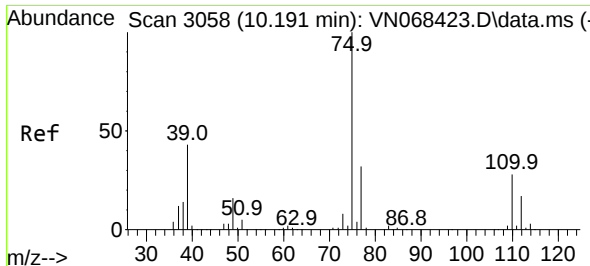

#54  
 cis-1,3-Dichloropropene  
 Concen: 8.761 ug/l  
 RT: 10.245 min Scan# 3078  
 Delta R.T. 0.054 min  
 Lab File: VN068595.D  
 Acq: 21 Sep 2021 20:38




Instrument :  
 MSVOA\_N  
 ClientSampled :


Tgt Ion: 75 Resp: 104074  
 Ion Ratio Lower Upper  
 75 100  
 77 0.4 25.3 37.9#  
 39 34.2 34.6 52.0#

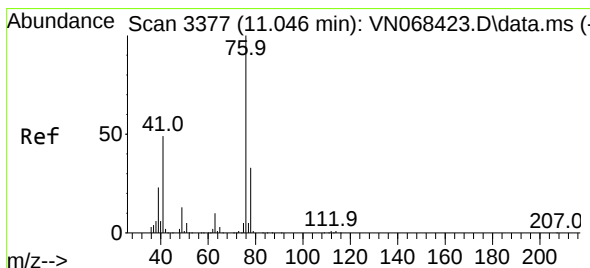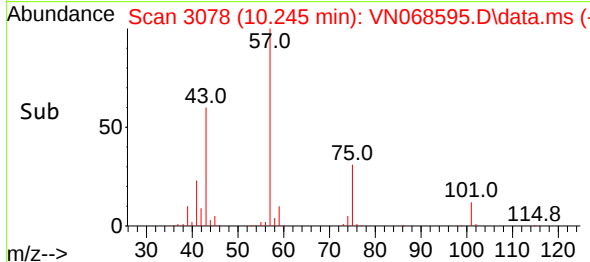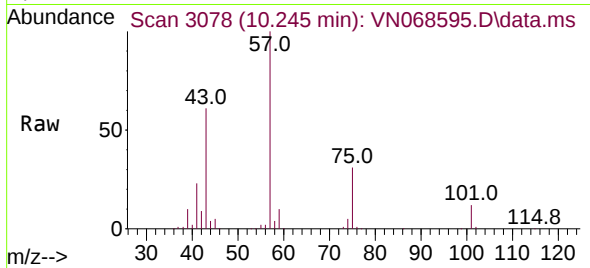

#57  
 1,3-Dichloropropane  
 Concen: 5.080 ug/l  
 RT: 11.092 min Scan# 3394  
 Delta R.T. 0.046 min  
 Lab File: VN068595.D  
 Acq: 21 Sep 2021 20:38

Tgt Ion: 76 Resp: 63959  
 Ion Ratio Lower Upper  
 76 100  
 78 0.3 25.9 38.9#


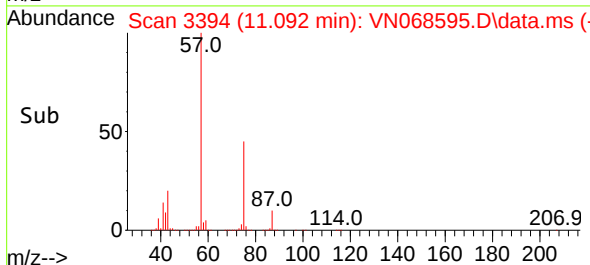
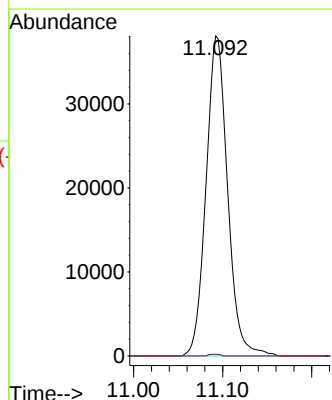
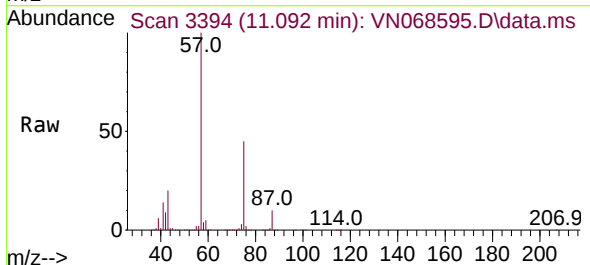




#59  
2-Hexanone  
Concen: 162.069 ug/l  
RT: 11.092 min Scan# 3394  
Delta R.T. 0.005 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 43 Resp: 871662  
Ion Ratio Lower Upper  
43 100  
58 18.6 30.0 90.1#

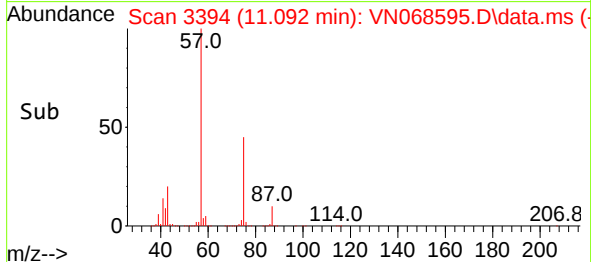

#60  
Dibromochloromethane  
Concen: 1.867 ug/l  
RT: 11.494 min Scan# 3544  
Delta R.T. 0.254 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Tgt Ion:129 Resp: 747  
Ion Ratio Lower Upper  
129 100  
127 0.0 38.5 115.3#


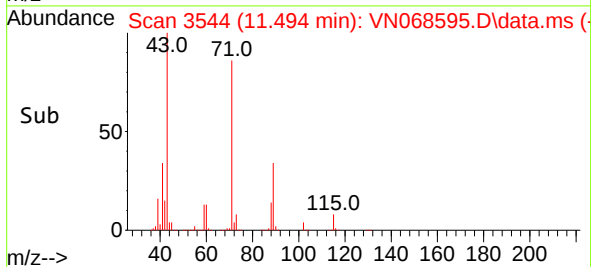
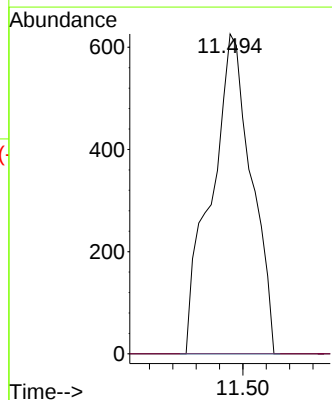
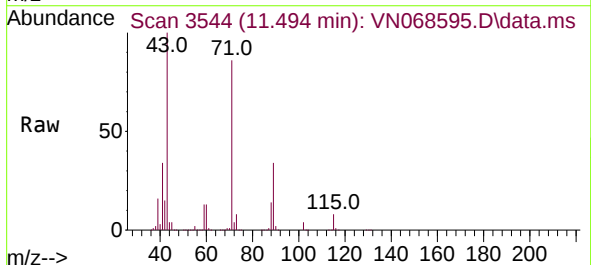


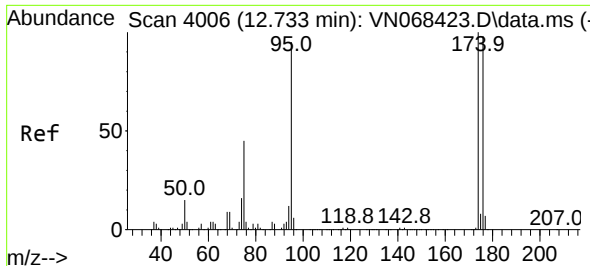

#62  
4-Bromofluorobenzene  
Concen: 45.732 ug/l  
RT: 12.734 min Scan# 4006  
Delta R.T. 0.001 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 95 Resp: 464897  
Ion Ratio Lower Upper  
95 100  
174 93.7 0.0 214.0  
176 90.5 0.0 205.4

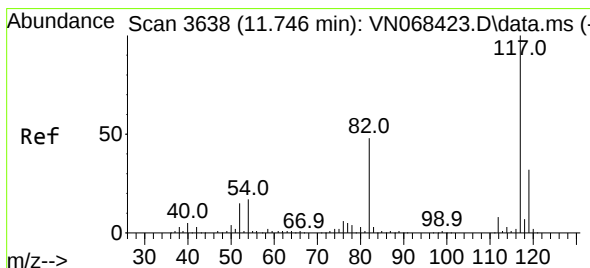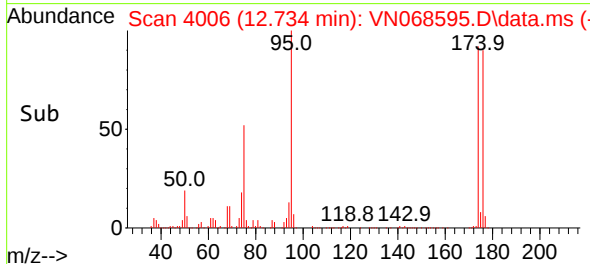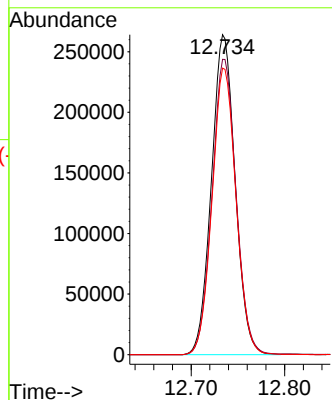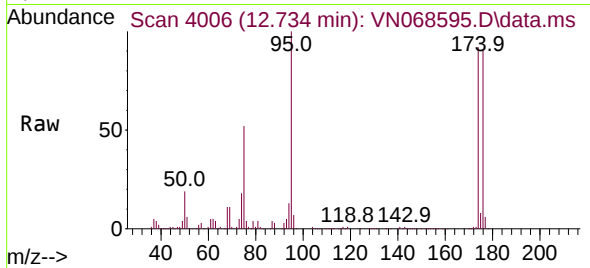

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.747 min Scan# 3638  
Delta R.T. 0.001 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Tgt Ion: 117 Resp: 1182438  
Ion Ratio Lower Upper  
117 100  
82 52.2 38.7 58.1  
119 31.7 25.5 38.3


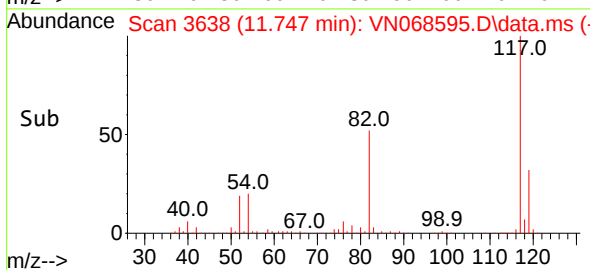
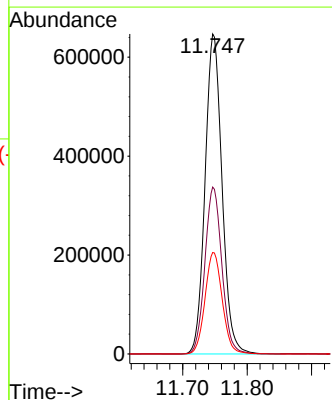
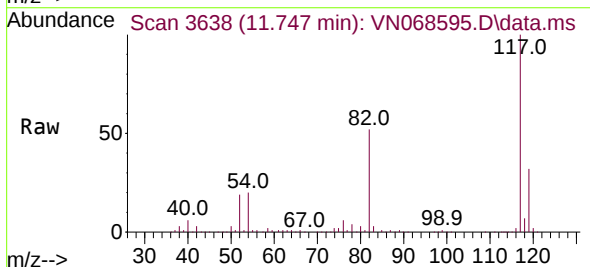


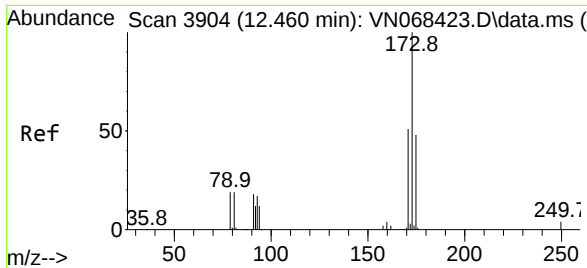

#71  
Bromoform  
Concen: 2.620 ug/l  
RT: 12.723 min Scan# 4002  
Delta R.T. 0.263 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion:173 Resp: 893  
Ion Ratio Lower Upper  
173 100  
175 0.0 24.1 72.3#  
254 0.0 0.0 0.0

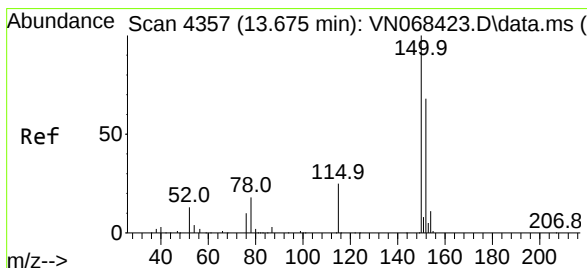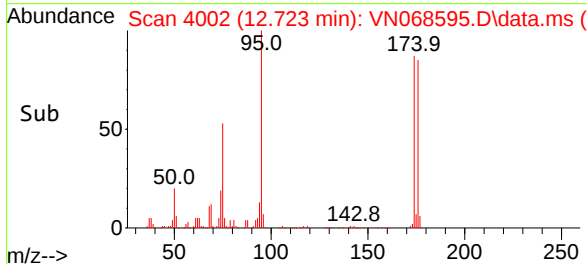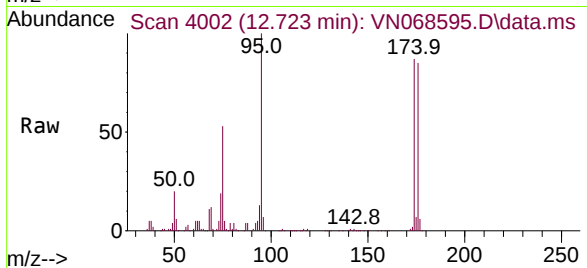

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.678 min Scan# 4358  
Delta R.T. 0.003 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38

Tgt Ion:152 Resp: 456493  
Ion Ratio Lower Upper  
152 100  
115 55.7 25.6 76.6  
150 156.1 0.0 346.8


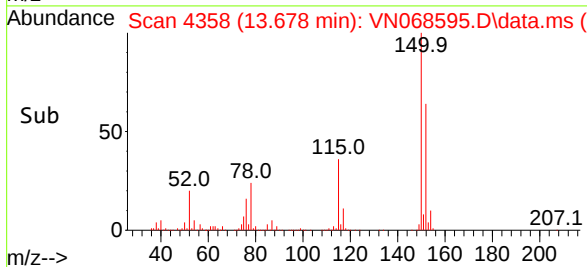

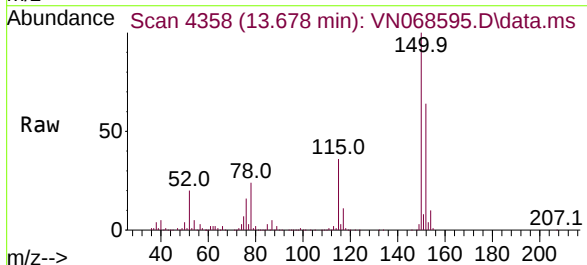


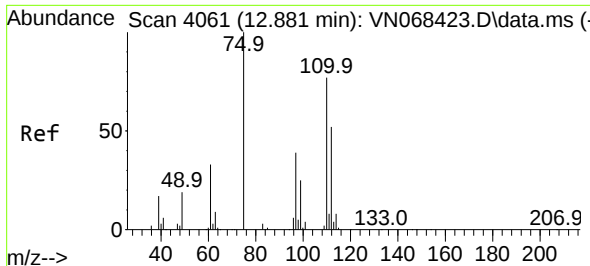

#76  
1,2,3-Trichloropropane  
Concen: 38.655 ug/l  
RT: 12.734 min Scan# 4006  
Delta R.T. -0.147 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 75 Resp: 244222  
Ion Ratio Lower Upper  
75 100  
77 1.0 100.9 302.7#

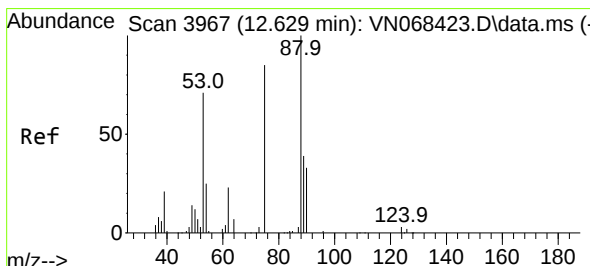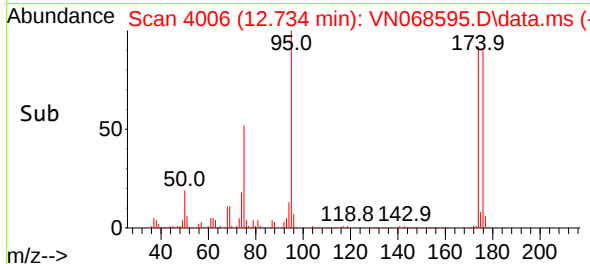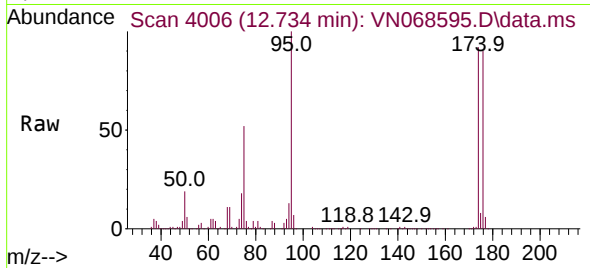

#81  
trans-1,4-Dichloro-2-butene  
Concen: 118.566 ug/l  
RT: 12.734 min Scan# 4006  
Delta R.T. 0.105 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38


Tgt Ion: 75 Resp: 244222  
Ion Ratio Lower Upper  
75 100  
53 0.1 70.6 105.8#  
89 0.0 39.5 59.3#

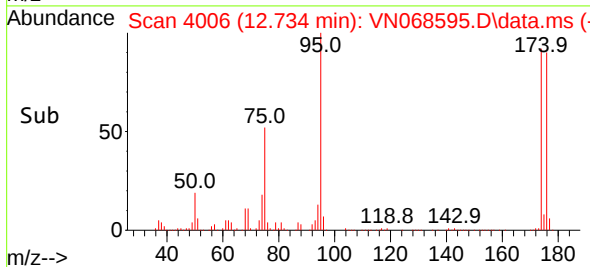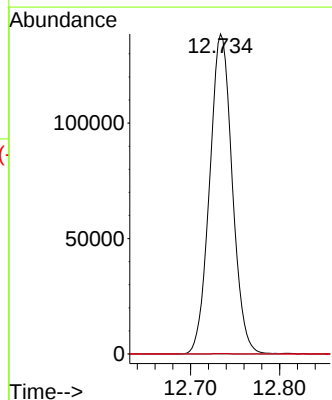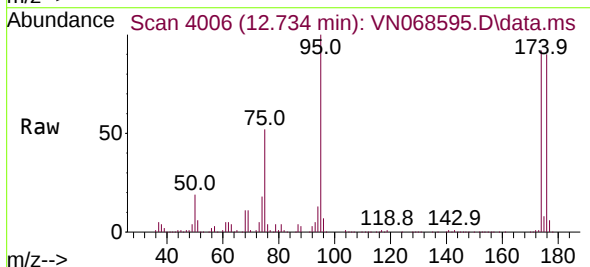






#93  
1,2,4-Trichlorobenzene  
Concen: 2.978 ug/l  
RT: 15.263 min Scan# 4949  
Delta R.T. -0.002 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38


Instrument :  
MSVOA\_N  
ClientSampled :





Tgt Ion:180 Resp: 167  
Ion Ratio Lower Upper  
180 100  
182 0.0 47.5 142.6#  
145 0.0 14.1 42.4#




#95  
Naphthalene  
Concen: 3.509 ug/l  
RT: 15.501 min Scan# 5038  
Delta R.T. -0.006 min  
Lab File: VN068595.D  
Acq: 21 Sep 2021 20:38




Tgt Ion:128 Resp: 251  
Ion Ratio Lower Upper  
128 100  
127 0.0 10.6 15.8#  
129 0.0 8.6 13.0#

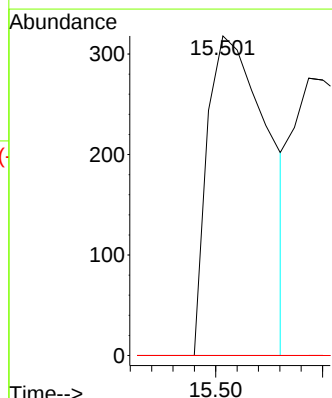



#96  
 1,2,3-Trichlorobenzene  
 Concen: 2.984 ug/l  
 RT: 15.705 min Scan# 5114  
 Delta R.T. 0.003 min  
 Lab File: VN068595.D  
 Acq: 21 Sep 2021 20:38

Instrument :  
 MSVOA\_N  
 ClientSampled :

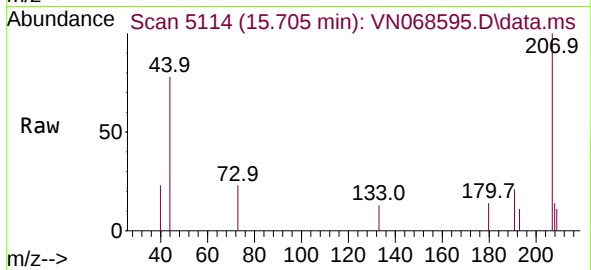

Tgt Ion:180 Resp: 83  
 Ion Ratio Lower Upper  
 180 100  
 182 94.0 47.9 143.6  
 145 0.0 15.2 45.5#

