

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN092121\  
 Data File : VN068576.D  
 Acq On : 21 Sep 2021 12:30  
 Operator : JC/MD  
 Sample : VN0921WBL01  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 VN0921WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N090721W.M

Title : SW846 8260

Signal : TIC: VN068576.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.735       | 269           | 278         | 295          | rVB3     | 15439          | 33910         | 1.12%           | 0.216%        |
| 2         | 5.106       | 1137          | 1162        | 1184         | rBV4     | 13509          | 43991         | 1.45%           | 0.280%        |
| 3         | 8.024       | 2223          | 2250        | 2261         | rBV3     | 423857         | 1014386       | 33.50%          | 6.456%        |
| 4         | 8.088       | 2262          | 2274        | 2321         | rVB      | 816108         | 1910002       | 63.08%          | 12.156%       |
| 5         | 8.440       | 2384          | 2405        | 2433         | rBV      | 398003         | 942450        | 31.13%          | 5.998%        |
| 6         | 8.971       | 2583          | 2603        | 2636         | rBV      | 1034814        | 2198422       | 72.61%          | 13.992%       |
| 7         | 10.443      | 3133          | 3152        | 3187         | rBV      | 1562930        | 3027770       | 100.00%         | 19.270%       |
| 8         | 11.746      | 3618          | 3638        | 3665         | rBV      | 1416177        | 2616359       | 86.41%          | 16.652%       |
| 9         | 12.733      | 3987          | 4006        | 4032         | rBV      | 1054875        | 1847152       | 61.01%          | 11.756%       |
| 10        | 13.677      | 4343          | 4358        | 4377         | rVB      | 1117579        | 1943500       | 64.19%          | 12.369%       |
| 11        | 15.268      | 4938          | 4951        | 4967         | rVB5     | 21153          | 37917         | 1.25%           | 0.241%        |
| 12        | 15.512      | 5025          | 5042        | 5061         | rVB2     | 22415          | 46597         | 1.54%           | 0.297%        |
| 13        | 15.702      | 5093          | 5113        | 5129         | rVB4     | 23093          | 49878         | 1.65%           | 0.317%        |




Sum of corrected areas: 15712334

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN092121\  
Data File : VN068576.D  
Acq On : 21 Sep 2021 12:30  
Operator : JC/MD  
Sample : VN0921WBL01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0921WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N090721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

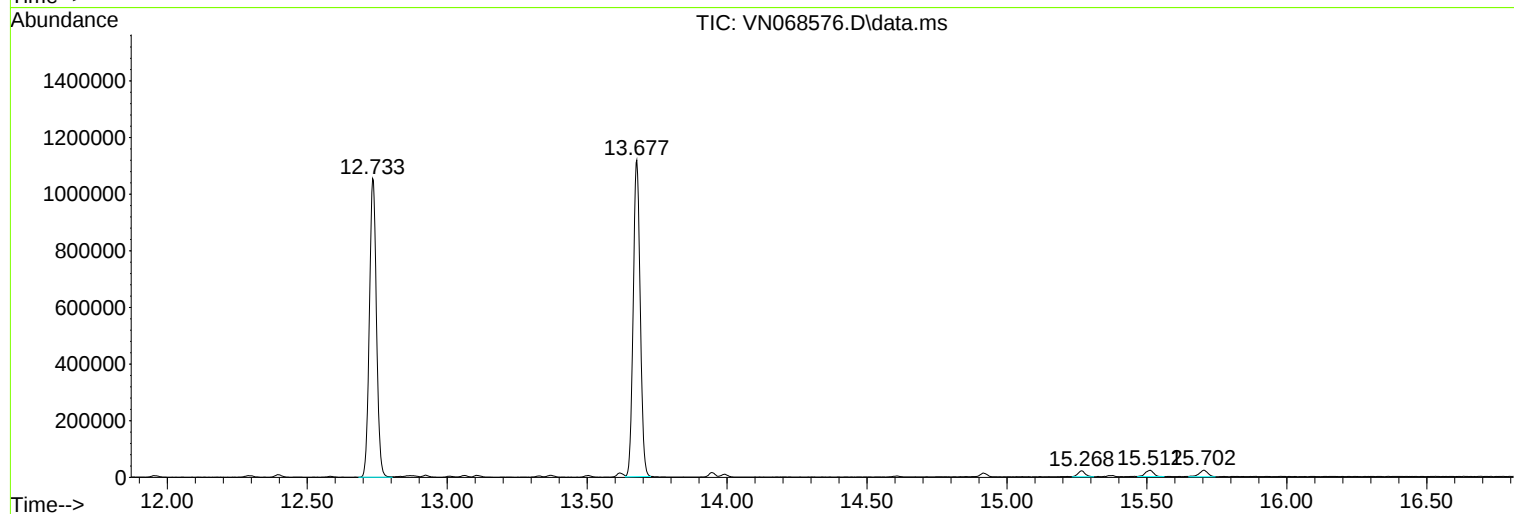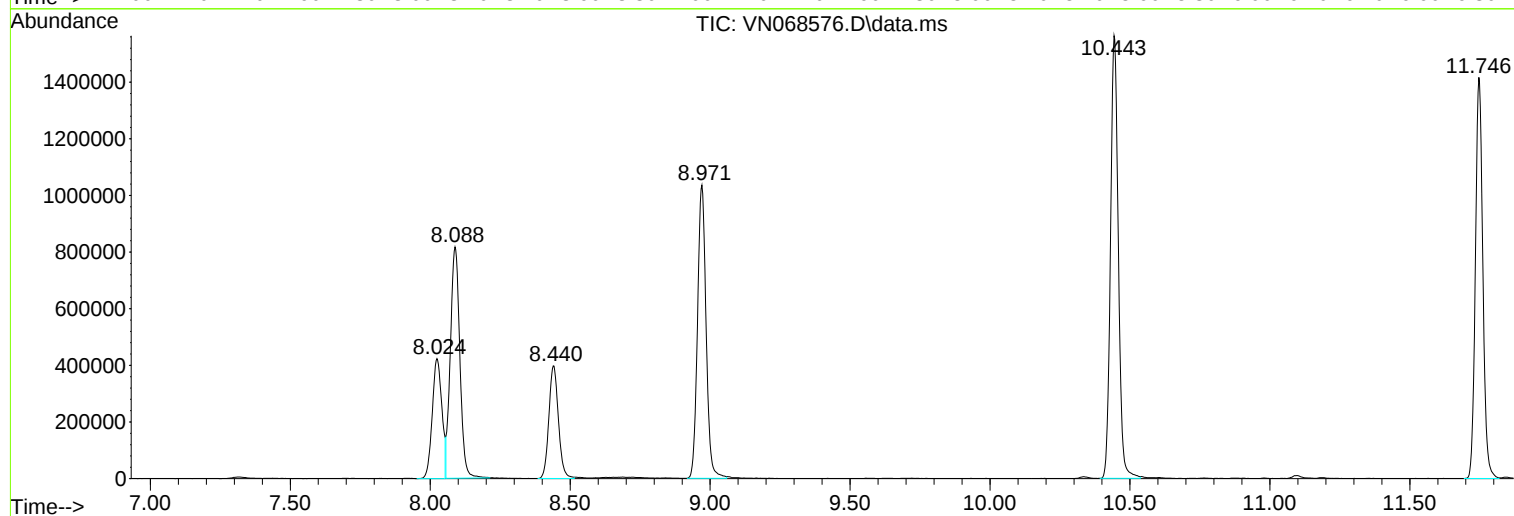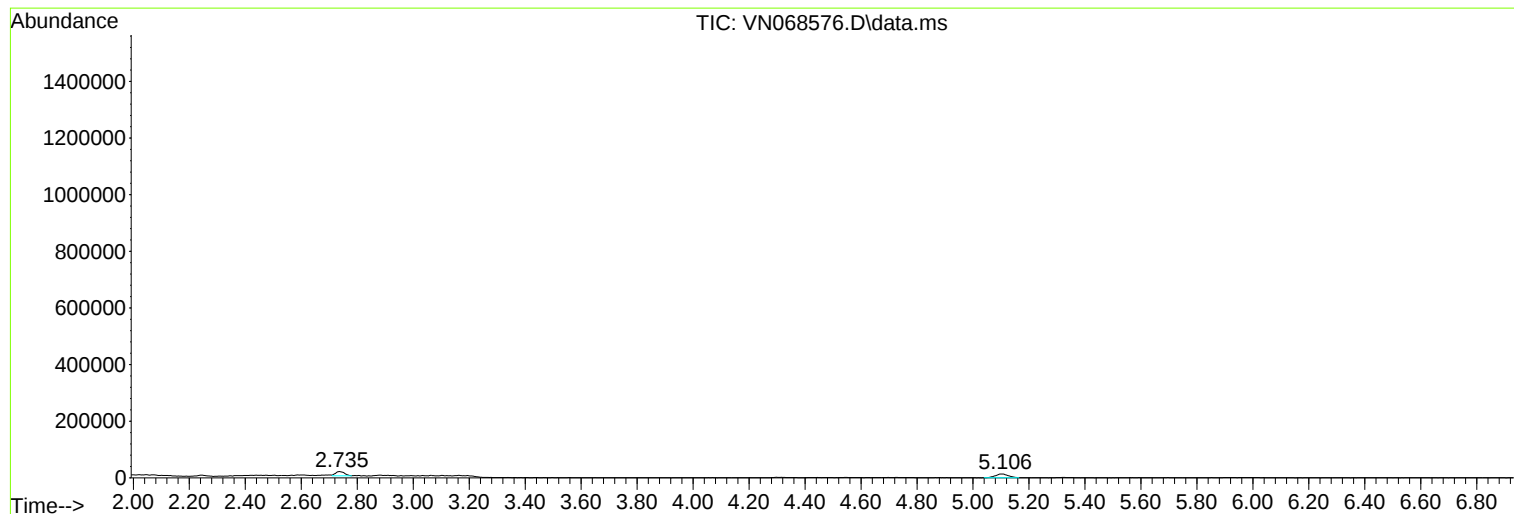

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN092121\  
Data File : VN068576.D  
Acq On : 21 Sep 2021 12:30  
Operator : JC/MD  
Sample : VN0921WBL01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0921WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N090721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN092121\  
Data File : VN068576.D  
Acq On : 21 Sep 2021 12:30  
Operator : JC/MD  
Sample : VN0921WBL01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0921WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N090721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----