
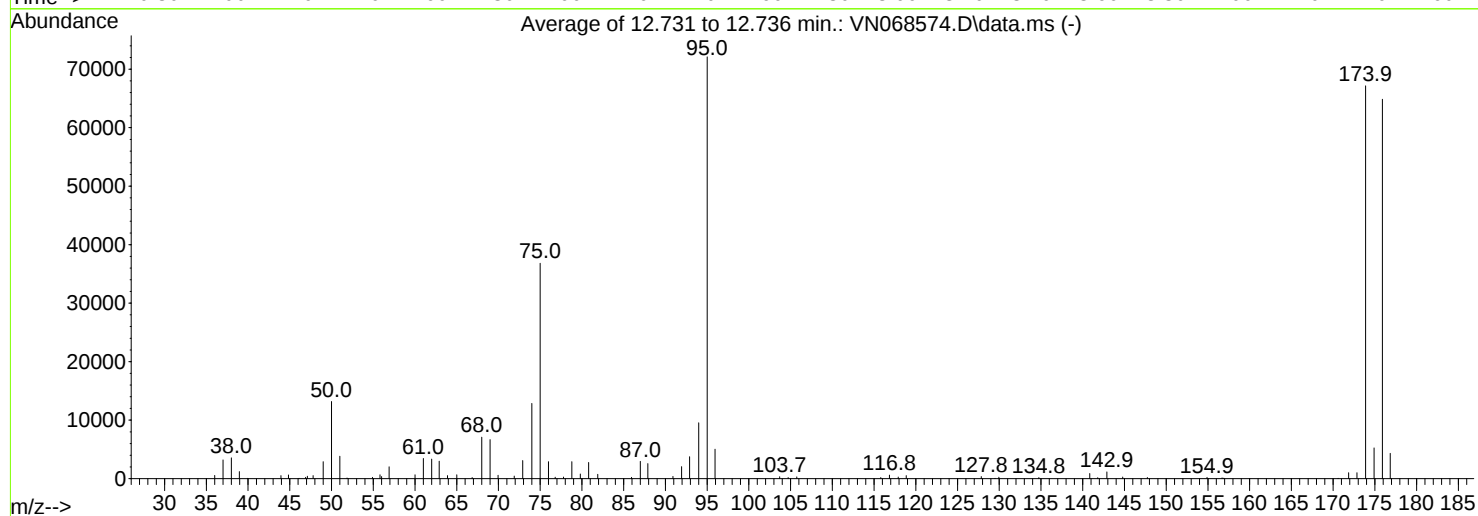


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092121\
Data File : VN068574.D
Acq On : 21 Sep 2021 10:14
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
Title : SW846 8260
Last Update : Fri Sep 17 11:02:11 2021

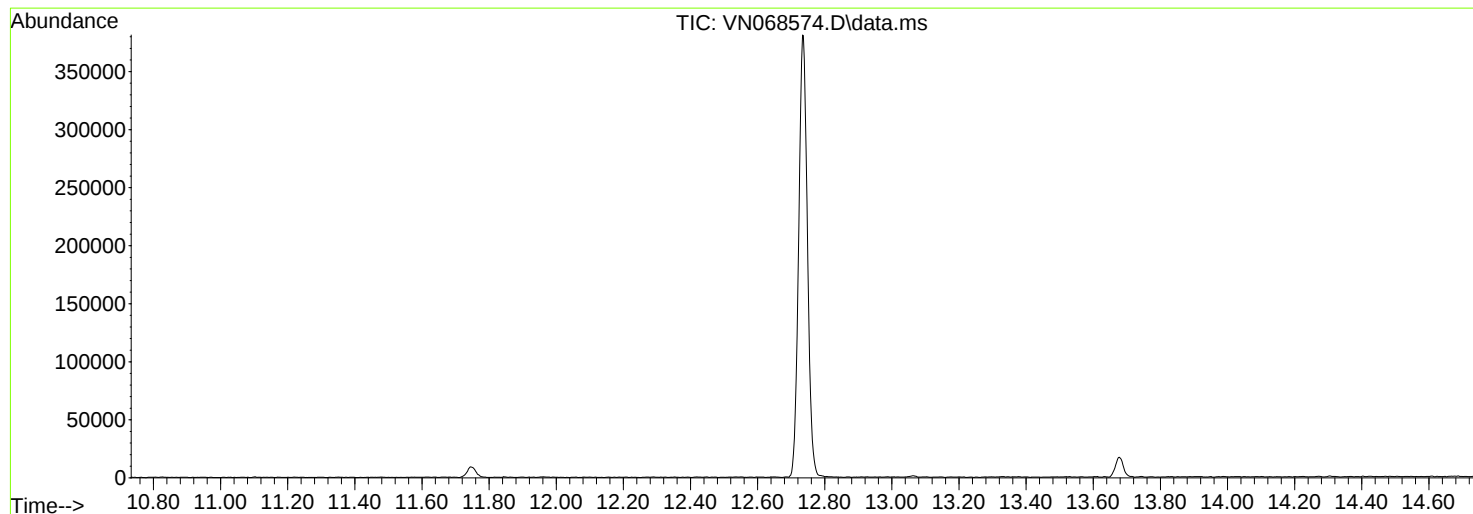

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	13180	PASS
75	95	30	60	51.1	36827	PASS
95	95	100	100	100.0	72109	PASS
96	95	5	9	7.0	5043	PASS
173	174	0.00	2	1.5	1009	PASS
174	95	50	100	93.1	67155	PASS
175	174	5	9	7.8	5258	PASS
176	174	95	101	96.6	64853	PASS
177	176	5	9	6.7	4330	PASS