

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092122\
 Data File : VN074603.D
 Acq On : 21 Sep 2022 10:32
 Operator : JC\MD
 Sample : VN0921MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0921MBL01

Quant Time: Sep 22 06:56:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091522W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 15 19:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	312873	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	590703	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	478415	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	172707	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.363	65	272833	51.394	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 102.780%			
35) Dibromofluoromethane	7.945	113	198905	50.690	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.380%			
50) Toluene-d8	10.381	98	693125	45.675	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 91.340%			
62) 4-Bromofluorobenzene	12.674	95	205836	39.603	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 79.200%#			
Target Compounds						Qvalue
3) Chloromethane	2.281	50	2514	0.695	ug/l #	43
6) Chloroethane	2.869	64	5210	1.244	ug/l #	42
11) Tert butyl alcohol	5.228	59	837	0.484	ug/l #	72
12) 1,1-Dichloroethene	4.075	96	205	0.734	ug/l #	1
13) Acrolein	3.987	56	342	0.542	ug/l	92
16) Acetone	4.210	43	898	0.264	ug/l #	52
18) Methyl Acetate	4.781	43	2529	0.240	ug/l	93
20) Methylene Chloride	5.010	84	1109	0.245	ug/l #	63
21) trans-1,2-Dichloroethene	5.746	96	228	0.479	ug/l #	1
25) 2-Butanone	7.269	43	2809	0.498	ug/l	97
29) Tetrahydrofuran	7.616	42	1542	0.416	ug/l #	74
31) Cyclohexane	8.010	56	9402	0.998	ug/l #	25
36) 1,1-Dichloropropene	8.016	75	30754	4.428	ug/l #	48
38) Carbon Tetrachloride	8.010	117	34363	5.359	ug/l #	21
49) 1,4-Dioxane	9.504	88	223	1.557	ug/l #	29
51) 4-Methyl-2-Pentanone	10.275	43	3150	0.287	ug/l	96
58) 2-Chloroethyl Vinyl ether	9.975	63	1707	0.407	ug/l #	63
59) 2-Hexanone	11.033	43	4483	0.535	ug/l	94
68) m/p-Xylenes	11.898	106	1940	0.238	ug/l	92
74) N-amyl acetate	12.345	43	2438	0.220	ug/l #	59
76) 1,2,3-Trichloropropane	12.669	75	125251	23.561	ug/l #	1
77) Bromobenzene	12.804	156	879	0.233	ug/l	65
81) trans-1,4-Dichloro-2-b...	12.669	75	125251	50.852	ug/l #	10
82) 4-Chlorotoluene	13.045	91	2520	0.211	ug/l #	49
87) 1,3-Dichlorobenzene	13.551	146	2348	0.338	ug/l #	60
88) 1,4-Dichlorobenzene	13.627	146	1725	0.247	ug/l #	1
91) 1,2-Dichlorobenzene	13.921	146	1817	0.252	ug/l	76
92) 1,2-Dibromo-3-Chloropr...	14.557	75	406	0.259	ug/l	81
95) Naphthalene	15.433	128	14430	2.534	ug/l #	94
96) 1,2,3-Trichlorobenzene	15.615	180	1151	1.652	ug/l #	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092122\
Data File : VN074603.D
Acq On : 21 Sep 2022 10:32
Operator : JC\MD
Sample : VN0921MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01

Quant Time: Sep 22 06:56:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091522W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 15 19:20:33 2022
Response via : Initial Calibration




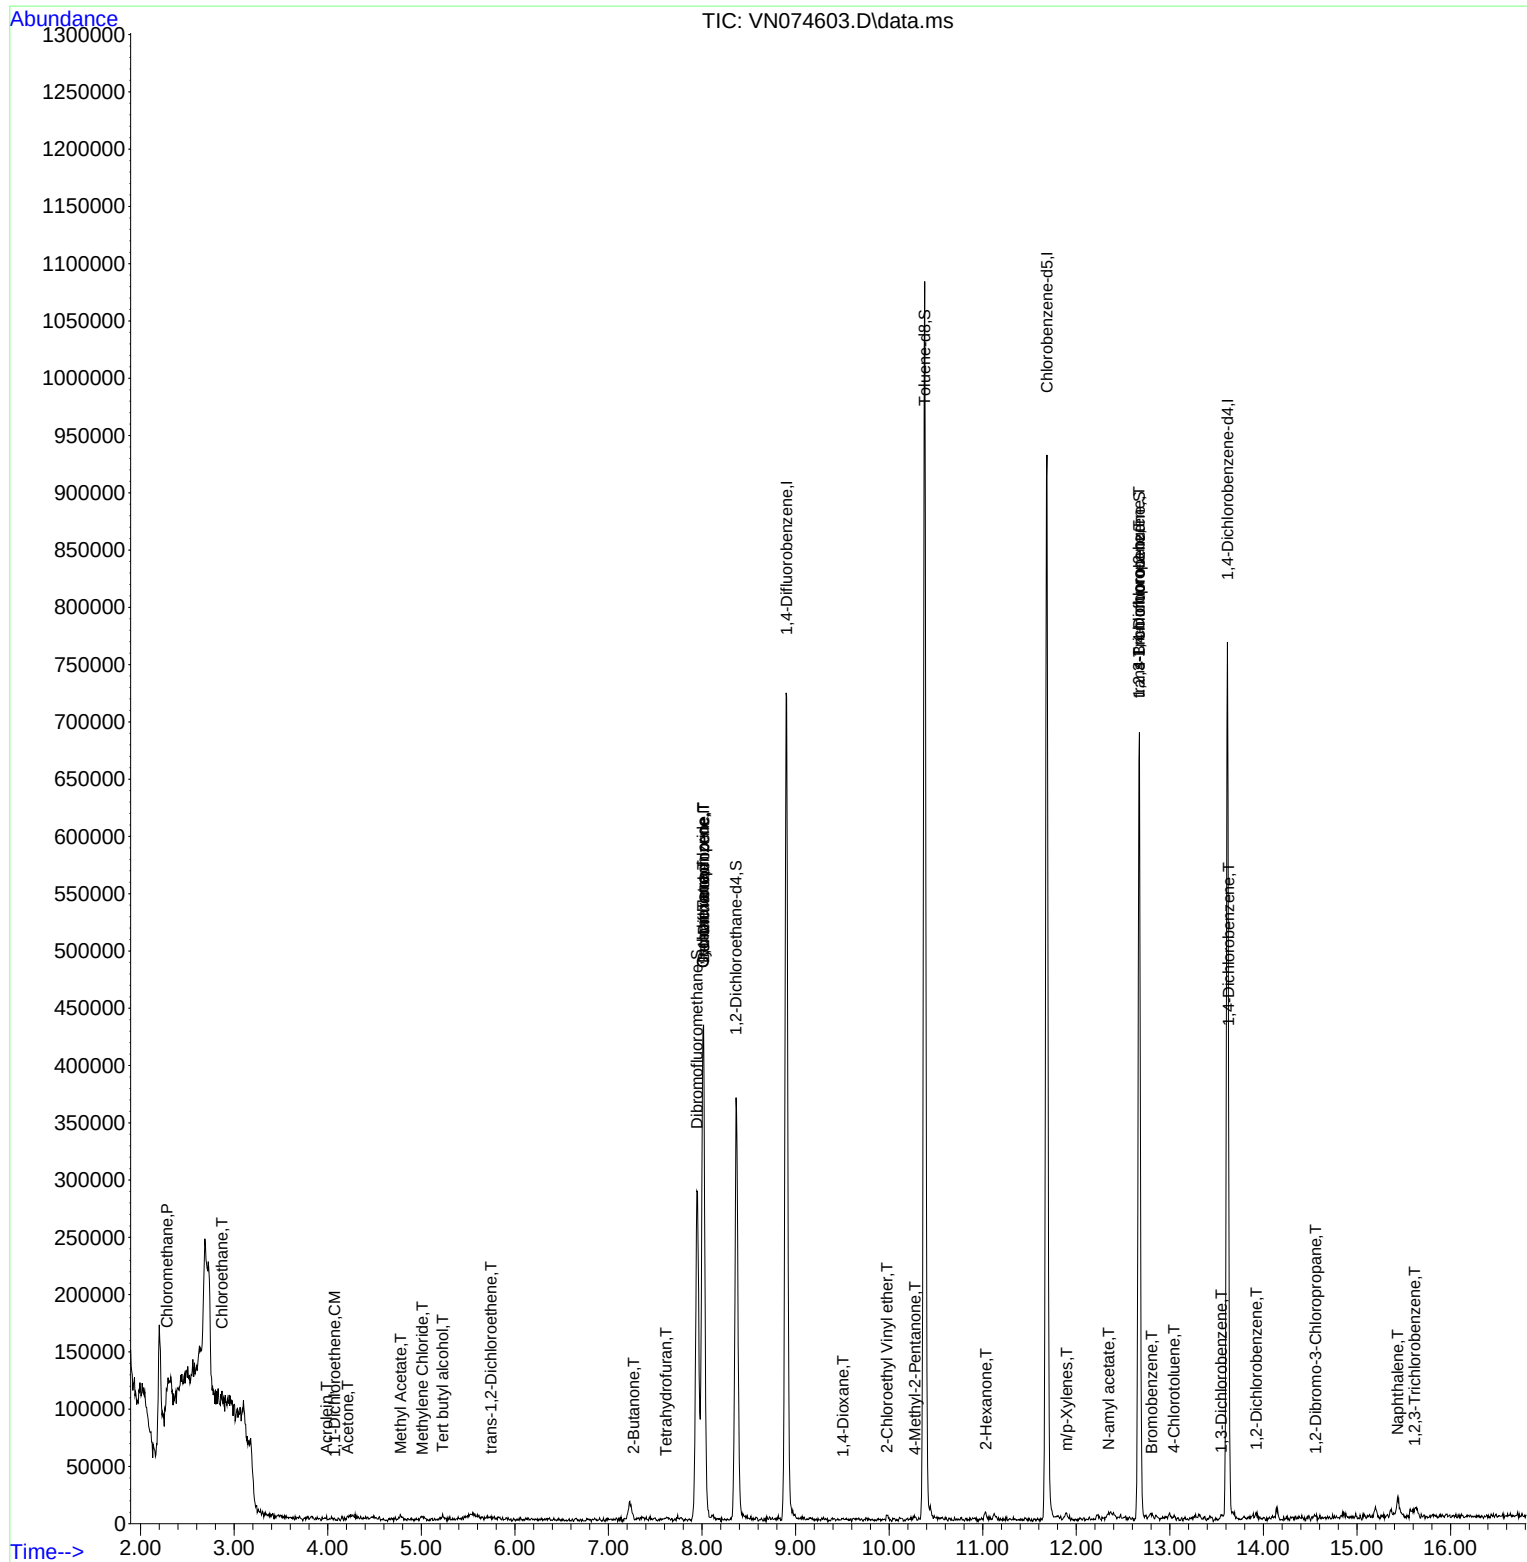




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01


Tgt Ion:168 Resp: 312873
Ion Ratio Lower Upper
168 100
99 52.4 42.3 63.5



#3
Chloromethane
Concen: 0.695 ug/l
RT: 2.281 min Scan# 67
Delta R.T. 0.018 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion: 50 Resp: 2514
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5#


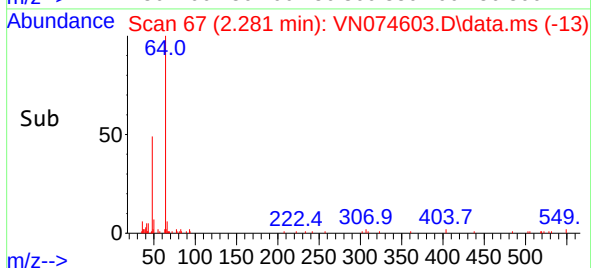






#6
Chloroethane
Concen: 1.244 ug/l
RT: 2.869 min Scan# 11
Delta R.T. -0.082 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01


Tgt Ion: 64 Resp: 5210
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

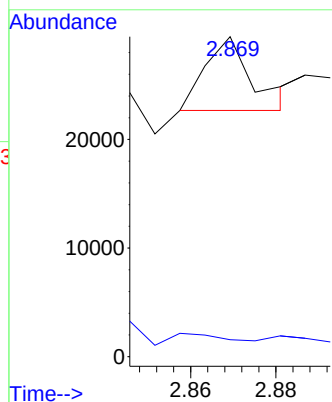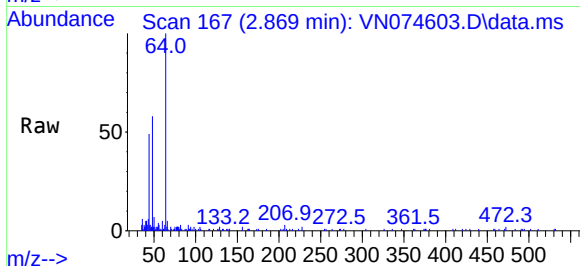

#11
Tert butyl alcohol
Concen: 0.484 ug/l
RT: 5.228 min Scan# 568
Delta R.T. -0.053 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion: 59 Resp: 837
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


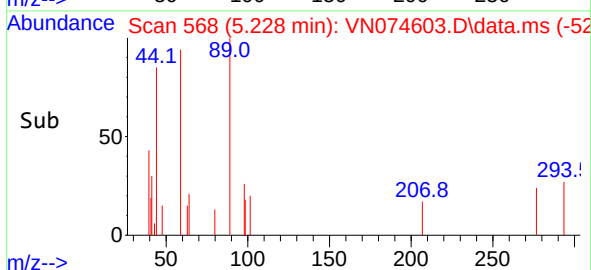

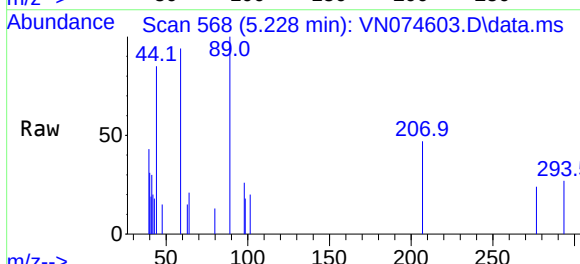




#12
1,1-Dichloroethene
Concen: 0.734 ug/l
RT: 4.075 min Scan# 31
Delta R.T. -0.029 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01


Tgt Ion: 96 Resp: 205
Ion Ratio Lower Upper
96 100
61 0.0 127.6 191.4#
98 0.0 51.2 76.8#

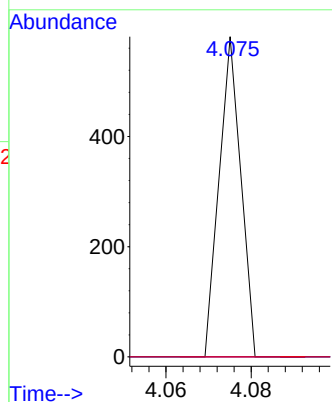

#13
Acrolein
Concen: 0.542 ug/l
RT: 3.987 min Scan# 357
Delta R.T. 0.012 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion: 56 Resp: 342
Ion Ratio Lower Upper
56 100
55 62.0 54.8 82.2


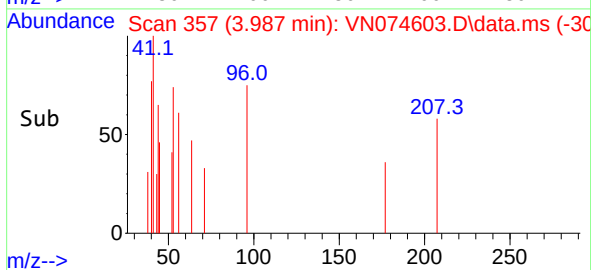






#16
Acetone
Concen: 0.264 ug/l
RT: 4.210 min Scan# 395
Delta R.T. -0.006 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01


Tgt Ion: 43 Resp: 898
Ion Ratio Lower Upper
43 100
58 59.2 26.0 39.0#

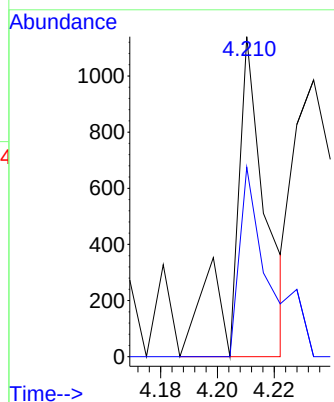

#18
Methyl Acetate
Concen: 0.240 ug/l
RT: 4.781 min Scan# 492
Delta R.T. 0.012 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion: 43 Resp: 2529
Ion Ratio Lower Upper
43 100
74 30.9 21.6 32.4


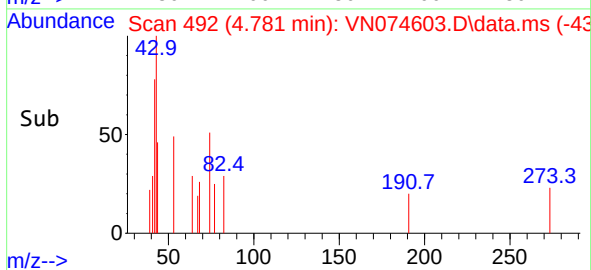
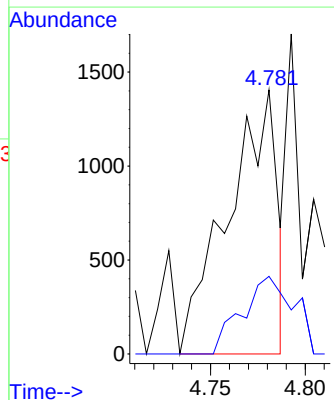



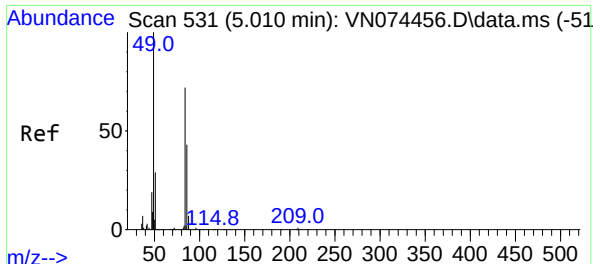

#20
Methylene Chloride
Concen: 0.245 ug/l
RT: 5.010 min Scan# 511
Delta R.T. 0.000 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01


Tgt Ion:	84	Resp:	1109
Ion	Ratio	Lower	Upper
84	100		
49	157.5	88.3	132.5#
51	0.0	28.2	42.2#
86	54.0	50.6	76.0

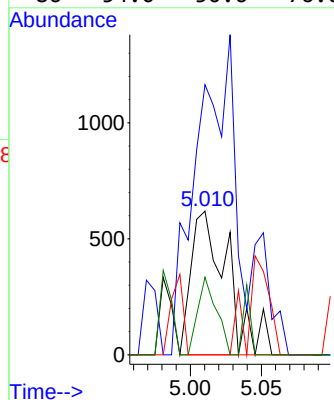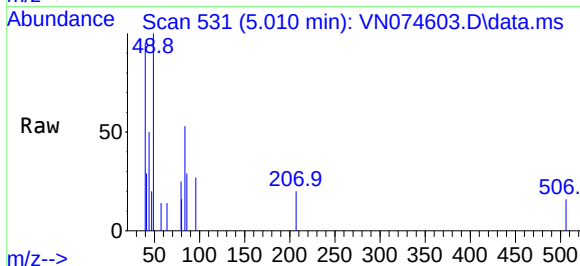

#21
trans-1,2-Dichloroethene
Concen: 0.479 ug/l
RT: 5.746 min Scan# 656
Delta R.T. 0.242 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion:	96	Resp:	228
Ion	Ratio	Lower	Upper
96	100		
61	0.0	105.8	158.8#
98	0.0	50.3	75.5#

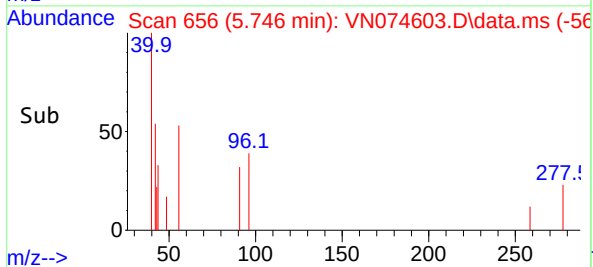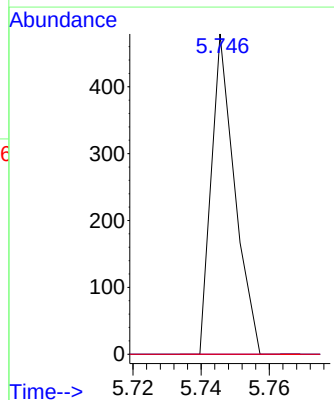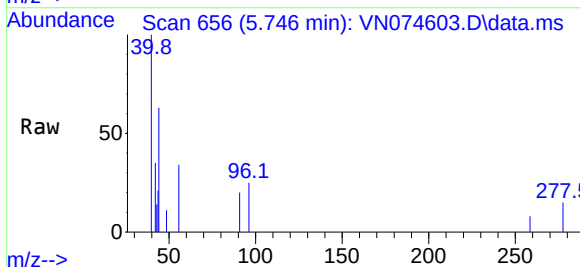



#25

2-Butanone

Concen: 0.498 ug/l

RT: 7.269 min Scan# 91

Delta R.T. 0.012 min

Lab File: VN074603.D

Acq: 21 Sep 2022 10:32

Instrument :

MSVOA_N

ClientSampleId :





VN0921MBL01

Tgt Ion: 43 Resp: 2809

Ion Ratio Lower Upper

43 100

72 31.5 23.7 35.5

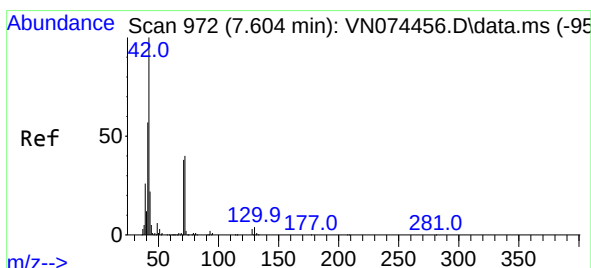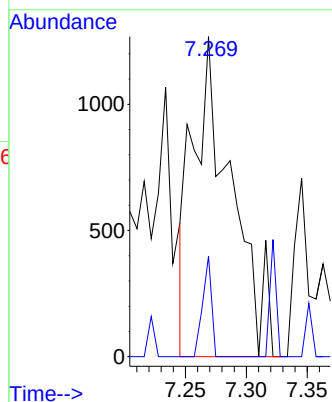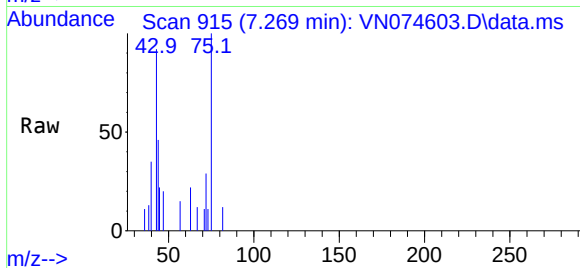

#29

Tetrahydrofuran

Concen: 0.416 ug/l

RT: 7.616 min Scan# 974

Delta R.T. 0.012 min

Lab File: VN074603.D

Acq: 21 Sep 2022 10:32




Tgt Ion: 42 Resp: 1542


Ion Ratio Lower Upper

42 100

72 30.5 39.7 59.5#

71 30.2 36.6 55.0#

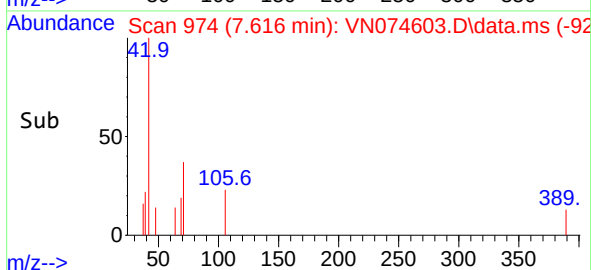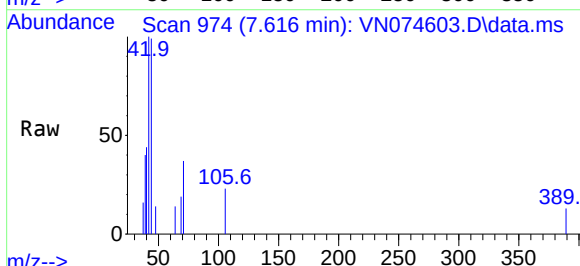



#31

Cyclohexane

Concen: 0.998 ug/l

RT: 8.010 min Scan# 1101

Delta R.T. -0.012 min

Lab File: VN074603.D

Acq: 21 Sep 2022 10:32

Instrument :

MSVOA_N

ClientSampleId :

VN0921MBL01





Tgt Ion: 56 Resp: 9402

Ion Ratio Lower Upper

56 100

69 90.5 27.8 41.8#

84 161.6 76.9 115.3#

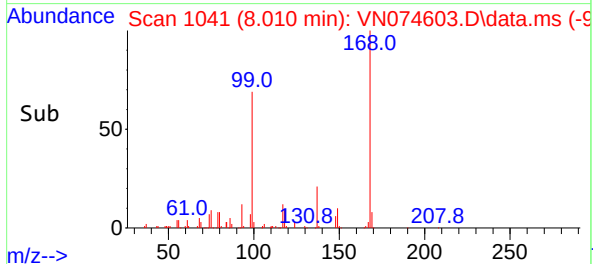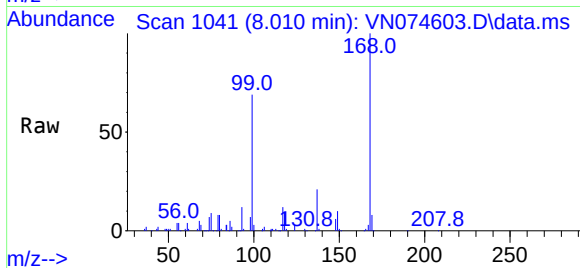

#33

1,2-Dichloroethane-d4

Concen: 51.394 ug/l

RT: 8.363 min Scan# 1101

Delta R.T. -0.006 min

Lab File: VN074603.D




Acq: 21 Sep 2022 10:32


Tgt Ion: 65 Resp: 272833

Ion Ratio Lower Upper

65 100

67 52.1 0.0 104.8

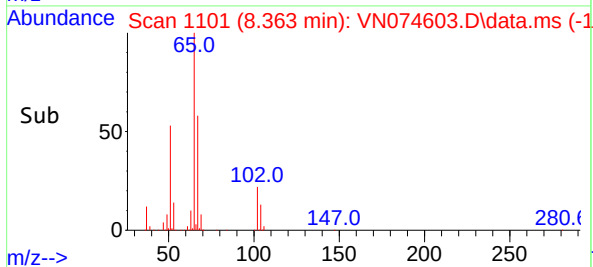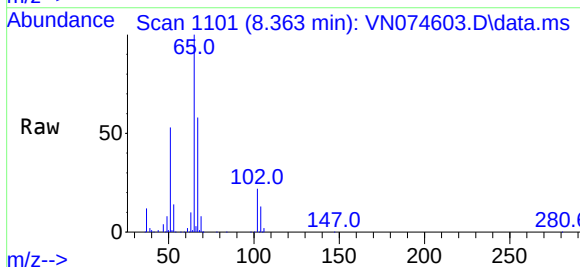




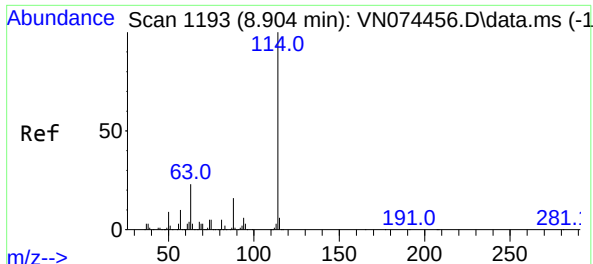


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.904 min Scan# 1193
Delta R.T. 0.000 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01

Tgt Ion:114 Resp: 590703




Ion	Ratio	Lower	Upper
114	100		
63	24.1	0.0	40.0
88	13.0	0.0	32.6

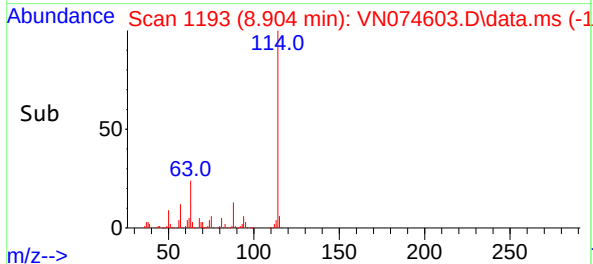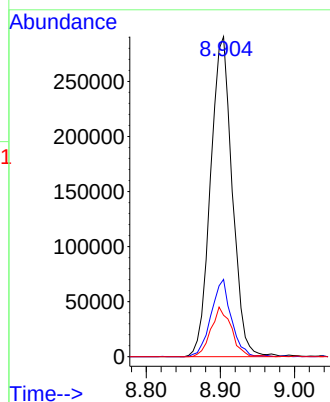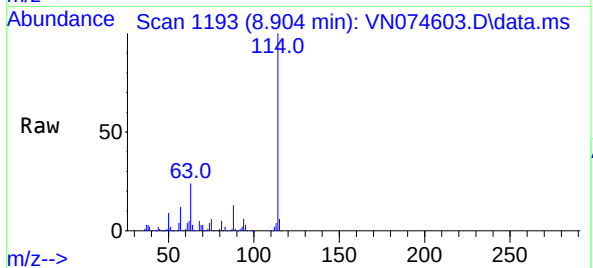


#35
Dibromofluoromethane
Concen: 50.690 ug/l
RT: 7.945 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion:113 Resp: 198905

Ion	Ratio	Lower	Upper
113	100		
111	103.9	81.4	122.0
192	17.5	17.0	25.6

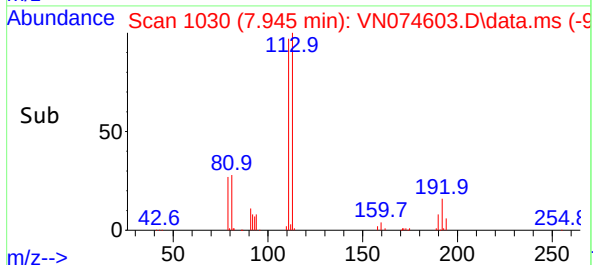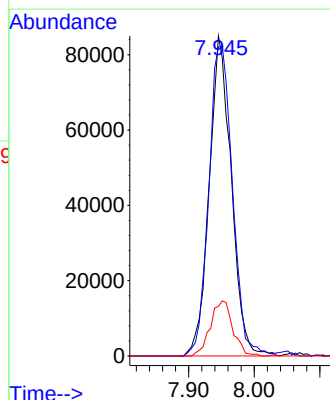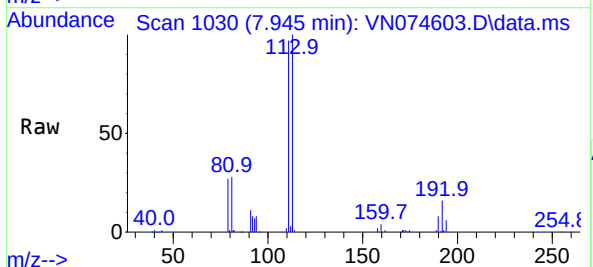

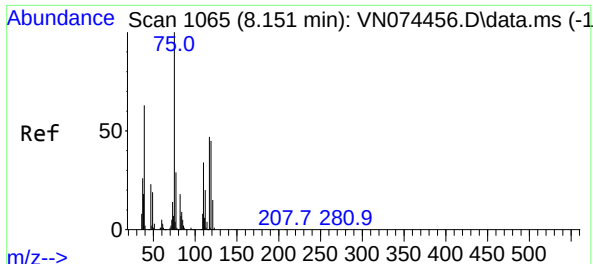

#36

1,1-Dichloropropene

Concen: 4.428 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.135 min

Lab File: VN074603.D

Acq: 21 Sep 2022 10:32

Instrument :

MSVOA_N

ClientSampleId :

VN0921MBL01





Tgt Ion: 75 Resp: 30754

Ion Ratio Lower Upper

75 100

110 7.7 18.3 54.8#

77 0.0 25.1 37.7#

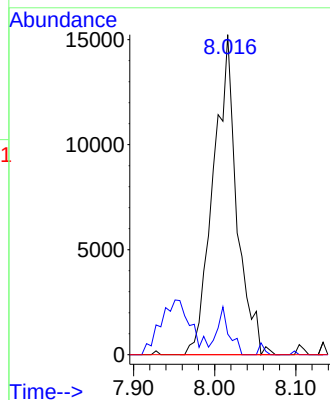

#38

Carbon Tetrachloride

Concen: 5.359 ug/l

RT: 8.010 min Scan# 1041

Delta R.T. -0.123 min

Lab File: VN074603.D

Acq: 21 Sep 2022 10:32




Tgt Ion: 117 Resp: 34363


Ion Ratio Lower Upper

117 100

119 11.0 75.8 113.8#

121 0.0 24.6 37.0#


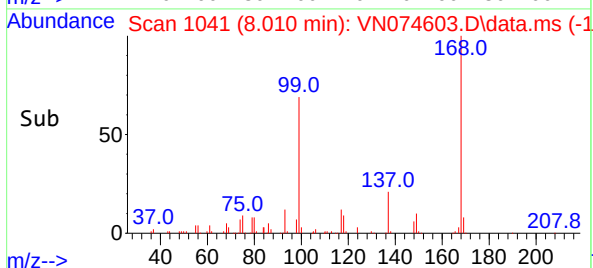
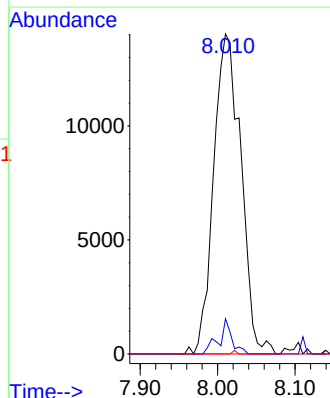
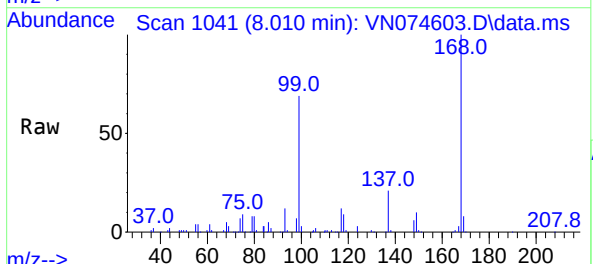




#49
1,4-Dioxane
Concen: 1.557 ug/l
RT: 9.504 min Scan# 1295
Delta R.T. 0.000 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01


Tgt Ion: 88 Resp: 223
Ion Ratio Lower Upper
88 100
43 131.4 20.2 30.4#
58 52.0 54.2 81.4#

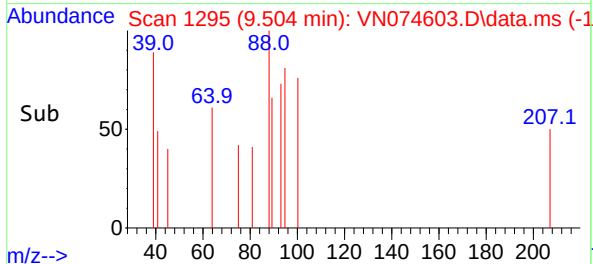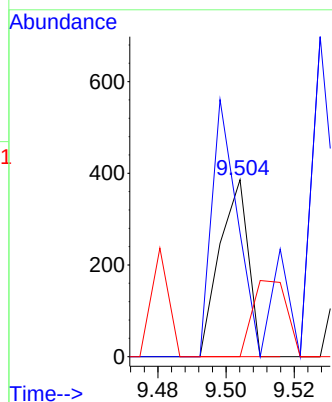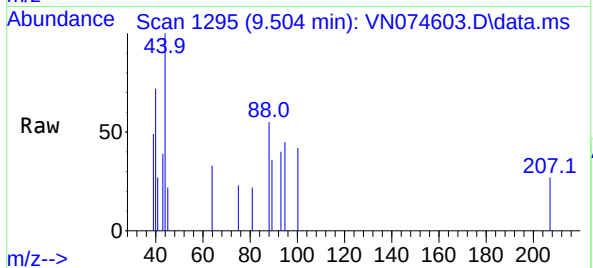

#50
Toluene-d8
Concen: 45.675 ug/l
RT: 10.381 min Scan# 1444
Delta R.T. 0.001 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion: 98 Resp: 693125
Ion Ratio Lower Upper
98 100
100 63.6 52.6 78.8


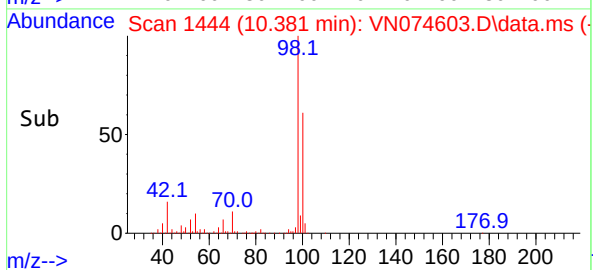
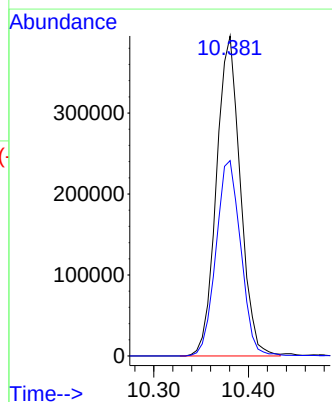
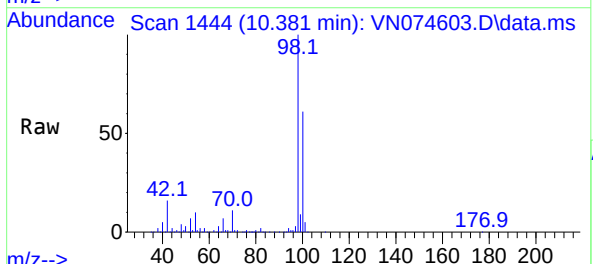




#51
4-Methyl-2-Pentanone
Concen: 0.287 ug/l
RT: 10.275 min Scan# 1425
Delta R.T. 0.006 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01


Tgt Ion: 43 Resp: 3150
Ion Ratio Lower Upper
43 100
58 45.1 34.1 51.1

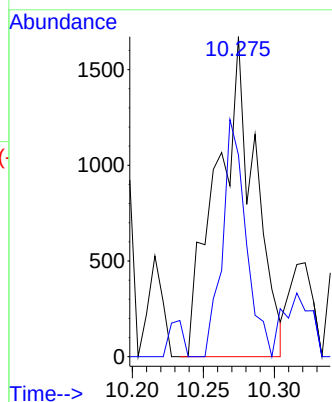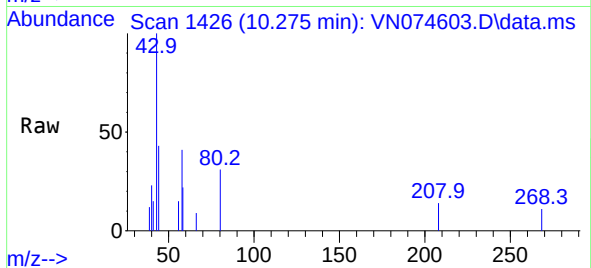

#58
2-Chloroethyl Vinyl ether
Concen: 0.407 ug/l
RT: 9.975 min Scan# 1375
Delta R.T. -0.005 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion: 63 Resp: 1707
Ion Ratio Lower Upper
63 100
106 10.4 24.6 36.8#


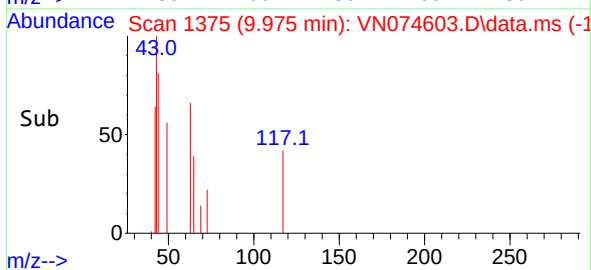
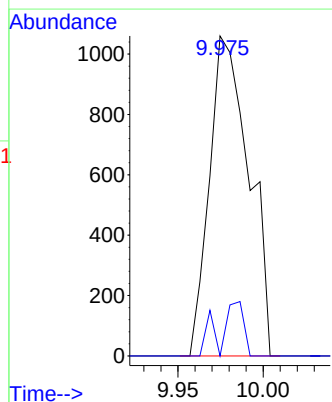





#59
2-Hexanone
Concen: 0.535 ug/l
RT: 11.033 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01


Tgt Ion: 43 Resp: 4483
Ion Ratio Lower Upper
43 100
58 54.8 29.7 89.1



#62
4-Bromofluorobenzene
Concen: 39.603 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion: 95 Resp: 205836
Ion Ratio Lower Upper
95 100
174 75.9 0.0 167.6
176 75.1 0.0 163.4


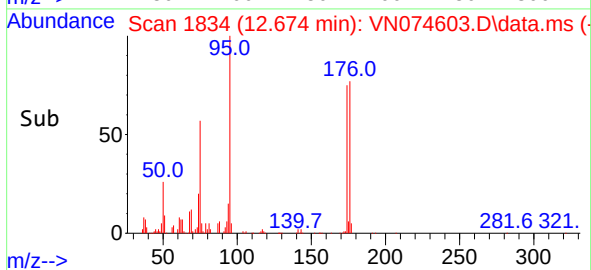




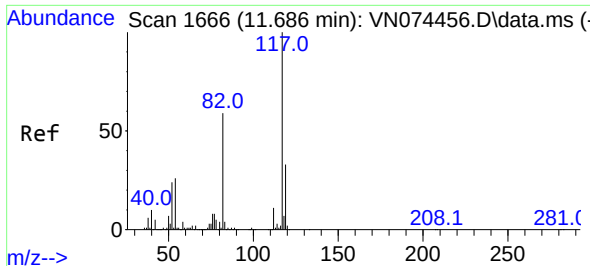

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01


Tgt Ion:117 Resp: 478415
Ion Ratio Lower Upper
117 100
82 59.3 44.2 66.2
119 32.9 25.4 38.0

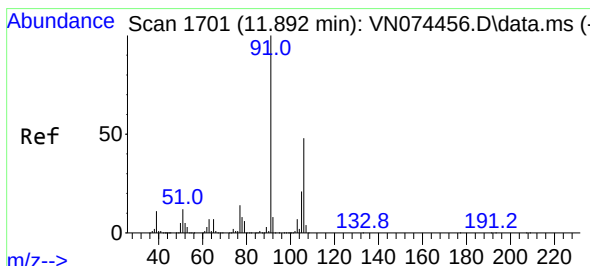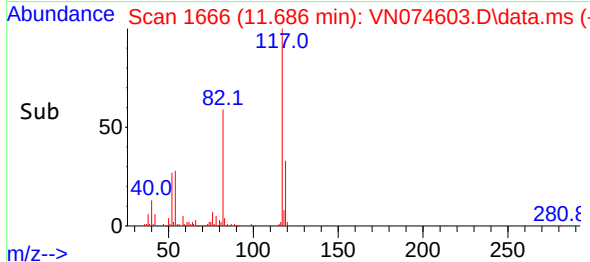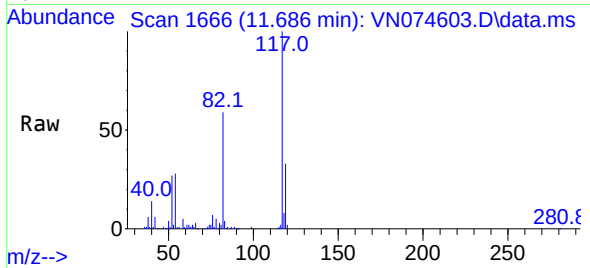

#68
m/p-Xylenes
Concen: 0.238 ug/l
RT: 11.898 min Scan# 1702
Delta R.T. 0.006 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32


Tgt Ion:106 Resp: 1940
Ion Ratio Lower Upper
106 100
91 211.2 158.9 238.3

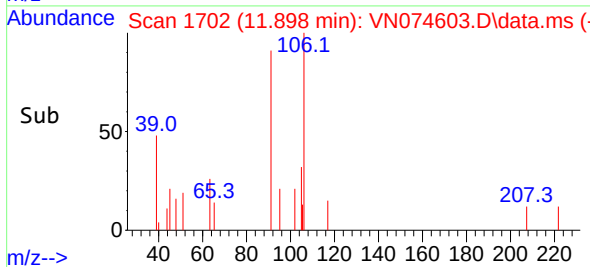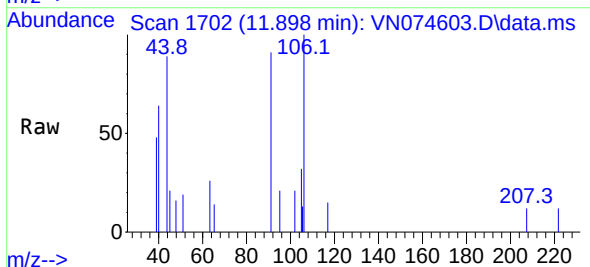



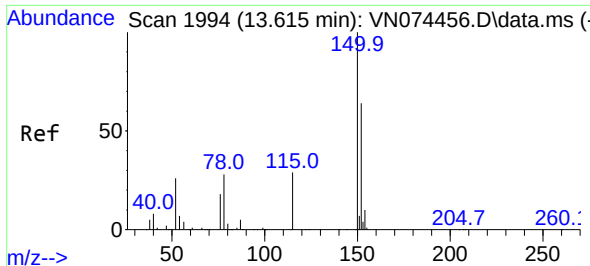


#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.616 min Scan# 1994
 Delta R.T. 0.001 min
 Lab File: VN074603.D
 Acq: 21 Sep 2022 10:32


Instrument :
 MSVOA_N
 ClientSampleId :
 VN0921MBL01

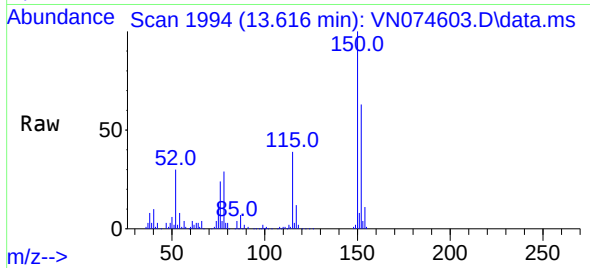



Tgt Ion:152 Resp: 172707
 Ion Ratio Lower Upper
 152 100
 115 60.7 28.9 86.7
 150 159.5 0.0 356.2

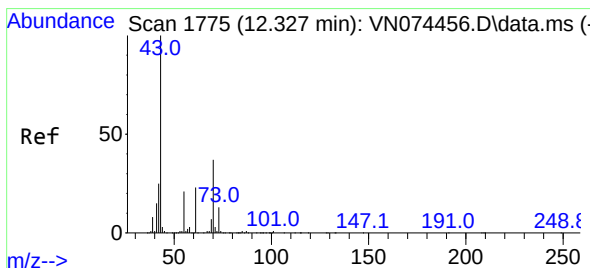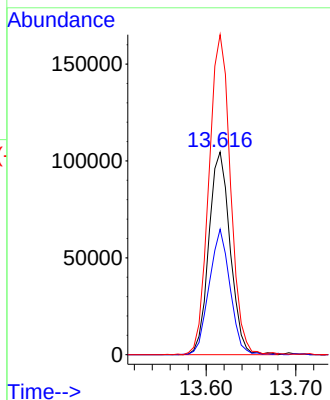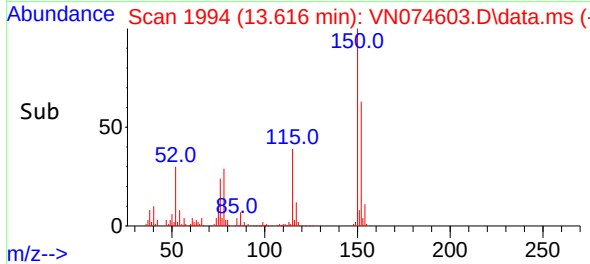


#74
 N-ethyl acetate
 Concen: 0.220 ug/l
 RT: 12.345 min Scan# 1778
 Delta R.T. 0.018 min
 Lab File: VN074603.D
 Acq: 21 Sep 2022 10:32

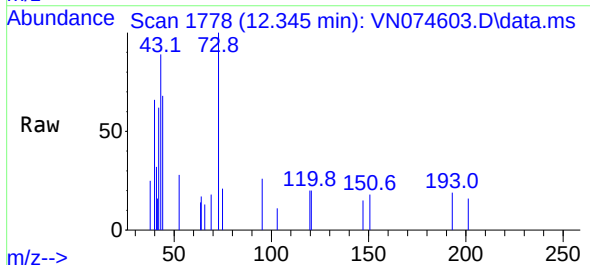

Tgt Ion: 43 Resp: 2438
 Ion Ratio Lower Upper
 43 100
 70 13.4 39.0 58.4#
 55 21.4 21.1 31.7
 61 0.0 21.1 31.7#



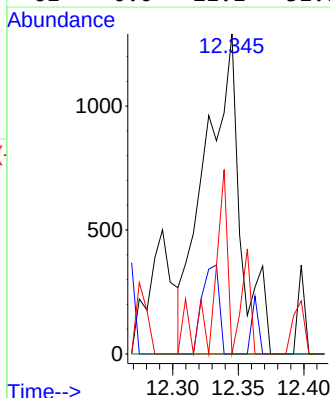
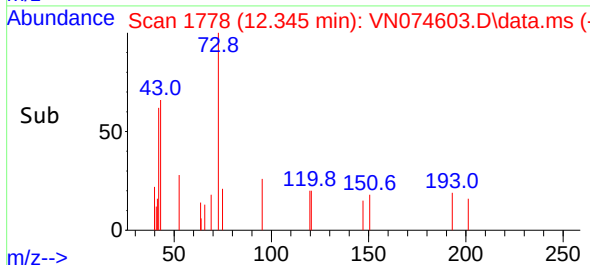




#76
1,2,3-Trichloropropane
Concen: 23.561 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.152 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01


Tgt Ion: 75 Resp: 125251
Ion Ratio Lower Upper
75 100
77 2.2 98.5 295.5#

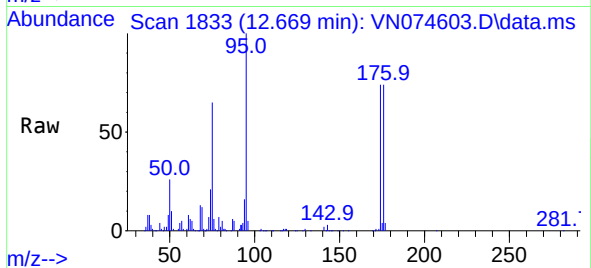

#77
Bromobenzene
Concen: 0.233 ug/l
RT: 12.804 min Scan# 1856
Delta R.T. -0.000 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion:156 Resp: 879
Ion Ratio Lower Upper
156 100
77 157.7 100.5 301.5
158 51.1 48.9 146.6


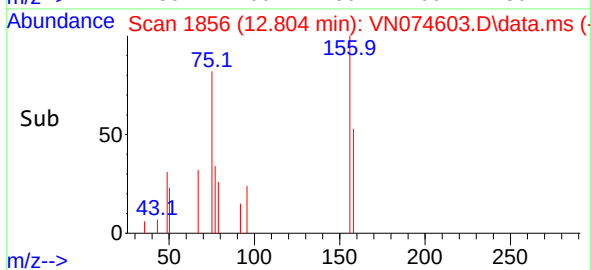




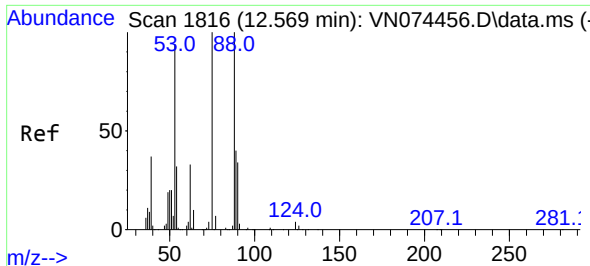

#81
trans-1,4-Dichloro-2-butene
Concen: 50.852 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. 0.100 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32




Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01


Tgt Ion: 75 Resp: 125251
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#

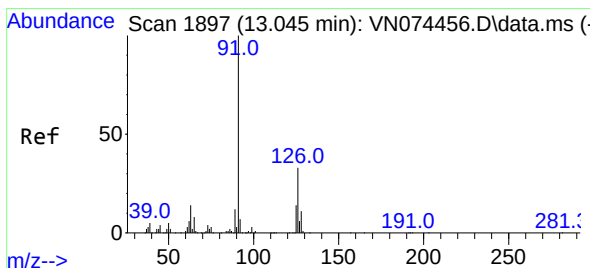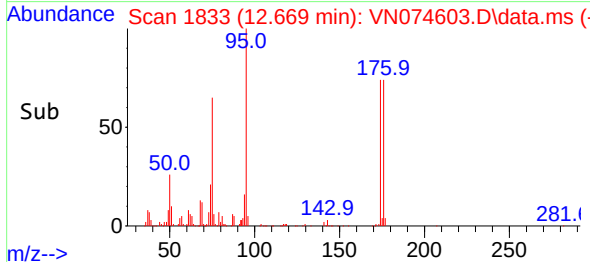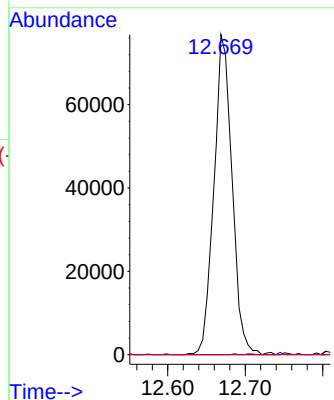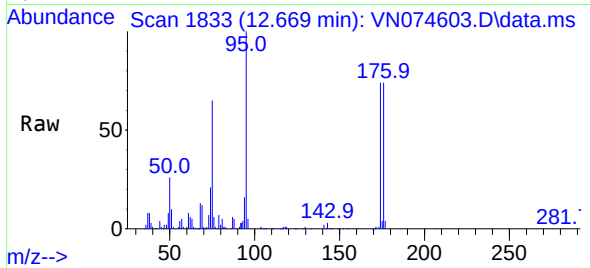

#82
4-Chlorotoluene
Concen: 0.211 ug/l
RT: 13.045 min Scan# 1897
Delta R.T. 0.000 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion: 91 Resp: 2520
Ion Ratio Lower Upper
91 100
126 5.2 17.2 51.6#

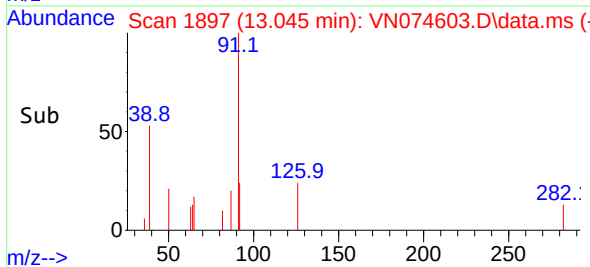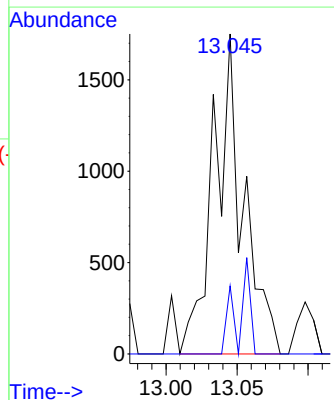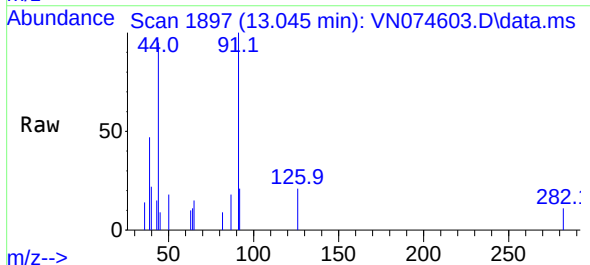



#87

1,3-Dichlorobenzene

Concen: 0.338 ug/l

RT: 13.551 min Scan# 1983

Delta R.T. -0.006 min

Lab File: VN074603.D

Acq: 21 Sep 2022 10:32

Instrument :

MSVOA_N

ClientSampleId :

VN0921MBL01





Tgt Ion:146 Resp: 2348

Ion Ratio Lower Upper

146 100

111 31.7 20.0 60.0

148 20.3 32.0 96.0#

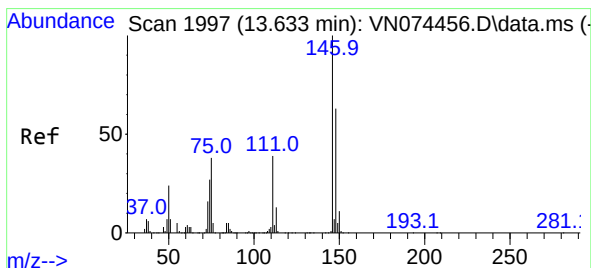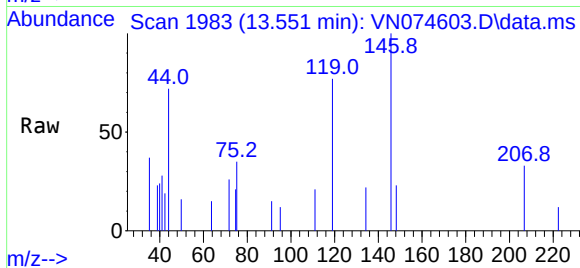

#88

1,4-Dichlorobenzene

Concen: 0.247 ug/l

RT: 13.627 min Scan# 1996

Delta R.T. -0.006 min

Lab File: VN074603.D

Acq: 21 Sep 2022 10:32




Tgt Ion:146 Resp: 1725


Ion Ratio Lower Upper

146 100

111 0.0 19.1 57.1#

148 200.8 31.4 94.3#

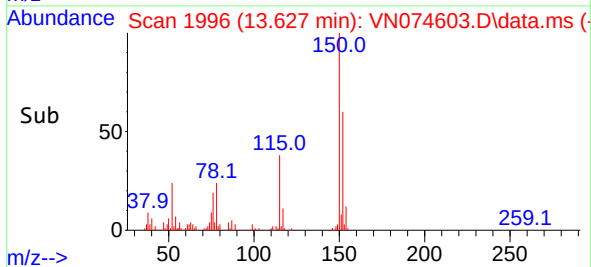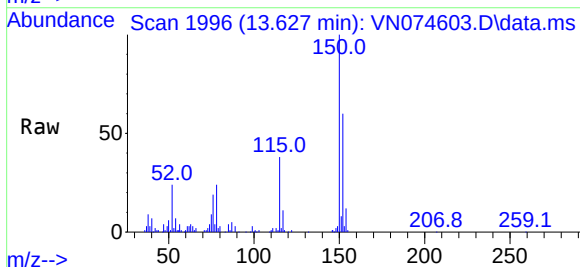



#91

1,2-Dichlorobenzene

Concen: 0.252 ug/l

RT: 13.921 min Scan# 2046

Delta R.T. -0.006 min

Lab File: VN074603.D

Acq: 21 Sep 2022 10:32

Instrument :

MSVOA_N

ClientSampleId :

VN0921MBL01





Tgt Ion:146 Resp: 1817

Ion Ratio Lower Upper

146 100

111 48.0 20.9 62.8

148 38.5 32.1 96.3

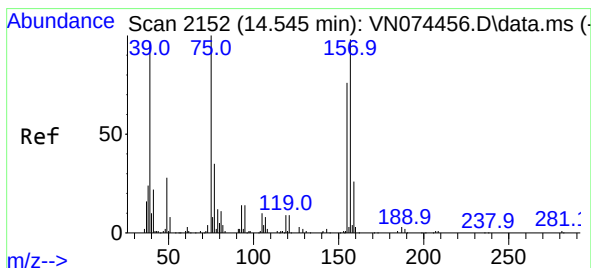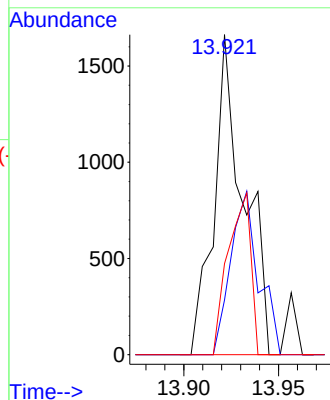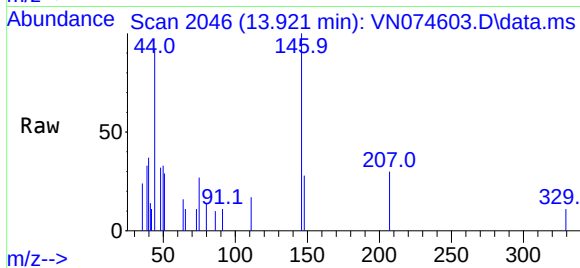

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.259 ug/l

RT: 14.557 min Scan# 2154

Delta R.T. 0.012 min

Lab File: VN074603.D

Acq: 21 Sep 2022 10:32




Tgt Ion: 75 Resp: 406


Ion Ratio Lower Upper

75 100

155 83.7 44.9 134.5

157 85.5 59.0 176.8


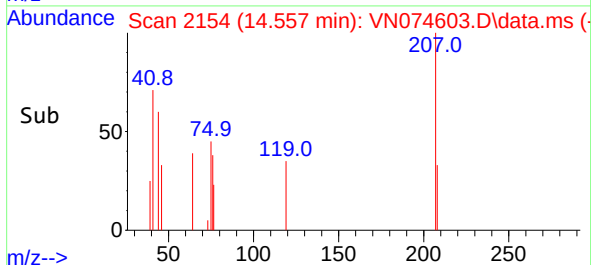
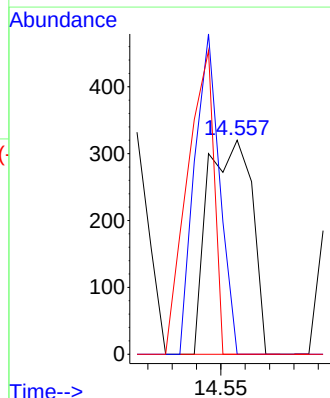
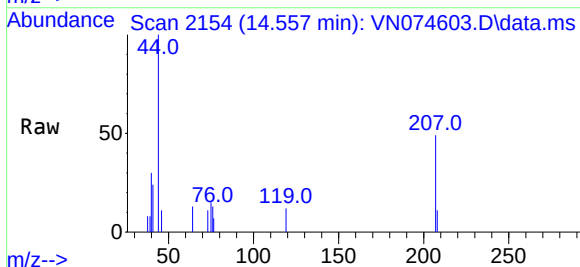




#95
Naphthalene
Concen: 2.534 ug/l
RT: 15.433 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Instrument :
MSVOA_N
ClientSampleId :
VN0921MBL01

Tgt Ion:128 Resp: 14430
Ion Ratio Lower Upper
128 100
127 10.3 10.3 15.5#
129 9.1 8.6 13.0

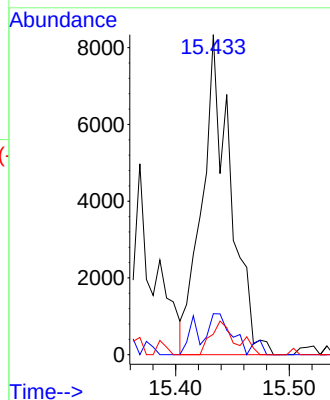

#96
1,2,3-Trichlorobenzene
Concen: 1.652 ug/l
RT: 15.615 min Scan# 2334
Delta R.T. -0.012 min
Lab File: VN074603.D
Acq: 21 Sep 2022 10:32

Tgt Ion:180 Resp: 1151
Ion Ratio Lower Upper
180 100
182 54.4 47.8 143.3
145 94.5 15.5 46.5#

