
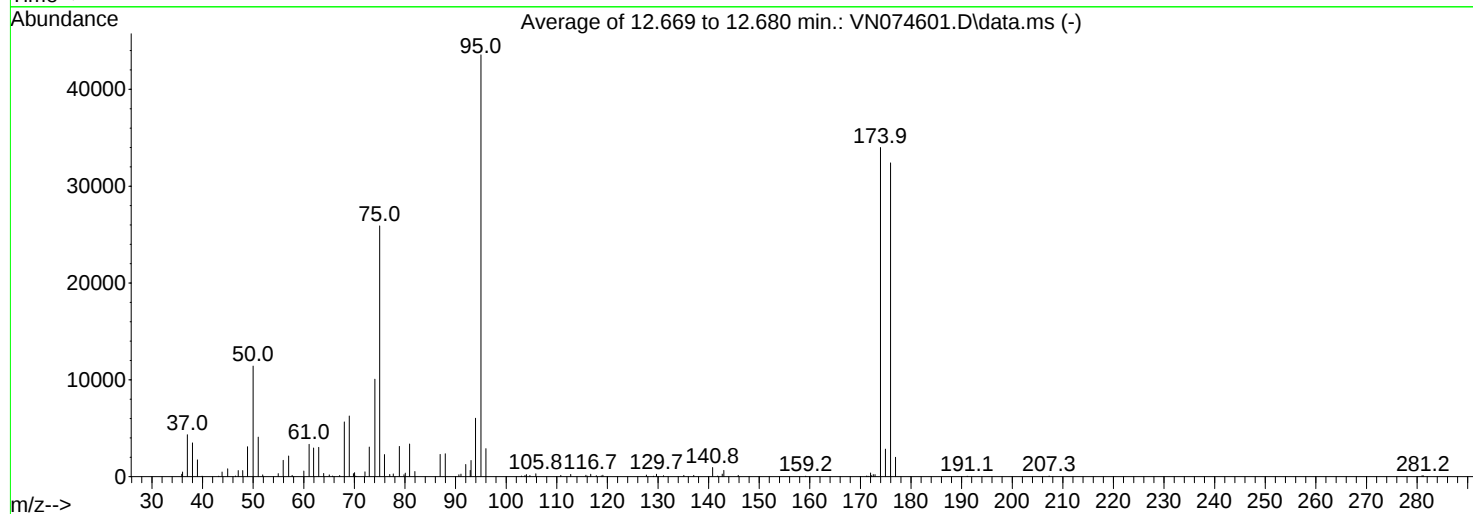


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092122\
 Data File : VN074601.D
 Acq On : 21 Sep 2022 07:57
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091522W.M
 Title : SW846 8260
 Last Update : Thu Sep 15 19:20:33 2022

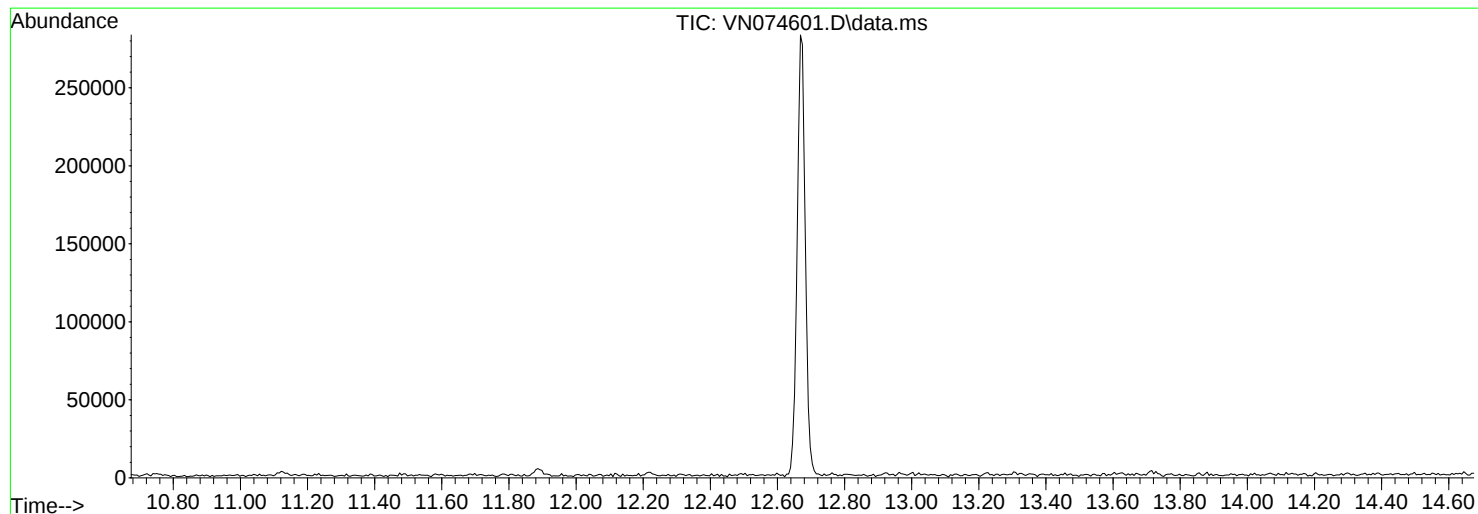

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.2	11424	PASS
75	95	30	60	59.4	25888	PASS
95	95	100	100	100.0	43565	PASS
96	95	5	9	6.7	2901	PASS
173	174	0.00	2	0.6	217	PASS
174	95	50	100	78.0	33987	PASS
175	174	5	9	8.3	2837	PASS
176	174	95	101	95.4	32411	PASS
177	176	5	9	6.2	1994	PASS