



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092123\
Data File : VN079313.D
Acq On : 21 Sep 2023 08:14
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 05:05:24 2023

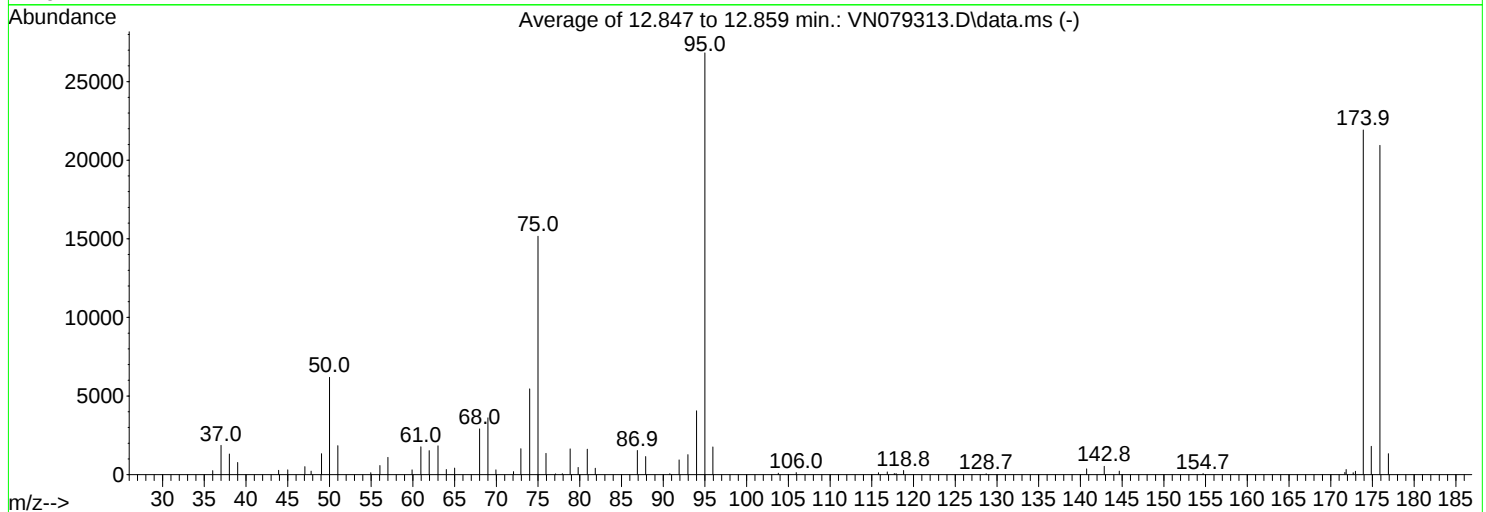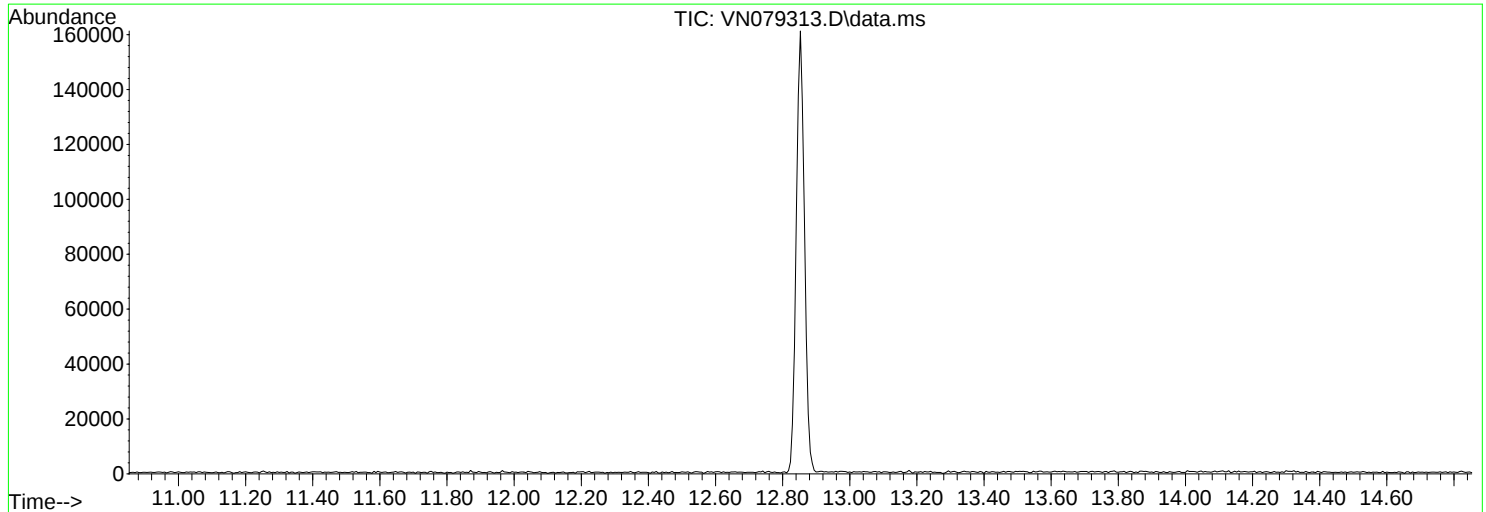

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	6193	PASS
75	95	30	60	56.5	15166	PASS
95	95	100	100	100.0	26829	PASS
96	95	5	9	6.6	1764	PASS
173	174	0.00	2	1.0	219	PASS
174	95	50	100	81.7	21925	PASS
175	174	5	9	8.2	1804	PASS
176	174	95	101	95.5	20949	PASS
177	176	5	9	6.3	1330	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	259	54.95	124	69.95	306	81.85	401
37.00	1859	56.05	578	72.05	196	86.90	153
38.00	1312	57.00	1100	72.95	1650	87.90	114
39.00	776	59.90	308	74.00	5459	90.80	6
43.90	273	60.95	1771	75.00	15166	91.90	938
45.00	304	61.95	1522	75.95	1355	92.95	1272
47.05	513	63.00	1832	77.10	54	94.00	4060
47.80	221	64.00	331	77.90	58	95.00	26829
49.05	1332	65.00	420	78.85	1634	95.95	1764
50.00	6193	68.00	2911	79.80	460	103.80	90
51.00	1839	69.00	3609	80.90	1618	105.95	128

Average of 12.847 to 12.859 min.: VN079313.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
115.80	118	171.85	325				
116.85	176	172.70	123				
117.70	68	172.95	219				
117.90	76	173.90	21925				
118.80	260	174.85	1804				
128.70	63	175.90	20949				
140.75	370	176.90	1330				
142.85	532						
144.65	227						
154.70	75						
171.70	138						

Instrument :

MSVOA_N

ClientSampleId :

BFB