
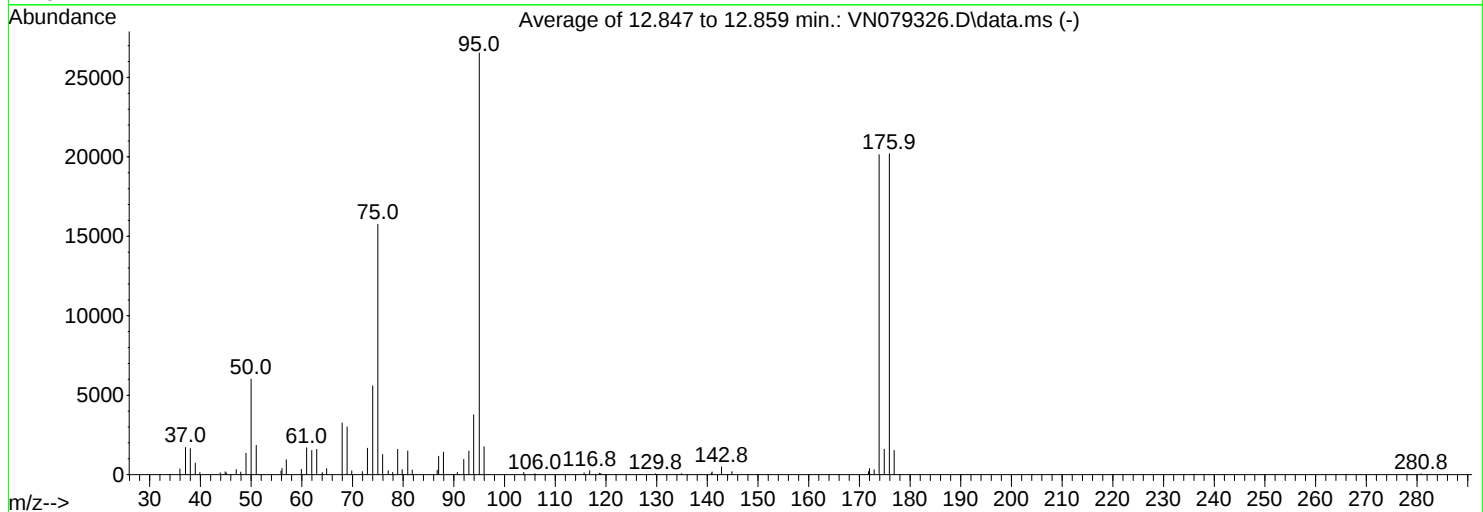


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092223\
 Data File : VN079326.D
 Acq On : 22 Sep 2023 08:23
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090723W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Sep 08 05:09:17 2023

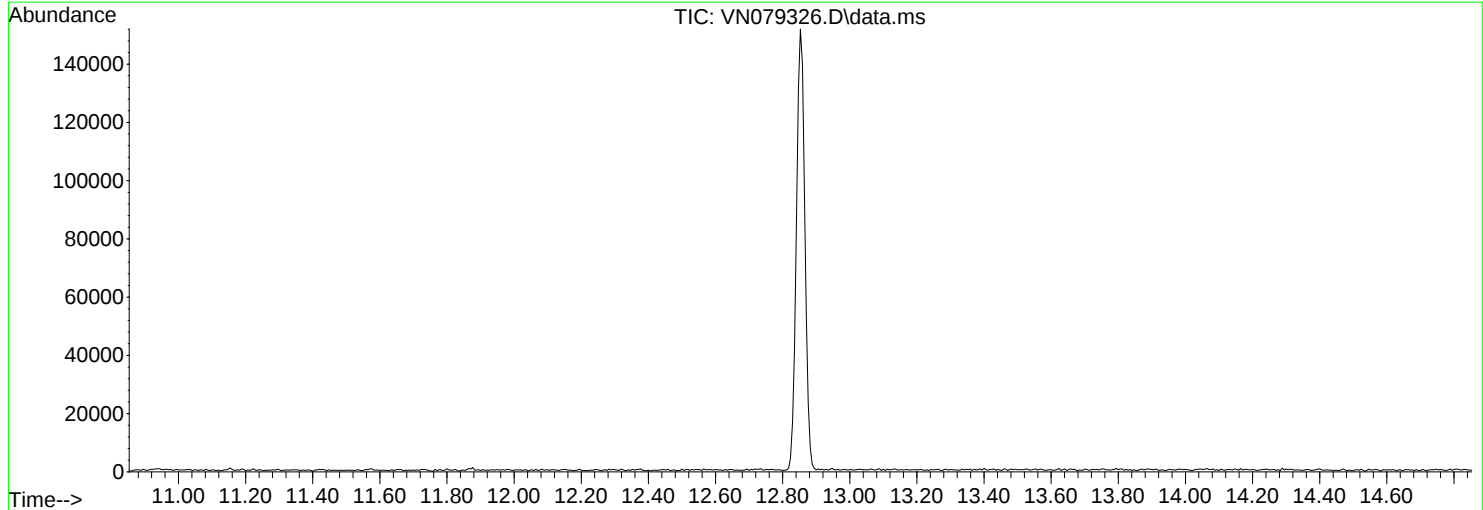

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	6015	PASS
75	95	30	60	59.4	15756	PASS
95	95	100	100	100.0	26547	PASS
96	95	5	9	6.6	1751	PASS
173	174	0.00	2	1.5	310	PASS
174	95	50	100	75.9	20144	PASS
175	174	5	9	7.9	1597	PASS
176	174	95	101	100.3	20200	PASS
177	176	5	9	7.5	1522	PASS