
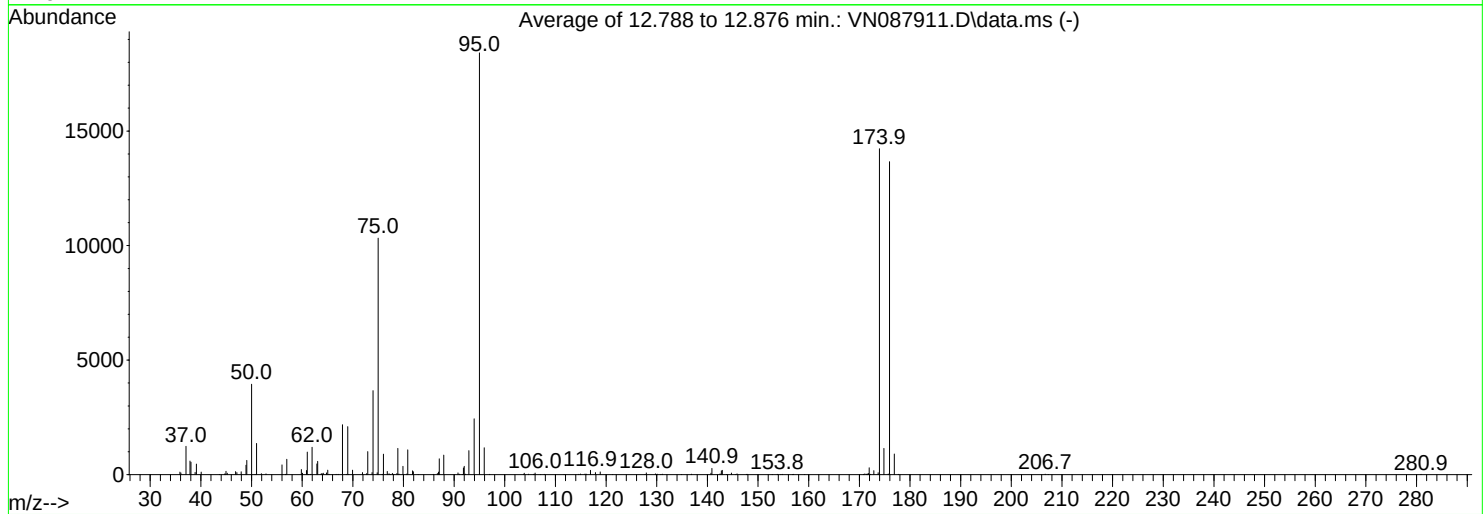


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN092225\  
Data File : VN087911.D  
Acq On : 22 Sep 2025 09:54  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N090425W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Fri Sep 05 03:29:53 2025

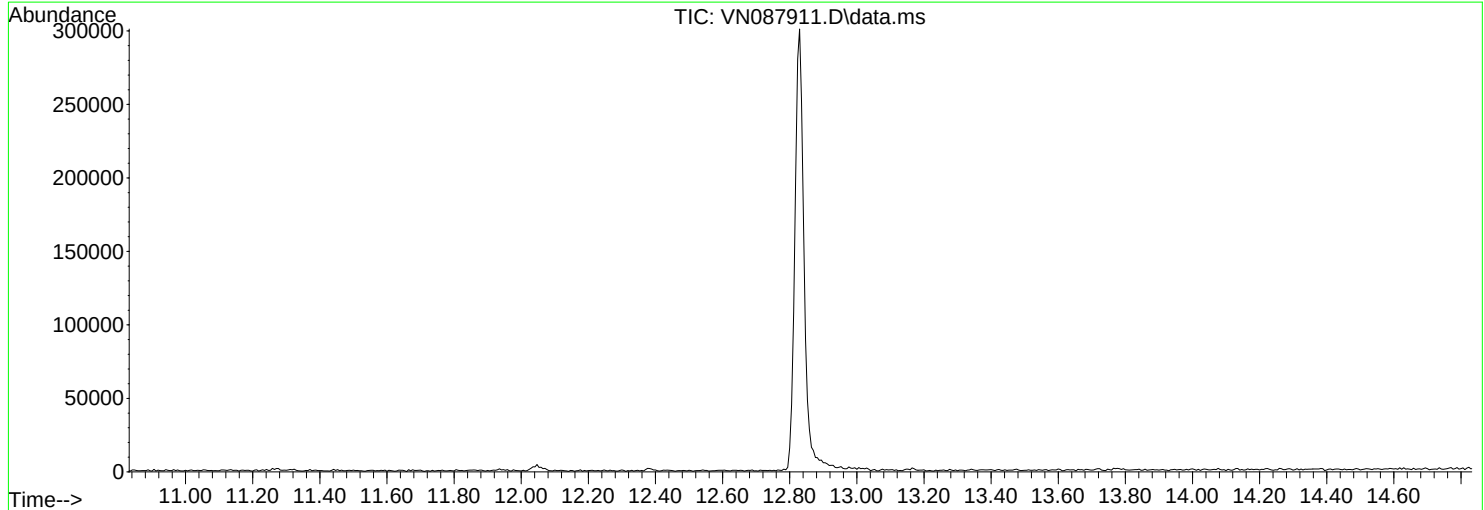

AutoFind: Averaged scan 1842 to 1857; Bkg corrected with scan 1841

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 21.4  | 3949  | PASS      |
| 75     | 95      | 30     | 60     | 56.1  | 10326 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 18413 | PASS      |
| 96     | 95      | 5      | 9      | 6.4   | 1176  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.3   | 178   | PASS      |
| 174    | 95      | 50     | 100    | 77.3  | 14225 | PASS      |
| 175    | 174     | 5      | 9      | 8.1   | 1149  | PASS      |
| 176    | 174     | 95     | 101    | 96.0  | 13663 | PASS      |
| 177    | 176     | 5      | 9      | 6.6   | 903   | PASS      |