

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN092318\
 Data File : VN051422.D
 Acq On : 23 Sep 2018 18:53
 Operator : MD\SY
 Sample : J5023-08
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 NB-PIT-2

Quant Time: Sep 24 06:48:10 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092318W.M
 Quant Title : SW846 8260
 QLast Update : Mon Sep 24 06:41:32 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	649280	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1022284	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	845330	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	313525	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	449194	55.23	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.46%	
35) Dibromofluoromethane	7.59	113	394768	48.29	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.58%	
50) Toluene-d8	10.09	98	1403130	45.58	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.16%	
62) 4-Bromofluorobenzene	12.40	95	387101	38.87	ug/l	0.00
Spiked Amount 50.000			Recovery	=	77.74%	
Target Compounds						
					Qvalue	
5) Bromomethane	2.57	94	1330	0.267	ug/l	90
8) Diethyl Ether	3.41	74	530	Below Cal		60
11) Tert butyl alcohol	4.78	59	201	0.438	ug/l #	78
13) Acrolein	3.60	56	282	0.619	ug/l #	59
14) Allyl chloride	4.55	41	8783	0.725	ug/l #	26
16) Acetone	3.82	43	49271	3.543	ug/l	98
17) Carbon Disulfide	4.06	76	4729	0.223	ug/l #	76
18) Methyl Acetate	4.33	43	16824	2.716	ug/l	97
20) Methylene Chloride	4.55	84	224138	27.849	ug/l	99
25) 2-Butanone	6.85	43	8503	3.054	ug/l	98
28) Bromochloromethane	7.37	49	1553	0.241	ug/l #	12
29) Tetrahydrofuran	7.21	42	602	0.341	ug/l #	34
30) Chloroform	7.37	83	19622	1.417	ug/l	96
31) Cyclohexane	7.67	56	12033	0.940	ug/l #	1
36) 1,1-Dichloropropene	7.67	75	45839	3.872	ug/l #	48
38) Carbon Tetrachloride	7.67	117	59113	4.774	ug/l #	17
43) Isopropyl Acetate	8.17	43	257431	20.916	ug/l	94
47) Bromodichloromethane	9.40	83	5004	0.424	ug/l #	90
48) Methyl methacrylate	9.18	41	6410	1.045	ug/l #	23
51) 4-Methyl-2-Pentanone	9.99	43	2342	0.346	ug/l	98
59) 2-Hexanone	10.76	43	8981	2.047	ug/l #	58
76) 1,2,3-Trichloropropane	12.40	75	190702	36.640	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.40	75	190702	112.666	ug/l #	12
95) Naphthalene	15.13	128	9480	8.727	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN092318\
Data File : VN051422.D
Acq On : 23 Sep 2018 18:53
Operator : MD\SY
Sample : J5023-08
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NB-PIT-2

Quant Time: Sep 24 06:48:10 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N092318W.M
Quant Title : SW846 8260
QLast Update : Mon Sep 24 06:41:32 2018
Response via : Initial Calibration

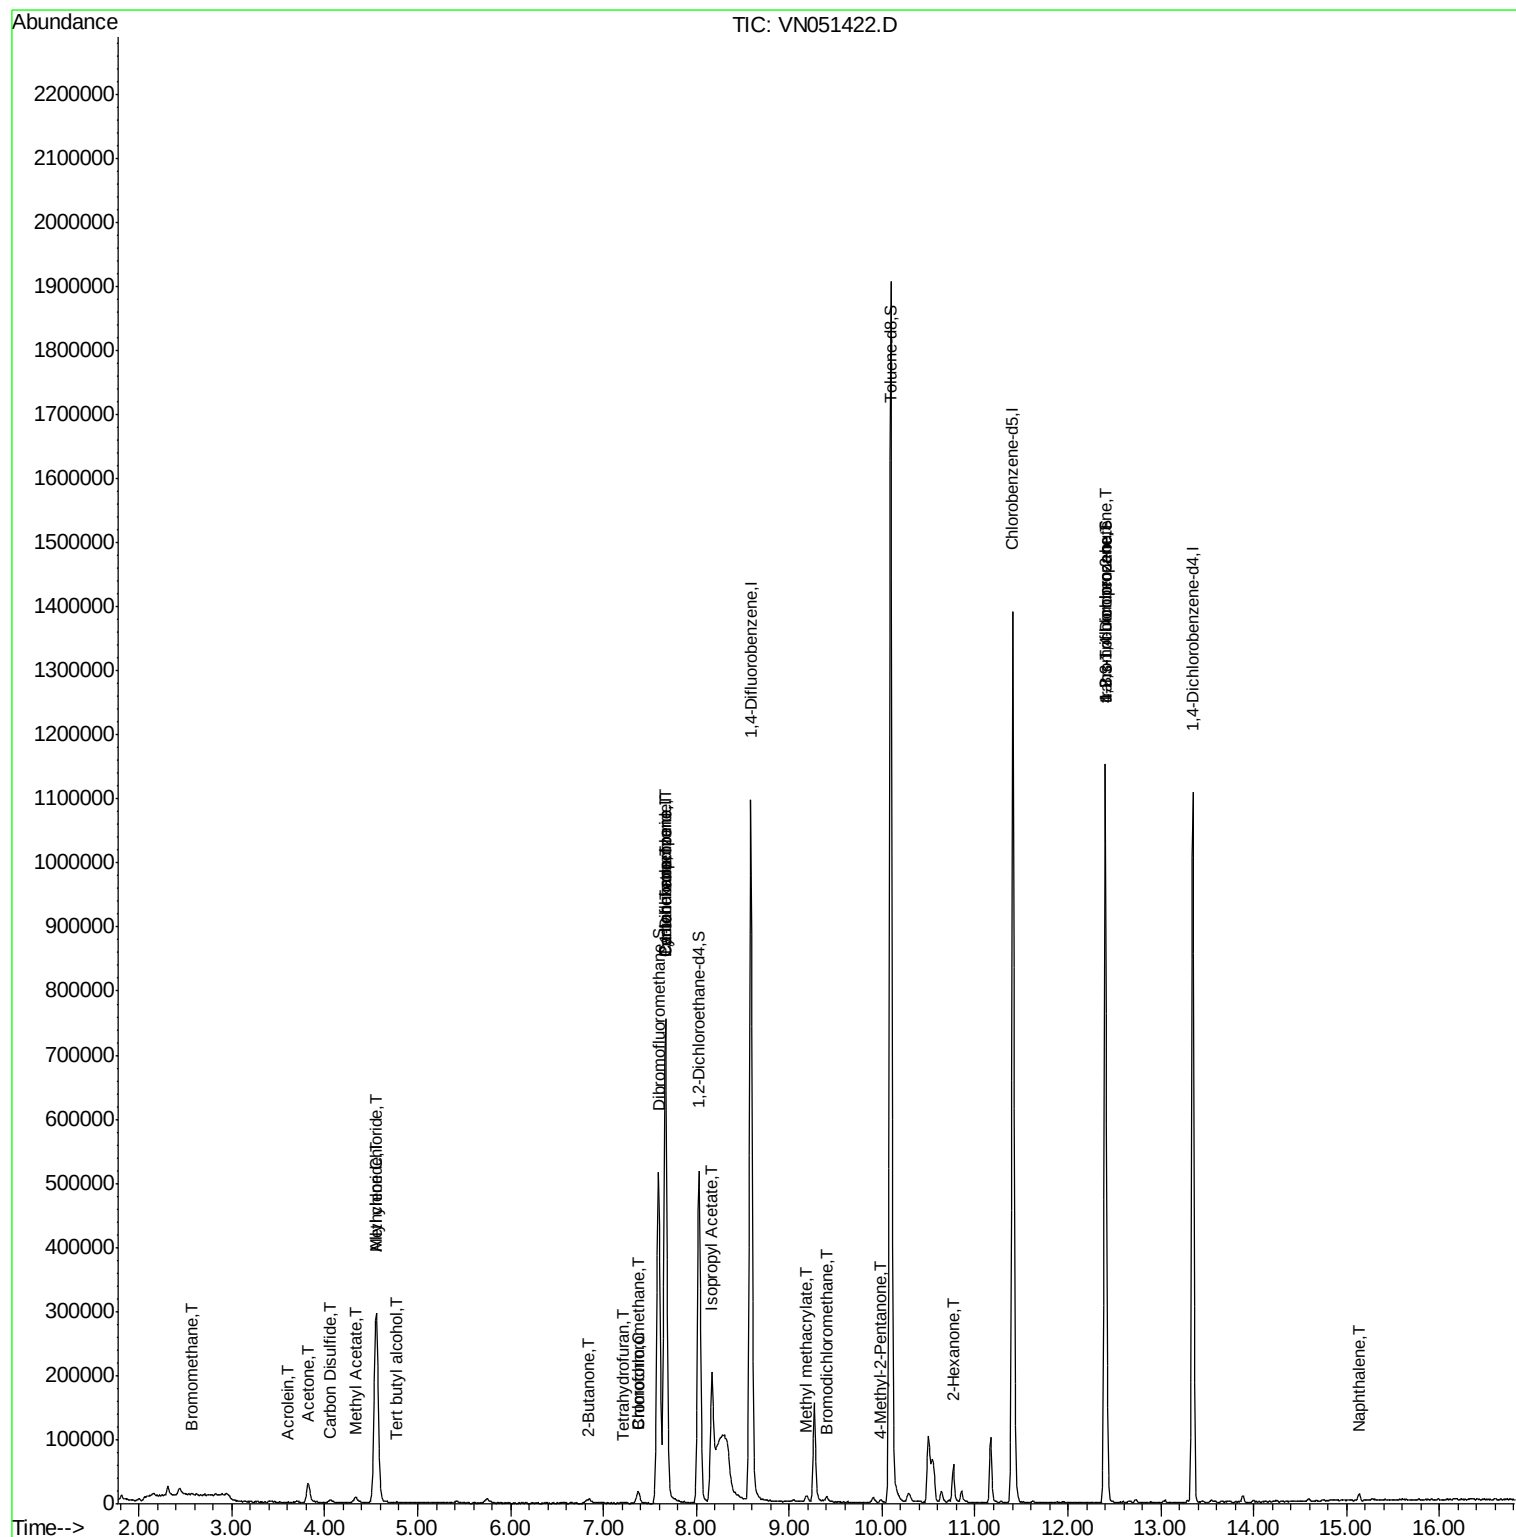

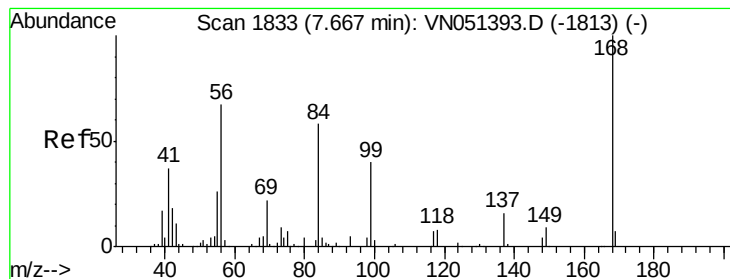

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :


NB-PIT-2

Tgt Ion:168 Resp: 649280

Ion Ratio Lower Upper

168 100

99 51.9 40.2 60.2



Abundance Ion 167.90 (167.60 to 168.60): VN051393.D (-1813) (-)

Ion 98.90 (98.60 to 99.60): VN051393.D (-1813) (-)

7.67

250000

200000



150000

100000

50000

0

Time-->

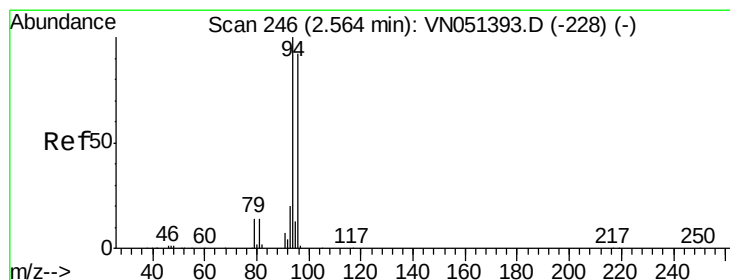

#5

Bromomethane

Concen: 0.267 ug/l

RT: 2.57 min Scan# 248

Delta R.T. 0.01 min

Lab File: VN051422.D


Acq: 23 Sep 2018 18:53

Tgt Ion: 94 Resp: 1330

Ion Ratio Lower Upper

94 100

96 82.5 73.6 110.4



Abundance Ion 93.90 (93.60 to 94.60): VN051393.D (-228) (-)

Ion 95.90 (95.60 to 96.60): VN051393.D (-228) (-)

2.57

800


600


400

200

0

Time-->





#8

Diethyl Ether

Concen: Below Cal

RT: 3.41 min Scan# 509

Delta R.T. -0.00 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :


NB-PIT-2

Tgt Ion: 74 Resp: 530

Ion Ratio Lower Upper


74 100

45 60.8 50.2 150.7


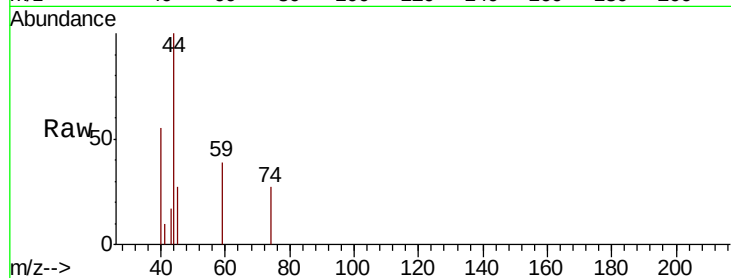


Abundance Ion 74.00 (73.70 to 74.70): VN0

Ion 45.00 (44.70 to 45.70): VN0

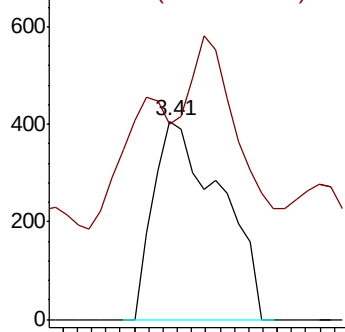

Time-->

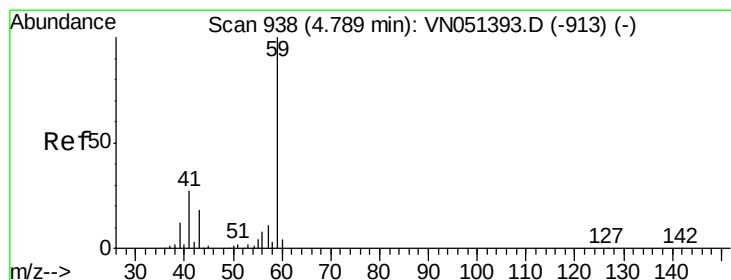

#11

Tert butyl alcohol

Concen: 0.438 ug/l

RT: 4.78 min Scan# 934

Delta R.T. -0.01 min

Lab File: VN051422.D


Acq: 23 Sep 2018 18:53

Tgt Ion: 59 Resp: 201

Ion Ratio Lower Upper


59 100

57 0.0 6.2 9.2#

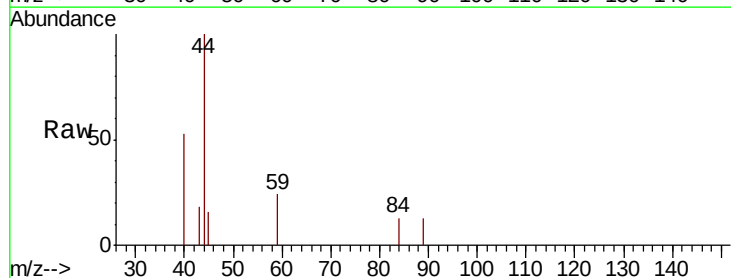



Abundance Ion 59.00 (58.70 to 59.70): VN0

Ion 57.00 (56.70 to 57.70): VN0

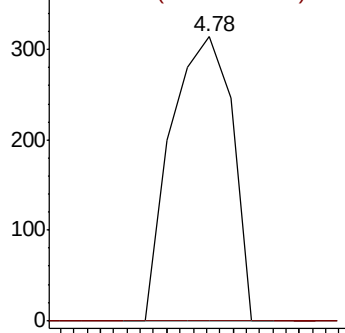

Time-->







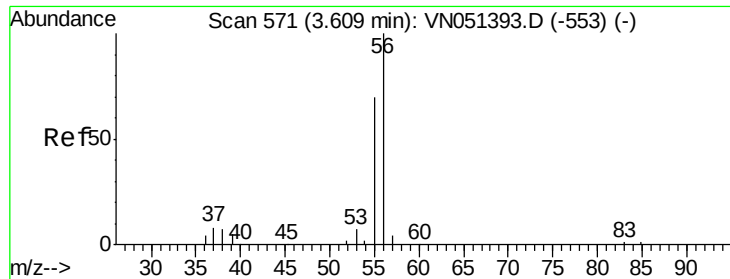

#13
 Acrolein
 Concen: 0.619 ug/l
 RT: 3.60 min Scan# 569
 Delta R.T. -0.01 min
 Lab File: VN051422.D
 Acq: 23 Sep 2018 18:53




Instrument :
 MSVOA_N
 ClientSampled :
 NB-PIT-2


Tgt Ion: 56 Resp: 282
 Ion Ratio Lower Upper
 56 100
 55 37.9 57.8 86.8#

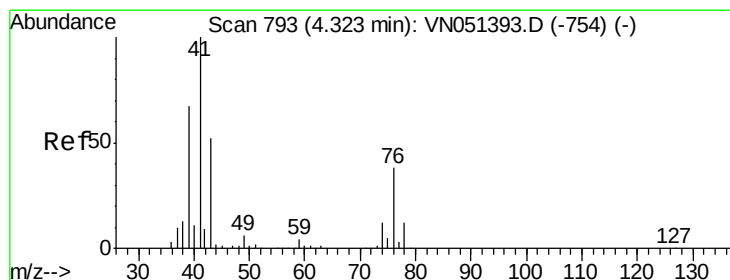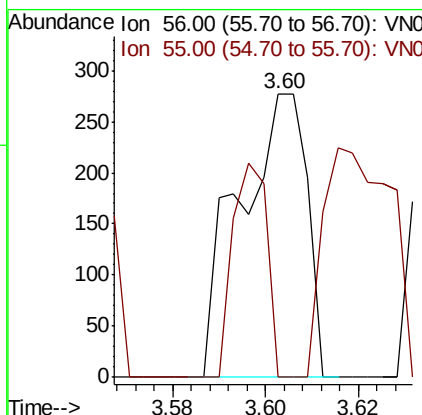

#14
 Allyl chloride
 Concen: 0.725 ug/l
 RT: 4.55 min Scan# 865
 Delta R.T. 0.23 min
 Lab File: VN051422.D
 Acq: 23 Sep 2018 18:53

Tgt Ion: 41 Resp: 8783
 Ion Ratio Lower Upper
 41 100
 39 0.0 51.4 77.2#
 76 0.0 28.1 42.1#

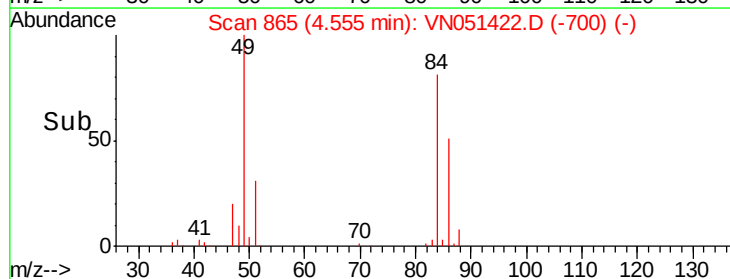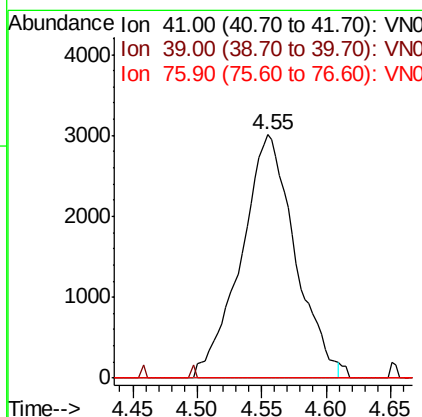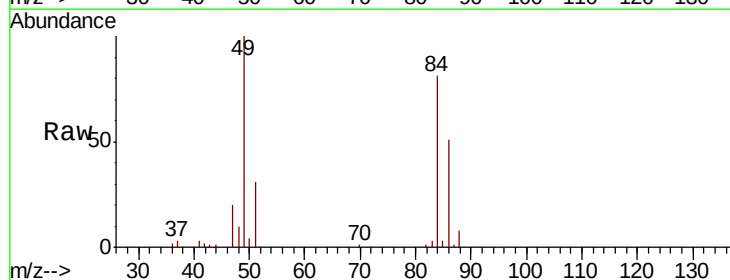

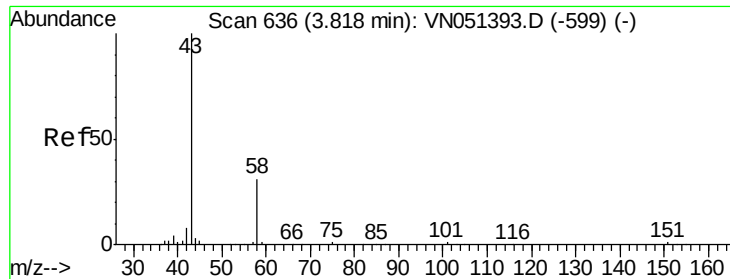

#16

Acetone

Concen: 3.543 ug/l

RT: 3.82 min Scan# 637

Delta R.T. 0.00 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53

Instrument :

MSVOA_N

ClientSampled :





NB-PIT-2

Tgt Ion: 43 Resp: 49271

Ion Ratio Lower Upper

43 100

58 32.1 25.0 37.4

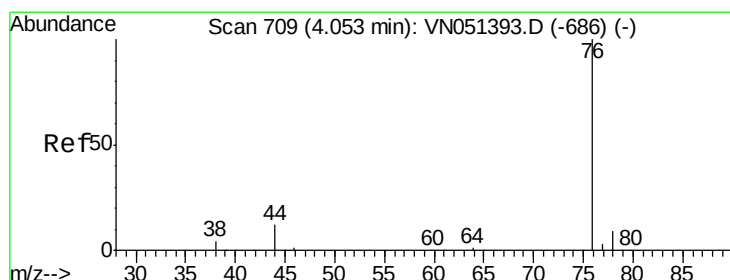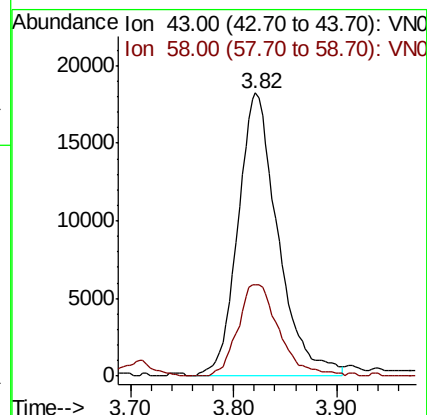

#17

Carbon Disulfide

Concen: 0.223 ug/l

RT: 4.06 min Scan# 711

Delta R.T. 0.01 min

Lab File: VN051422.D




Acq: 23 Sep 2018 18:53


Tgt Ion: 76 Resp: 4729

Ion Ratio Lower Upper

76 100

78 17.9 7.3 10.9#


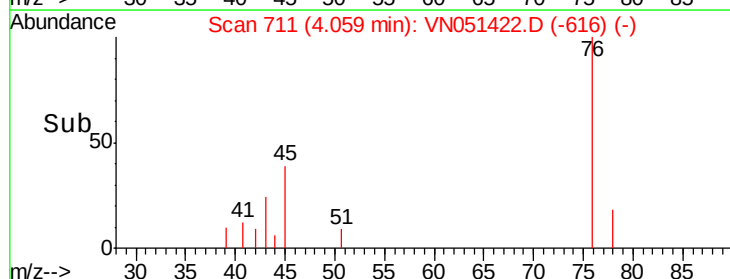
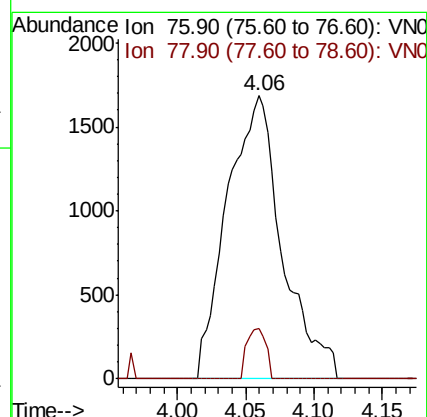
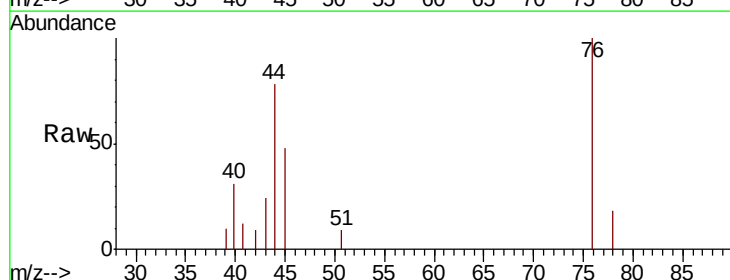




#18
Methyl Acetate
Concen: 2.716 ug/l
RT: 4.33 min Scan# 796
Delta R.T. 0.01 min
Lab File: VN051422.D
Acq: 23 Sep 2018 18:53




Instrument :
MSVOA_N
ClientSampleId :
NB-PIT-2


Tgt Ion: 43 Resp: 16824
Ion Ratio Lower Upper
43 100
74 22.2 18.8 28.2

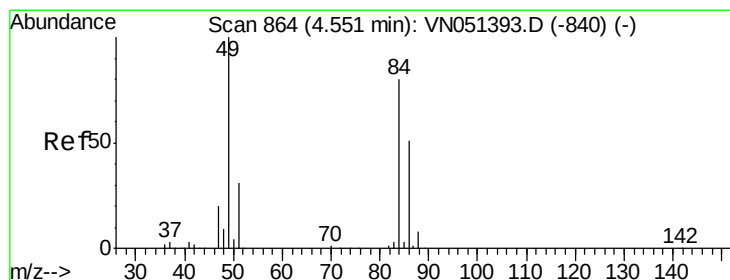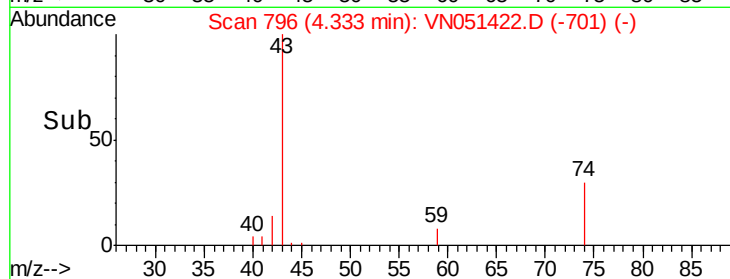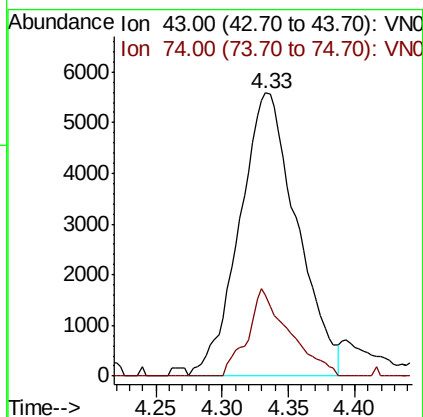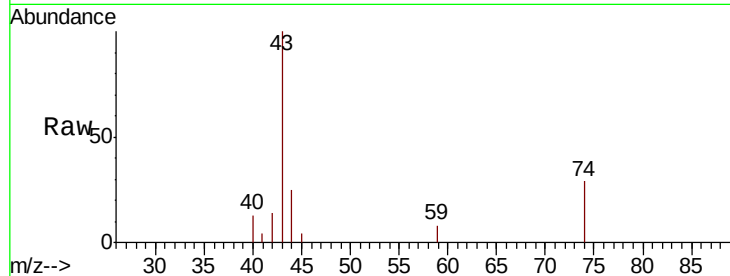

#20
Methylene Chloride
Concen: 27.849 ug/l
RT: 4.55 min Scan# 865
Delta R.T. 0.00 min
Lab File: VN051422.D
Acq: 23 Sep 2018 18:53

Tgt Ion: 84 Resp: 224138
Ion Ratio Lower Upper
84 100
49 124.1 99.9 149.9
51 38.5 31.4 47.2
86 63.7 50.9 76.3

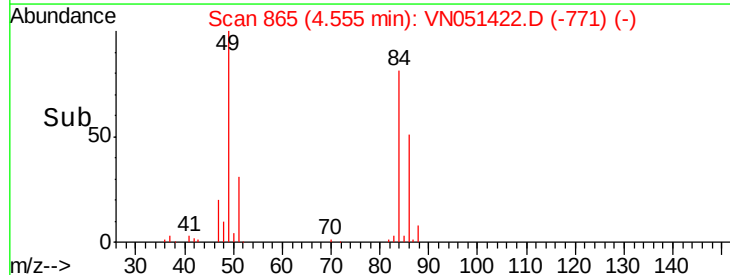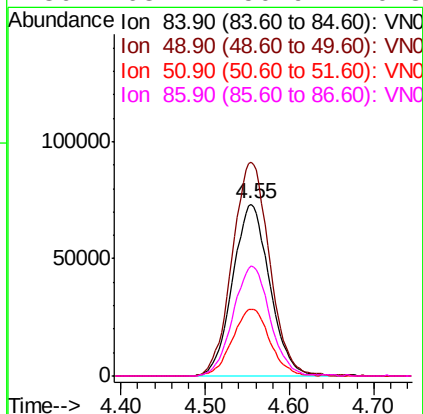

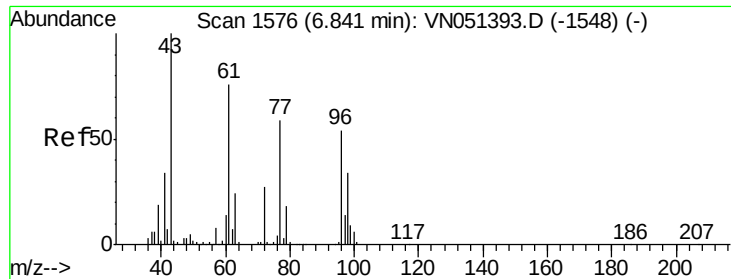

#25

2-Butanone

Concen: 3.054 ug/l

RT: 6.85 min Scan# 1578

Delta R.T. 0.01 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53

Instrument :

MSVOA_N

ClientSampled :


NB-PIT-2

Tgt Ion: 43 Resp: 8503

Ion Ratio Lower Upper




43 100

72 28.2 21.8 32.6

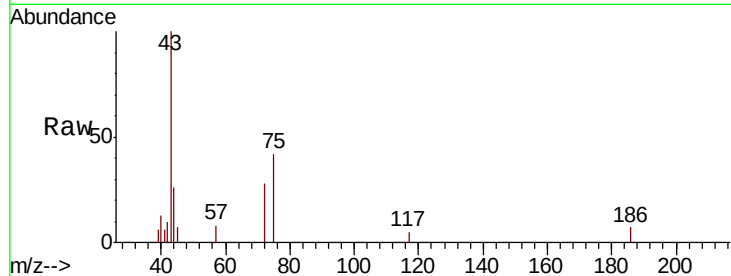

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

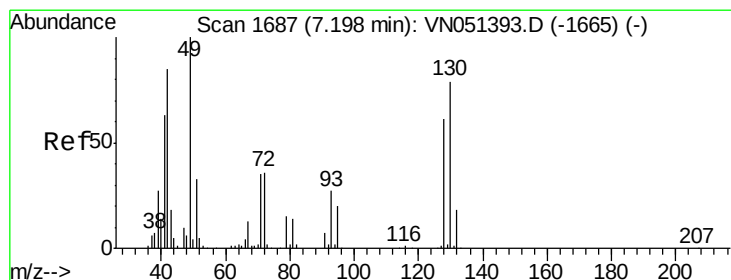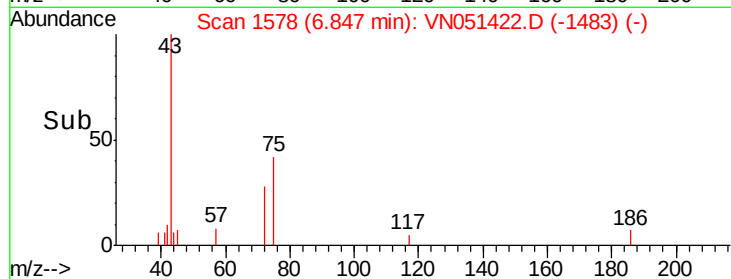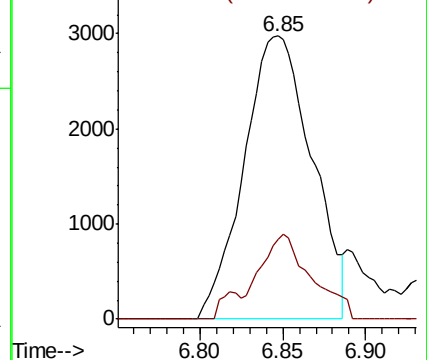

#28

Bromochloromethane

Concen: 0.241 ug/l

RT: 7.37 min Scan# 1742

Delta R.T. 0.18 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53


Tgt Ion: 49 Resp: 1553

Ion Ratio Lower Upper

49 100

129 0.0 0.0 3.8



130 0.0 63.0 94.4#

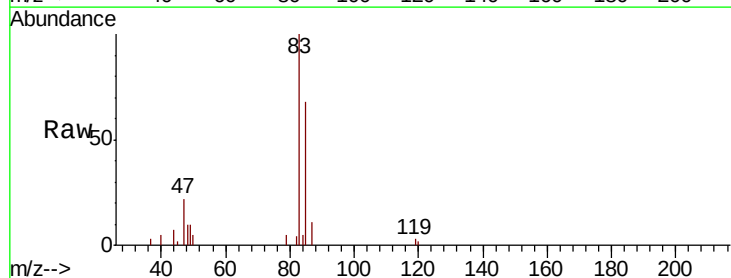


Abundance Ion 48.90 (48.60 to 49.60): VN0

Ion 128.80 (128.50 to 129.50): V

Ion 129.80 (129.50 to 130.50): V

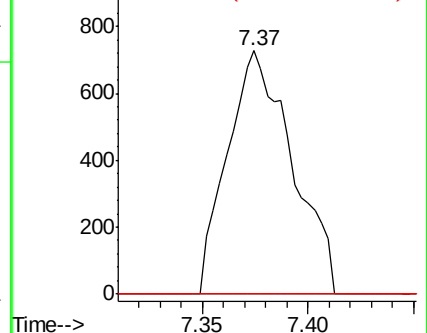







#29
Tetrahydrofuran
Concen: 0.341 ug/l
RT: 7.21 min Scan# 1692
Delta R.T. -0.00 min
Lab File: VN051422.D
Acq: 23 Sep 2018 18:53

Instrument :
MSVOA_N
ClientSampled :
NB-PIT-2

Tgt Ion: 42 Resp: 602
Ion Ratio Lower Upper
42 100
72 0.0 34.3 51.5#
71 0.0 32.2 48.4#

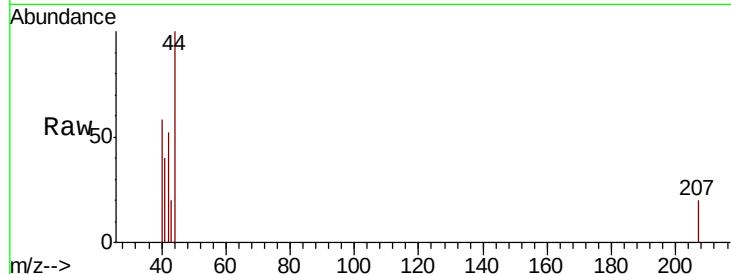


Abundance Ion 42.00 (41.70 to 42.70): VN0
Ion 72.00 (71.70 to 72.70): VN0
Ion 71.00 (70.70 to 71.70): VN0

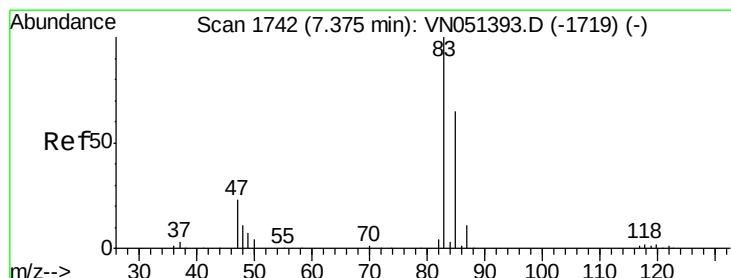
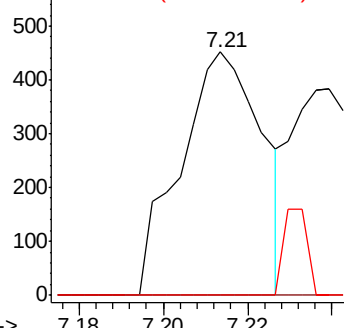



#30
Chloroform
Concen: 1.417 ug/l
RT: 7.37 min Scan# 1742
Delta R.T. -0.00 min
Lab File: VN051422.D
Acq: 23 Sep 2018 18:53

Tgt Ion: 83 Resp: 19622
Ion Ratio Lower Upper
83 100
85 67.9 51.8 77.6

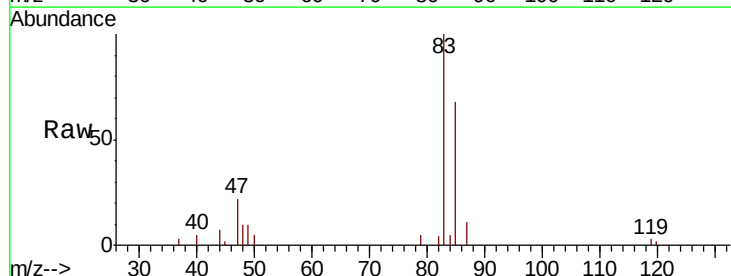

Abundance Ion 82.90 (82.60 to 83.60): VN0
Ion 84.90 (84.60 to 85.60): VN0

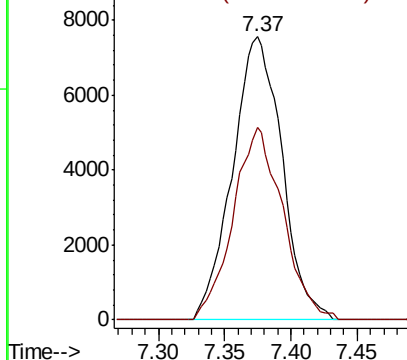

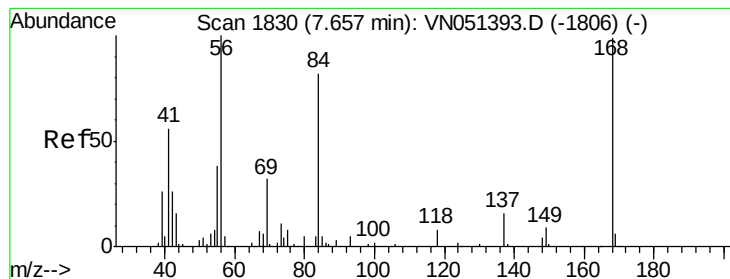

#31

Cyclohexane

Concen: 0.940 ug/l

RT: 7.67 min Scan# 1834

Delta R.T. 0.01 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :

NB-PIT-2


Tgt Ion: 56 Resp: 12033

Ion Ratio Lower Upper

56 100

69 159.1 25.8 38.6#




84 138.2 66.0 99.0#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

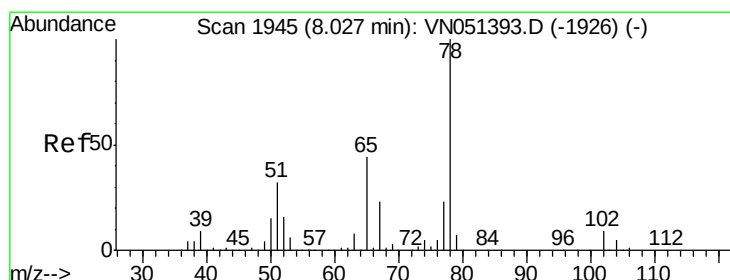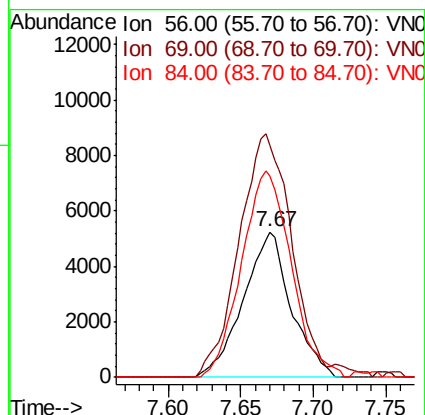

#33

1,2-Dichloroethane-d4

Concen: 55.228 ug/l

RT: 8.03 min Scan# 1946

Delta R.T. 0.00 min

Lab File: VN051422.D


Acq: 23 Sep 2018 18:53

Tgt Ion: 65 Resp: 449194

Ion Ratio Lower Upper



65 100


67 53.0 0.0 107.8



Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

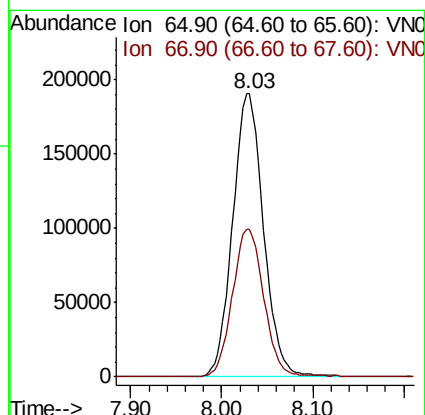

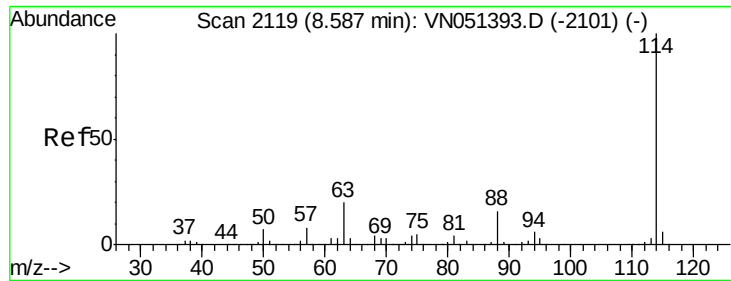

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. -0.00 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :

NB-PIT-2


Tgt Ion:114 Resp: 1022284

Ion Ratio Lower Upper

114 100

63 20.2 0.0 40.2




88 15.7 0.0 31.4

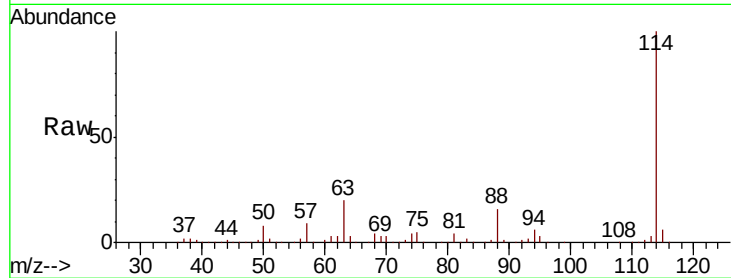

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

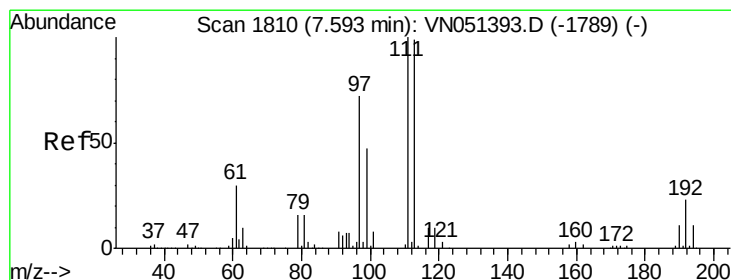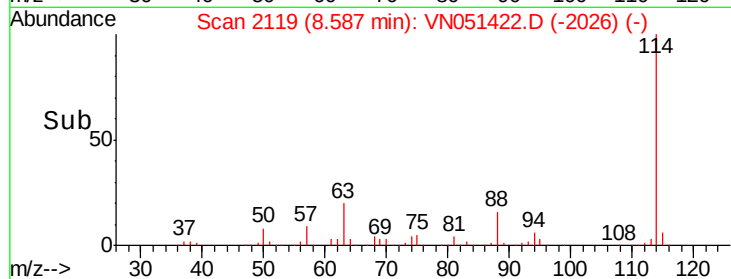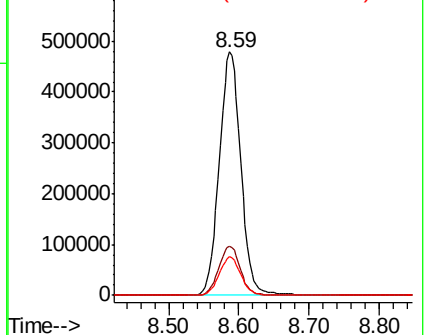

#35

Dibromofluoromethane

Concen: 48.291 ug/l

RT: 7.59 min Scan# 1810

Delta R.T. -0.00 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53


Tgt Ion:113 Resp: 394768

Ion Ratio Lower Upper

113 100

111 101.6 82.6 123.8



192 22.5 18.0 27.0

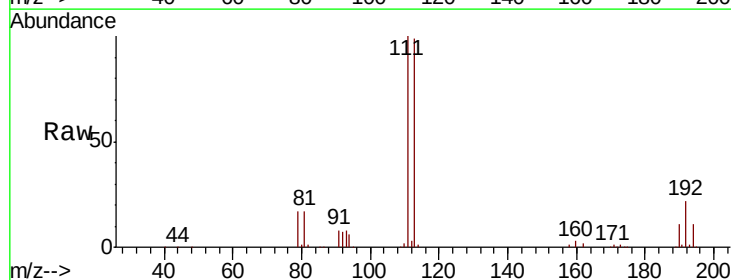


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



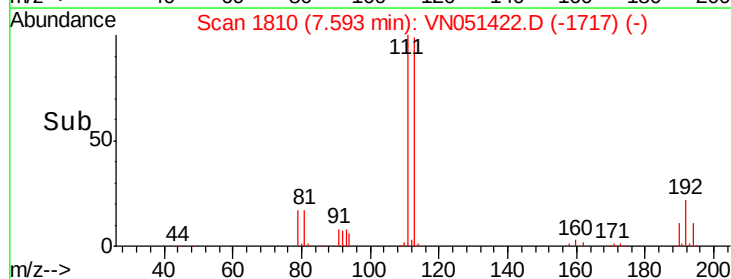
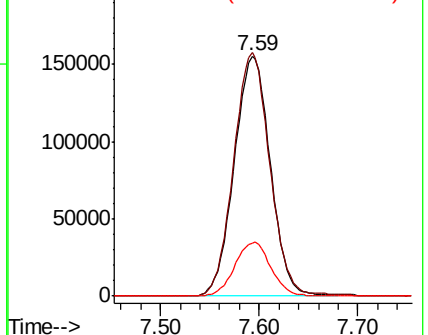


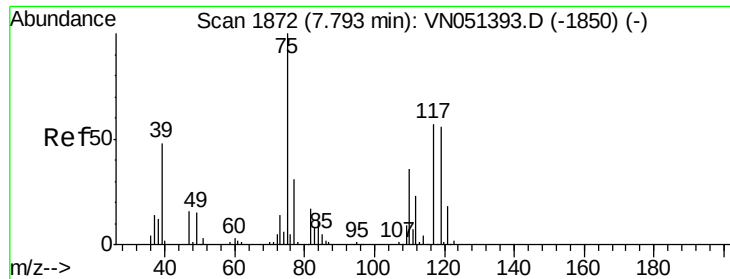

#36
 1,1-Dichloropropene
 Concen: 3.872 ug/l
 RT: 7.67 min Scan# 1833
 Delta R.T. -0.13 min
 Lab File: VN051422.D
 Acq: 23 Sep 2018 18:53




Instrument :
 MSVOA_N
 ClientSampled :
 NB-PIT-2


Tgt Ion: 75 Resp: 45839
 Ion Ratio Lower Upper
 75 100
 110 8.9 18.1 54.3#
 77 0.0 25.6 38.4#

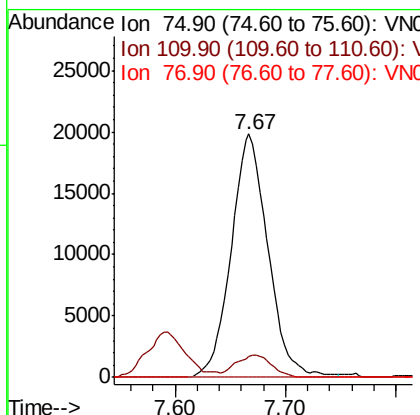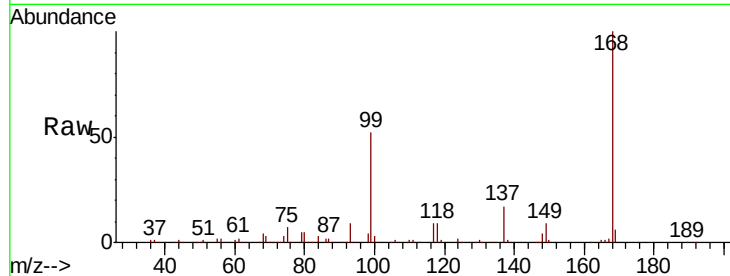

#38
 Carbon Tetrachloride
 Concen: 4.774 ug/l
 RT: 7.67 min Scan# 1833
 Delta R.T. -0.11 min
 Lab File: VN051422.D
 Acq: 23 Sep 2018 18:53

Tgt Ion: 117 Resp: 59113
 Ion Ratio Lower Upper
 117 100
 119 6.3 76.9 115.3#
 121 0.0 24.6 37.0#

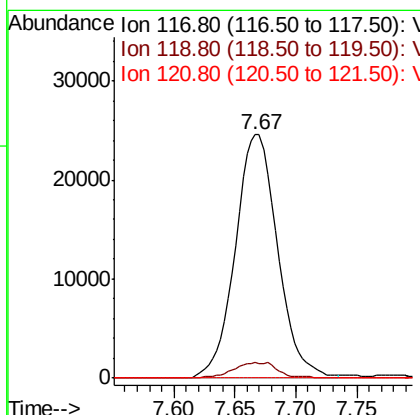



#43

Isopropyl Acetate

Concen: 20.916 ug/l

RT: 8.17 min Scan# 1989

Delta R.T. 0.00 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :

NB-PIT-2


Tgt Ion: 43 Resp: 257431

Ion Ratio Lower Upper

43 100

61 17.9 16.8 25.2




87 11.4 10.7 16.1

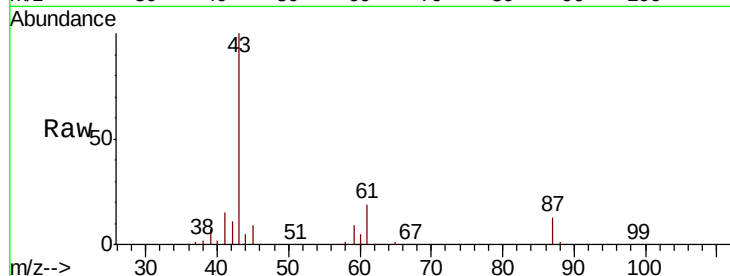

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

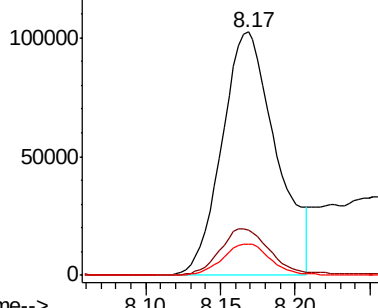

#47

Bromodichloromethane

Concen: 0.424 ug/l

RT: 9.40 min Scan# 2372

Delta R.T. -0.00 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53


Tgt Ion: 83 Resp: 5004

Ion Ratio Lower Upper

83 100

85 56.3 51.8 77.6



127 6.8 7.4 11.2#




Abundance Ion 82.90 (82.60 to 83.60): VN0

Ion 84.90 (84.60 to 85.60): VN0

Ion 126.80 (126.50 to 127.50): V

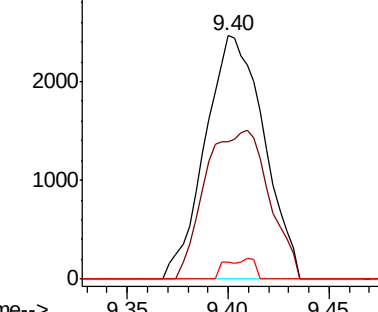


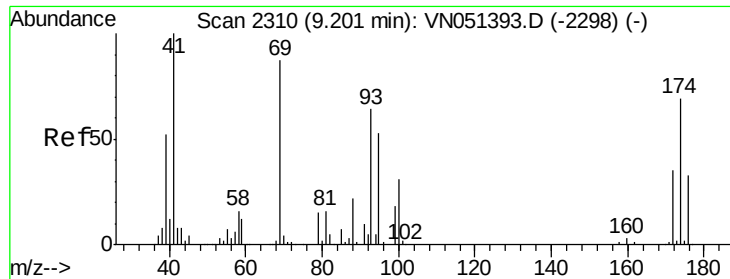




#48
Methyl methacrylate
Concen: 1.045 ug/l
RT: 9.18 min Scan# 2303
Delta R.T. -0.02 min
Lab File: VN051422.D
Acq: 23 Sep 2018 18:53

Instrument :
MSVOA_N
ClientSampled :
NB-PIT-2

Tgt Ion: 41 Resp: 6410
Ion Ratio Lower Upper
41 100
69 0.0 70.4 105.6#
39 18.8 43.8 65.8#




Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 39.00 (38.70 to 39.70): VN0


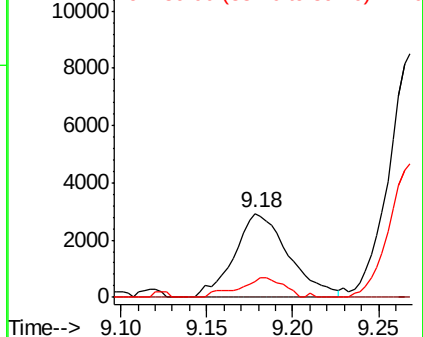



#50
Toluene-d8
Concen: 45.581 ug/l
RT: 10.09 min Scan# 2587
Delta R.T. -0.00 min
Lab File: VN051422.D
Acq: 23 Sep 2018 18:53

Tgt Ion: 98 Resp: 1403130
Ion Ratio Lower Upper
98 100
100 63.6 50.6 75.8



Abundance Ion 98.00 (97.70 to 98.70): VN0
Ion 100.00 (99.70 to 100.70): VN0




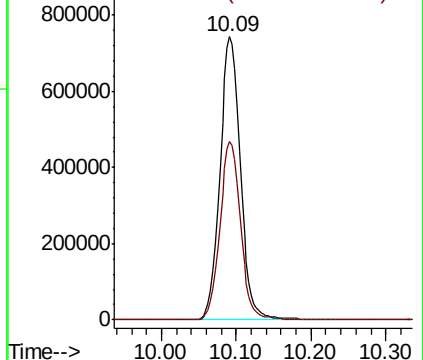




#51
 4-Methyl-2-Pentanone
 Concen: 0.346 ug/l
 RT: 9.99 min Scan# 2555
 Delta R.T. 0.00 min
 Lab File: VN051422.D
 Acq: 23 Sep 2018 18:53




Instrument :
 MSVOA_N
 ClientSampled :
 NB-PIT-2


Tgt Ion: 43 Resp: 2342
 Ion Ratio Lower Upper
 43 100
 58 40.8 31.5 47.3

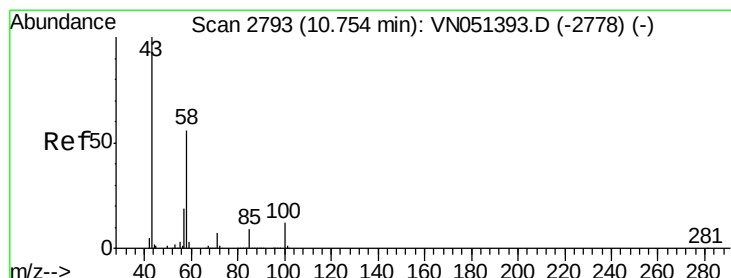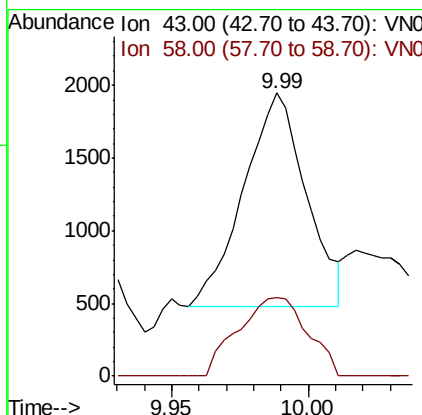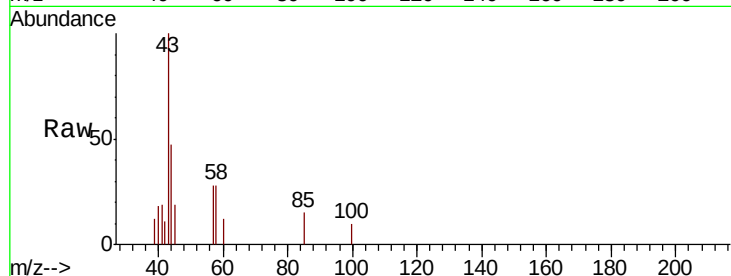

#59
 2-Hexanone
 Concen: 2.047 ug/l
 RT: 10.76 min Scan# 2795
 Delta R.T. 0.01 min
 Lab File: VN051422.D
 Acq: 23 Sep 2018 18:53

Tgt Ion: 43 Resp: 8981
 Ion Ratio Lower Upper
 43 100
 58 24.9 27.7 83.0#

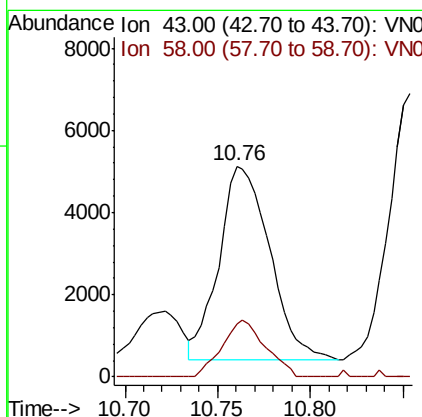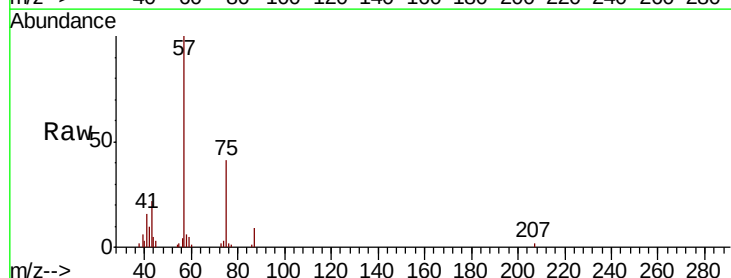



#62

4-Bromofluorobenzene

Concen: 38.872 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :

NB-PIT-2


Tgt Ion: 95 Resp: 387101

Ion Ratio Lower Upper

95 100

174 89.5 0.0 181.6




176 87.5 0.0 176.4

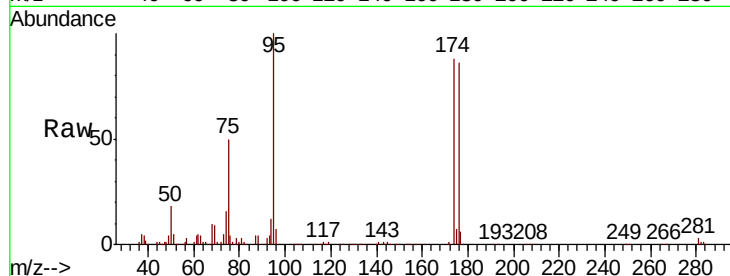

Abundance Ion 94.90 (94.60 to 95.60): VN051393.D (-3290) (-)

Ion 173.80 (173.50 to 174.50): VN051393.D (-3290) (-)

Ion 175.80 (175.50 to 176.50): VN051393.D (-3290) (-)

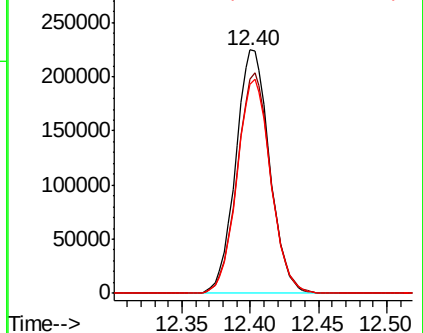

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. -0.00 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53


Tgt Ion: 117 Resp: 845330

Ion Ratio Lower Upper

117 100

82 55.1 44.2 66.2



119 32.4 25.9 38.9




Abundance Ion 116.90 (116.60 to 117.60): VN051393.D (-2981) (-)

Ion 82.00 (81.70 to 82.70): VN051393.D (-2981) (-)

Ion 118.90 (118.60 to 119.60): VN051393.D (-2981) (-)

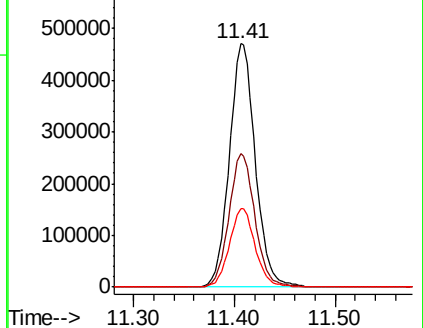

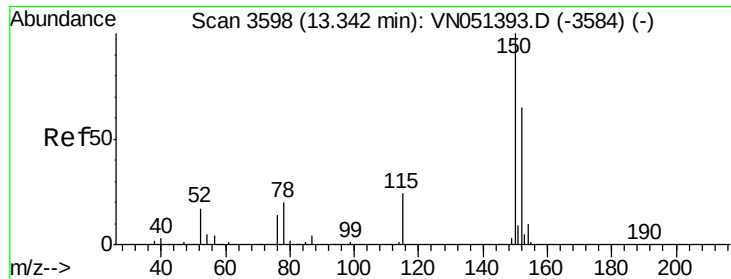

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3599

Delta R.T. 0.00 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :

NB-PIT-2


Tgt Ion:152 Resp: 313525

Ion Ratio Lower Upper

152 100

115 56.4 28.3 84.9




150 158.4 0.0 353.6

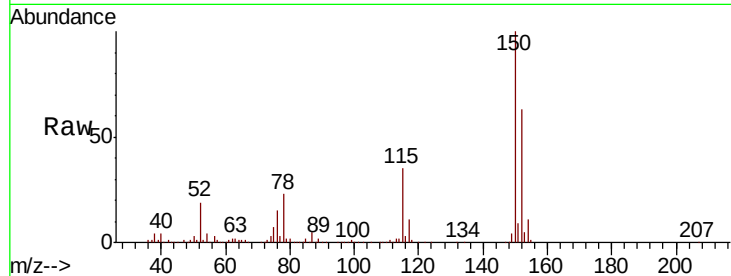

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

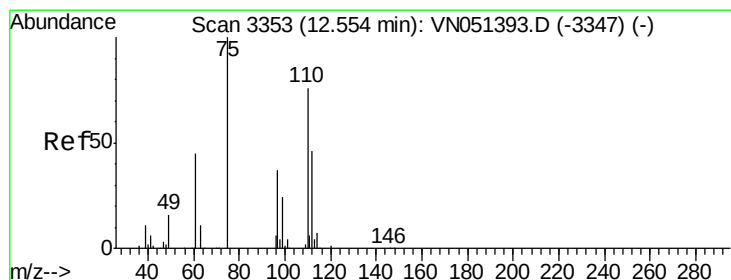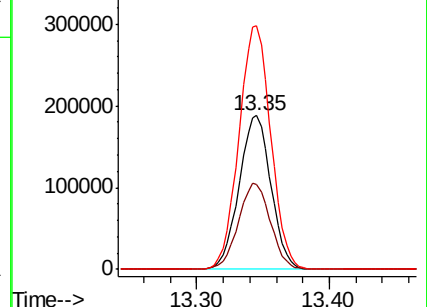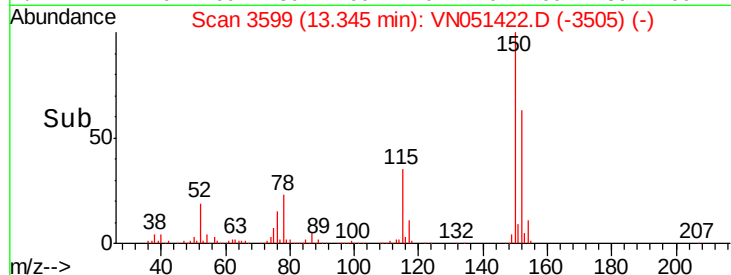

#76

1,2,3-Trichloropropane

Concen: 36.640 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. -0.15 min

Lab File: VN051422.D


Acq: 23 Sep 2018 18:53

Tgt Ion: 75 Resp: 190702

Ion Ratio Lower Upper



75 100


77 1.1 0.0 0.0#

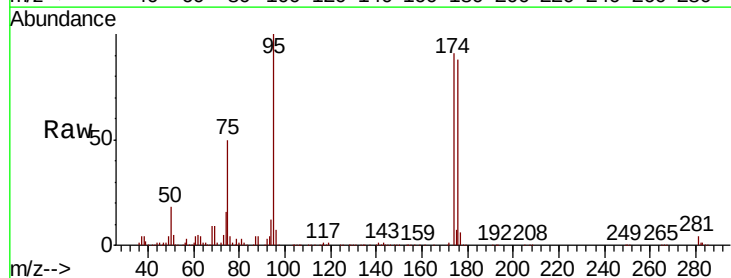

Abundance Ion 74.90 (74.60 to 75.60): V

Ion 77.00 (76.70 to 77.70): V

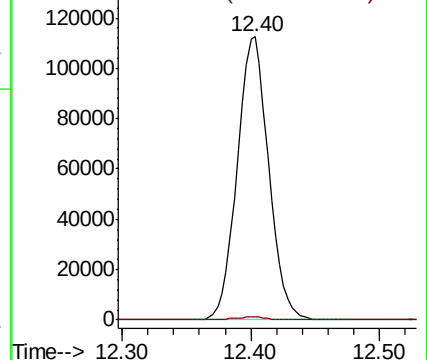



#81

trans-1,4-Dichloro-2-butene

Concen: 112.666 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.10 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53

Instrument :

MSVOA_N

ClientSampleId :

NB-PIT-2


Tgt Ion: 75 Resp: 190702

Ion Ratio Lower Upper

75 100

53 0.1 73.9 110.9#




89 0.1 36.7 55.1#

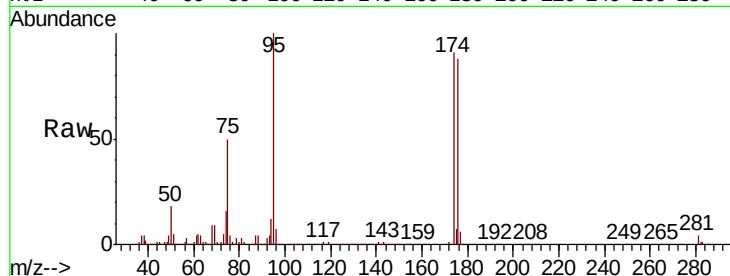

Abundance Ion 74.90 (74.60 to 75.60): VN051422.D (-3181) (-)

Ion 53.00 (52.70 to 53.70): VN051422.D (-3181) (-)

Ion 88.90 (88.60 to 89.60): VN051422.D (-3181) (-)

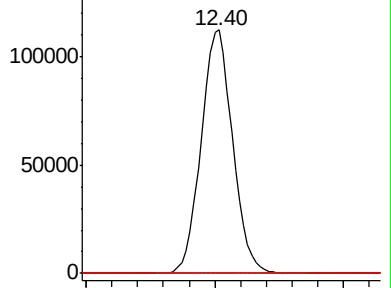

#95

Naphthalene

Concen: 8.727 ug/l

RT: 15.13 min Scan# 4155

Delta R.T. -0.00 min

Lab File: VN051422.D

Acq: 23 Sep 2018 18:53


Tgt Ion: 128 Resp: 9480

Ion Ratio Lower Upper

128 100

127 12.9 10.5 15.7

129 11.6 8.6 12.8



Abundance Ion 128.00 (127.70 to 128.70): VN051422.D (-4062) (-)

Ion 127.00 (126.70 to 127.70): VN051422.D (-4062) (-)

Ion 129.00 (128.70 to 129.70): VN051422.D (-4062) (-)

