


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN092318\
 Data File : VN051390.D
 Acq On : 22 Sep 2018 11:16
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092318W.M
 Title : SW846 8260
 Last Update : Mon Sep 24 06:41:32 2018

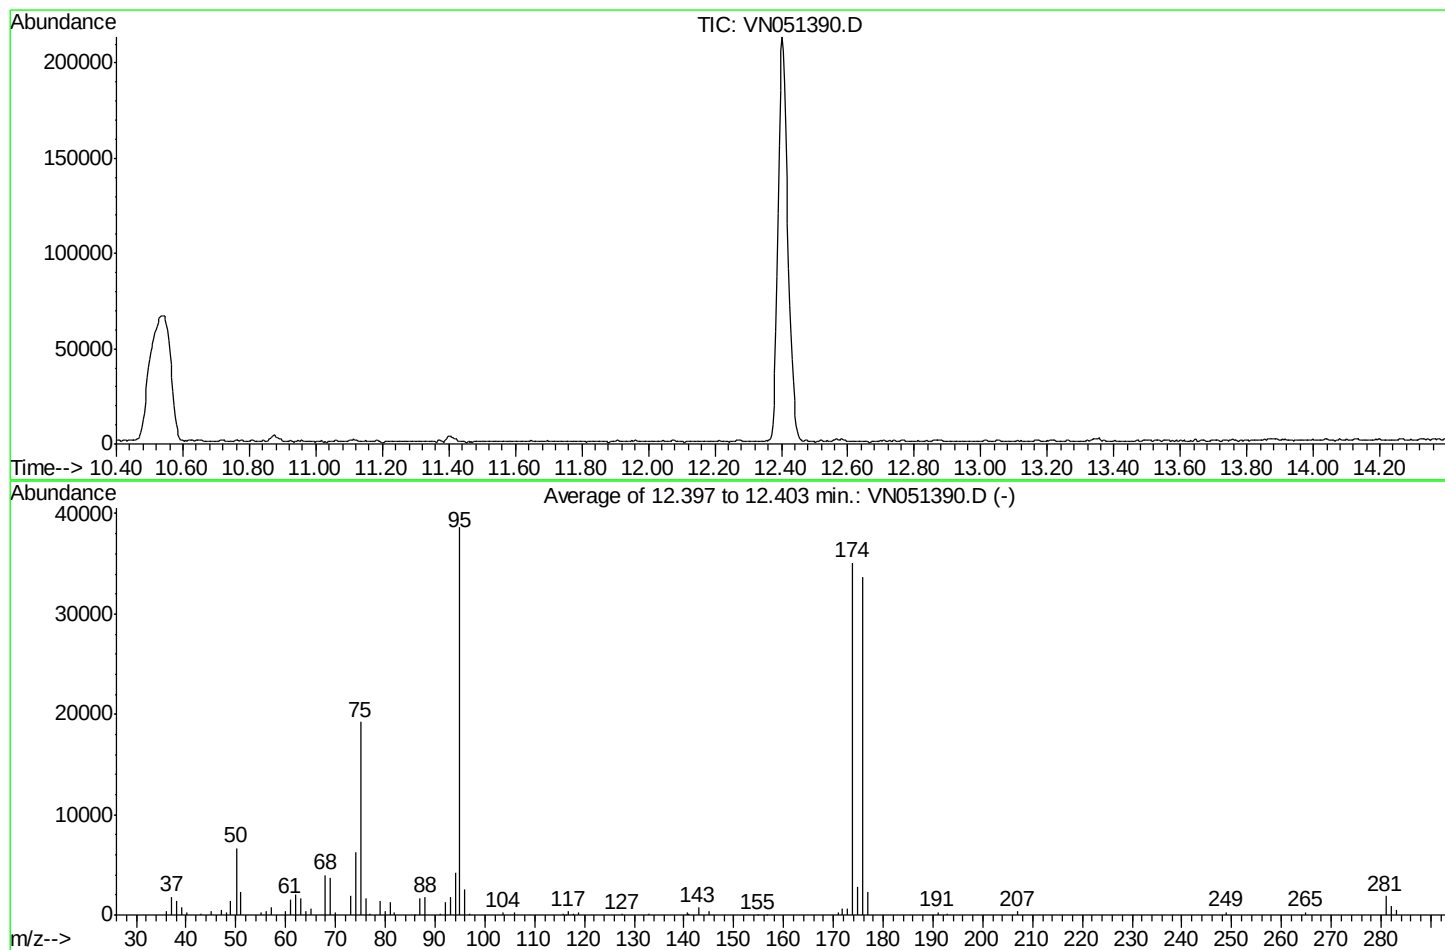

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	6682	PASS
75	95	30	60	49.8	19224	PASS
95	95	100	100	100.0	38637	PASS
96	95	5	9	6.5	2493	PASS
173	174	0.00	2	1.7	613	PASS
174	95	50	100	90.8	35096	PASS
175	174	5	9	8.2	2863	PASS
176	174	95	101	96.2	33746	PASS
177	176	5	9	6.8	2292	PASS