


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN092318\
Data File : VN051424.D
Acq On : 23 Sep 2018 20:06
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092318W.M
Title : SW846 8260
Last Update : Mon Sep 24 06:41:32 2018

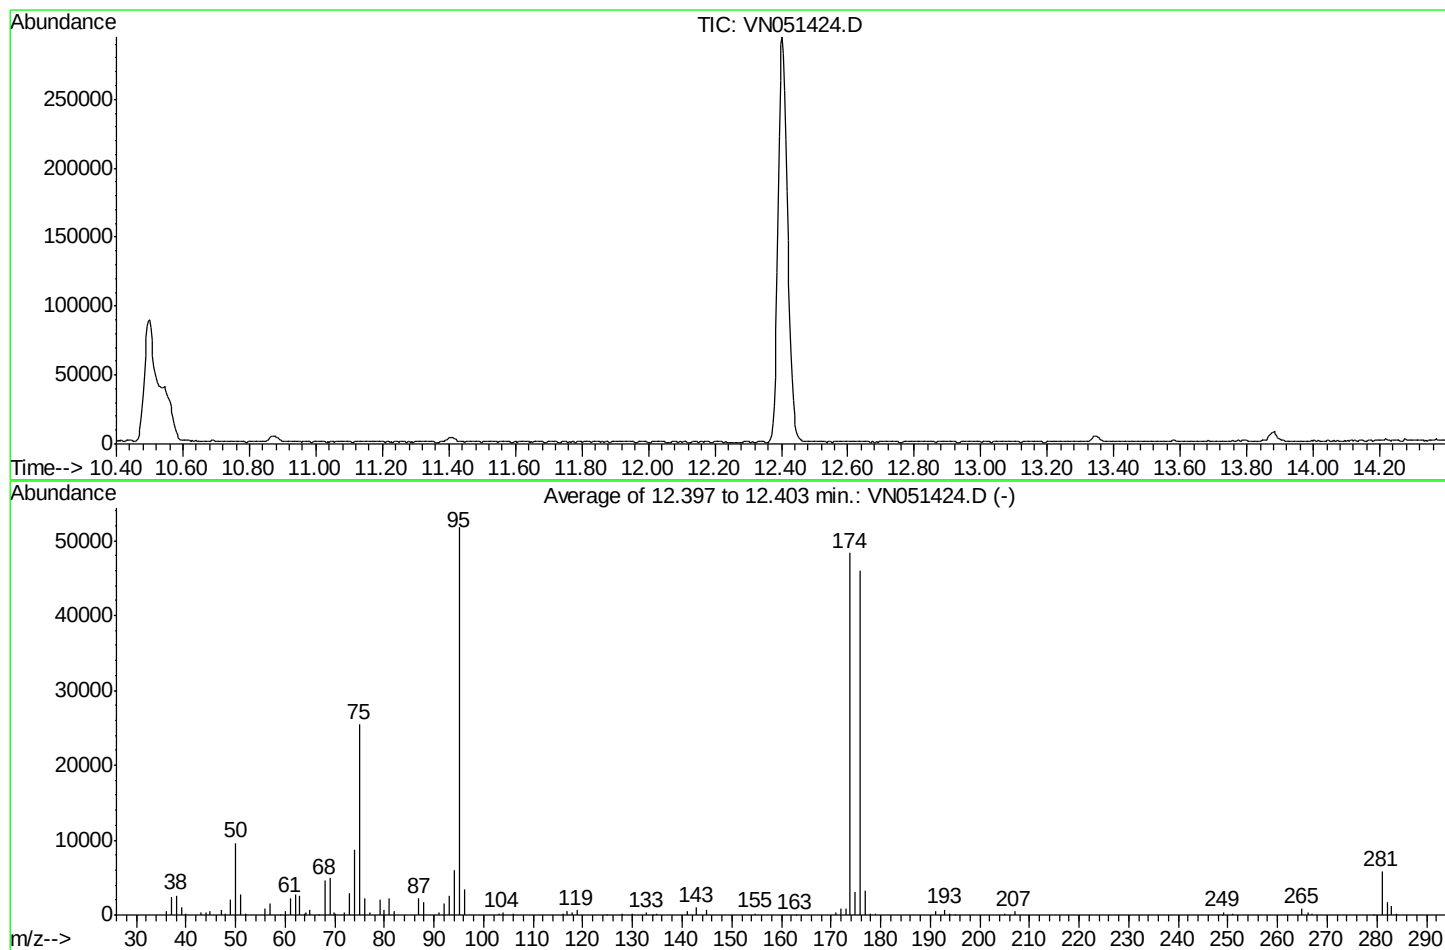

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	9581	PASS
75	95	30	60	49.1	25434	PASS
95	95	100	100	100.0	51784	PASS
96	95	5	9	6.8	3500	PASS
173	174	0.00	2	1.6	781	PASS
174	95	50	100	93.3	48336	PASS
175	174	5	9	6.5	3131	PASS
176	174	95	101	95.0	45925	PASS
177	176	5	9	7.2	3285	PASS