

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN092320\
 Data File : VN063617.D
 Acq On : 24 Sep 2020 3:40
 Operator : JC/MD
 Sample : PB131813ZHE#16
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB131813ZHE#16

Quant Time: Sep 24 05:04:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091620W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 16 13:05:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.62
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.55
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.38
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.32

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN092320\
Data File : VN063617.D
Acq On : 24 Sep 2020 3:40
Operator : JC/MD
Sample : PB131813ZHE#16
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB131813ZHE#16

Quant Time: Sep 24 05:04:44 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N091620W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 16 13:05:20 2020
Response via : Initial Calibration

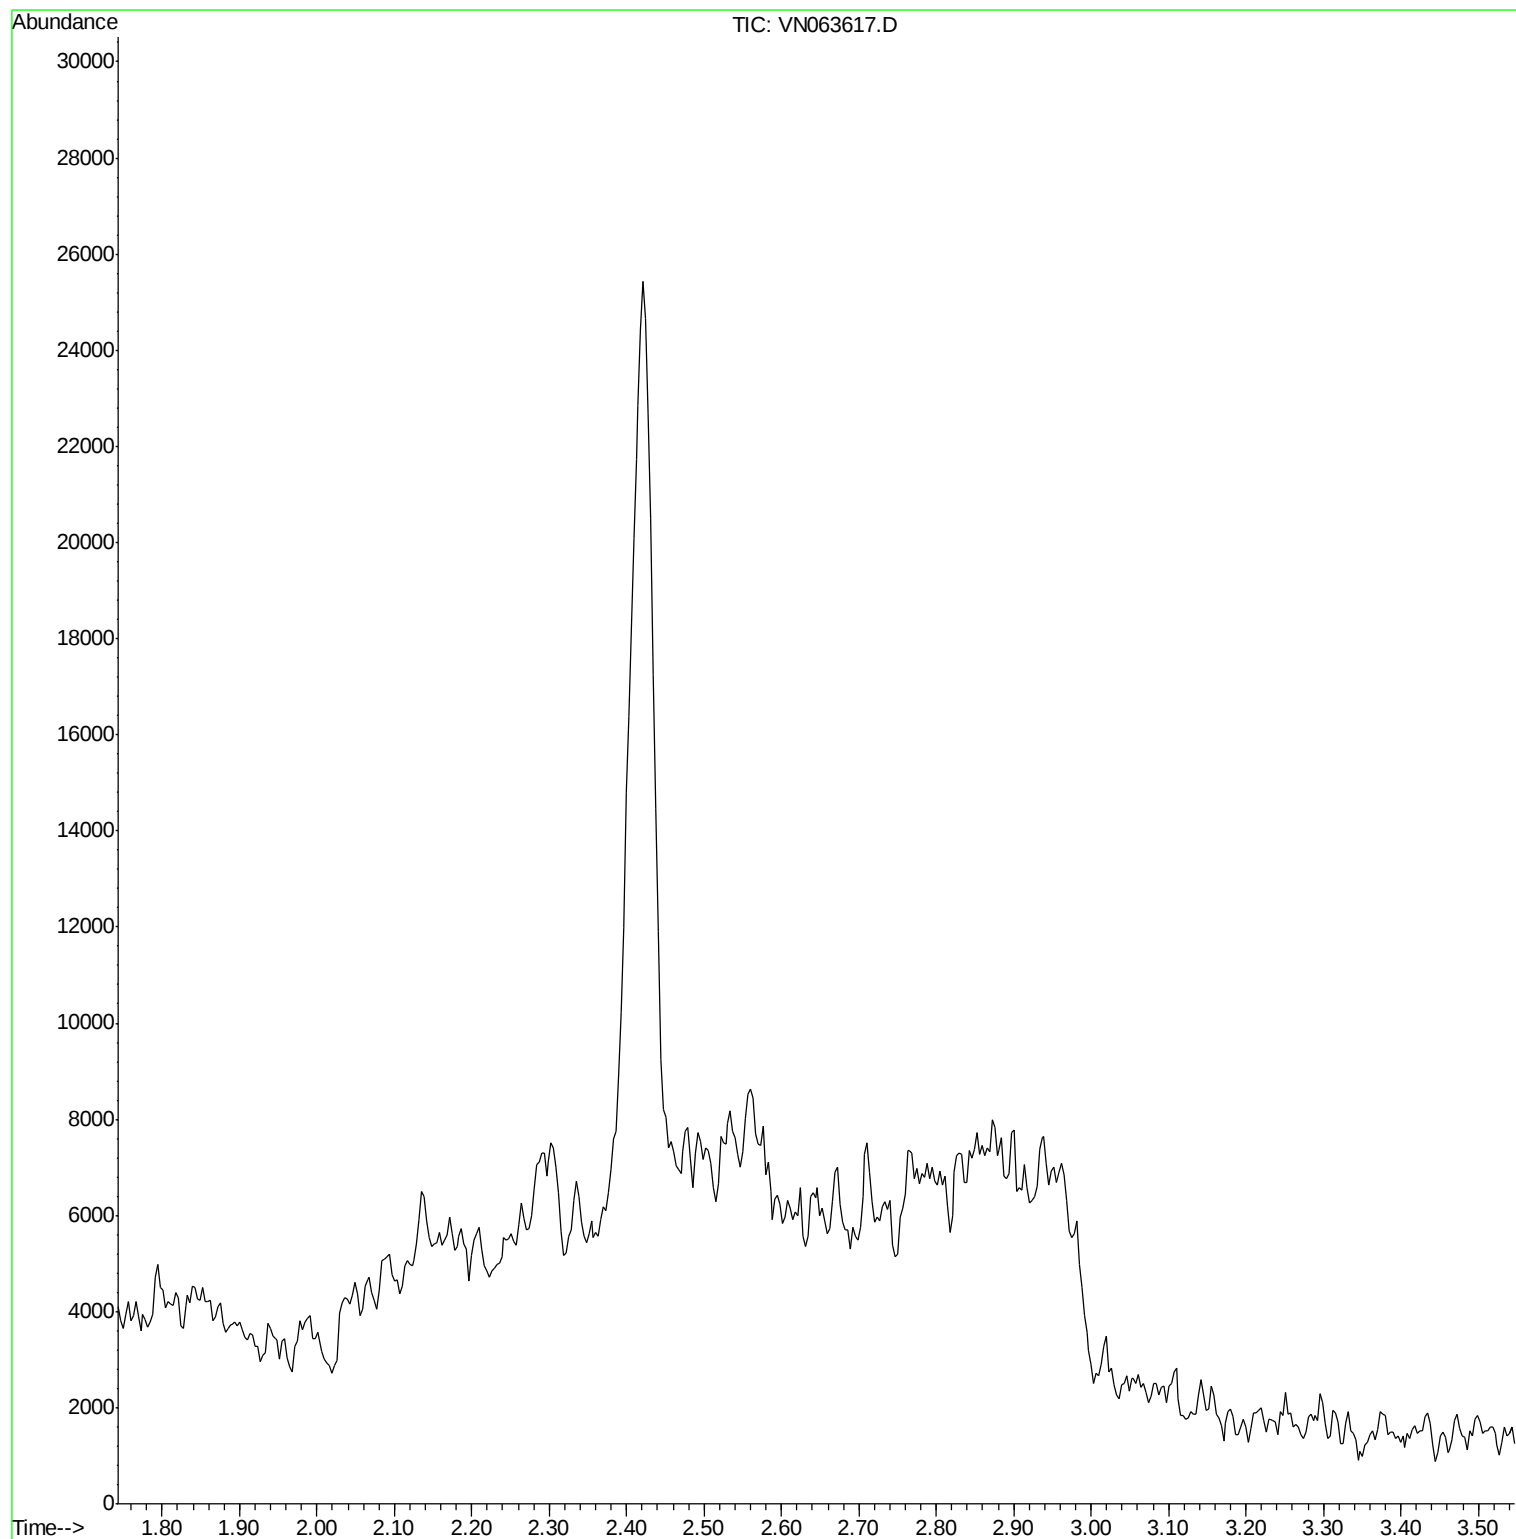


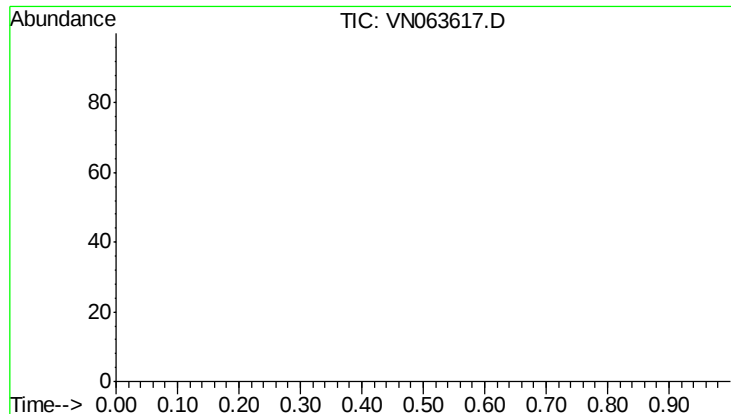


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 7.62 min

Lab File: VN063617.D
Acq: 24 Sep 2020 3:40

Instrument :
MSVOA_N
ClientSampleId :
PB131813ZHE#16


Tot Ion: 168
Sig Exp Ratio
168 100
99 66.3

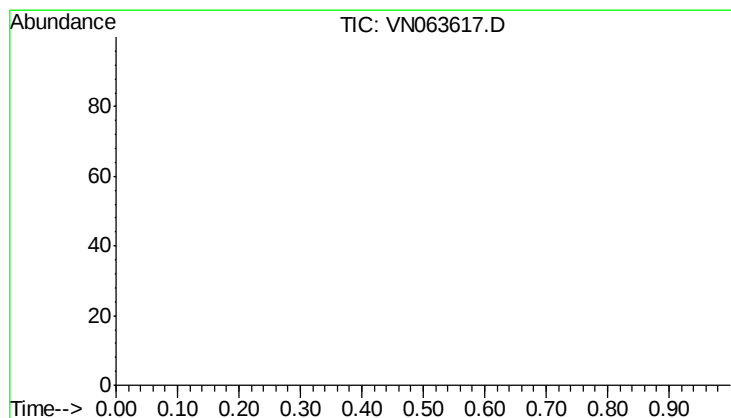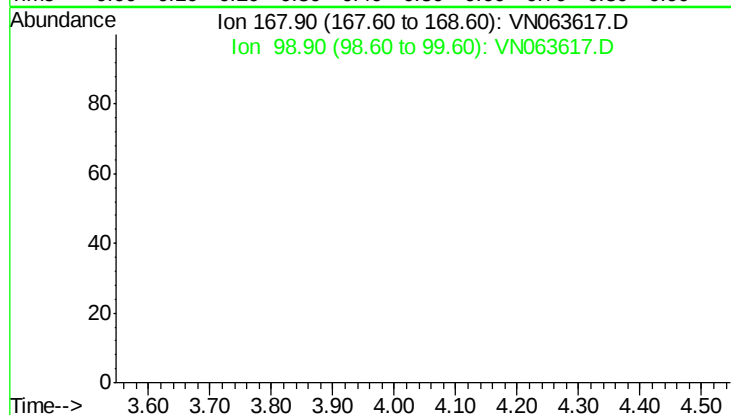


#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 7.99 min

Lab File: VN063617.D
Acq: 24 Sep 2020 3:40

Tgt Ion: 65
Sig Exp Ratio
65 100
67 52.1


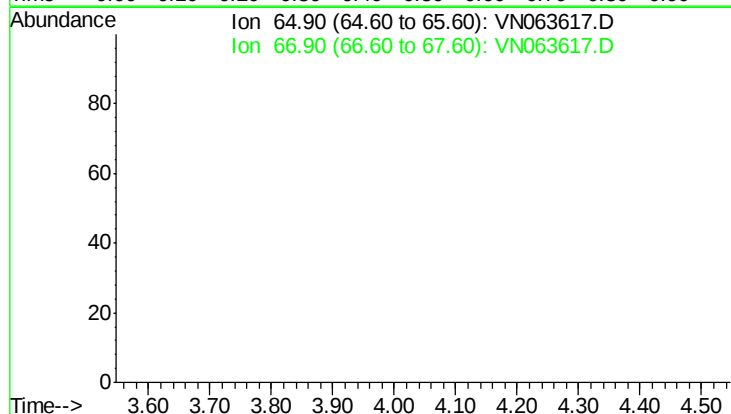


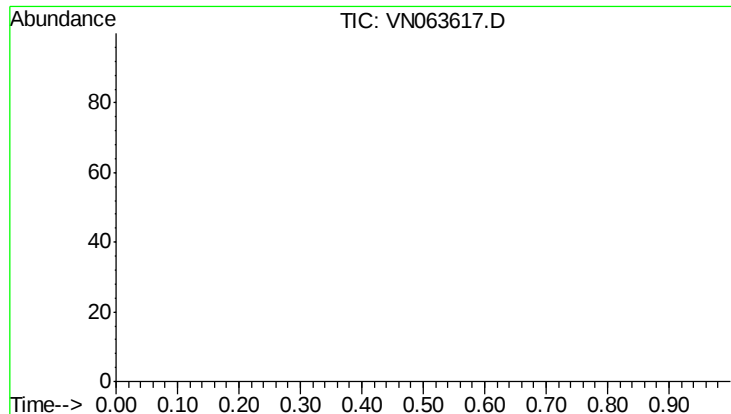

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.55 min
 Lab File: VN063617.D
 Acq: 24 Sep 2020 3:40


Instrument :
 MSVOA_N
 ClientSampleId :
 PB131813ZHE#16


Tot Ion: 114
 Sig Exp Ratio
 114 100
 63 23.2
 88 16.6

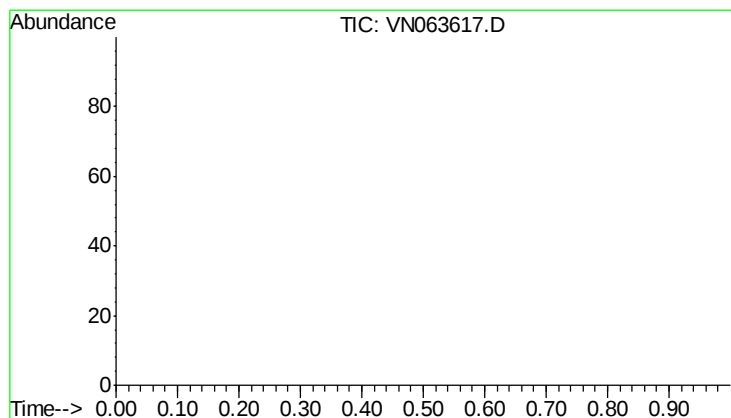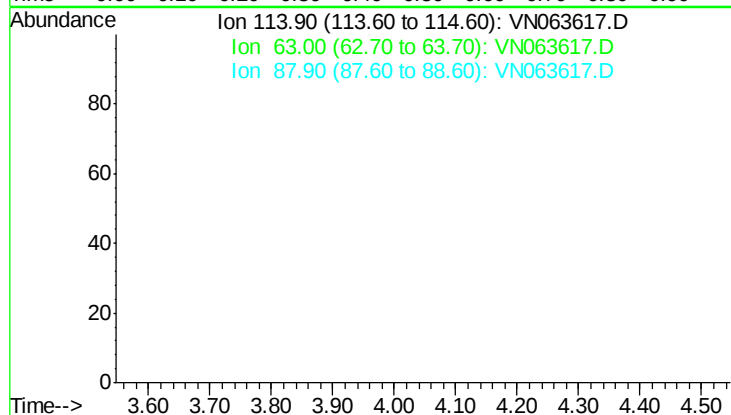

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.55 min
 Lab File: VN063617.D
 Acq: 24 Sep 2020 3:40

Tgt Ion: 113
 Sig Exp Ratio
 113 100
 111 103.6
 192 17.4


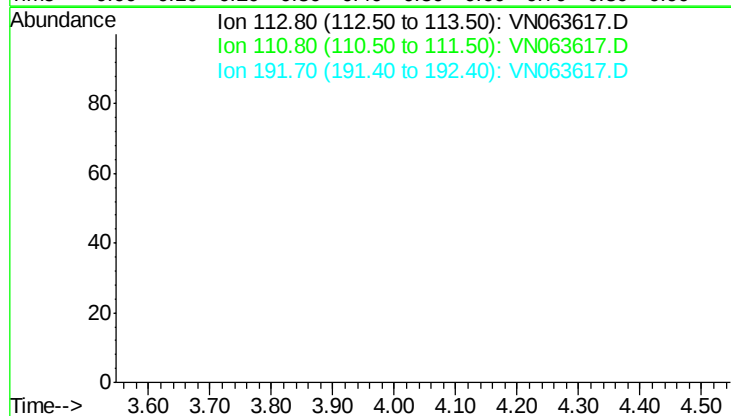


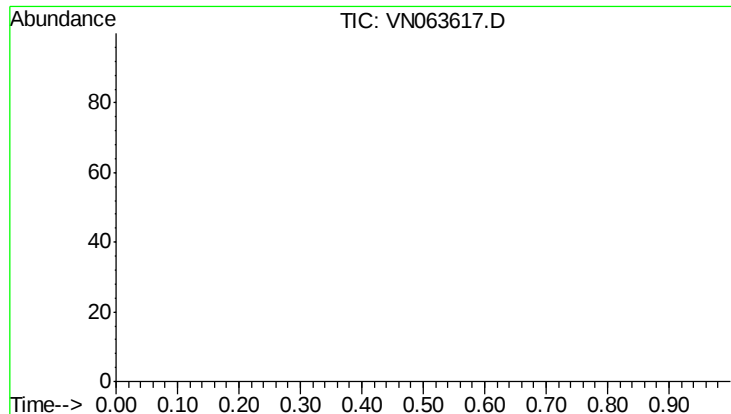

#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.06 min
Lab File: VN063617.D
Acq: 24 Sep 2020 3:40


Instrument :
MSVOA_N
ClientSampleId :
PB131813ZHE#16


Tot Ion	98
Sig	Exp Ratio
98	100
100	63.4

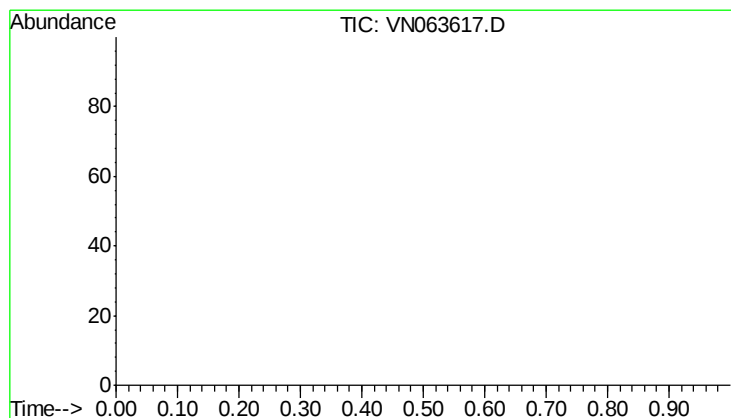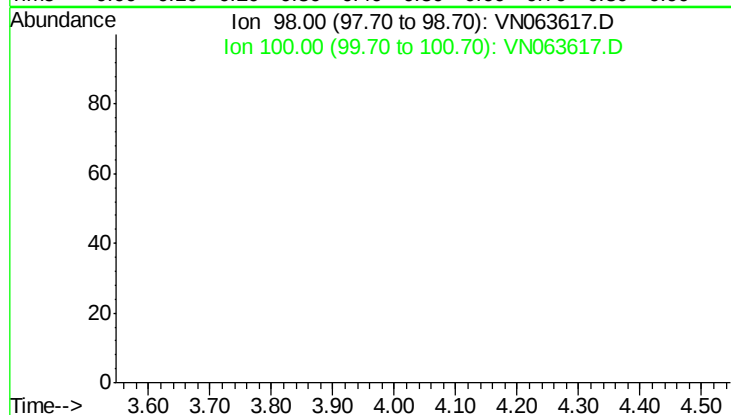

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.38 min
Lab File: VN063617.D
Acq: 24 Sep 2020 3:40

Tgt Ion	95
Sig	Exp Ratio
95	100
174	70.4
176	68.8


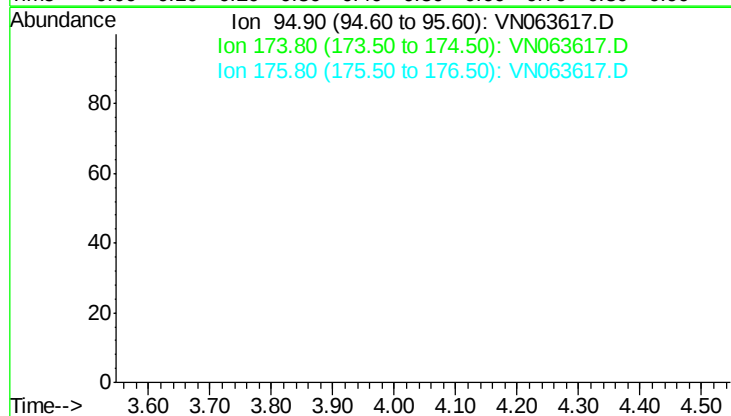


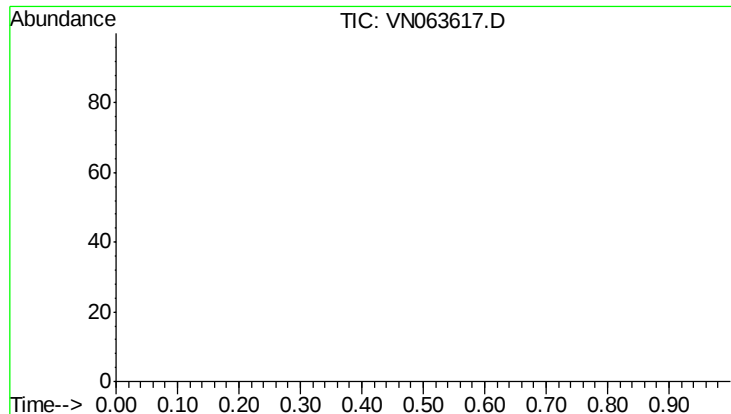

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.38 min
 Lab File: VN063617.D
 Acq: 24 Sep 2020 3:40

Instrument :
 MSVOA_N
 ClientSampleId :
 PB131813ZHE#16

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 61.5
 119 32.8

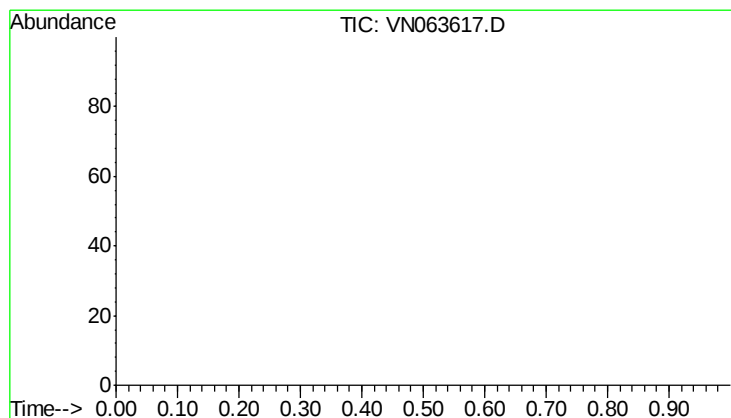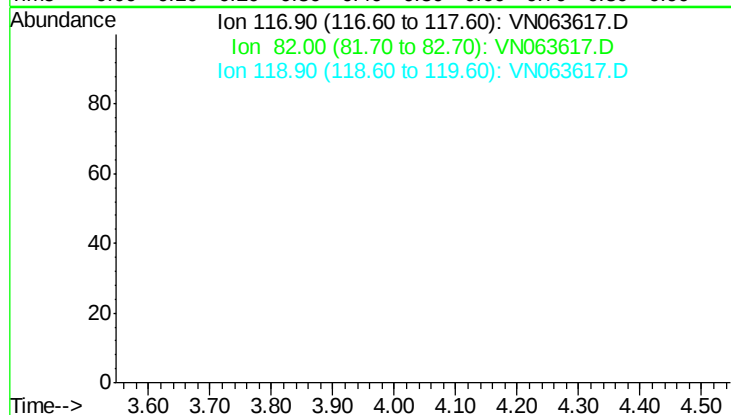

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.32 min
 Lab File: VN063617.D
 Acq: 24 Sep 2020 3:40

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 64.4
 150 171.7

