


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN092320\
 Data File : VN063579.D
 Acq On : 23 Sep 2020 10:55
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091620W.M
 Title : SW846 8260
 Last Update : Wed Sep 16 13:05:20 2020

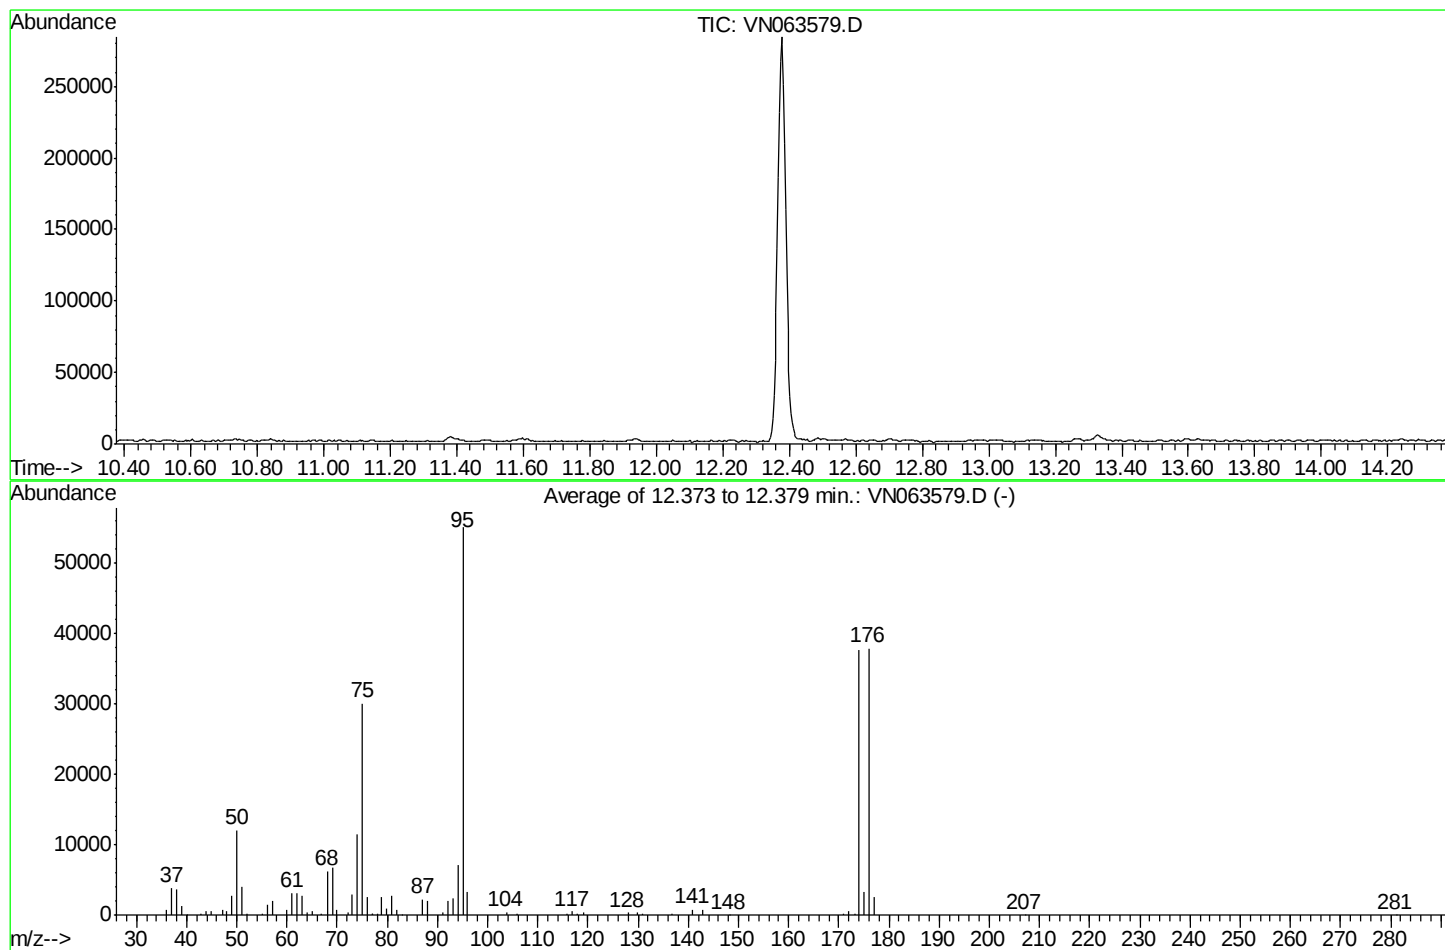

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	12034	PASS
75	95	30	60	54.6	30048	PASS
95	95	100	100	100.0	55024	PASS
96	95	5	9	5.9	3263	PASS
173	174	0.00	2	0.7	268	PASS
174	95	50	100	68.5	37677	PASS
175	174	5	9	8.7	3292	PASS
176	174	95	101	100.4	37818	PASS
177	176	5	9	6.5	2476	PASS