


Bromomethane

Response Ratio

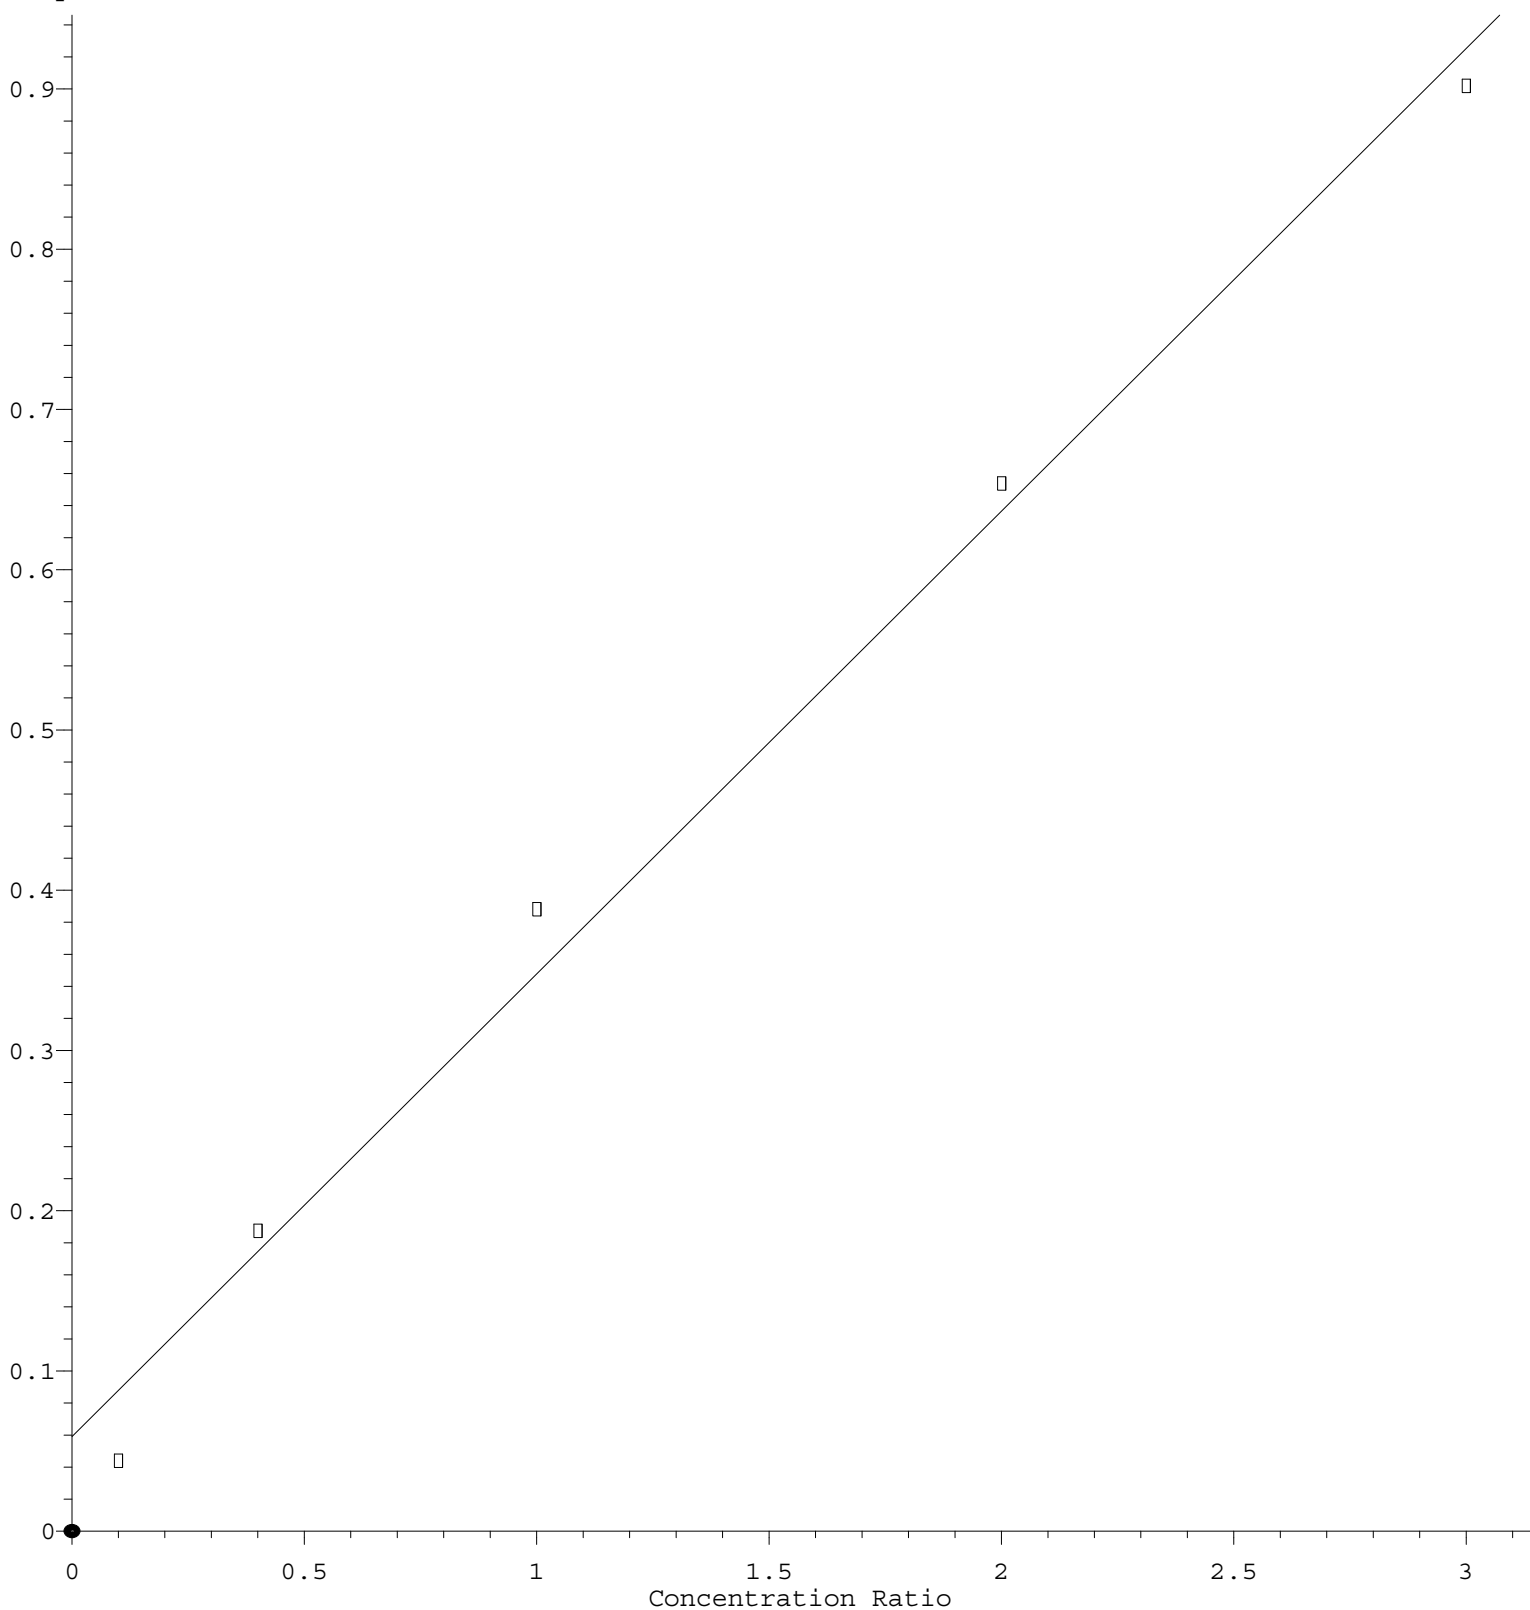

$$\text{Response} = 2.890\text{e-}001 * \text{Amt} + 5.931\text{e-}002$$


Coef of Det (r^2) = 0.990544 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092321W.M

Calibration Table Last Updated: Thu Sep 23 13:52:37 2021


Chloroethane

Response Ratio

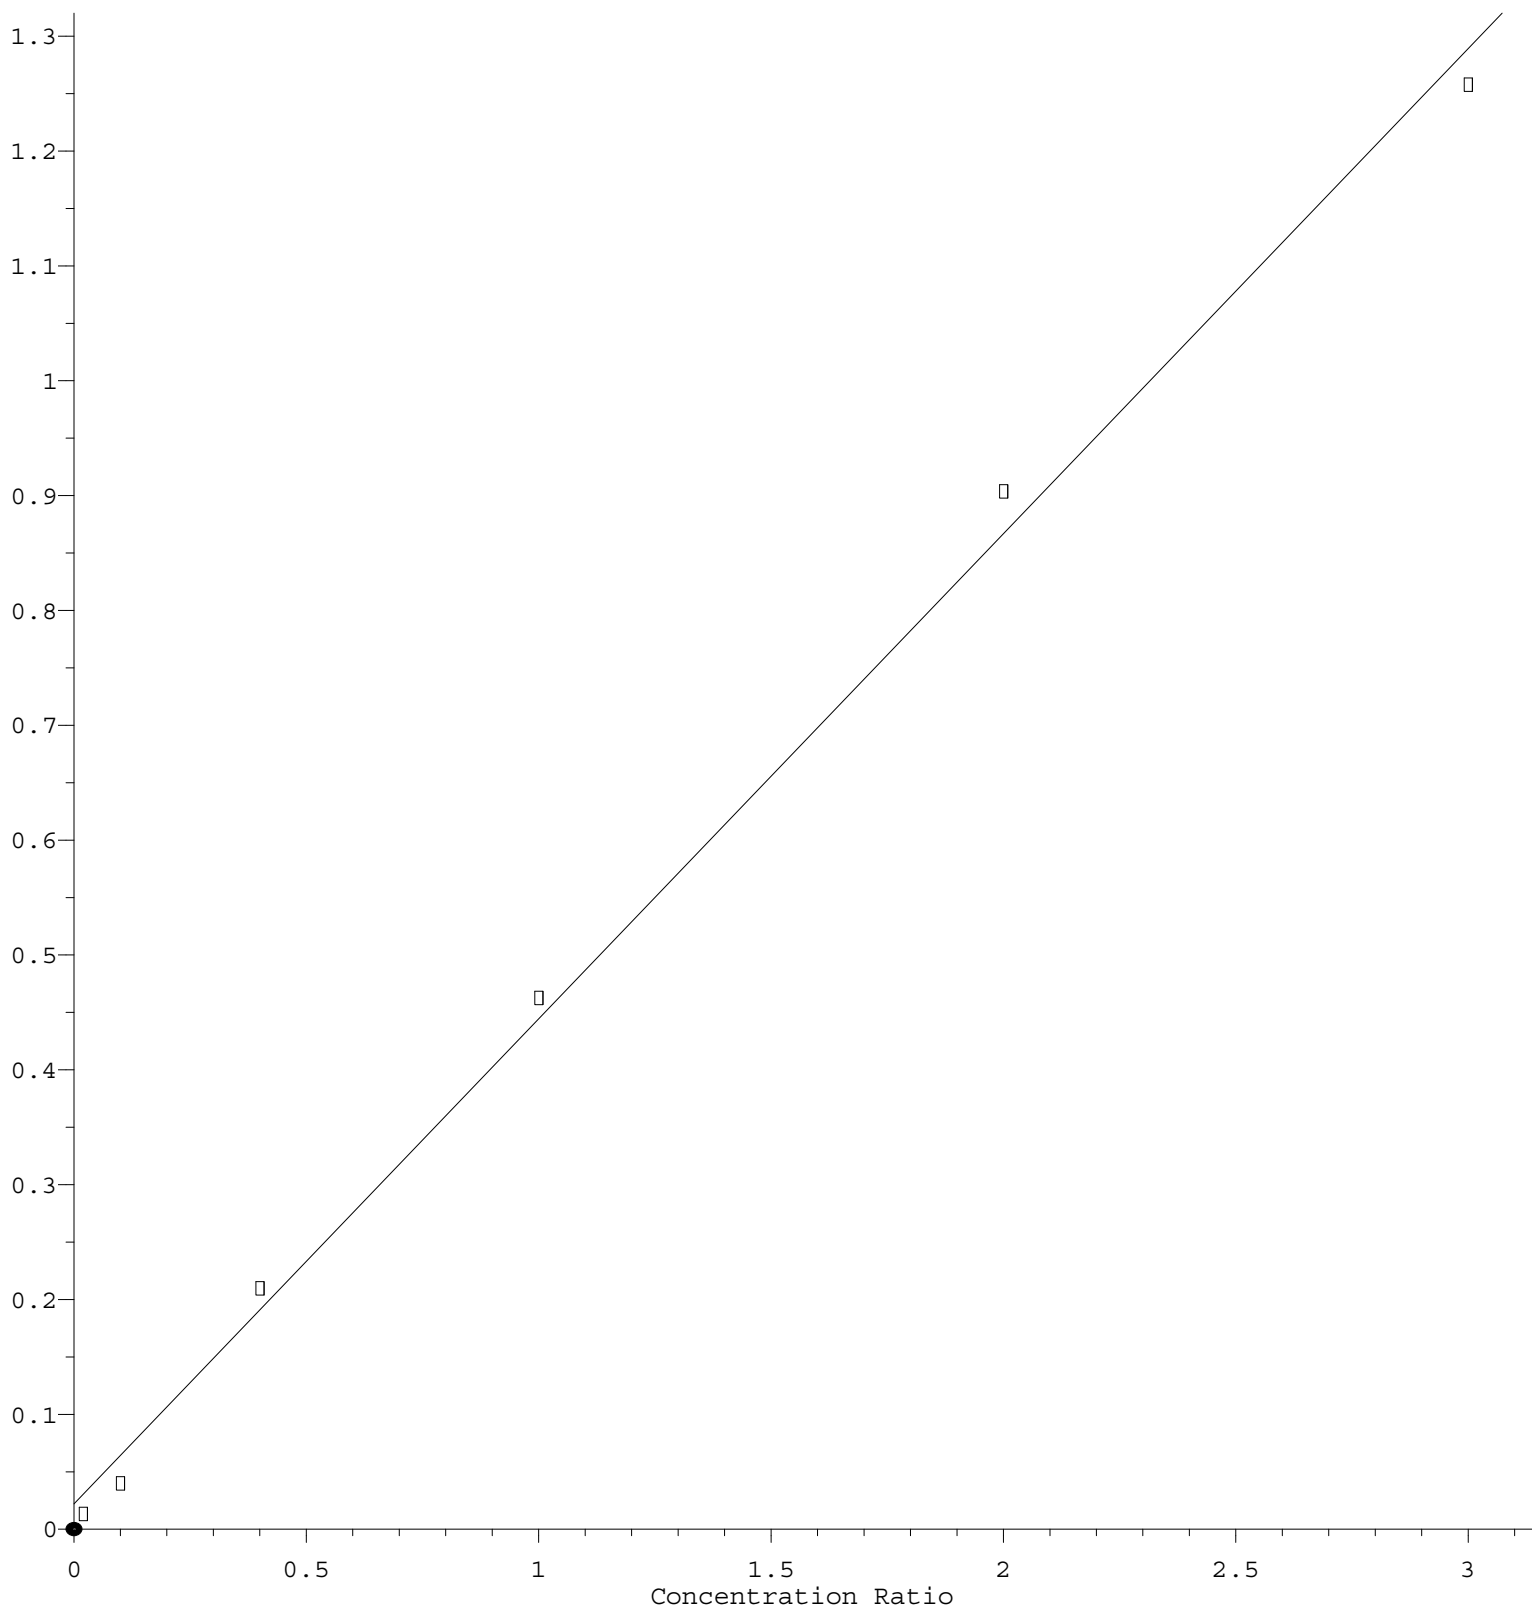

Response = $4.226 \times 10^{-1} \times \text{Amt} + 2.187 \times 10^{-2}$
Coef of Det (r^2) = 0.996911 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092321W.M
Calibration Table Last Updated: Thu Sep 23 13:52:37 2021


Acrolein

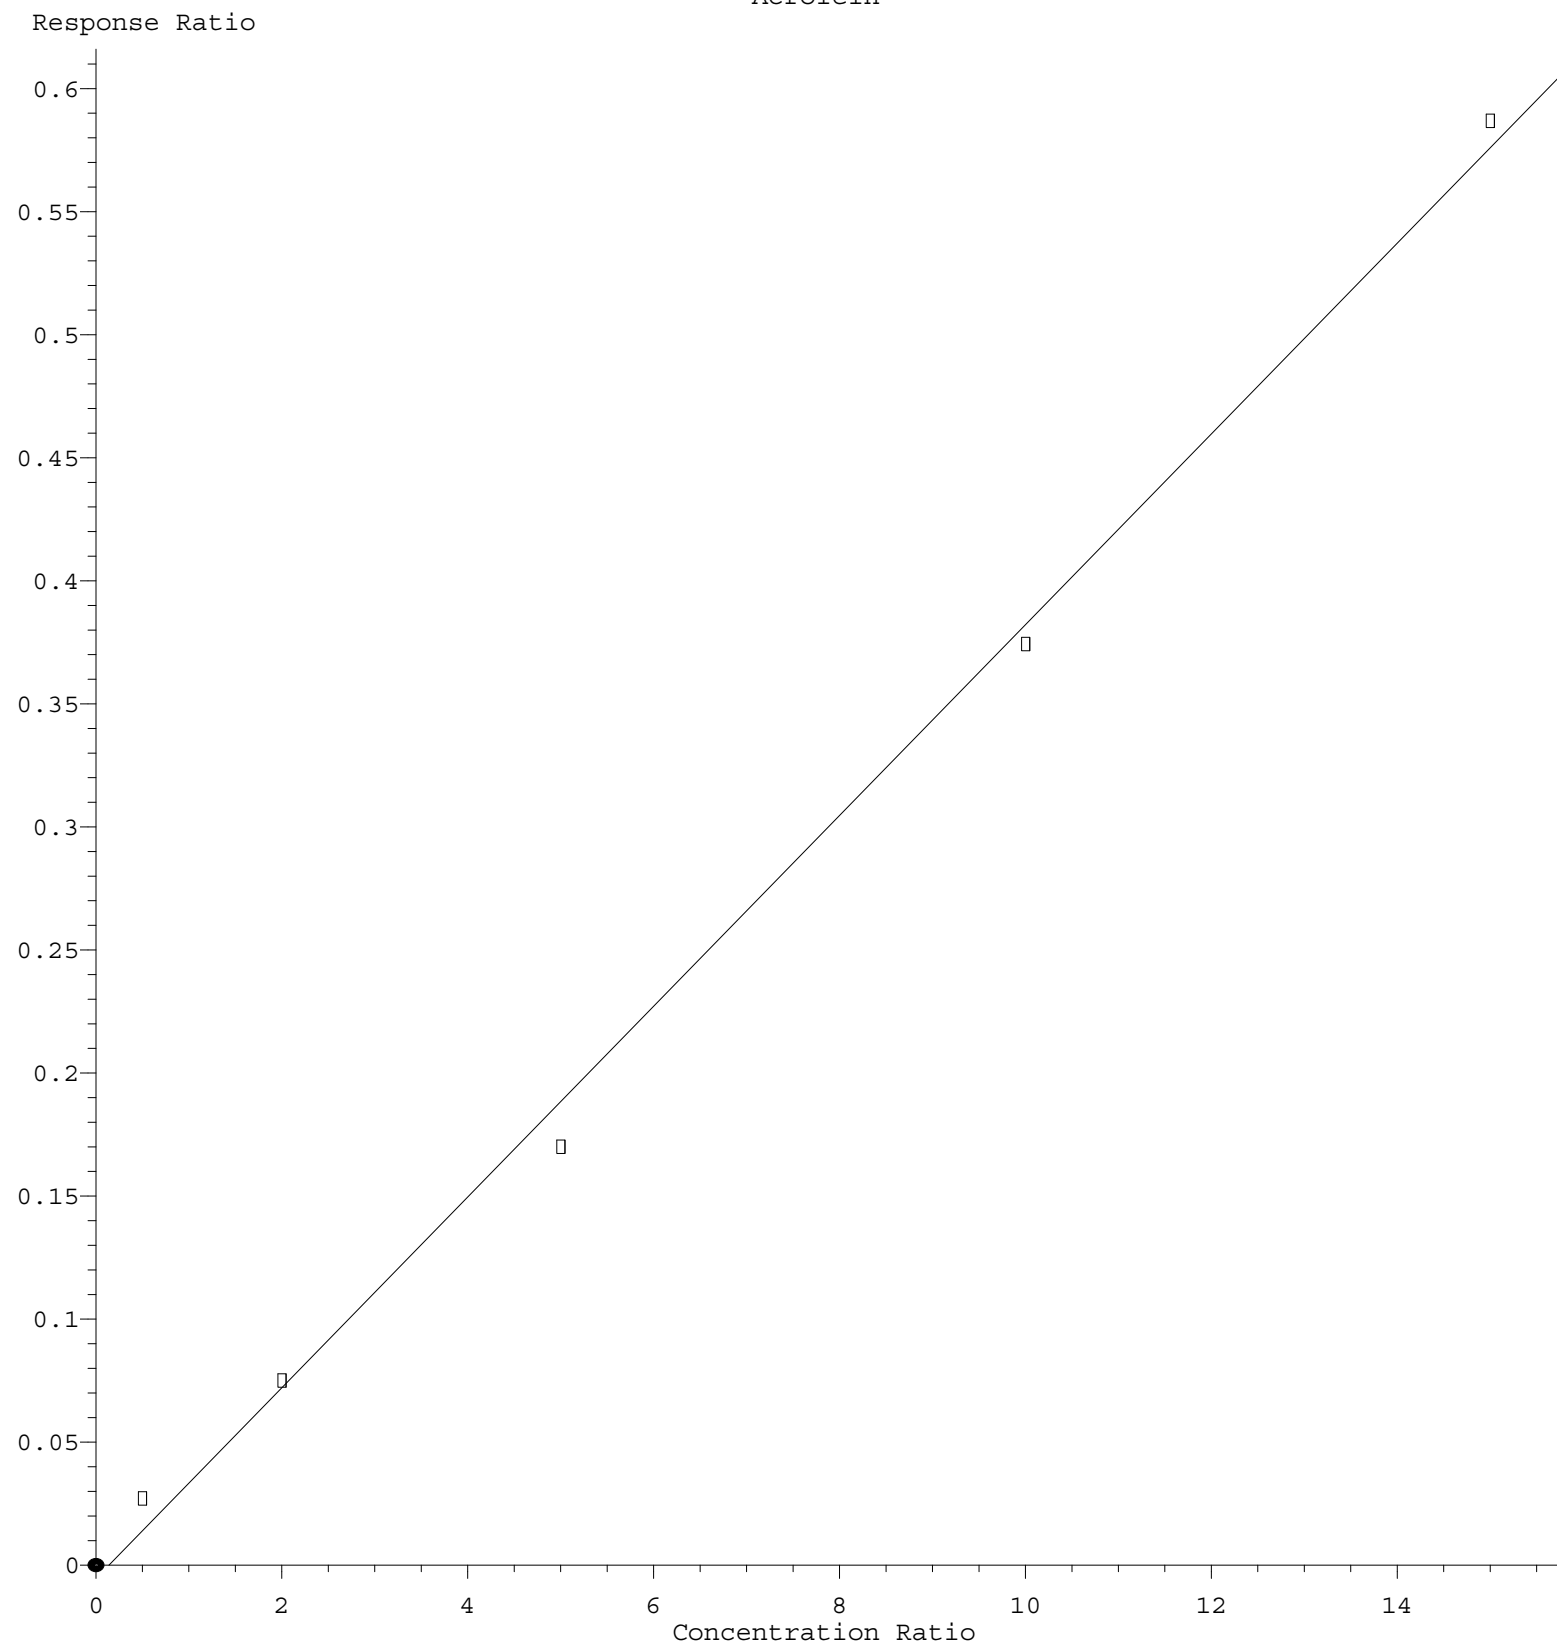

Response = $3.876 \times 10^{-2} \times \text{Amt} - 5.291 \times 10^{-3}$
 Coef of Det (r^2) = 0.996752 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092321W.M
 Calibration Table Last Updated: Thu Sep 23 13:52:37 2021

Acetone


Response Ratio

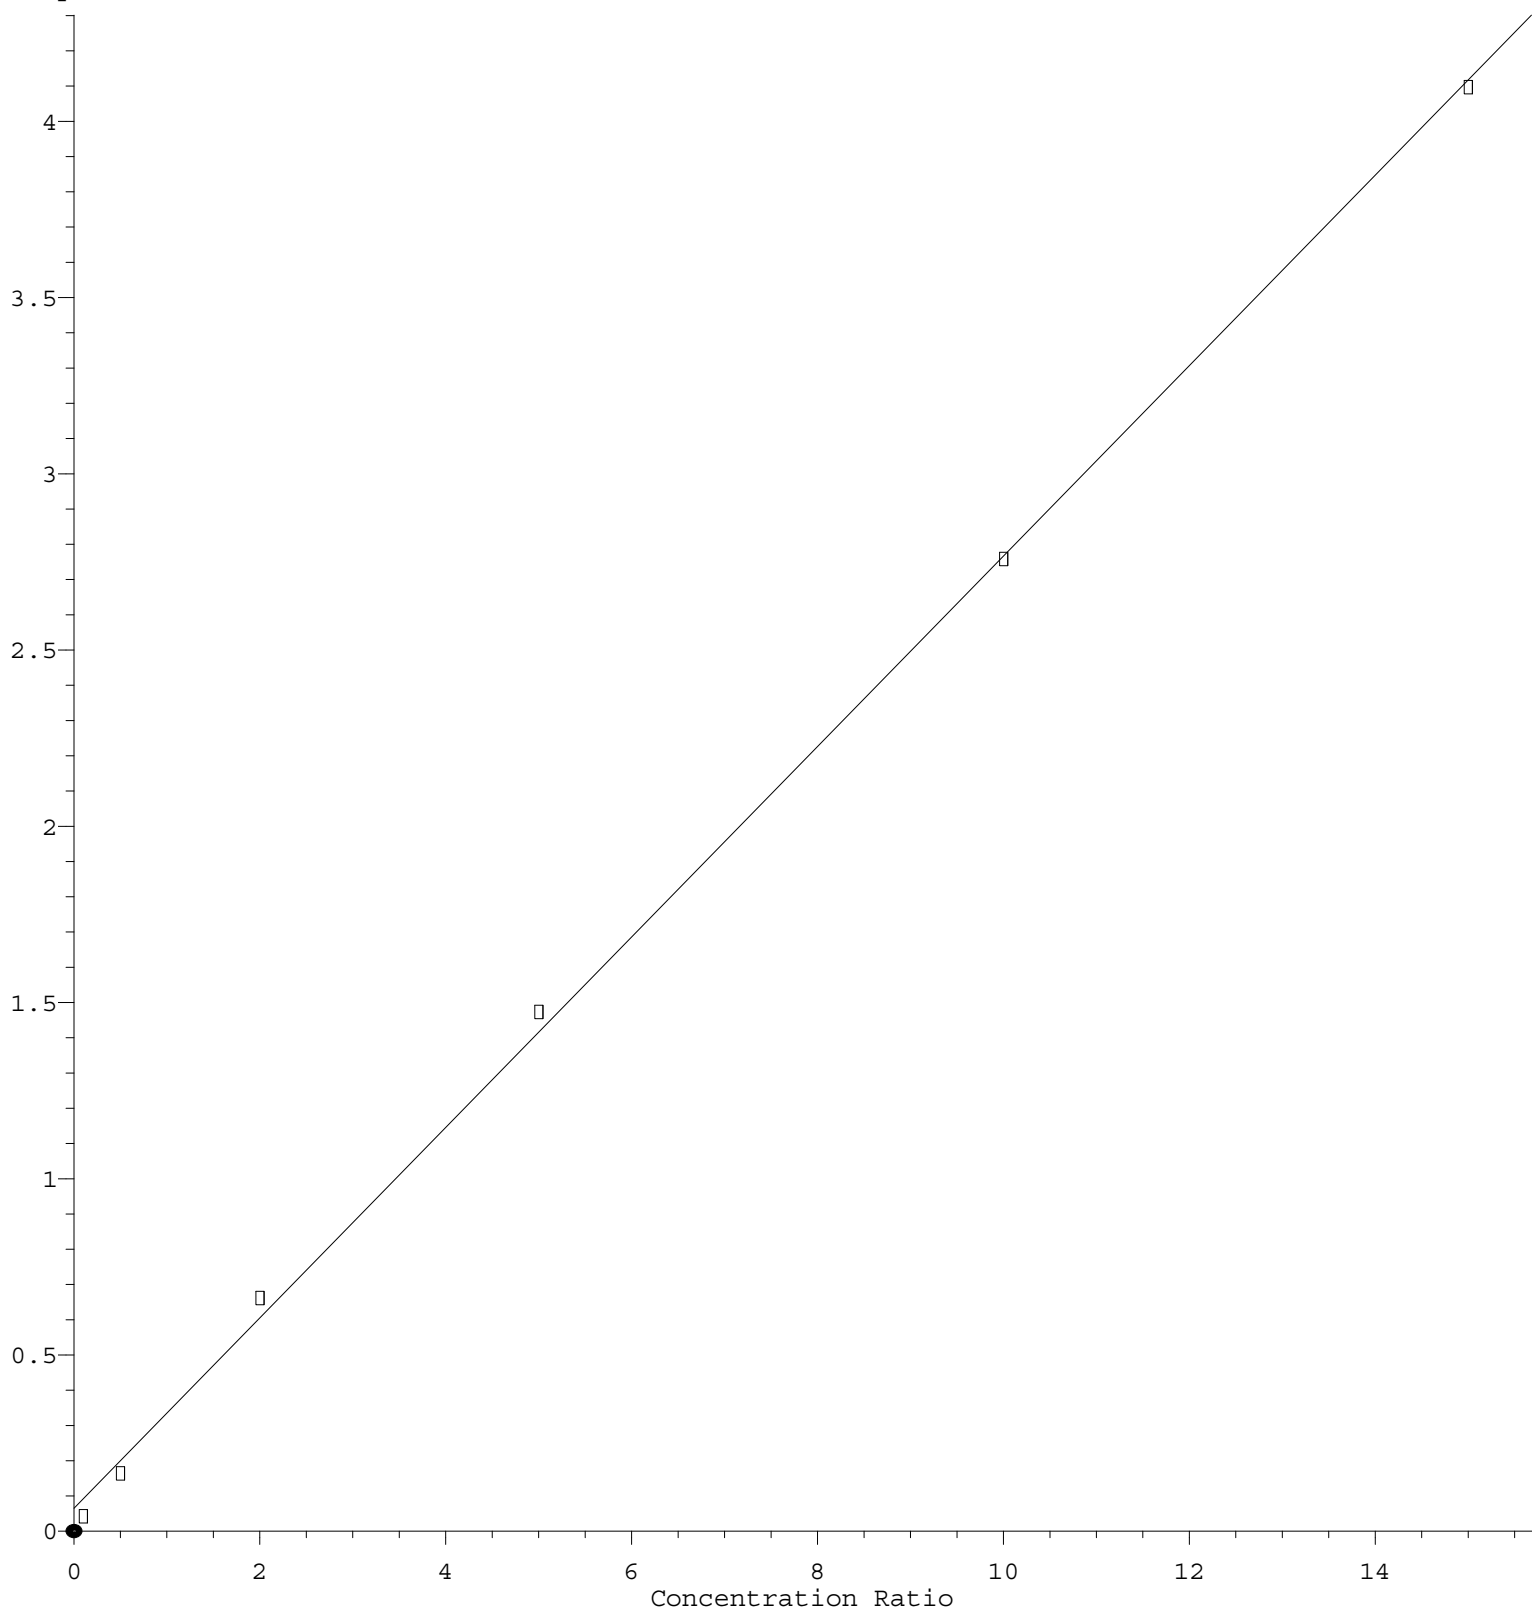

$\text{Response} = 2.701\text{e-}001 * \text{Amt} + 6.496\text{e-}002$
 Coef of Det (r^2) = 0.999171 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092321W.M
 Calibration Table Last Updated: Thu Sep 23 13:52:37 2021

Methylene Chloride

Response Ratio

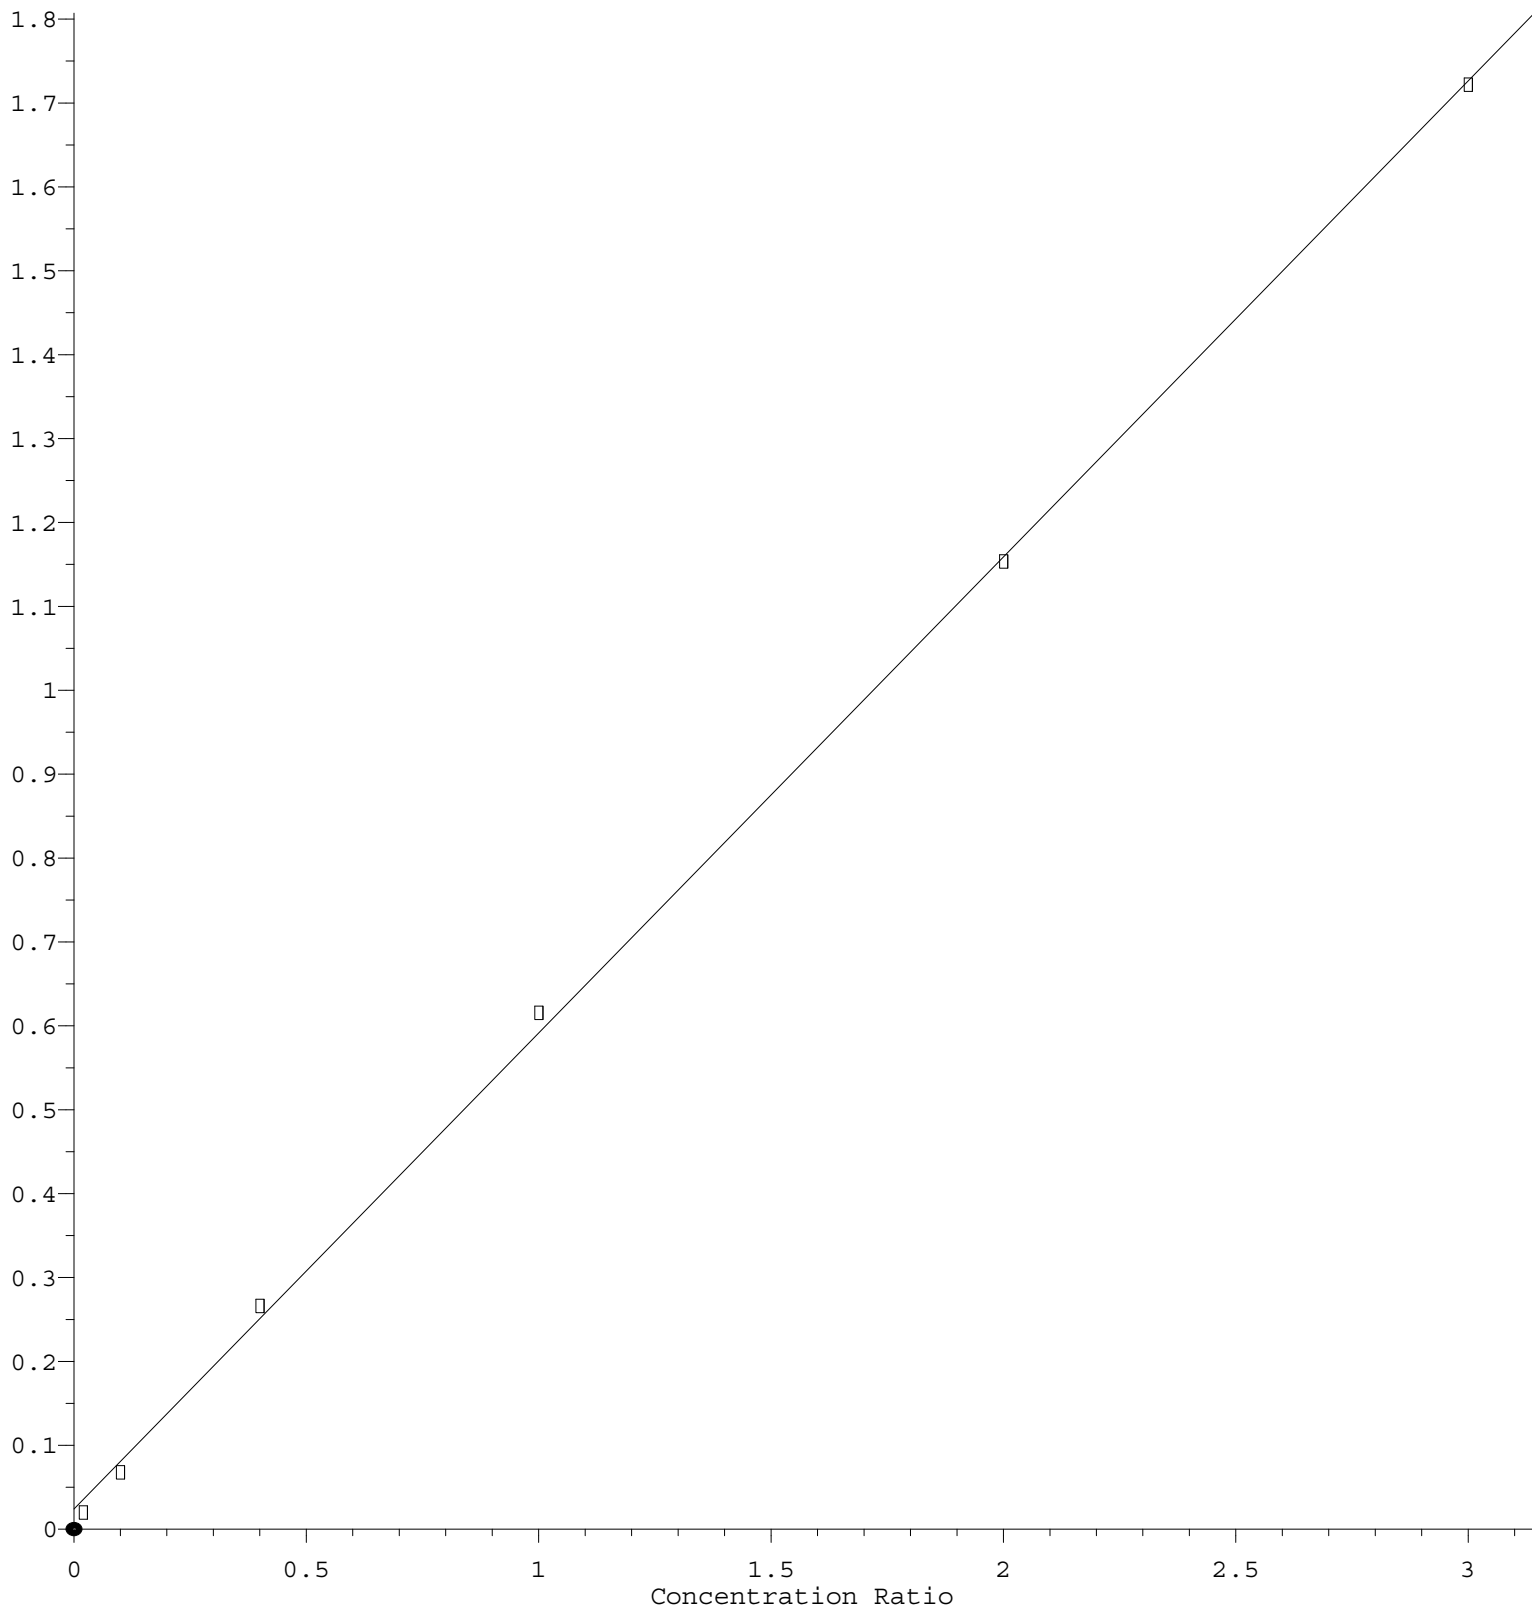

$$\text{Response} = 5.679\text{e-}001 * \text{Amt} + 2.351\text{e-}002$$


Coef of Det (r^2) = 0.999447 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092321W.M

Calibration Table Last Updated: Thu Sep 23 13:52:37 2021

1,2-Dichloroethane-d4

Response Ratio

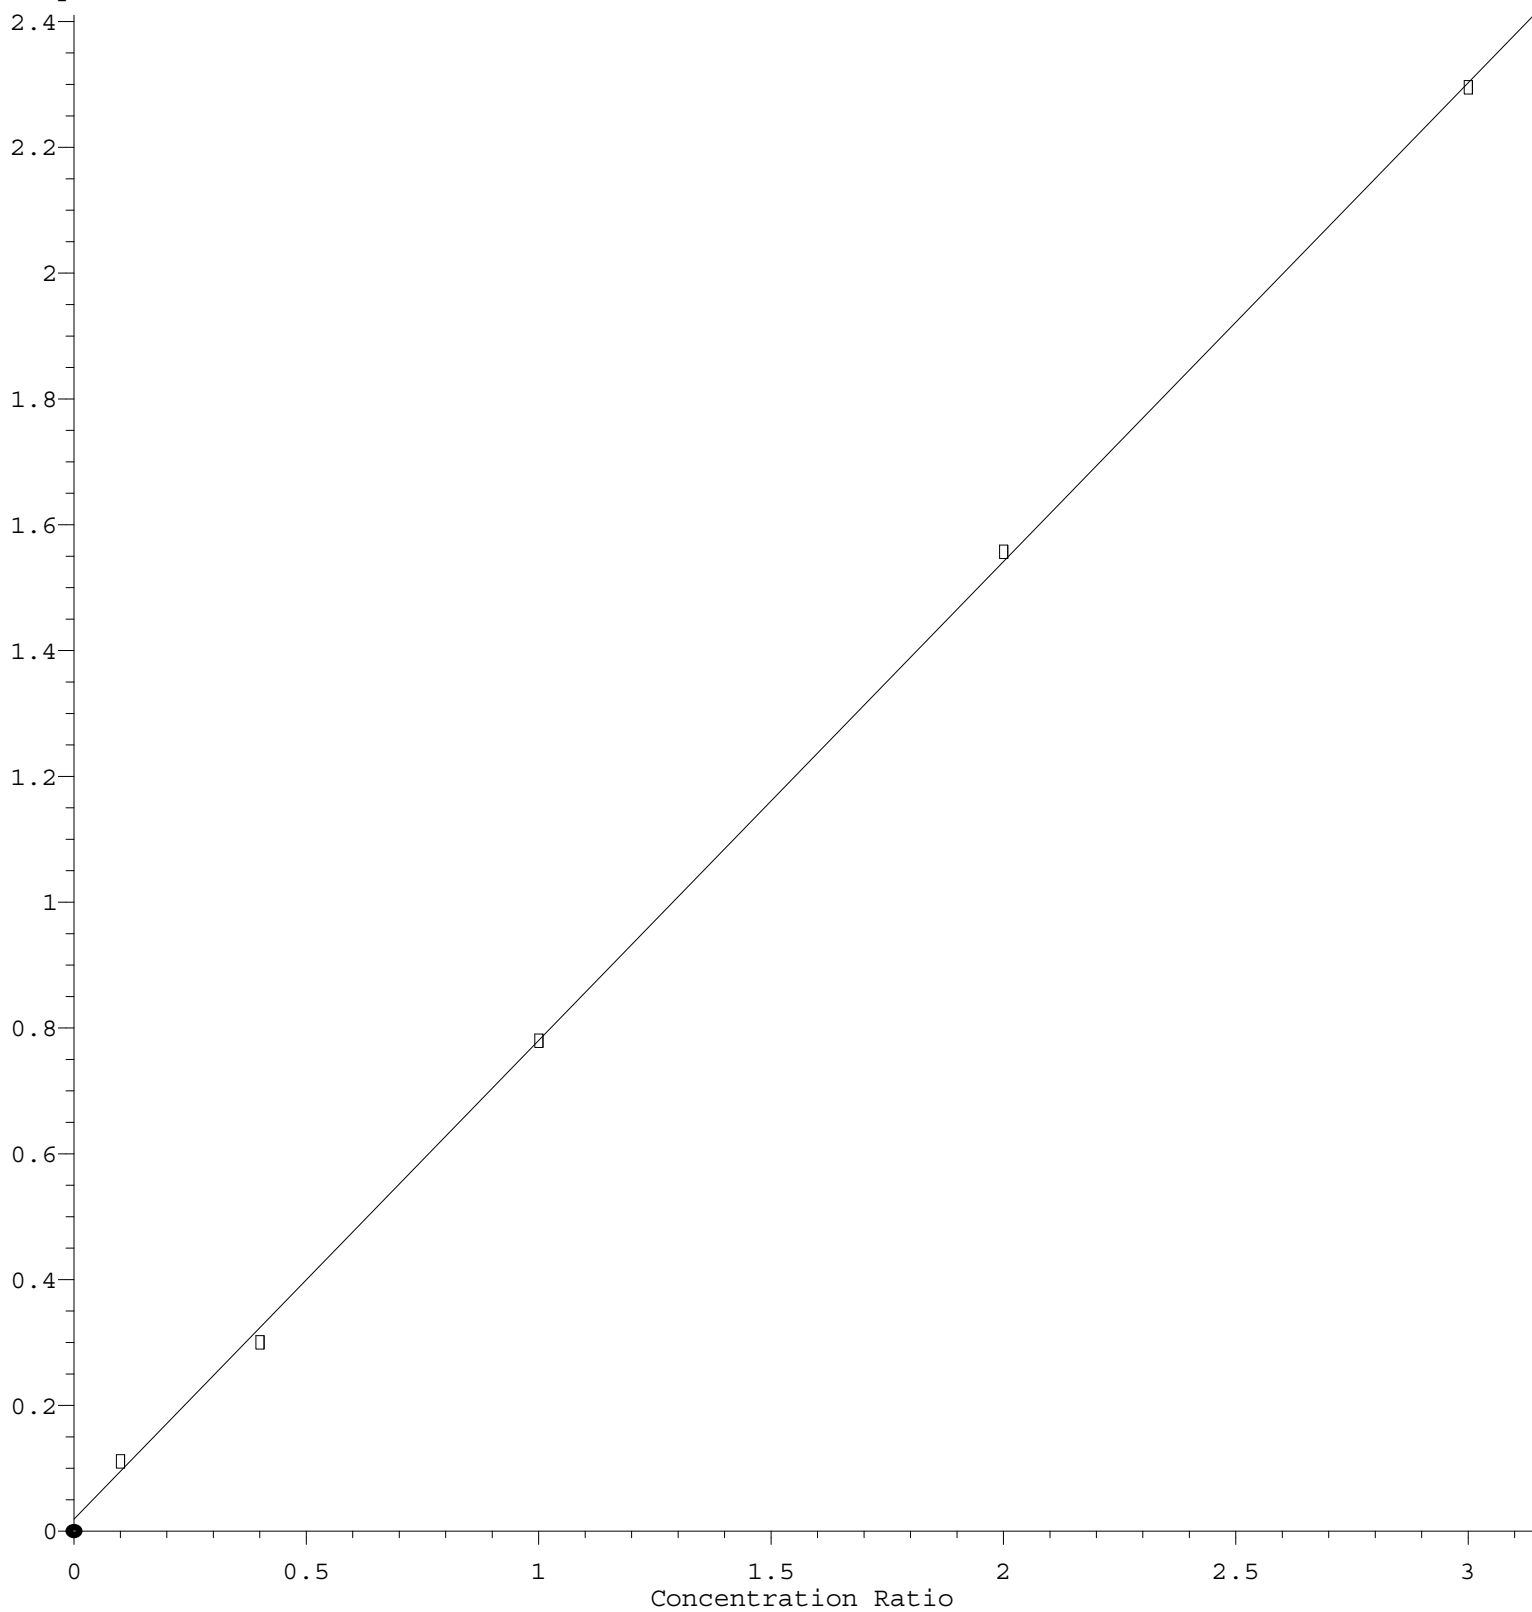

$$\text{Response} = 7.613\text{e-}001 * \text{Amt} + 1.890\text{e-}002$$


Coef of Det (r^2) = 0.999673 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092321W.M

Calibration Table Last Updated: Thu Sep 23 13:52:37 2021

Dibromofluoromethane

Response Ratio

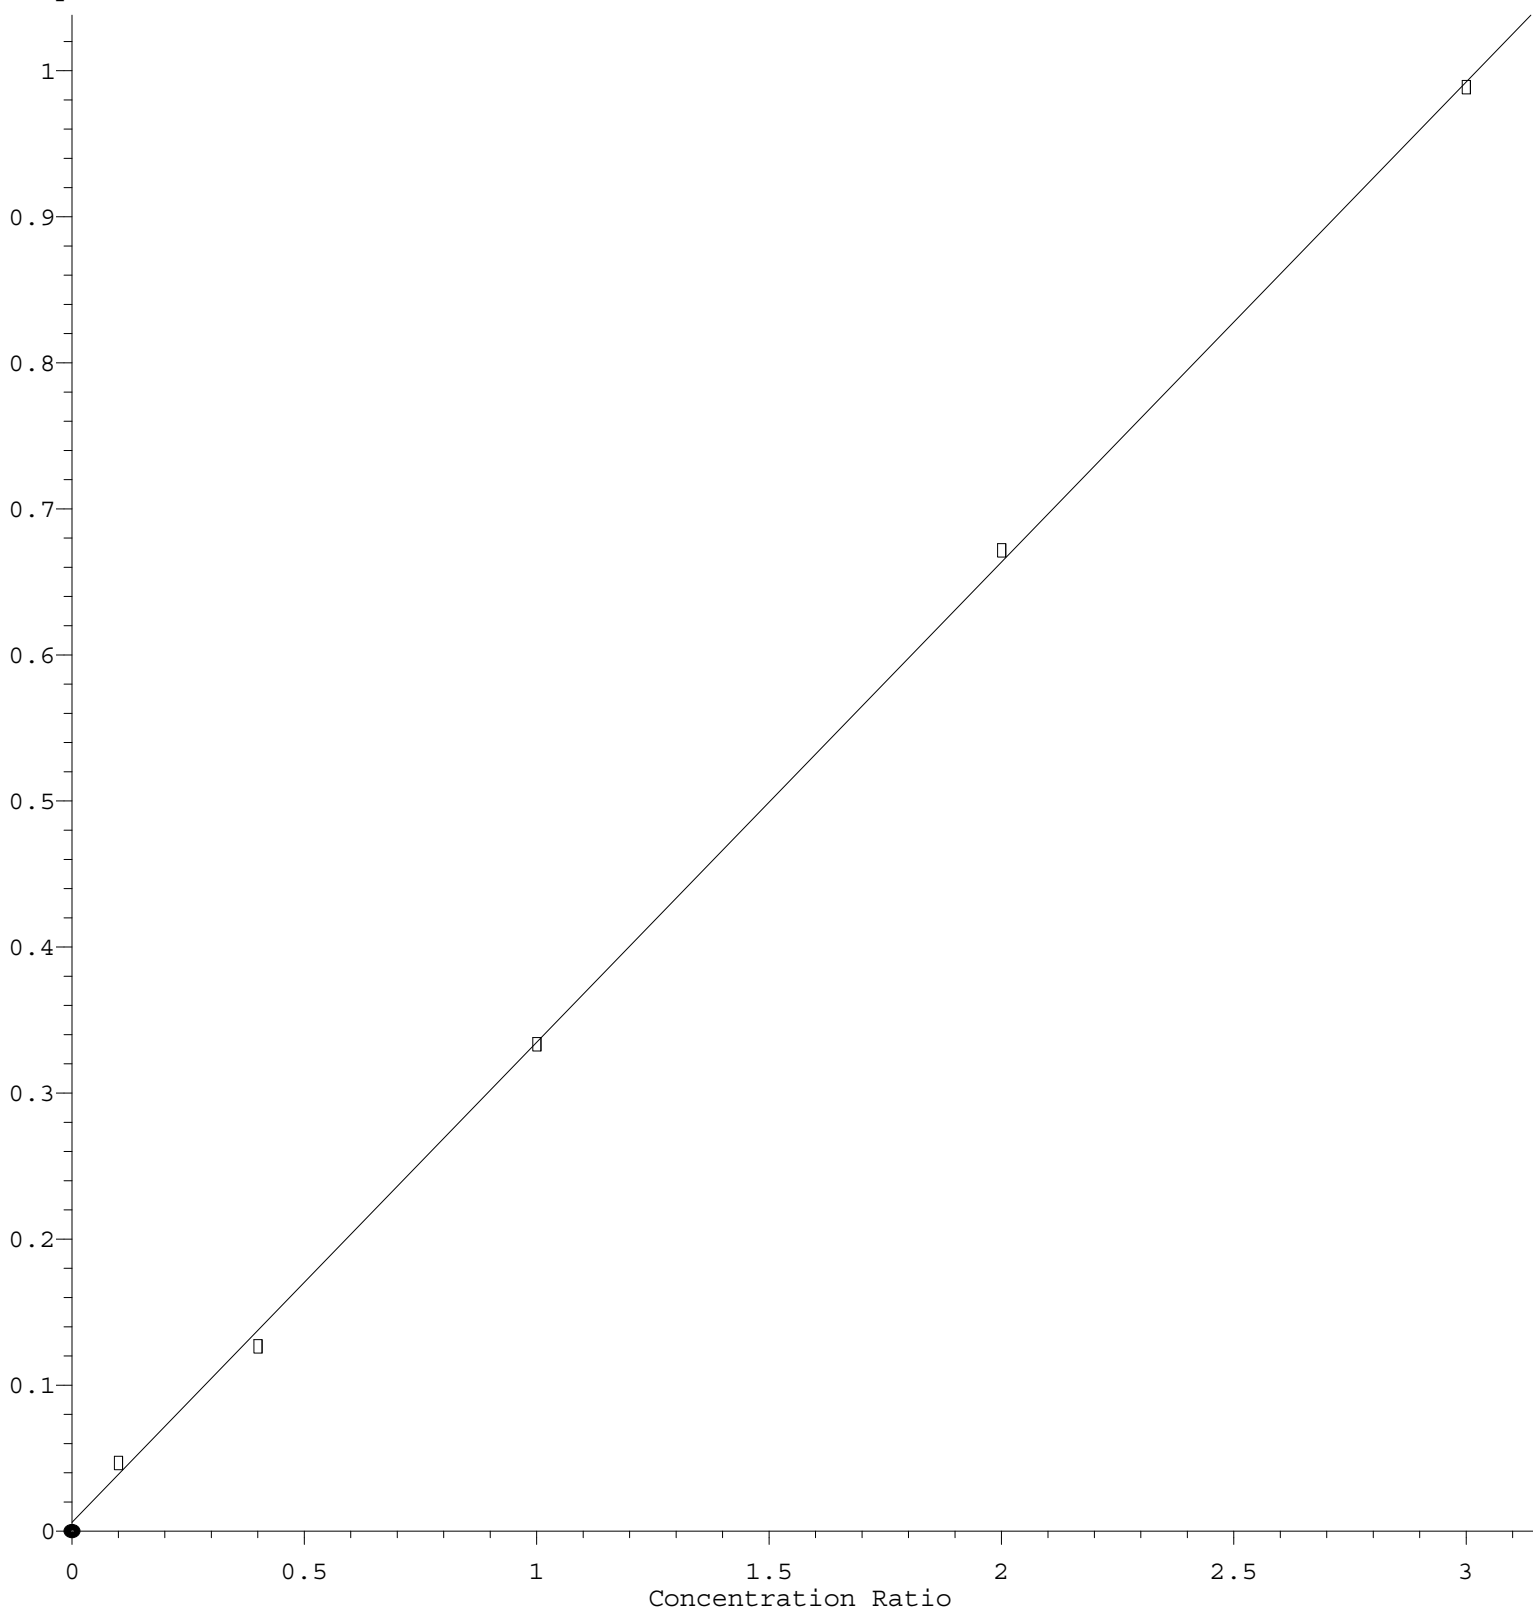

$$\text{Response} = 3.289 \times 10^{-1} \times \text{Amt} + 5.861 \times 10^{-3}$$


Coef of Det (r^2) = 0.999581 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092321W.M

Calibration Table Last Updated: Thu Sep 23 13:52:37 2021

Ethyl methacrylate

Response Ratio

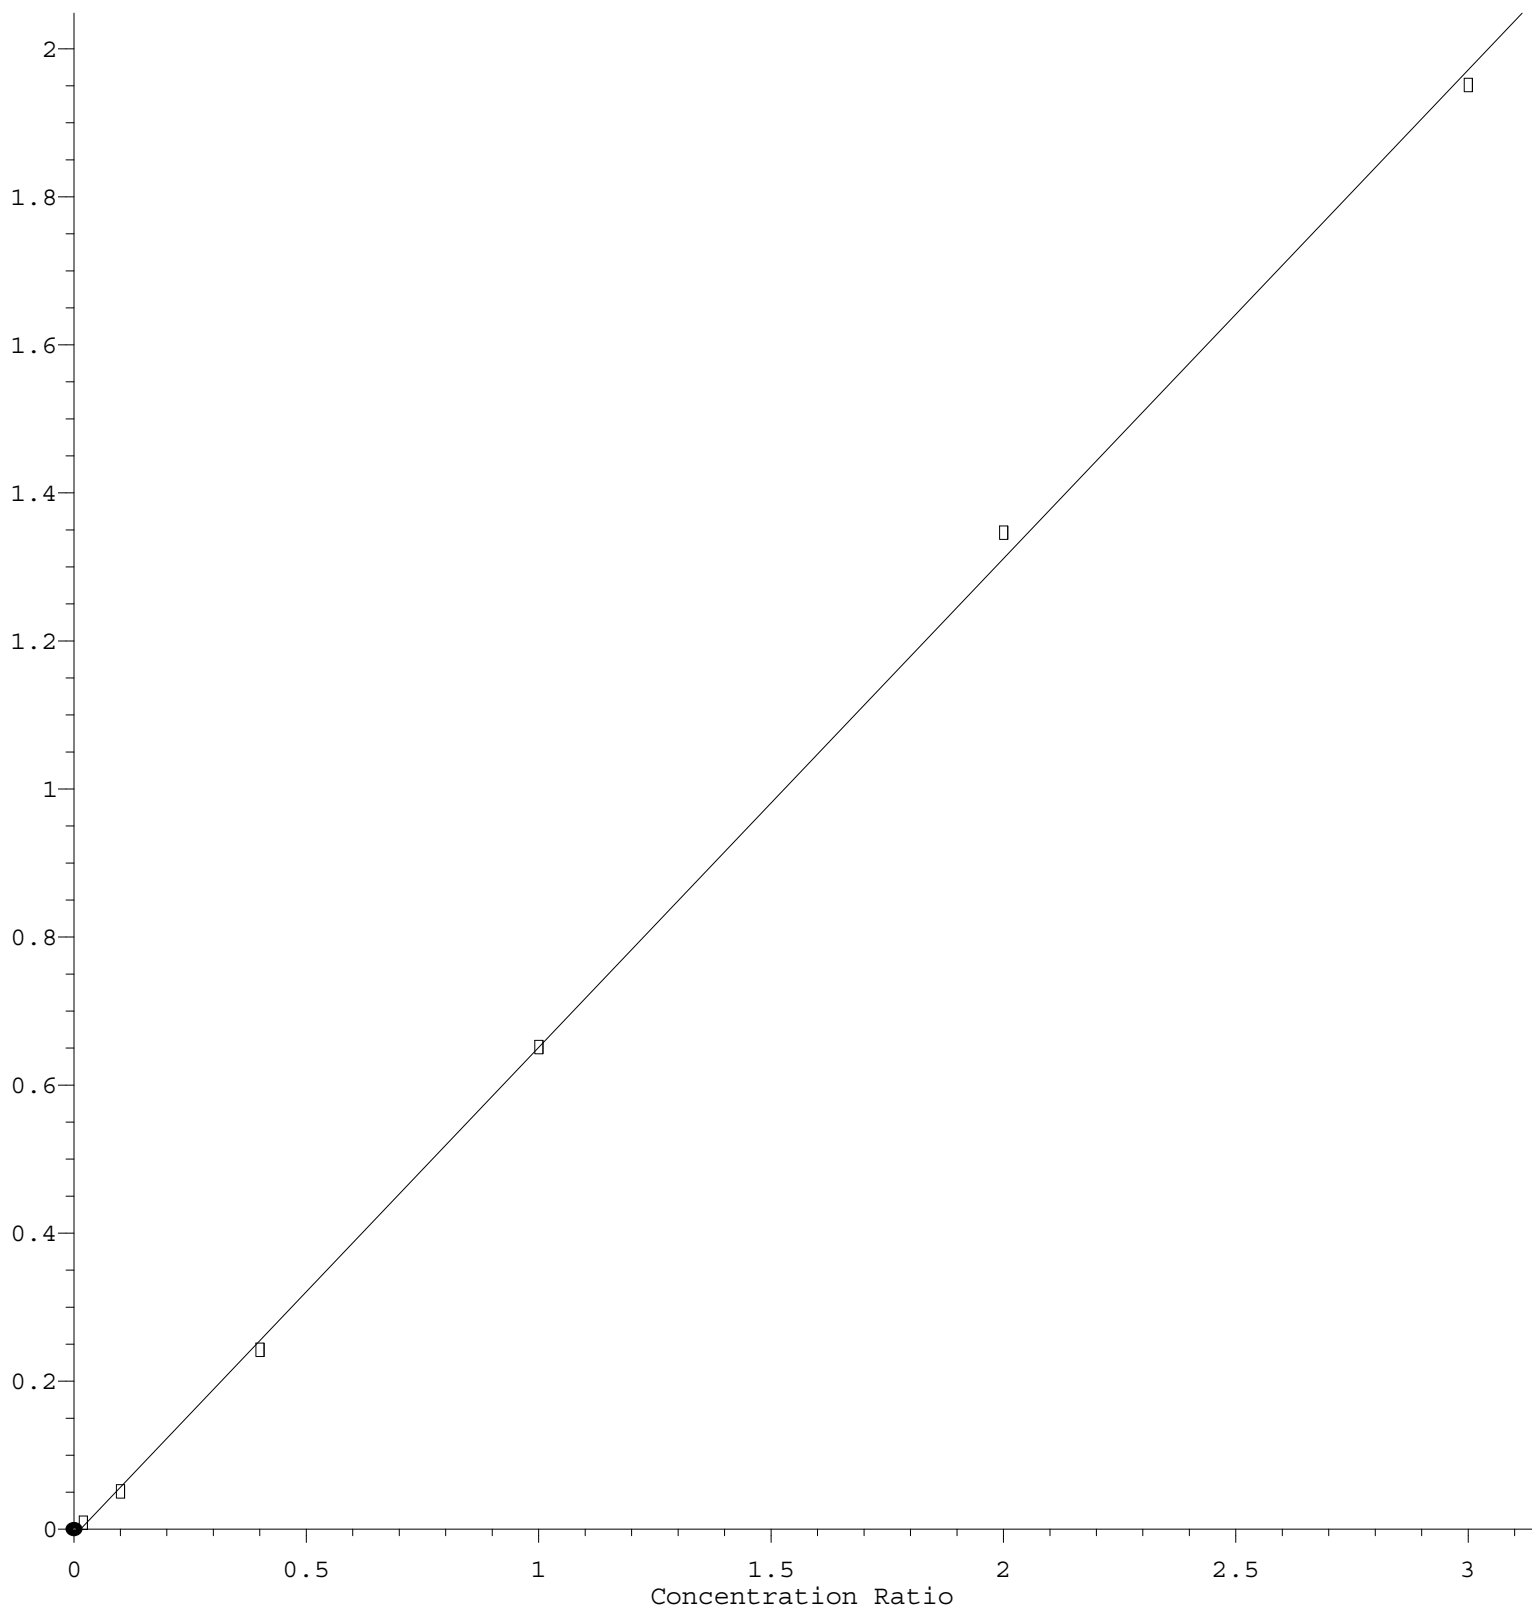

$$\text{Response} = 6.605\text{e-}001 * \text{Amt} - 9.320\text{e-}003$$


Coef of Det (r^2) = 0.999401 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092321W.M

Calibration Table Last Updated: Thu Sep 23 13:52:37 2021

2-Chloroethyl Vinyl ether

Response Ratio

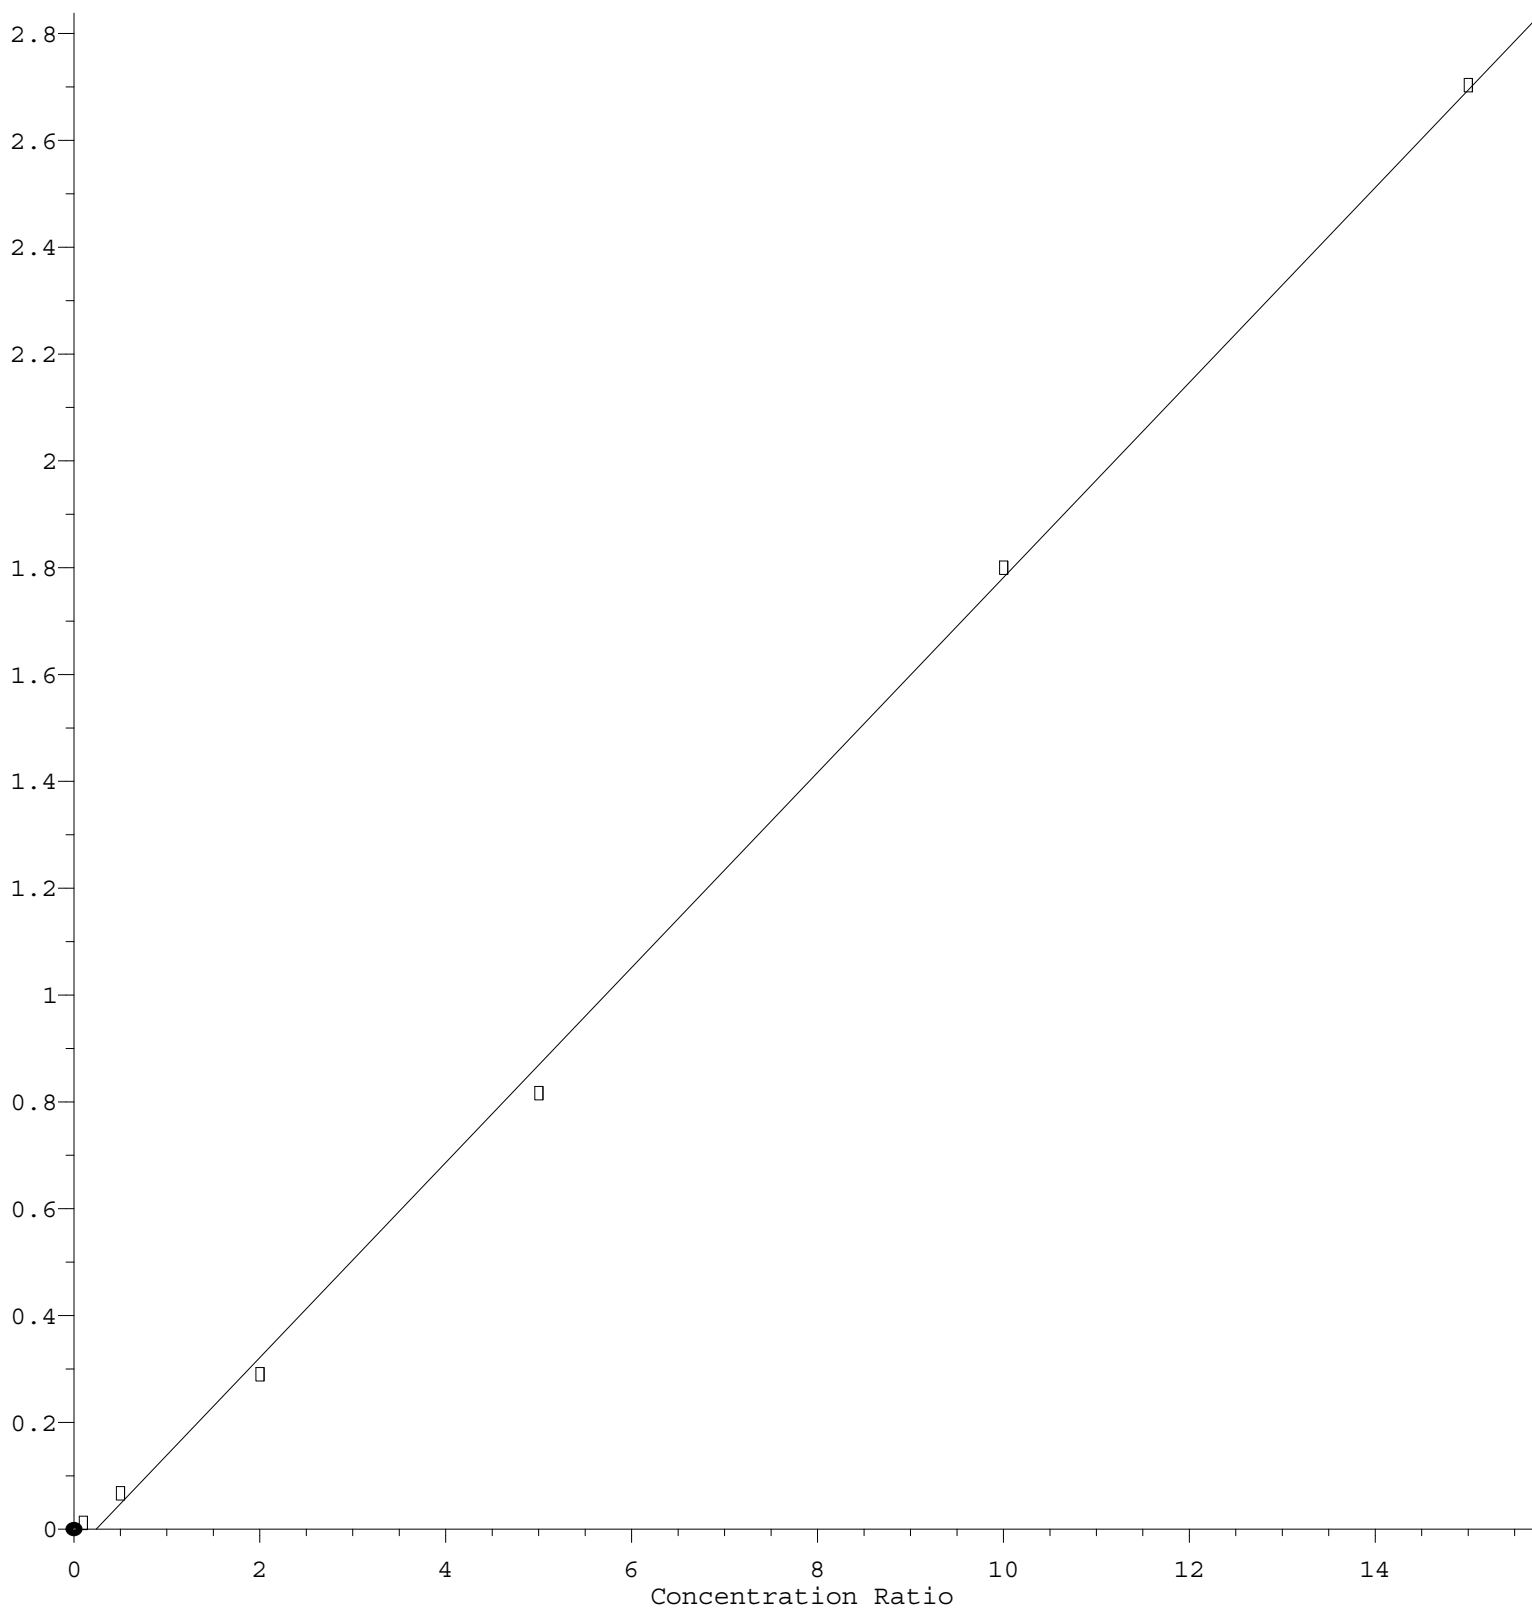

$$\text{Response} = 1.826\text{e-}001 * \text{Amt} - 4.389\text{e-}002$$


Coef of Det (r^2) = 0.998997 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092321W.M

Calibration Table Last Updated: Thu Sep 23 13:52:37 2021

Naphthalene

Response Ratio

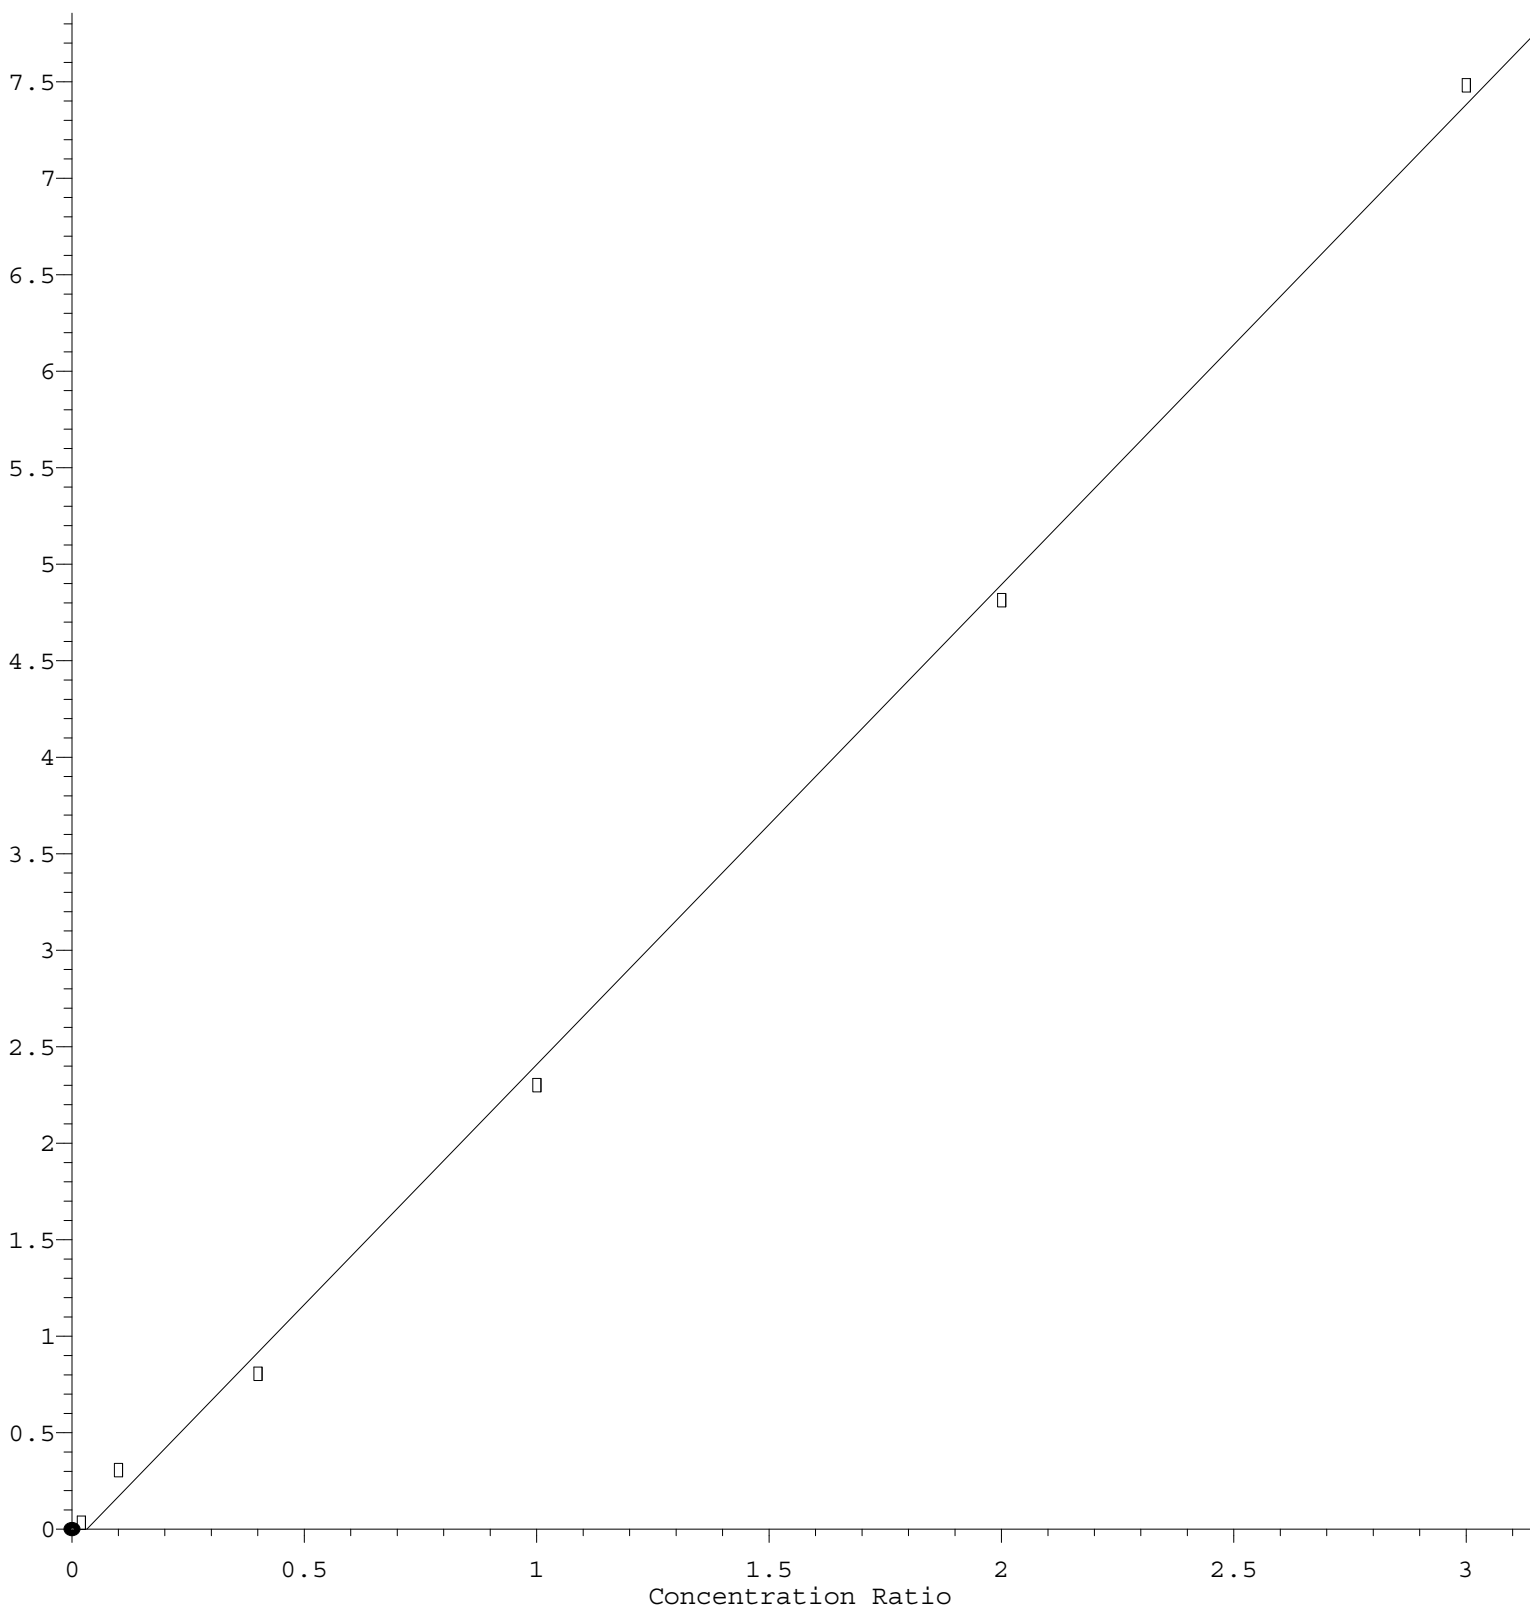

$$\text{Response} = 2.487\text{e}+000 * \text{Amt} - 7.942\text{e}-002$$

Coef of Det (r^2) = 0.998565 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N092321W.M

Calibration Table Last Updated: Thu Sep 23 13:52:37 2021