

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092324\
 Data File : VN084098.D
 Acq On : 23 Sep 2024 10:07
 Operator : JC\MD
 Sample : VN0923WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0923WBL01

Quant Time: Sep 24 01:27:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 11 15:18:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	175531	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	304776	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	258041	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	105851	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	133229	50.337	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 100.680%	
35) Dibromofluoromethane	8.165	113	99082	50.782	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 101.560%	
50) Toluene-d8	10.565	98	362159	53.691	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 107.380%	
62) 4-Bromofluorobenzene	12.847	95	129090	46.387	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 92.780%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092324\
Data File : VN084098.D
Acq On : 23 Sep 2024 10:07
Operator : JC\MD
Sample : VN0923WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0923WBL01


Quant Time: Sep 24 01:27:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 11 15:18:56 2024
Response via : Initial Calibration

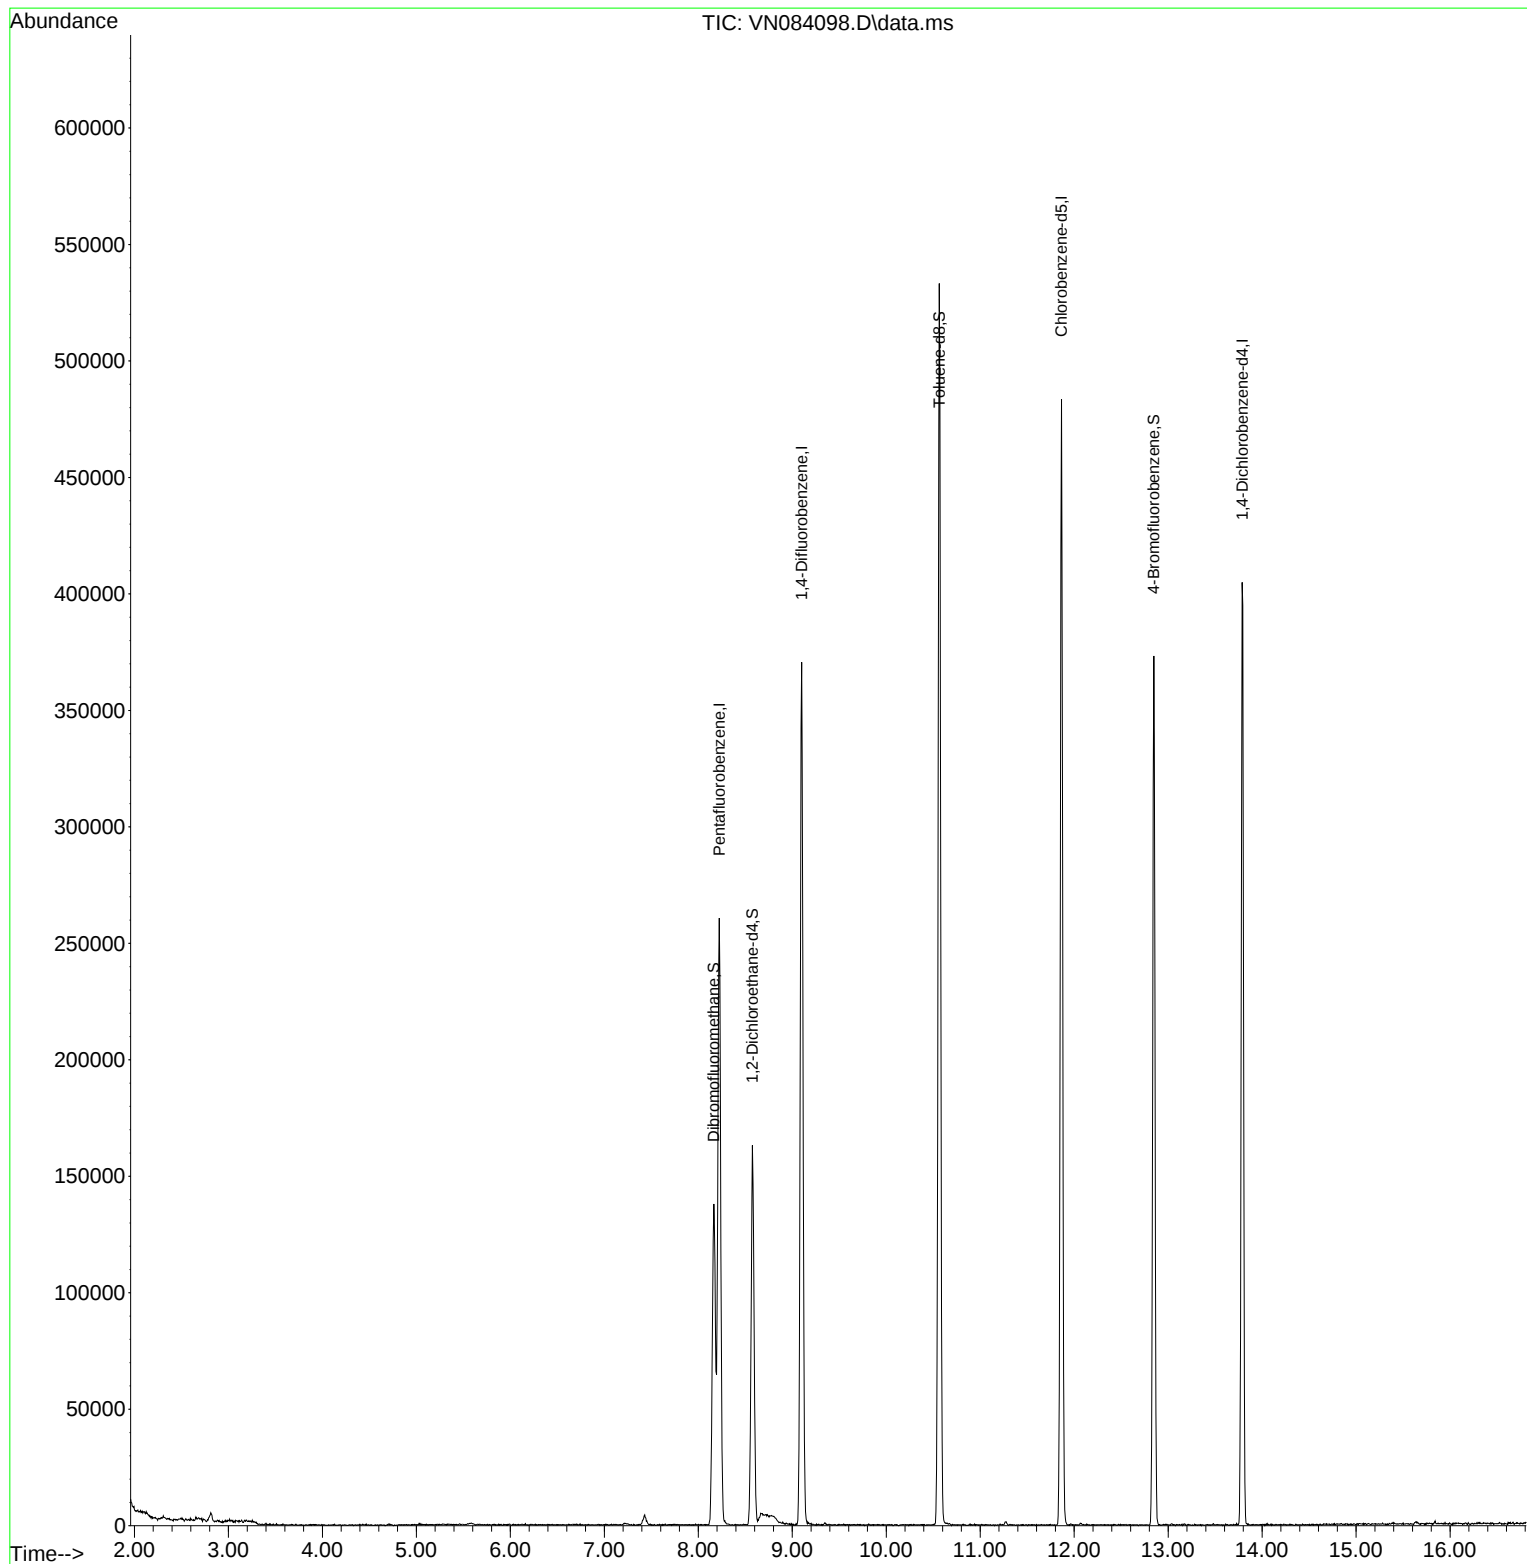



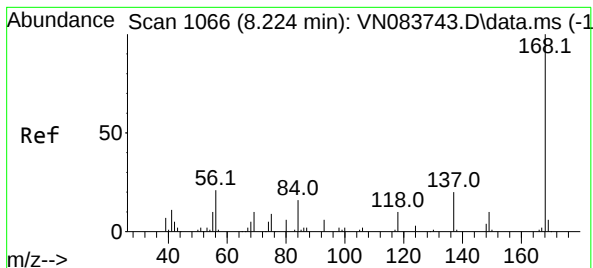


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN084098.D
Acq: 23 Sep 2024 10:07

Instrument :
MSVOA_N
ClientSampleId :
VN0923WBL01



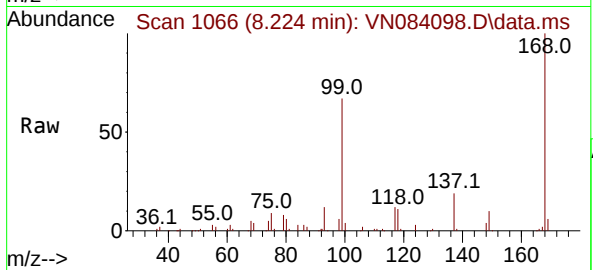


Tgt Ion:168 Resp: 175531
Ion Ratio Lower Upper
168 100
99 66.7 54.2 81.2

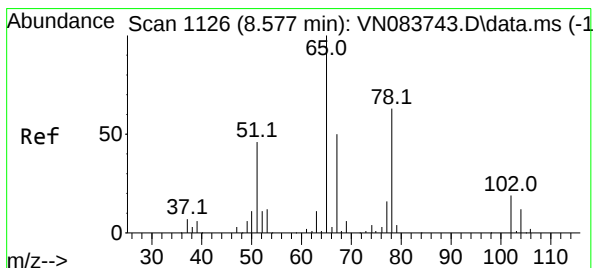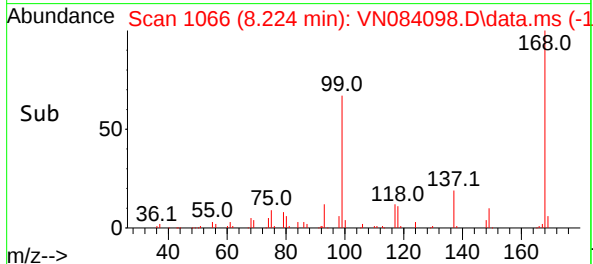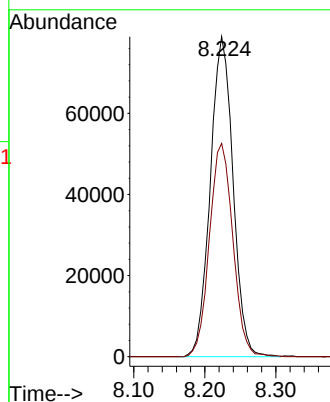

#33
1,2-Dichloroethane-d4
Concen: 50.337 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN084098.D
Acq: 23 Sep 2024 10:07

Tgt Ion: 65 Resp: 133229
Ion Ratio Lower Upper
65 100
67 50.0 0.0 100.8


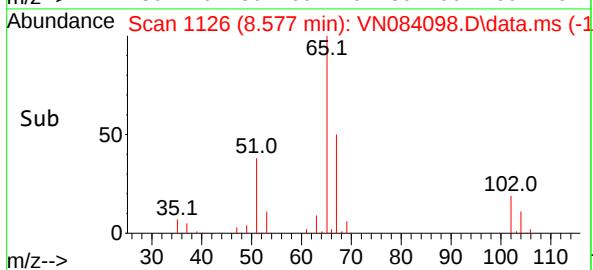
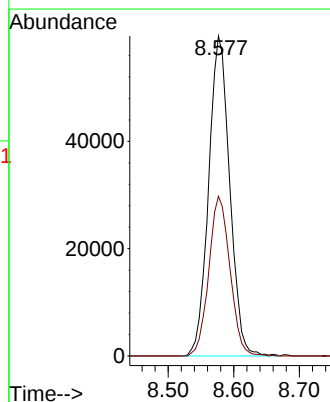
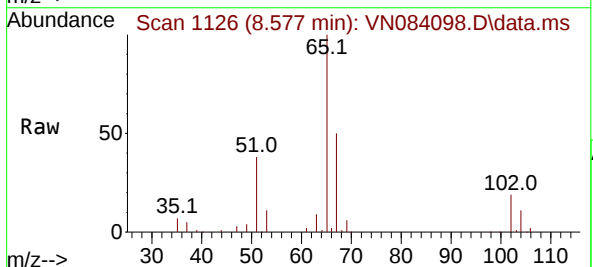




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN084098.D
Acq: 23 Sep 2024 10:07




Instrument :
MSVOA_N
ClientSampleId :
VN0923WBL01


Tgt Ion:114 Resp: 304776
Ion Ratio Lower Upper
114 100
63 22.8 0.0 43.4
88 17.1 0.0 32.6

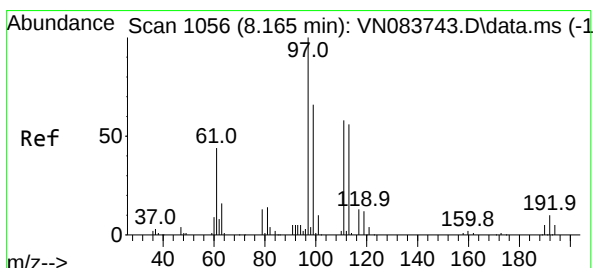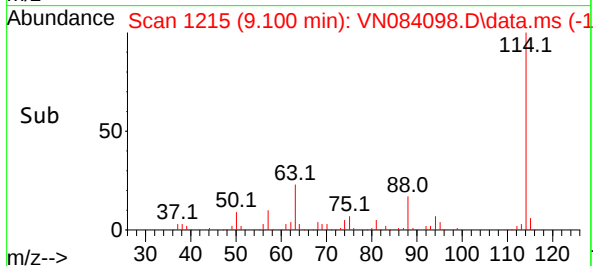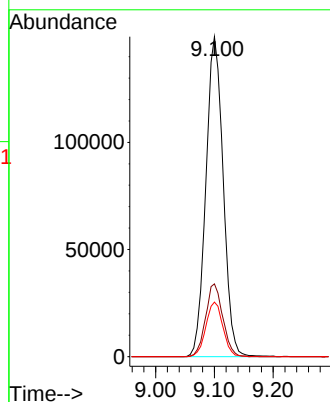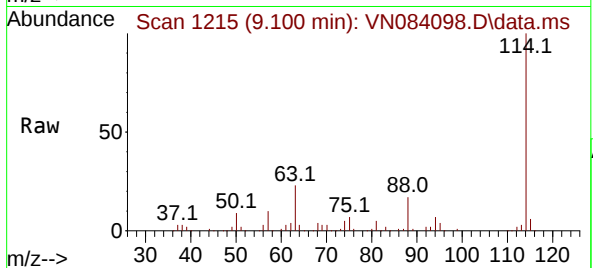

#35
Dibromofluoromethane
Concen: 50.782 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN084098.D
Acq: 23 Sep 2024 10:07

Tgt Ion:113 Resp: 99082
Ion Ratio Lower Upper
113 100
111 102.2 82.6 124.0
192 16.9 14.3 21.5


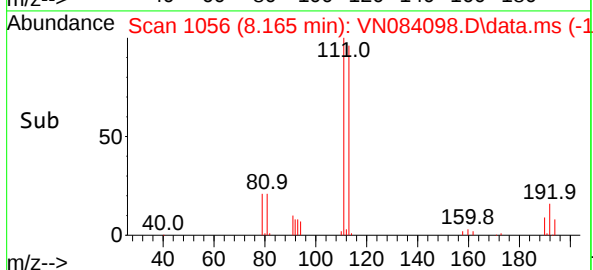
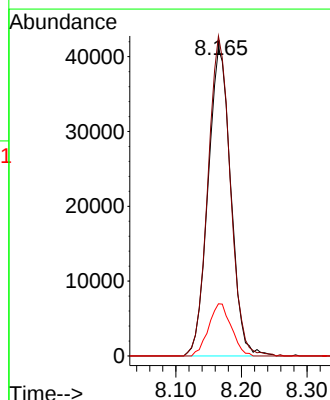
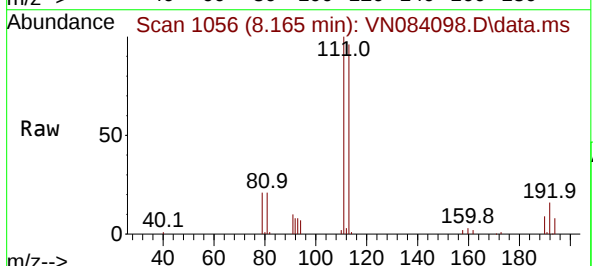


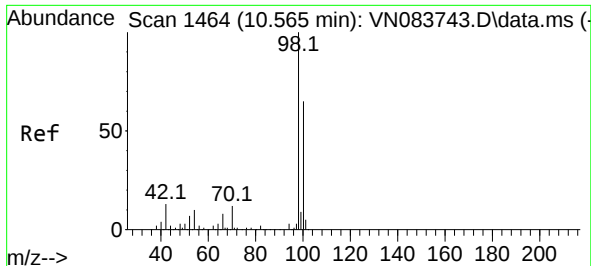

#50
Toluene-d8
Concen: 53.691 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN084098.D
Acq: 23 Sep 2024 10:07




Instrument :
MSVOA_N
ClientSampleId :
VN0923WBL01


Tgt Ion: 98 Resp: 362159
Ion Ratio Lower Upper
98 100
100 64.8 52.0 78.0

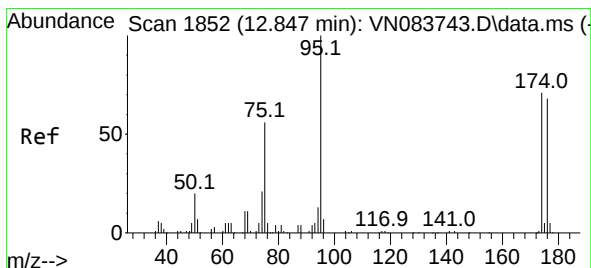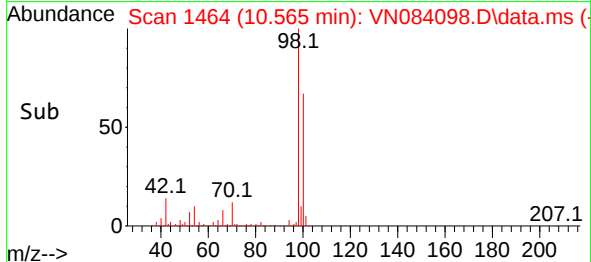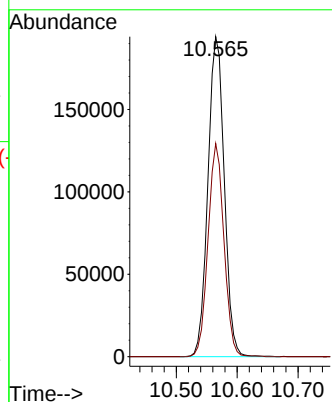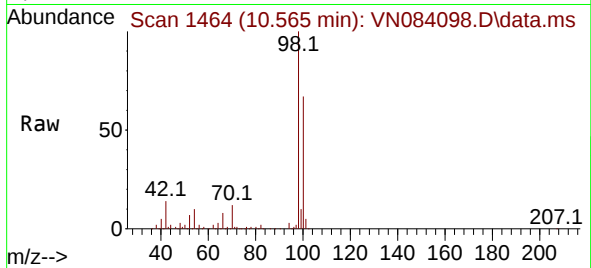

#62
4-Bromofluorobenzene
Concen: 46.387 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN084098.D
Acq: 23 Sep 2024 10:07

Tgt Ion: 95 Resp: 129090
Ion Ratio Lower Upper
95 100
174 71.2 0.0 139.8
176 67.8 0.0 131.4


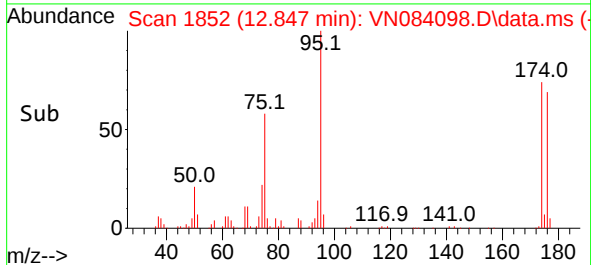
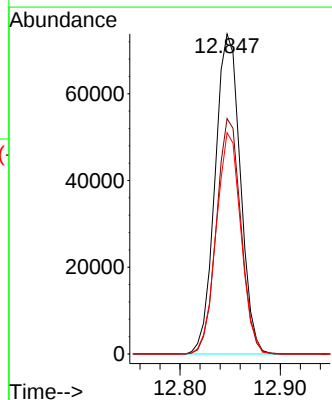
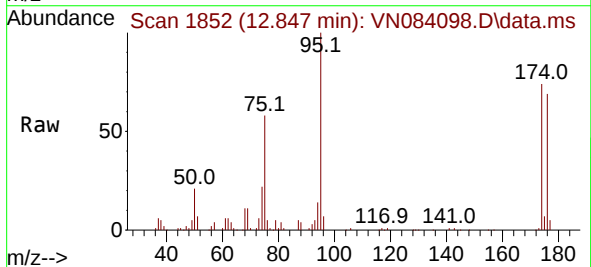


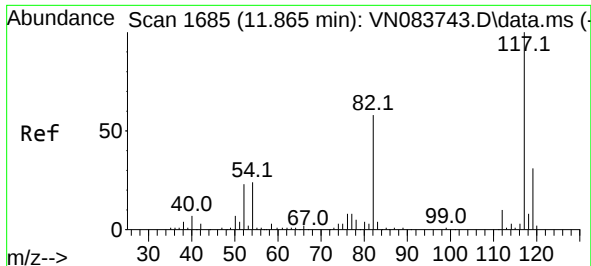

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN084098.D
Acq: 23 Sep 2024 10:07

Instrument :
MSVOA_N
ClientSampleId :
VN0923WBL01

Tgt Ion:117 Resp: 258041
Ion Ratio Lower Upper
117 100
82 59.2 47.4 71.0
119 32.6 26.3 39.5

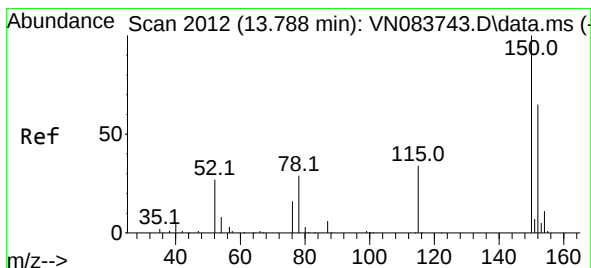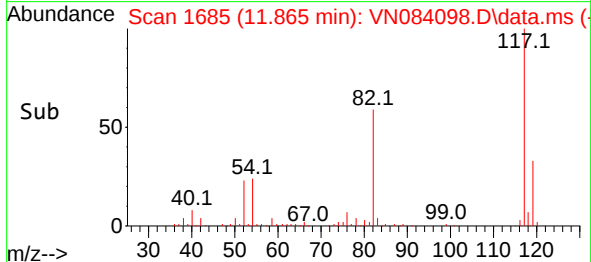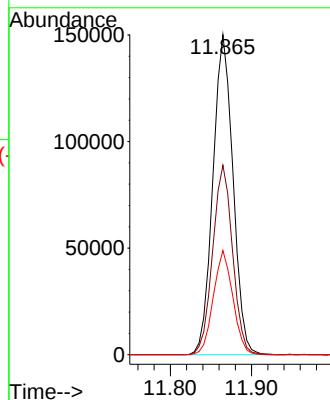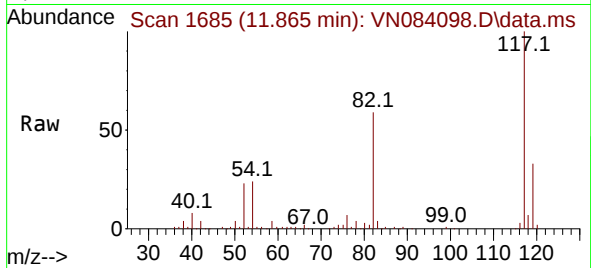

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN084098.D
Acq: 23 Sep 2024 10:07

Tgt Ion:152 Resp: 105851
Ion Ratio Lower Upper
152 100
115 62.6 32.2 96.6
150 157.4 0.0 348.6

