
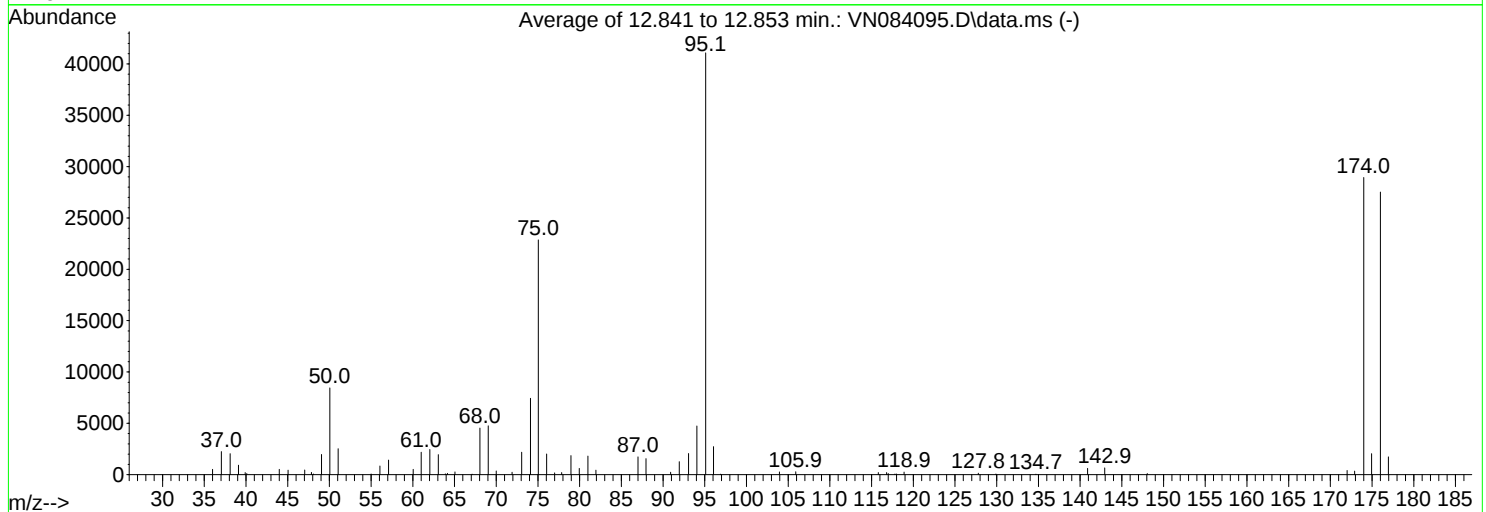


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092324\
Data File : VN084095.D
Acq On : 23 Sep 2024 08:33
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

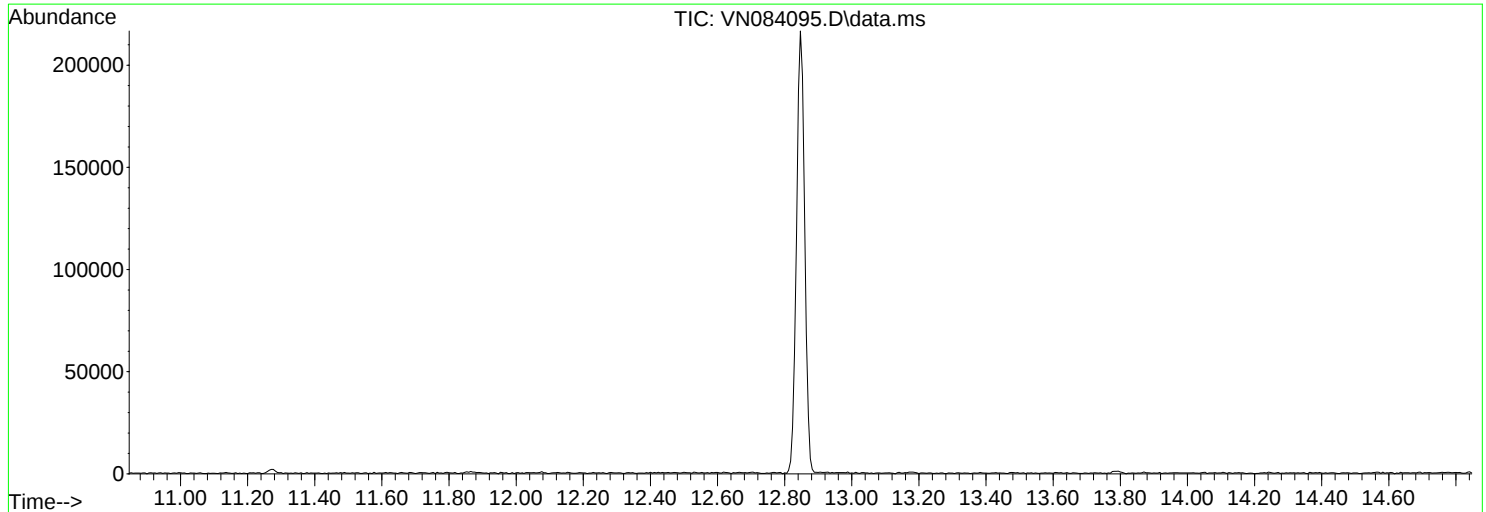

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	8449	PASS
75	95	30	60	55.7	22867	PASS
95	95	100	100	100.0	41083	PASS
96	95	5	9	6.6	2722	PASS
173	174	0.00	2	1.2	338	PASS
174	95	50	100	70.5	28944	PASS
175	174	5	9	7.1	2046	PASS
176	174	95	101	95.1	27523	PASS
177	176	5	9	6.3	1738	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	518	49.05	1959	64.15	118	77.00	161
37.05	2250	50.05	8449	65.05	269	77.85	207
38.10	2045	51.05	2520	67.10	55	78.95	186
39.10	923	55.00	68	68.05	4533	79.95	60
39.90	200	56.05	847	69.05	4752	81.00	1814
40.10	105	57.10	1427	70.00	356	81.95	431
44.00	519	60.05	513	71.90	236	87.00	1735
45.05	432	61.00	2190	73.05	2191	87.95	1561
47.05	447	62.05	2445	74.10	7434	90.90	232
47.85	224	63.05	1950	75.05	22867	91.95	1267
48.10	65	63.90	72	76.05	2015	93.05	2063

Average of 12.841 to 12.853 min.: VN084095.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	4734	118.90	247	176.00	27523		
95.10	41083	127.80	141	176.95	1738		
96.05	2722	129.90	64				
96.90	53	134.70	55				
103.95	265	140.90	616				
105.90	288	142.95	654				
115.80	198	148.05	111				
116.80	204	172.00	401				
117.00	111	172.90	338				
117.80	65	174.00	28944				
118.00	71	174.95	2046				

Instrument :

MSVOA_N

ClientSampleId :

BFB