


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN092418\
Data File : VN051445.D
Acq On : 24 Sep 2018 7:54
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N092318W.M
Title : SW846 8260
Last Update : Mon Sep 24 06:41:32 2018

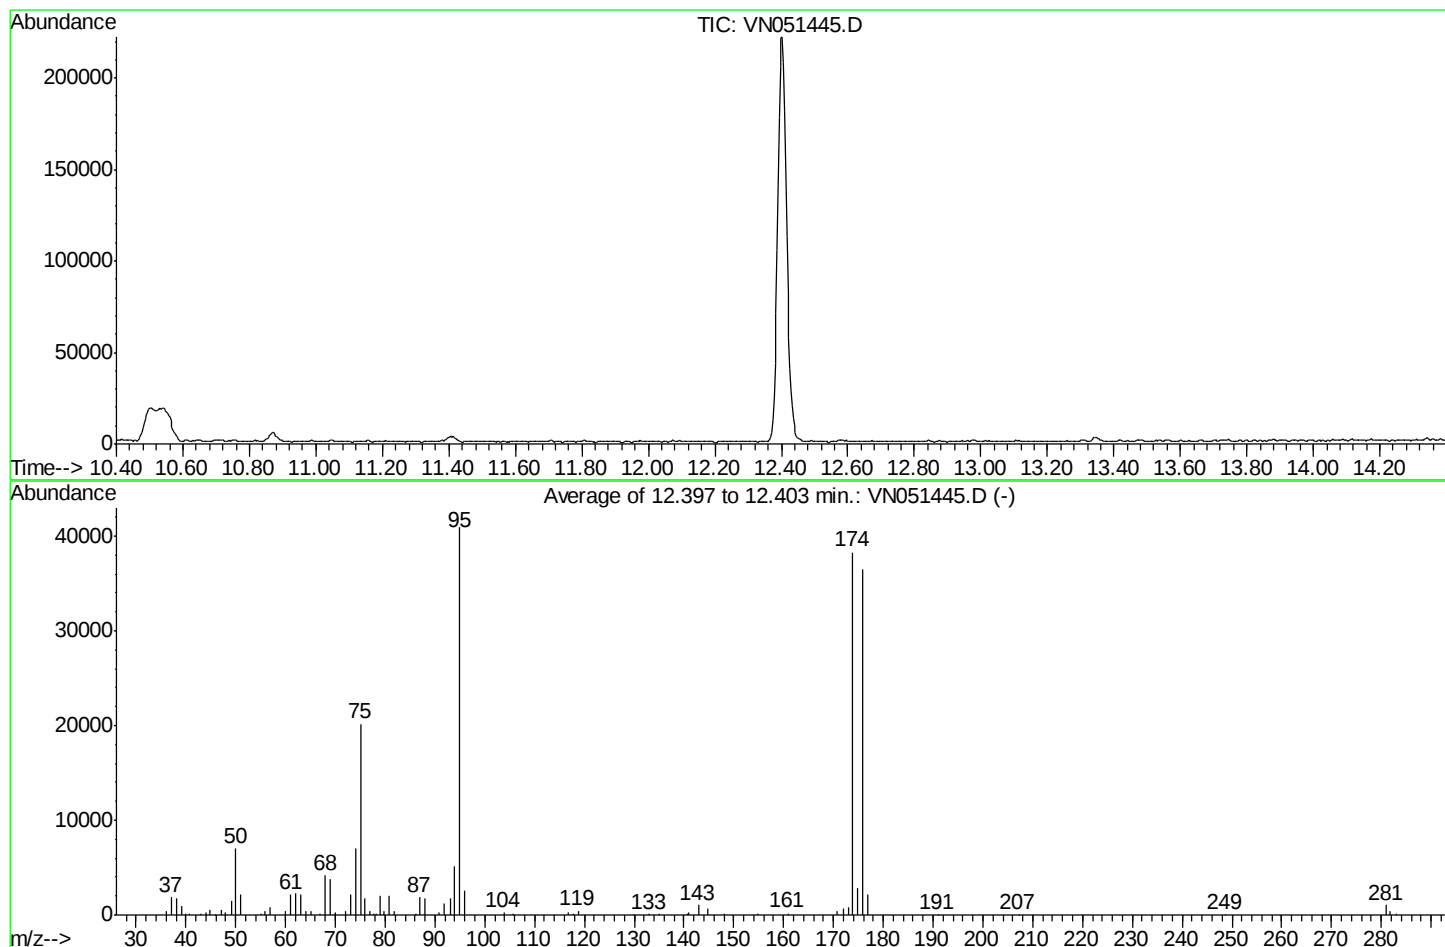

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	6987	PASS
75	95	30	60	49.3	20184	PASS
95	95	100	100	100.0	40922	PASS
96	95	5	9	6.3	2582	PASS
173	174	0.00	2	2.0	759	PASS
174	95	50	100	93.6	38309	PASS
175	174	5	9	7.6	2909	PASS
176	174	95	101	95.4	36549	PASS
177	176	5	9	5.8	2126	PASS