


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN092419\
Data File : VN058335.D
Acq On : 24 Sep 2019 9:15
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N092419W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Sep 25 01:36:25 2019

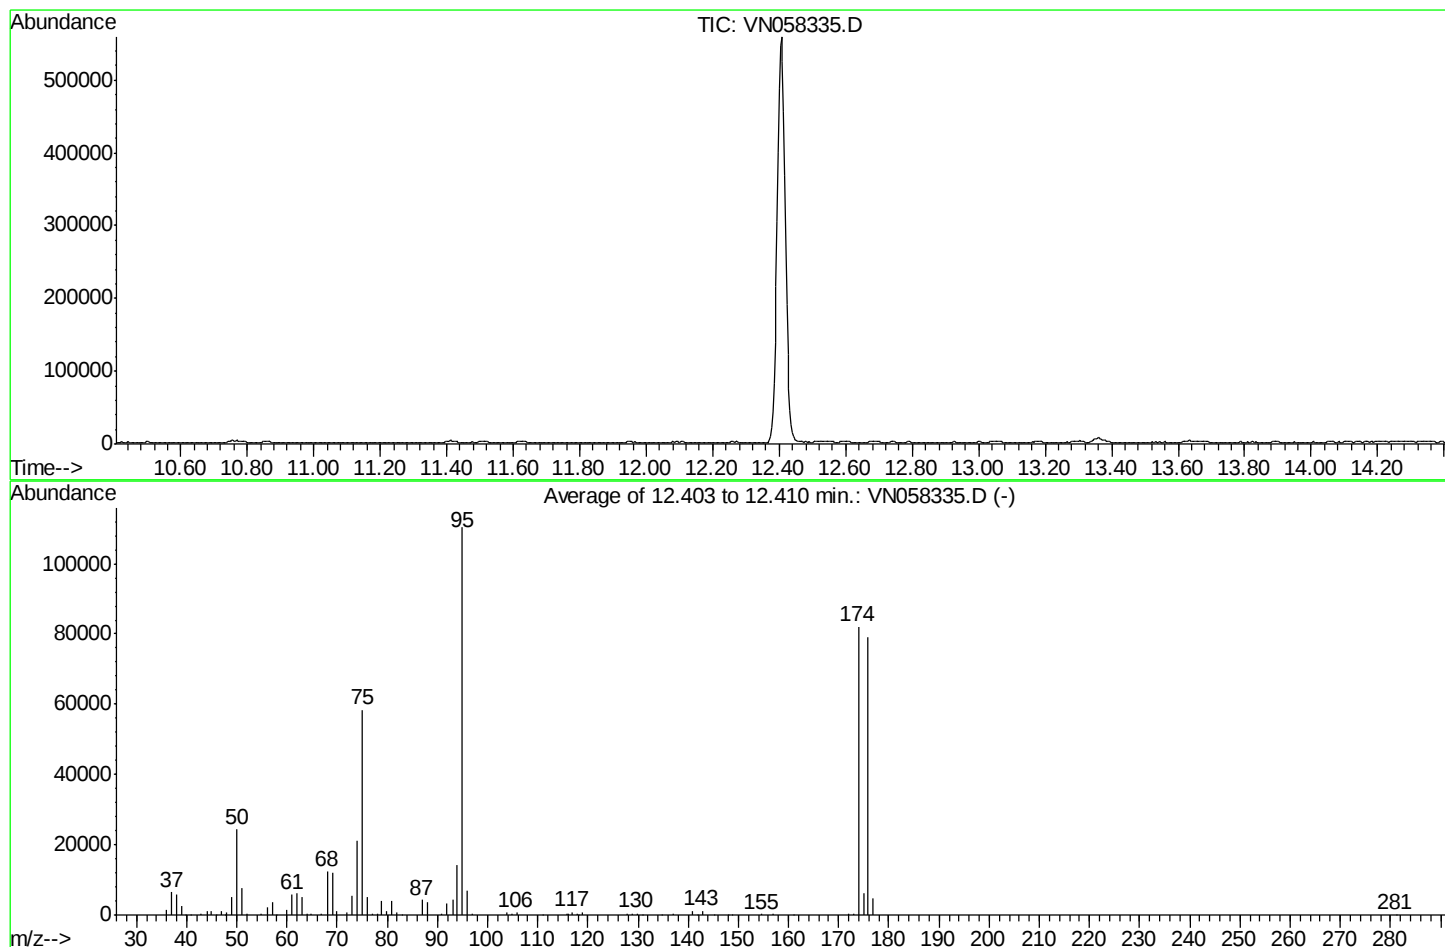

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	24397	PASS
75	95	30	60	53.0	58453	PASS
95	95	100	100	100.0	110362	PASS
96	95	5	9	6.2	6880	PASS
173	174	0.00	2	0.5	404	PASS
174	95	50	100	74.4	82109	PASS
175	174	5	9	7.6	6225	PASS
176	174	95	101	96.5	79266	PASS
177	176	5	9	5.9	4707	PASS