
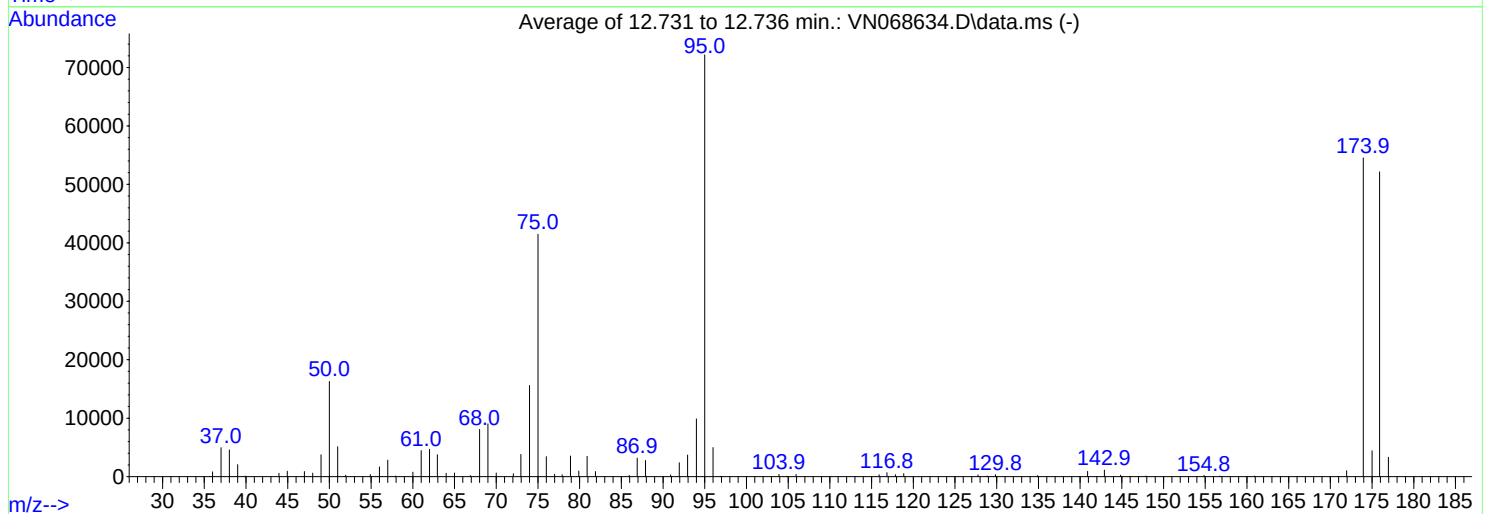


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092421\
Data File : VN068634.D
Acq On : 24 Sep 2021 11:34
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092321W.M
Title : SW846 8260
Last Update : Thu Sep 23 13:52:37 2021

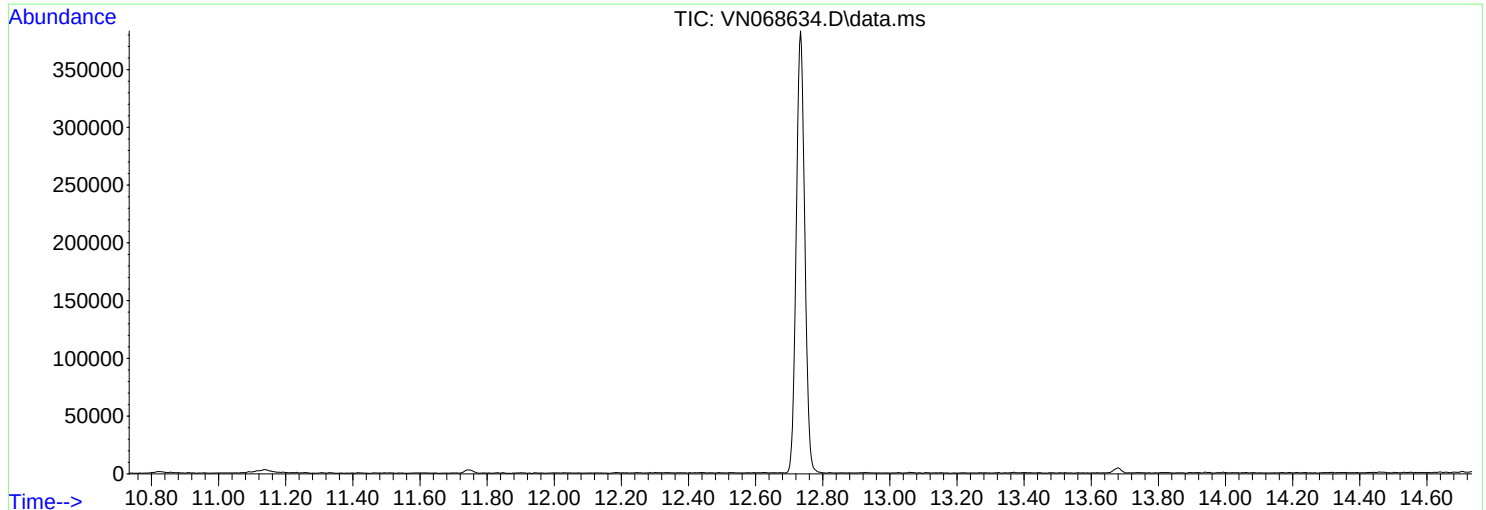

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	16292	PASS
75	95	30	60	57.5	41467	PASS
95	95	100	100	100.0	72160	PASS
96	95	5	9	6.9	4978	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.6	54531	PASS
175	174	5	9	8.1	4444	PASS
176	174	95	101	95.6	52141	PASS
177	176	5	9	6.4	3323	PASS