

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN092424\  
Data File : VN084131.D  
Acq On : 24 Sep 2024 13:55  
Operator : JC\MD  
Sample : P4116-04  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
DUPE04-20240916

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N091024W.M

Title : SW846 8260

Signal : TIC: VN084131.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 8.165       | 1045          | 1056        | 1061         | rBV2     | 121723         | 290958        | 34.70%          | 6.743%        |
| 2         | 8.224       | 1061          | 1066        | 1076         | rVB      | 214750         | 474477        | 56.58%          | 10.996%       |
| 3         | 8.577       | 1115          | 1126        | 1138         | rBV      | 136970         | 306861        | 36.59%          | 7.111%        |
| 4         | 9.100       | 1207          | 1215        | 1226         | rBV      | 311325         | 629957        | 75.12%          | 14.599%       |
| 5         | 10.565      | 1456          | 1464        | 1475         | rBV      | 457496         | 838605        | 100.00%         | 19.434%       |
| 6         | 11.865      | 1677          | 1685        | 1699         | rBV      | 395246         | 704760        | 84.04%          | 16.333%       |
| 7         | 12.847      | 1845          | 1852        | 1860         | rBV      | 314778         | 517636        | 61.73%          | 11.996%       |
| 8         | 13.788      | 2005          | 2012        | 2023         | rVB      | 325743         | 551794        | 65.80%          | 12.788%       |




Sum of corrected areas: 4315048

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN092424\  
Data File : VN084131.D  
Acq On : 24 Sep 2024 13:55  
Operator : JC\MD  
Sample : P4116-04  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
DUPE04-20240916

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N091024W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

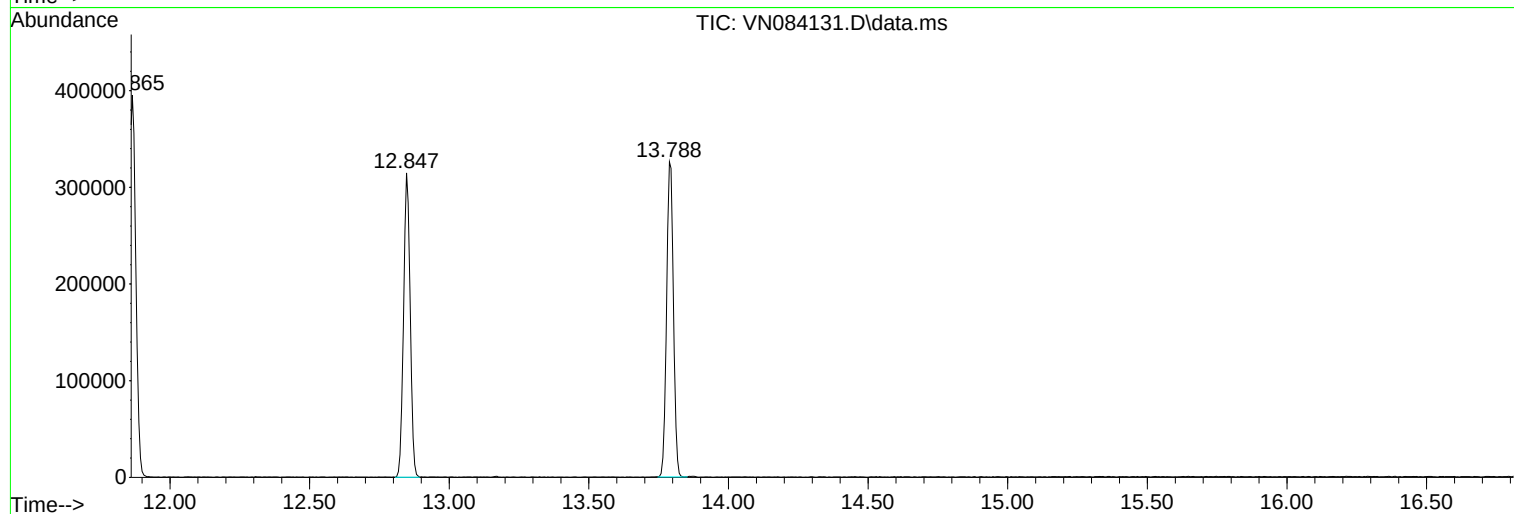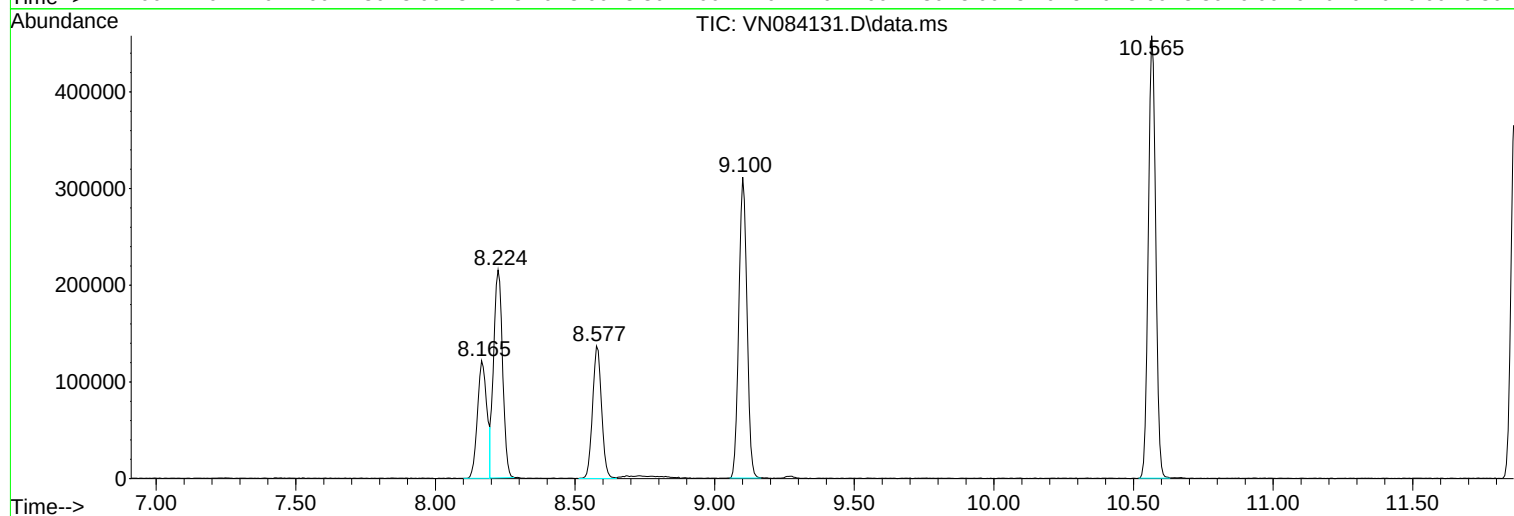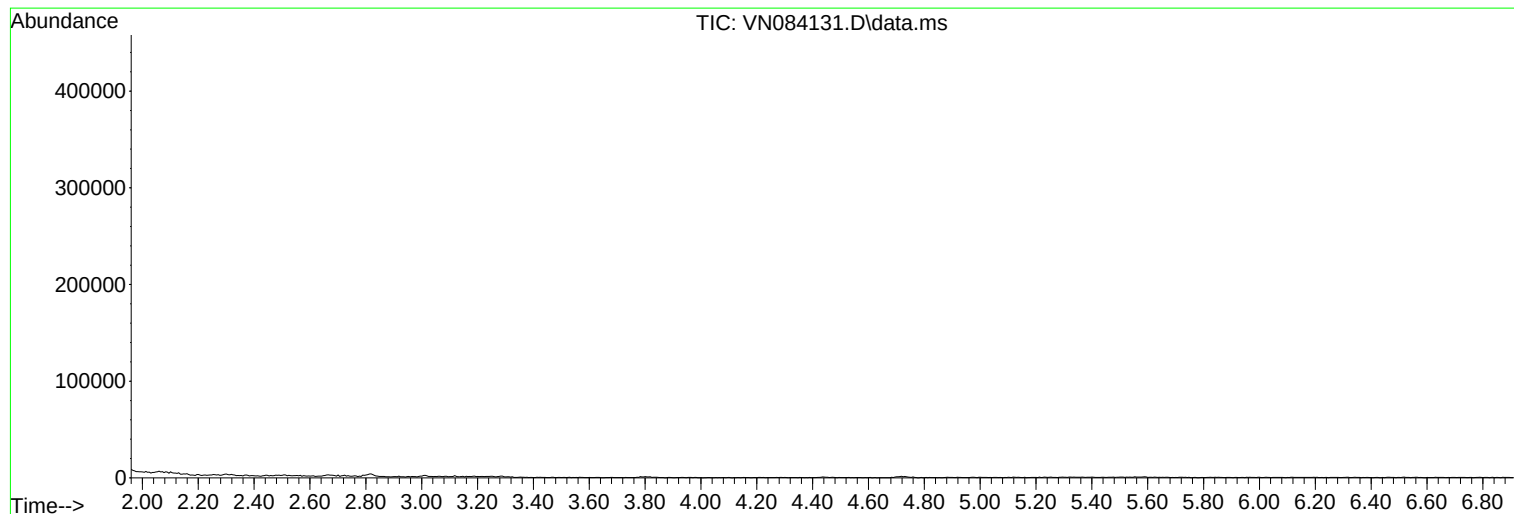

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN092424\  
Data File : VN084131.D  
Acq On : 24 Sep 2024 13:55  
Operator : JC\MD  
Sample : P4116-04  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
DUPE04-20240916

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N091024W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN092424\  
Data File : VN084131.D  
Acq On : 24 Sep 2024 13:55  
Operator : JC\MD  
Sample : P4116-04  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
DUPE04-20240916

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N091024W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |