
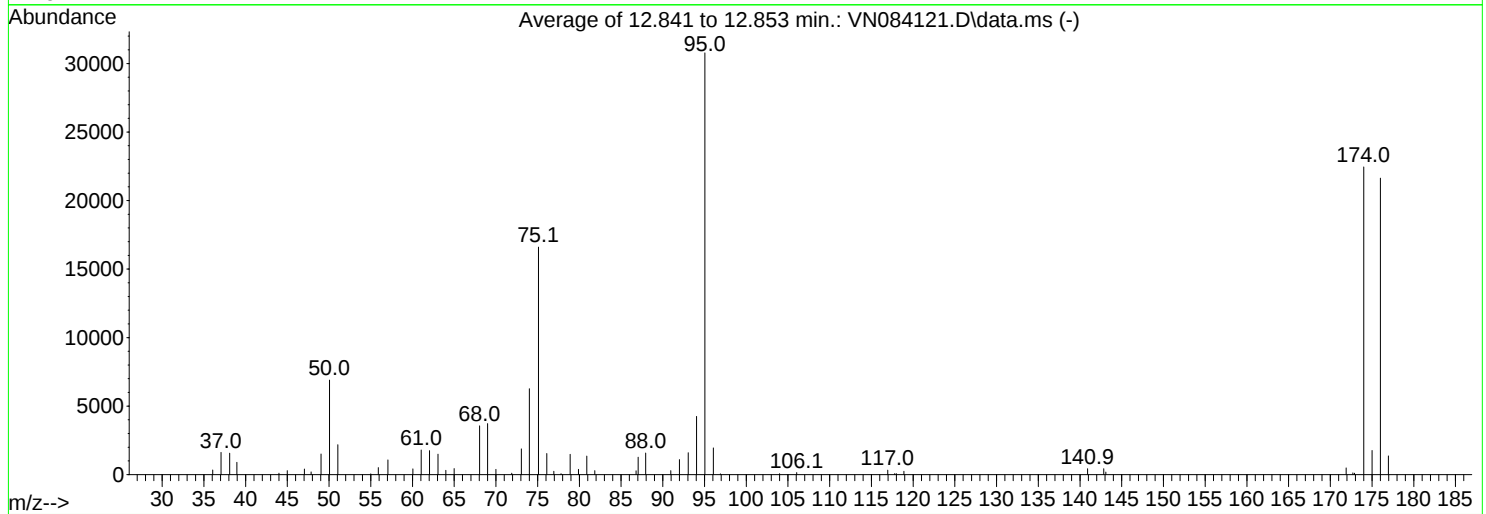


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092424\
Data File : VN084121.D
Acq On : 24 Sep 2024 08:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

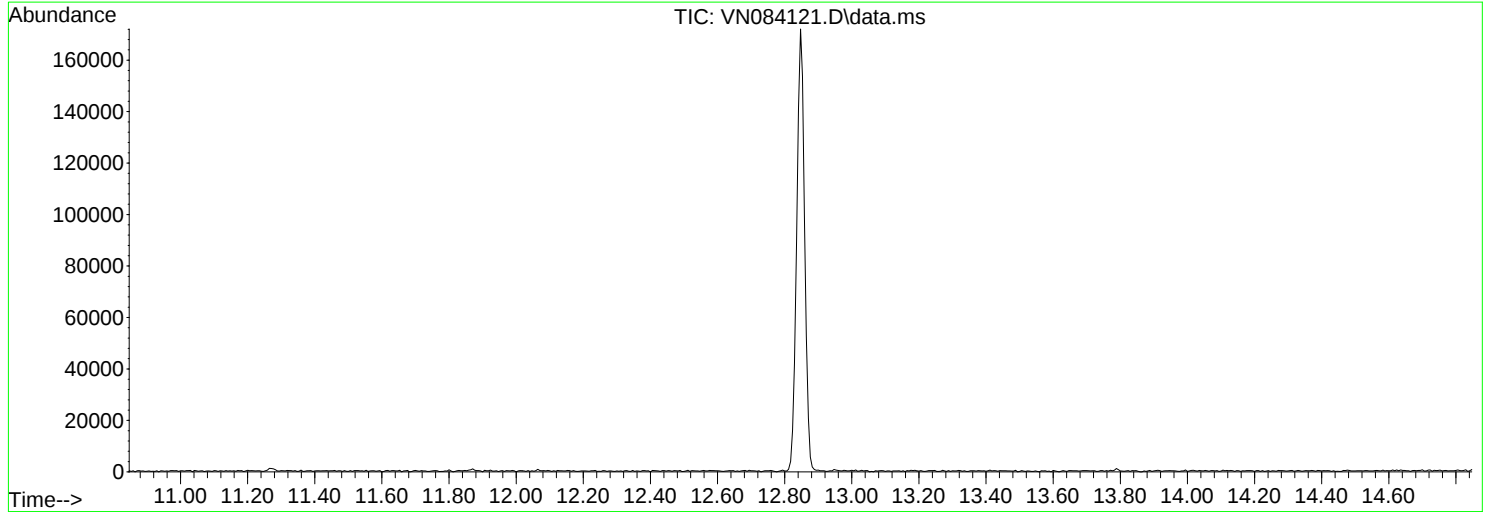

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	6900	PASS
75	95	30	60	53.9	16598	PASS
95	95	100	100	100.0	30779	PASS
96	95	5	9	6.3	1948	PASS
173	174	0.00	2	0.6	132	PASS
174	95	50	100	73.0	22456	PASS
175	174	5	9	7.8	1761	PASS
176	174	95	101	96.3	21632	PASS
177	176	5	9	6.3	1371	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	337	55.00	54	70.00	381	81.85	281
37.05	1618	55.90	512	71.90	107	86.80	281
38.10	1568	57.05	1070	73.05	1883	87.05	1271
38.95	904	60.05	424	74.00	6269	87.95	1571
44.00	110	61.05	1799	75.10	16598	90.95	289
45.00	293	62.05	1753	76.10	1546	92.00	1102
47.05	405	63.05	1493	76.95	250	93.05	1603
47.85	198	64.00	317	77.80	66	94.05	4248
49.05	1508	65.00	448	78.90	1481	95.05	30779
50.05	6900	68.05	3558	79.90	384	96.05	1948
51.05	2187	69.00	3727	80.90	1356	96.90	62

Average of 12.841 to 12.853 min.: VN084121.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
104.00	68	172.90	108				
106.05	147	174.00	22456				
116.95	328	175.00	1761				
117.80	79	176.00	21632				
118.00	74	176.95	1371				
118.90	248						
140.90	438						
142.85	438						
143.10	192						
171.90	494						
172.70	132						

Instrument :

MSVOA_N

ClientSampleId :

BFB