
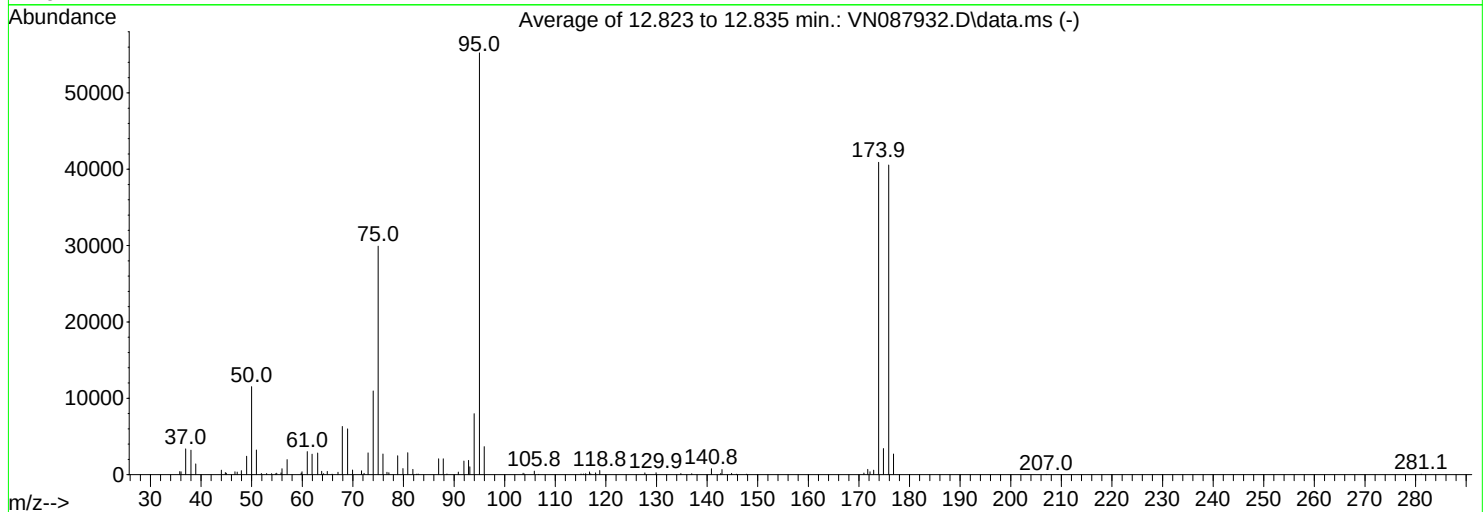


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092425\
Data File : VN087932.D
Acq On : 24 Sep 2025 07:41
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092325W.M
Title : SW846 8260
Last Update : Wed Sep 24 05:05:30 2025

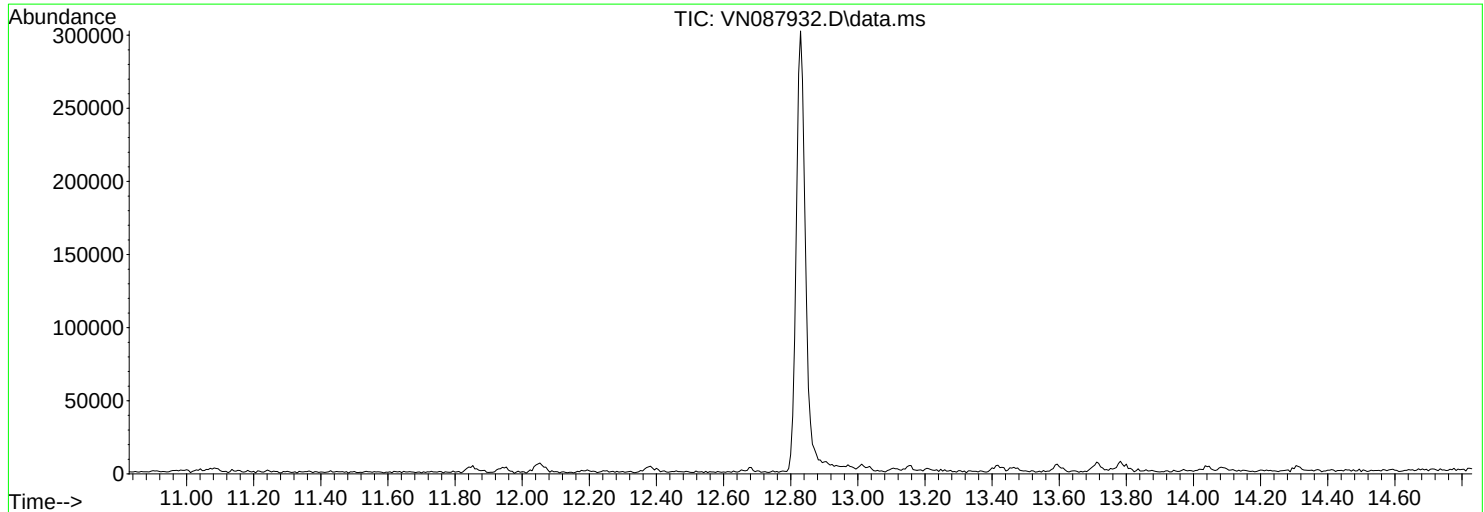

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	11523	PASS
75	95	30	60	54.2	29931	PASS
95	95	100	100	100.0	55245	PASS
96	95	5	9	6.7	3678	PASS
173	174	0.00	2	1.4	589	PASS
174	95	50	100	74.1	40912	PASS
175	174	5	9	8.4	3418	PASS
176	174	95	101	99.1	40560	PASS
177	176	5	9	6.7	2698	PASS

Average of 12.823 to 12.835 min.: VN087932.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	395	49.00	2406	59.80	203	68.95	599
36.05	382	50.00	11523	59.95	385	69.95	611
36.95	3368	50.95	3230	61.00	3027	71.70	50
38.00	3212	51.90	140	61.95	2691	72.20	16
38.95	1408	52.95	144	63.05	2821	73.00	2844
44.00	581	53.95	135	63.85	439	74.00	10971
44.80	282	54.70	111	64.20	120	75.00	29931
45.00	198	54.95	188	64.95	423	75.95	2699
46.70	382	55.80	227	65.90	55	76.75	314
47.15	342	56.00	769	67.05	320	77.10	249
47.95	523	57.00	1967	67.90	6304	78.85	2472

Average of 12.823 to 12.835 min.: VN087932.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.90	791	93.10	1029	116.75	362	144.85	163
80.85	2871	93.95	7977	117.00	115	145.80	61
81.85	702	95.00	55245	117.95	234	147.80	72
82.60	59	95.95	3678	118.80	550	171.00	211
82.90	91	103.65	184	127.70	233	171.75	682
86.95	2077	103.90	92	129.90	256	172.20	374
87.85	2068	105.85	455	134.80	146	172.90	589
88.60	84	106.70	50	136.95	116	173.90	40912
90.85	334	115.10	84	140.85	786	174.85	3418
91.95	1783	115.60	76	142.70	152	175.90	40560
92.85	1872	116.00	120	142.95	676	176.85	2698

Average of 12.823 to 12.835 min.: VN087932.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
207.00	35						
281.10	59						

Instrument :

MSVOA_N

ClientSampleId :

BFB