


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN092518\  
Data File : VN051471.D  
Acq On : 25 Sep 2018 8:10  
Operator : MD\SY  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\624N092518W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Wed Sep 26 01:56:49 2018

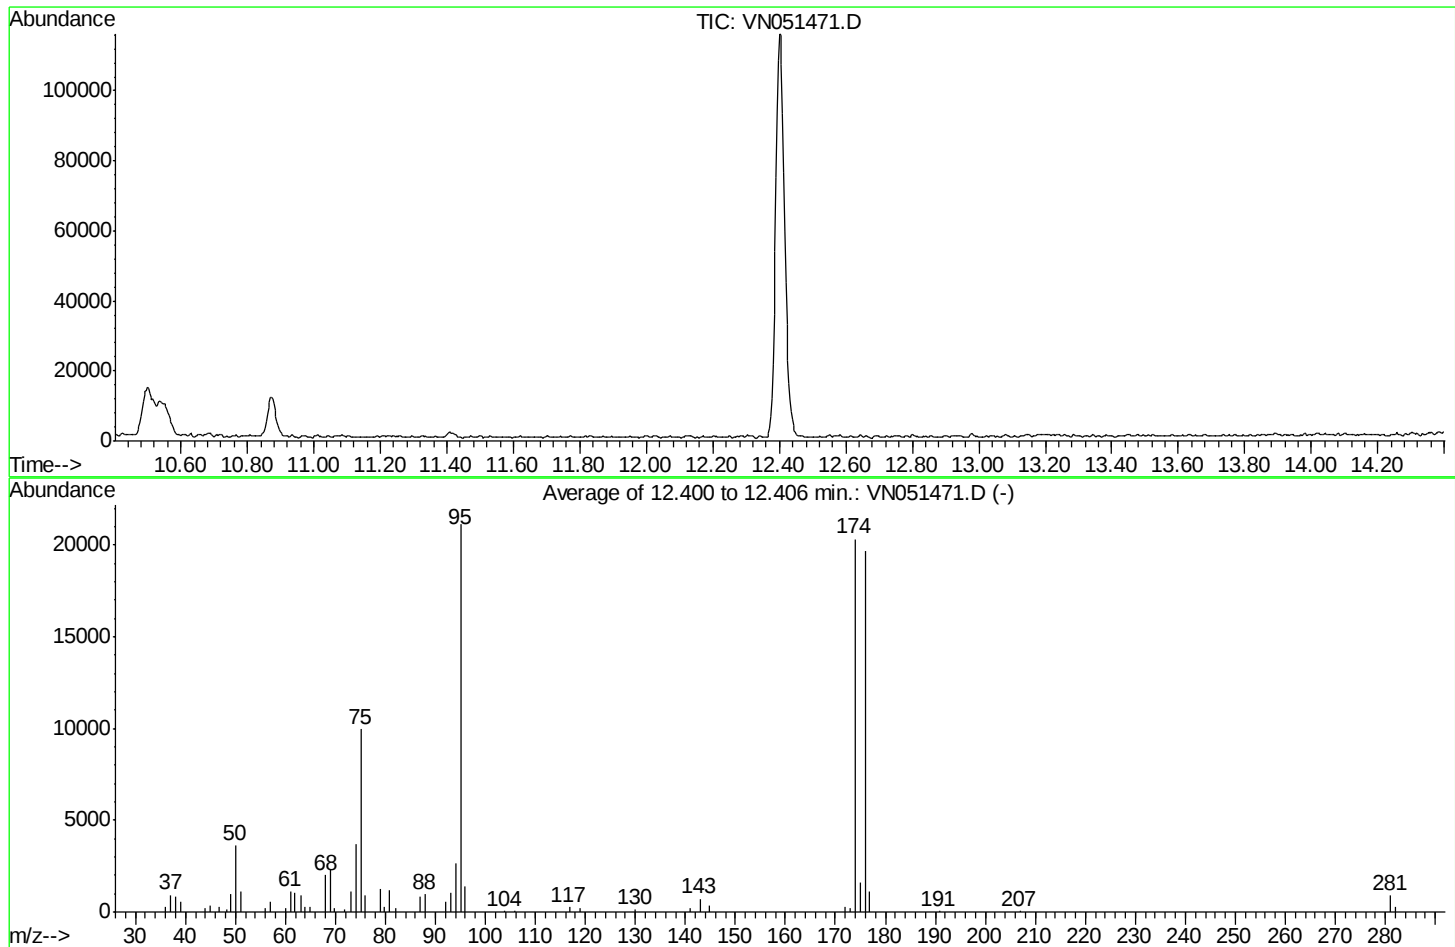

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3293

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.0      | 3596    | PASS             |
| 75          | 95           | 30           | 60           | 47.2      | 9969    | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 21133   | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 1399    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.1       | 225     | PASS             |
| 174         | 95           | 50           | 100          | 96.2      | 20322   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 1629    | PASS             |
| 176         | 174          | 95           | 101          | 96.8      | 19669   | PASS             |
| 177         | 176          | 5            | 9            | 5.5       | 1087    | PASS             |