


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN092519\
 Data File : VN058349.D
 Acq On : 25 Sep 2019 8:22
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091819W.M
 Title : SW846 8260
 Last Update : Thu Sep 19 09:27:53 2019

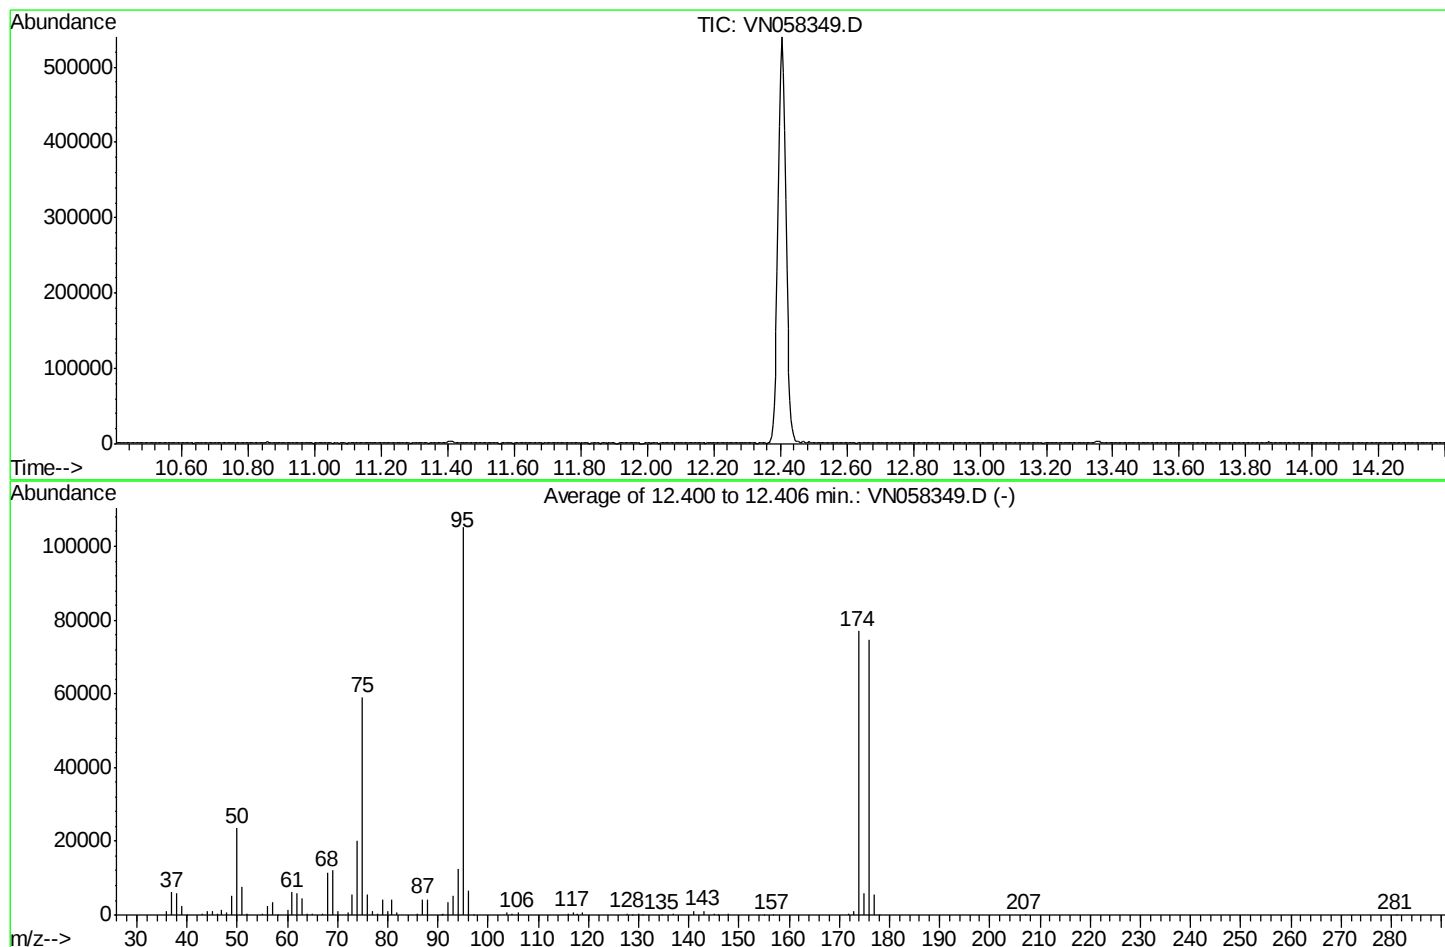

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	23477	PASS
75	95	30	60	56.1	59018	PASS
95	95	100	100	100.0	105146	PASS
96	95	5	9	6.2	6508	PASS
173	174	0.00	2	1.3	1026	PASS
174	95	50	100	73.2	76960	PASS
175	174	5	9	7.6	5861	PASS
176	174	95	101	97.1	74717	PASS
177	176	5	9	7.3	5428	PASS