


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092520\
 Data File : VN063672.D
 Acq On : 25 Sep 2020 10:28
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091620W.M
 Title : SW846 8260
 Last Update : Wed Sep 16 13:05:20 2020

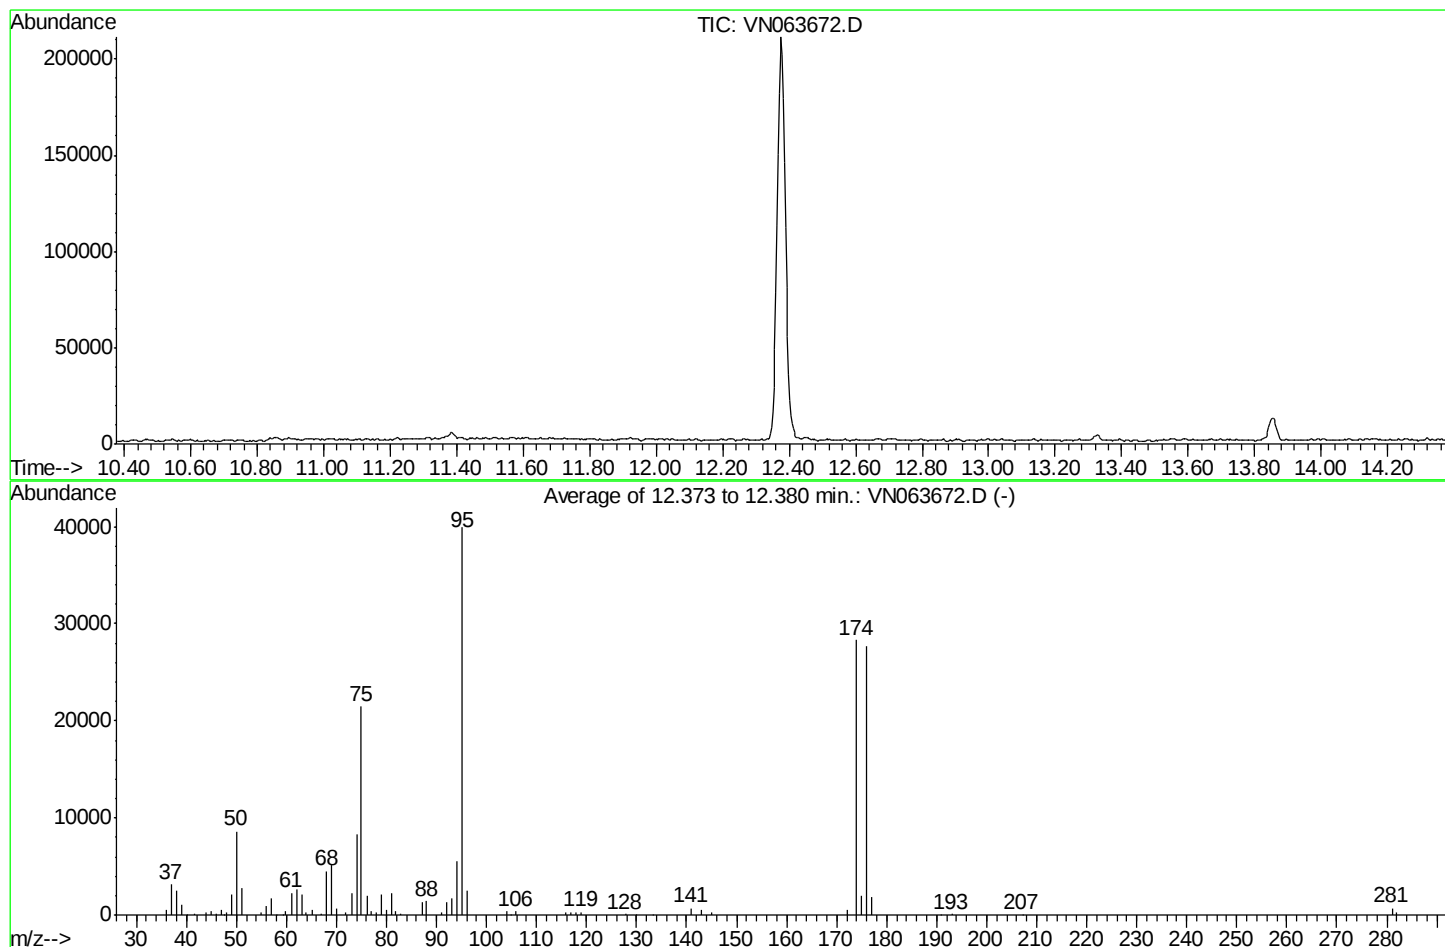

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	8578	PASS
75	95	30	60	53.8	21474	PASS
95	95	100	100	100.0	39930	PASS
96	95	5	9	6.4	2557	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.0	28333	PASS
175	174	5	9	7.0	1992	PASS
176	174	95	101	97.9	27746	PASS
177	176	5	9	6.4	1788	PASS