

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092521\
 Data File : VN068669.D
 Acq On : 25 Sep 2021 15:53
 Operator : JC/MD
 Sample : PB139323TB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB139323TB

Quant Time: Sep 27 04:44:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092321W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 23 13:52:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	515459	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.971	114	838255	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	838306	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	363104	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	397189	49.366	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	98.740%
35) Dibromofluoromethane	8.024	113	296459	52.881	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	105.760%
50) Toluene-d8	10.443	98	1277644	53.742	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	107.480%
62) 4-Bromofluorobenzene	12.734	95	578483	71.149	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	142.300%#


Target Compounds				Qvalue		
5) Bromomethane	2.869	94	858	Below Cal	#	72
6) Chloroethane	2.952	64	219	Below Cal	#	80
11) Tert butyl alcohol	5.363	59	640	0.517	ug/l	# 71
13) Acrolein	4.041	56	260	7.475	ug/l	# 67
16) Acetone	4.293	43	109770	27.395	ug/l	97
18) Methyl Acetate	4.870	43	7391	0.624	ug/l	# 58
20) Methylene Chloride	5.101	84	27315	2.595	ug/l	90
25) 2-Butanone	7.337	43	26746	5.452	ug/l	100
29) Tetrahydrofuran	7.697	42	2735	0.877	ug/l	# 75
31) Cyclohexane	8.083	56	11894	1.053	ug/l	# 19
36) 1,1-Dichloropropene	8.091	75	41809	4.938	ug/l	# 51
37) Ethyl Acetate	7.337	43	26746	2.783	ug/l	# 71
38) Carbon Tetrachloride	8.088	117	51905	5.936	ug/l	# 17
43) Isopropyl Acetate	8.566	43	62181	3.782	ug/l	# 86
45) 1,2-Dichloropropane	9.625	63	3581	0.547	ug/l	# 44
48) Methyl methacrylate	9.547	41	13029	1.735	ug/l	# 12
49) 1,4-Dioxane	9.614	88	162	1.479	ug/l	# 1
51) 4-Methyl-2-Pentanone	10.330	43	17126	1.722	ug/l	91
54) cis-1,3-Dichloropropene	10.245	75	100077	9.682	ug/l	# 63
56) Ethyl methacrylate	10.768	69	900	0.787	ug/l	# 19
57) 1,3-Dichloropropane	11.092	76	52937	4.968	ug/l	# 43
59) 2-Hexanone	11.092	43	890715	124.567	ug/l	# 52
68) m/p-Xylenes	11.956	106	2830	0.239	ug/l	97
74) N-amyl acetate	12.388	43	5353	0.385	ug/l	# 91
76) 1,2,3-Trichloropropane	12.734	75	312725	34.832	ug/l	# 100
80) 1,3,5-Trimethylbenzene	13.058	105	5528	0.216	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.734	75	312725	98.392	ug/l	# 6
87) 1,3-Dichlorobenzene	13.616	146	2744	0.217	ug/l	93
88) 1,4-Dichlorobenzene	13.616	146	2744	0.213	ug/l	94
93) 1,2,4-Trichlorobenzene	15.268	180	3379	0.555	ug/l	93
95) Naphthalene	15.512	128	13025	2.318	ug/l	# 95
96) 1,2,3-Trichlorobenzene	15.705	180	3465	0.582	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092521\
Data File : VN068669.D
Acq On : 25 Sep 2021 15:53
Operator : JC/MD
Sample : PB139323TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB139323TB

Quant Time: Sep 27 04:44:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092321W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 23 13:52:37 2021
Response via : Initial Calibration

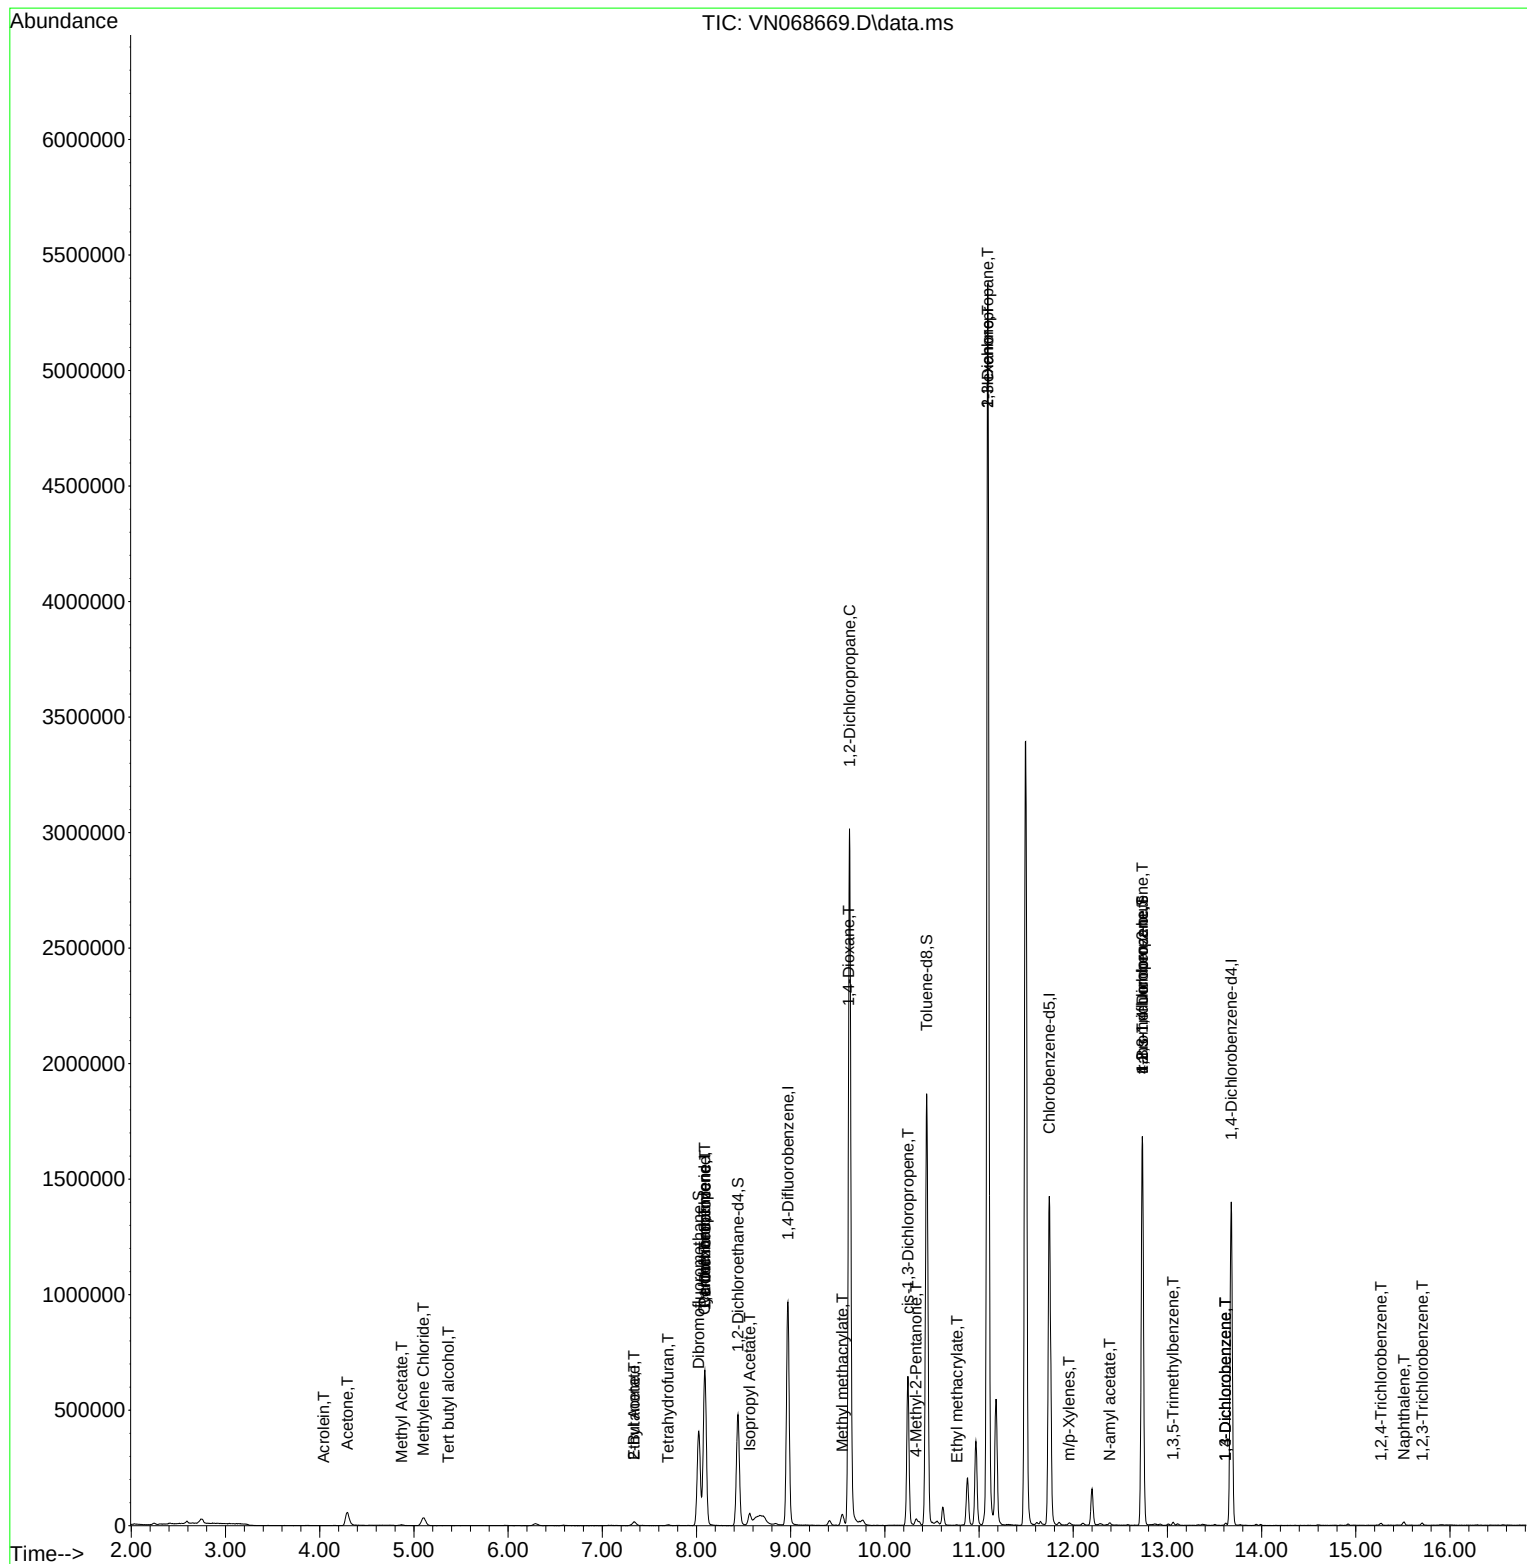



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. 0.000 min

Lab File: VN068669.D





Acq: 25 Sep 2021 15:53

Tgt Ion:168 Resp: 515459

Ion Ratio Lower Upper

168 100

99 60.0 62.9 94.3#

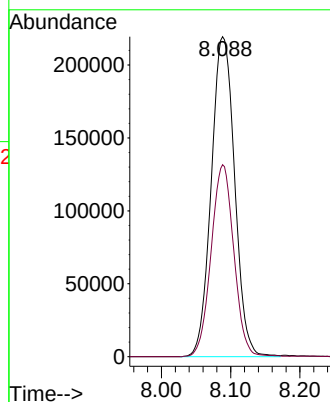

#5

Bromomethane

Concen: Below Cal

RT: 2.869 min Scan# 328

Delta R.T. 0.032 min

Lab File: VN068669.D




Acq: 25 Sep 2021 15:53


Tgt Ion: 94 Resp: 858

Ion Ratio Lower Upper

94 100

96 65.8 73.7 110.5#


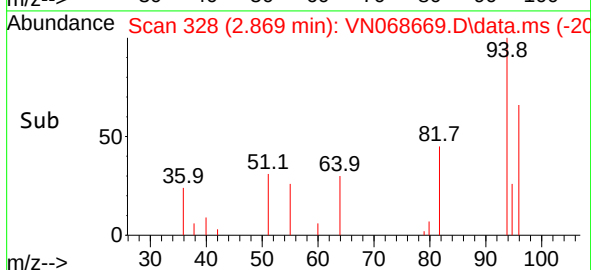
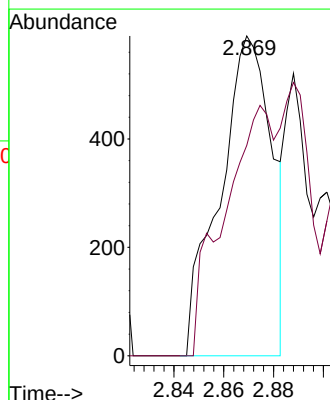



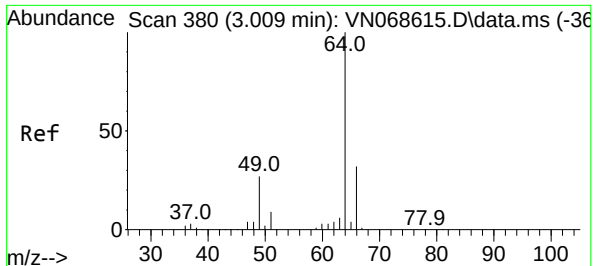

#6
Chloroethane
Concen: Below Cal
RT: 2.952 min Scan# 359
Delta R.T. -0.057 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampleId :
PB139323TB


Tgt Ion: 64 Resp: 219
Ion Ratio Lower Upper
64 100
66 41.9 24.7 37.1#

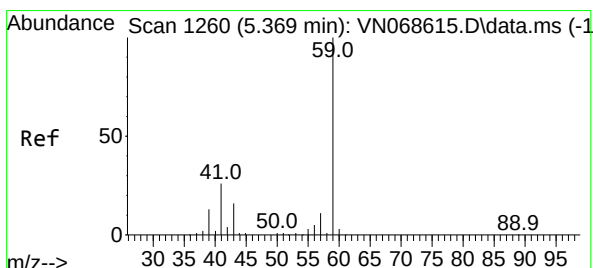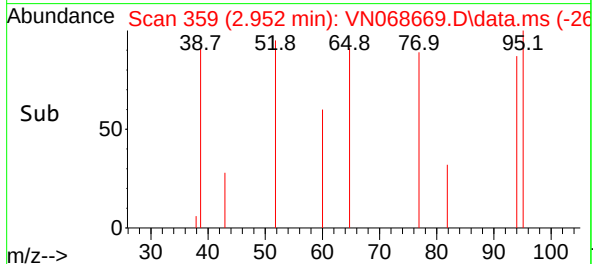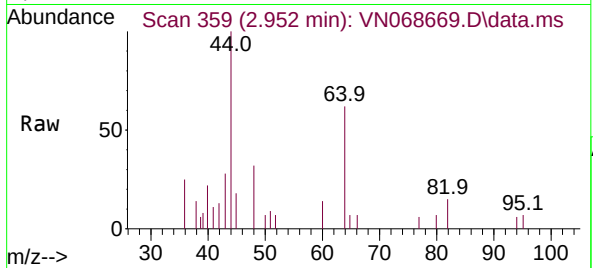

#11
Tert butyl alcohol
Concen: 0.517 ug/l
RT: 5.363 min Scan# 1258
Delta R.T. -0.006 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion: 59 Resp: 640
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


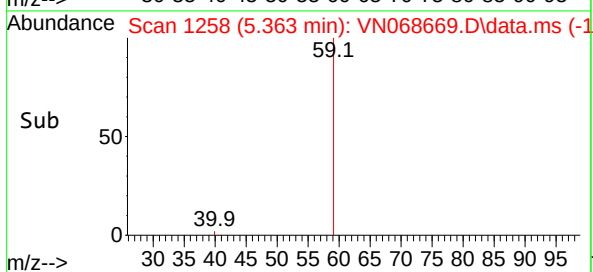

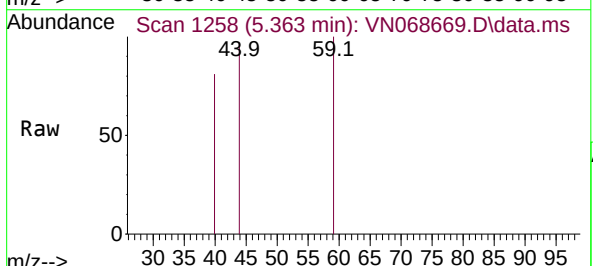




#13
Acrolein
Concen: 7.475 ug/l
RT: 4.041 min Scan# 765
Delta R.T. -0.003 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampleId :
PB139323TB


Tgt Ion: 56 Resp: 260
Ion Ratio Lower Upper
56 100
55 44.2 57.4 86.0#

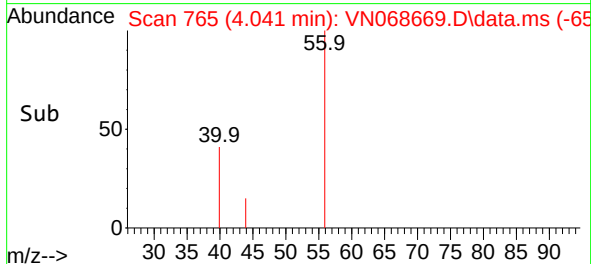

#16
Acetone
Concen: 27.395 ug/l
RT: 4.293 min Scan# 859
Delta R.T. 0.005 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion: 43 Resp: 109770
Ion Ratio Lower Upper
43 100
58 28.2 21.2 31.8




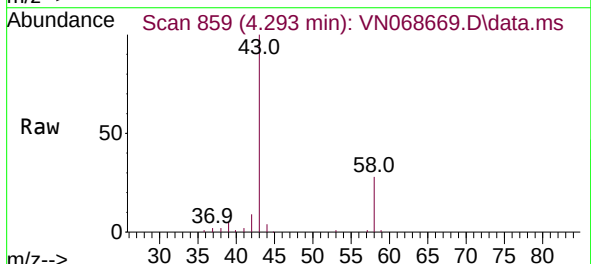


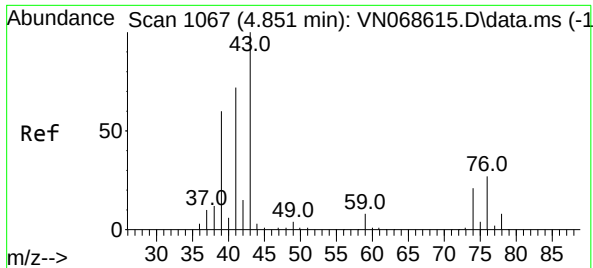

#18
Methyl Acetate
Concen: 0.624 ug/l
RT: 4.870 min Scan# 1074
Delta R.T. 0.019 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampleId :
PB139323TB


Tgt Ion: 43 Resp: 7391
Ion Ratio Lower Upper
43 100
74 1.9 17.4 26.0#

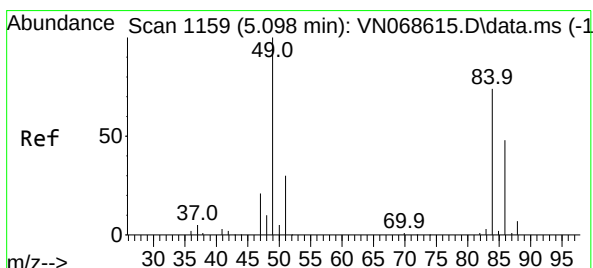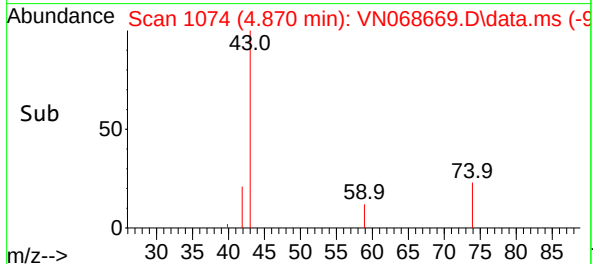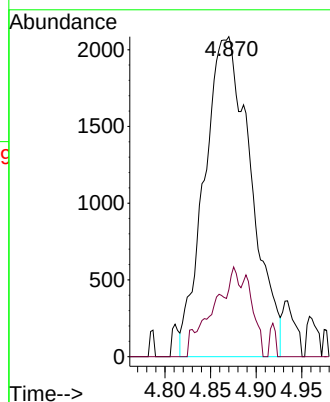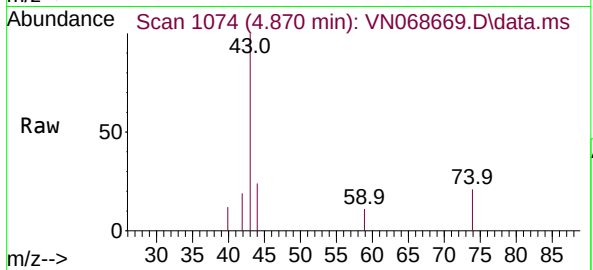

#20
Methylene Chloride
Concen: 2.595 ug/l
RT: 5.101 min Scan# 1160
Delta R.T. 0.003 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion: 84 Resp: 27315
Ion Ratio Lower Upper
84 100
49 122.5 110.9 166.3
51 39.9 32.6 49.0
86 58.5 51.6 77.4


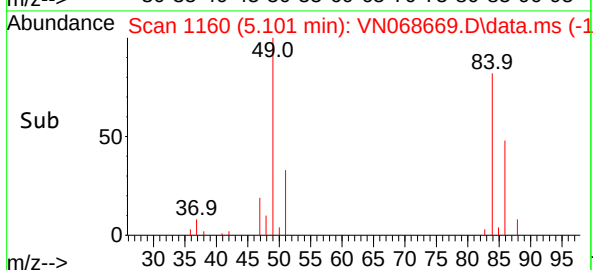
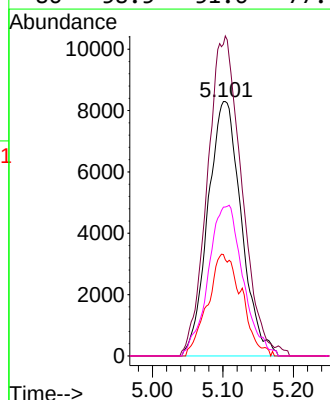
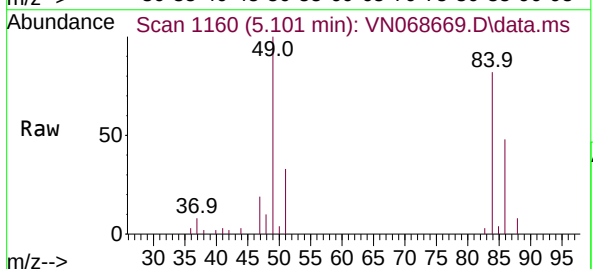


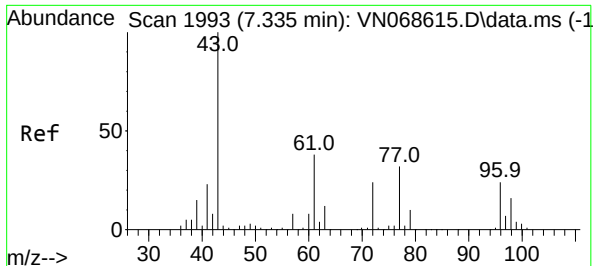

#25
2-Butanone
Concen: 5.452 ug/l
RT: 7.337 min Scan# 1994
Delta R.T. 0.002 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampled :
PB139323TB


Tgt Ion: 43 Resp: 26746
Ion Ratio Lower Upper
43 100
72 24.6 19.7 29.5

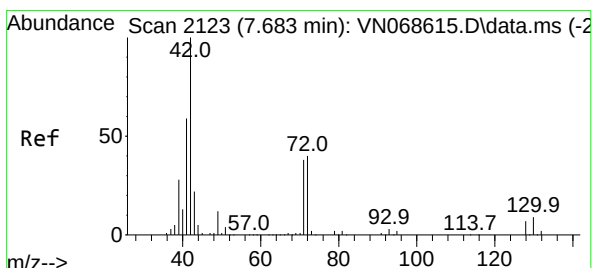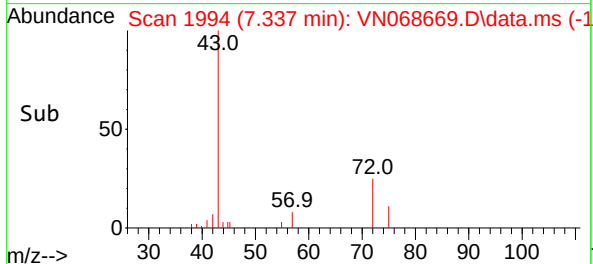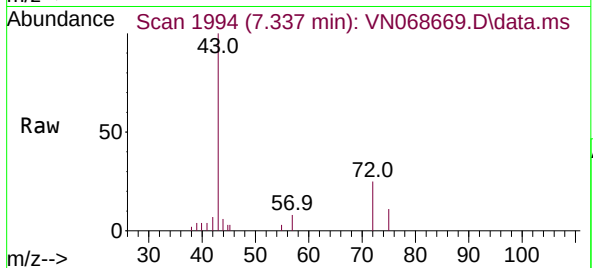

#29
Tetrahydrofuran
Concen: 0.877 ug/l
RT: 7.697 min Scan# 2128
Delta R.T. 0.014 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion: 42 Resp: 2735
Ion Ratio Lower Upper
42 100
72 26.0 32.8 49.2#
71 23.6 31.2 46.8#


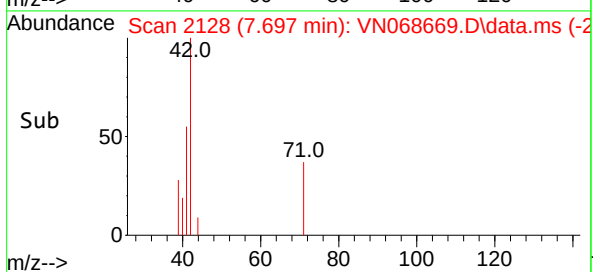

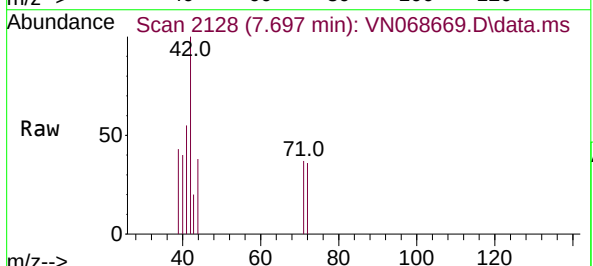




#31
Cyclohexane
Concen: 1.053 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.013 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampleId :
PB139323TB


Tgt Ion:	56	Resp:	11894
Ion	Ratio	Lower	Upper
56	100		
69	149.7	27.3	40.9#
84	108.6	64.9	97.3#

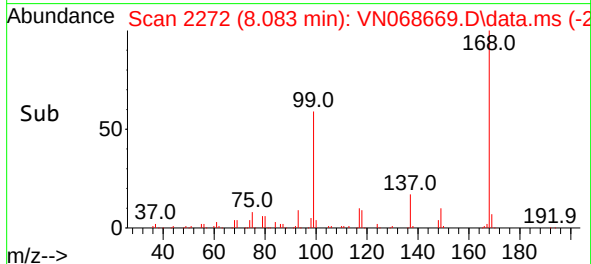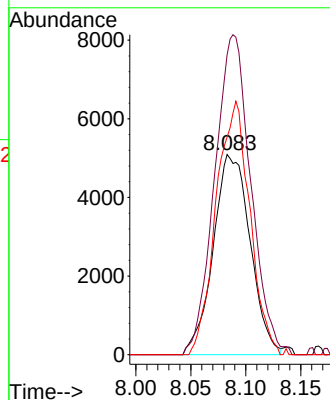

#33
1,2-Dichloroethane-d4
Concen: 49.366 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion:	65	Resp:	397189
Ion	Ratio	Lower	Upper
65	100		
67	51.2	0.0	98.6


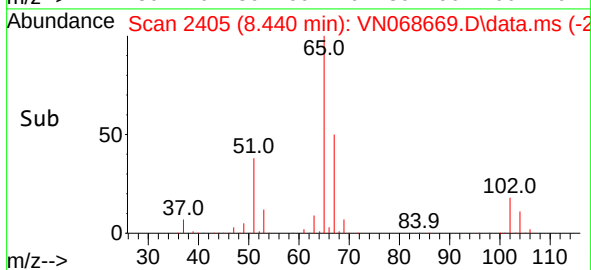
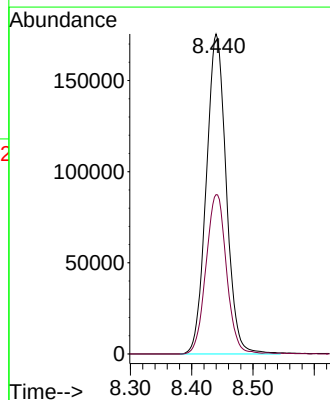
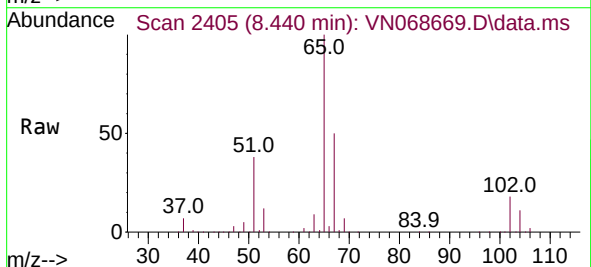




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampleId :
PB139323TB


Tgt Ion:114 Resp: 838255
Ion Ratio Lower Upper
114 100
63 20.9 0.0 49.0
88 15.3 0.0 36.6

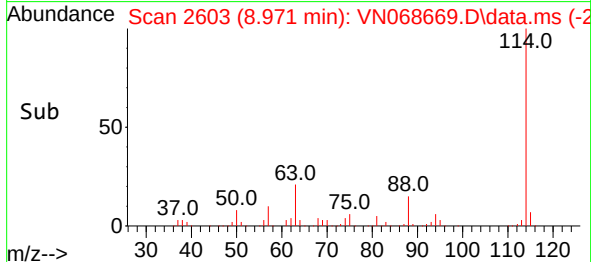

#35
Dibromofluoromethane
Concen: 52.881 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion:113 Resp: 296459
Ion Ratio Lower Upper
113 100
111 103.8 83.8 125.8
192 18.4 13.4 20.0


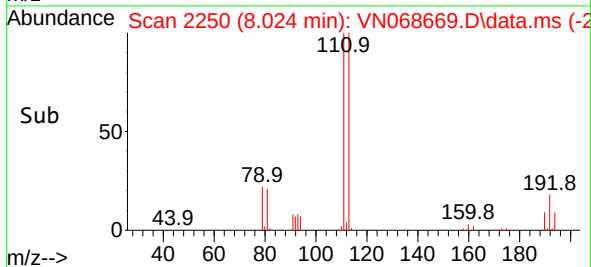

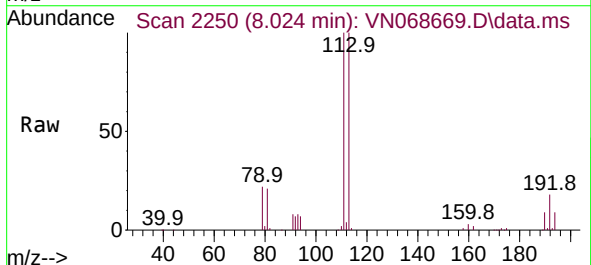




#36
1,1-Dichloropropene
Concen: 4.938 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. -0.132 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampled :
PB139323TB


Tgt Ion: 75 Resp: 41809
Ion Ratio Lower Upper
75 100
110 8.1 15.7 47.0#
77 0.0 24.6 37.0#

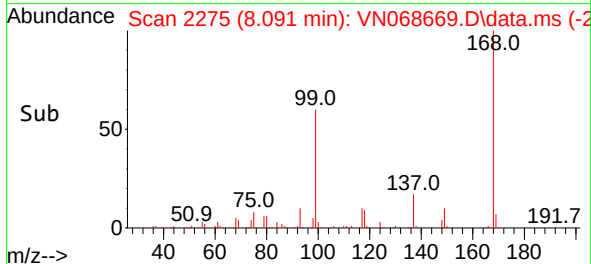

#37
Ethyl Acetate
Concen: 2.783 ug/l
RT: 7.337 min Scan# 1994
Delta R.T. -0.076 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion: 43 Resp: 26746
Ion Ratio Lower Upper
43 100
61 0.8 10.6 16.0#
70 0.0 8.1 12.1#


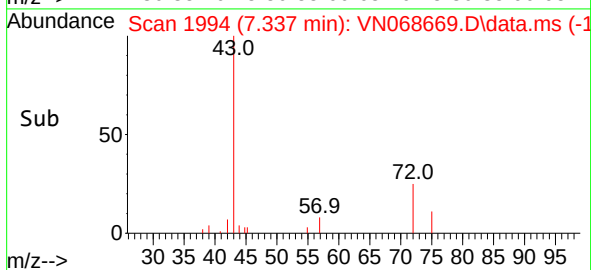

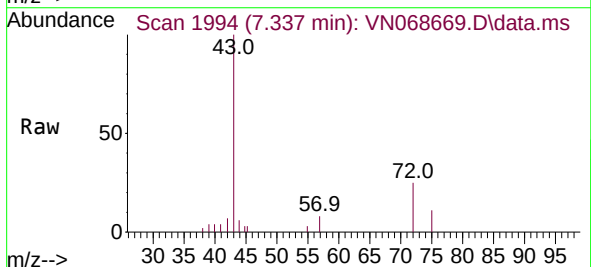




#38
Carbon Tetrachloride
Concen: 5.936 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.121 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampleId :
PB139323TB


Tgt Ion:117 Resp: 51905
Ion Ratio Lower Upper
117 100
119 5.8 75.4 113.2#
121 0.0 23.5 35.3#

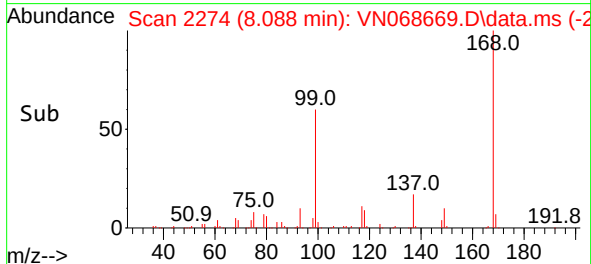

#43
Isopropyl Acetate
Concen: 3.782 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.006 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion: 43 Resp: 62181
Ion Ratio Lower Upper
43 100
61 14.7 19.0 28.4#
87 9.9 9.5 14.3

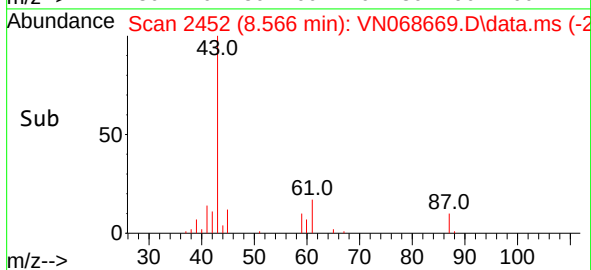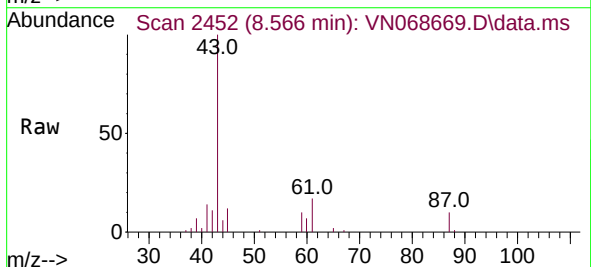







#45

1,2-Dichloropropane
Concen: 0.547 ug/l
RT: 9.625 min Scan# 2847
Delta R.T. 0.134 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Instrument :
MSVOA_N
ClientSampled :
PB139323TB




Tgt Ion: 63 Resp: 3581
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#

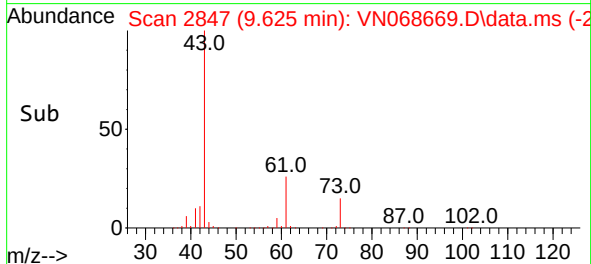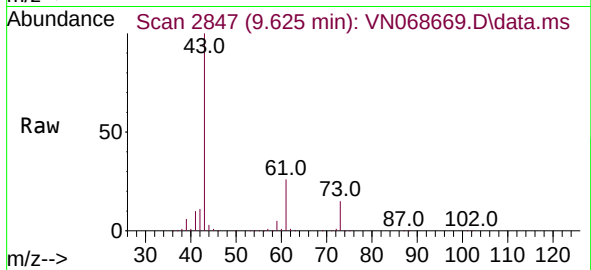


#48

Methyl methacrylate
Concen: 1.735 ug/l
RT: 9.547 min Scan# 2818
Delta R.T. -0.014 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion: 41 Resp: 13029
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

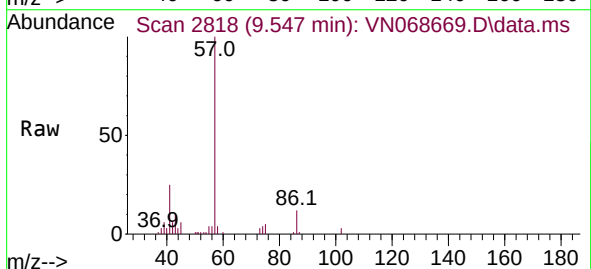



#49

1,4-Dioxane

Concen: 1.479 ug/l

RT: 9.614 min Scan# 2843

Delta R.T. 0.045 min

Lab File: VN068669.D

Acq: 25 Sep 2021 15:53

Instrument :

MSVOA_N

ClientSampleId :

PB139323TB





Tgt Ion: 88 Resp: 162

Ion Ratio Lower Upper

88 100

43 1871449.4 28.8 43.2#

58 7122.8 60.4 90.6#

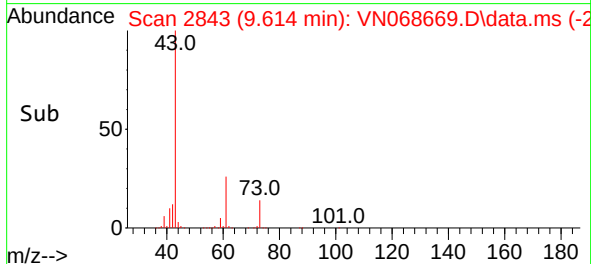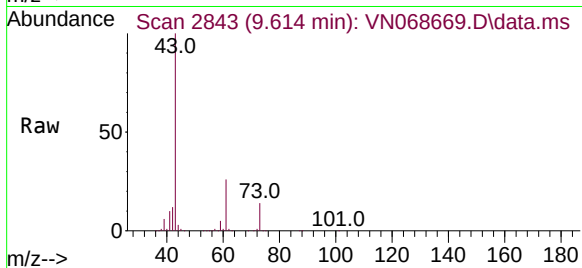

#50

Toluene-d8

Concen: 53.742 ug/l

RT: 10.443 min Scan# 3152

Delta R.T. 0.000 min

Lab File: VN068669.D




Acq: 25 Sep 2021 15:53


Tgt Ion: 98 Resp: 1277644

Ion Ratio Lower Upper

98 100

100 63.8 51.7 77.5


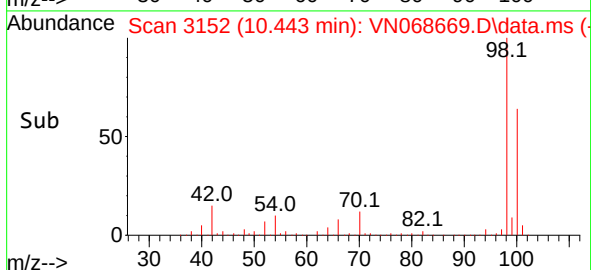

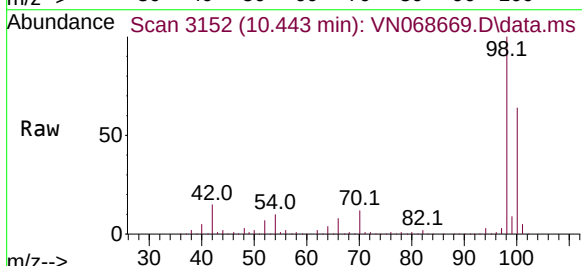




#51
4-Methyl-2-Pentanone
Concen: 1.722 ug/l
RT: 10.330 min Scan# 3110
Delta R.T. -0.001 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampled :
PB139323TB


Tgt Ion: 43 Resp: 17126
Ion Ratio Lower Upper
43 100
58 41.3 28.6 43.0



#54
cis-1,3-Dichloropropene
Concen: 9.682 ug/l
RT: 10.245 min Scan# 3078
Delta R.T. 0.054 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion: 75 Resp: 100077
Ion Ratio Lower Upper
75 100
77 0.5 24.6 37.0#
39 41.5 50.7 76.1#


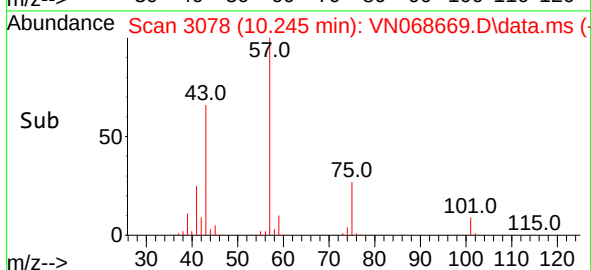






#56
Ethyl methacrylate
Concen: 0.787 ug/l
RT: 10.768 min Scan# 3273
Delta R.T. 0.006 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampled :
PB139323TB


Tgt Ion:	69	Resp:	900
Ion	Ratio	Lower	Upper
69	100		
41	0.0	58.6	88.0#
39	0.0	38.3	57.5#

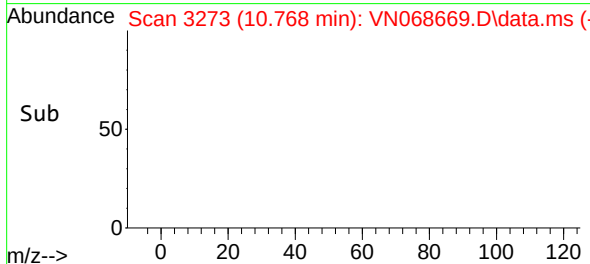

#57
1,3-Dichloropropane
Concen: 4.968 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.045 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion:	76	Resp:	52937
Ion	Ratio	Lower	Upper
76	100		
78	0.0	25.7	38.5#


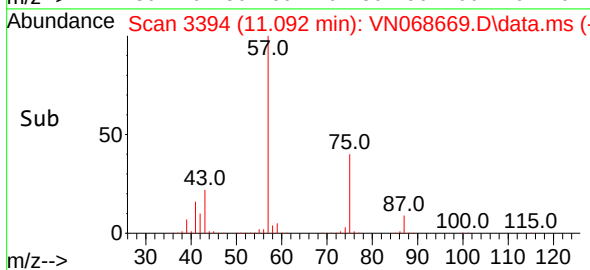

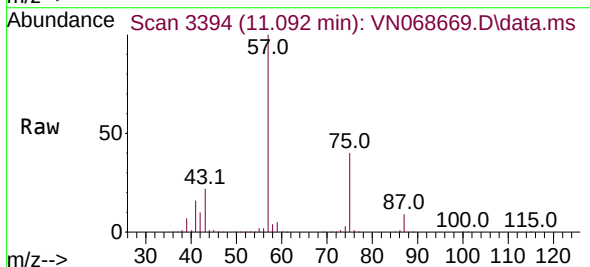


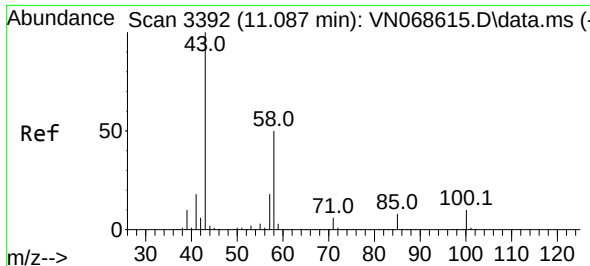

#59
2-Hexanone
Concen: 124.567 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.005 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampleId :
PB139323TB


Tgt Ion: 43 Resp: 890715
Ion Ratio Lower Upper
43 100
58 16.7 24.7 74.1#

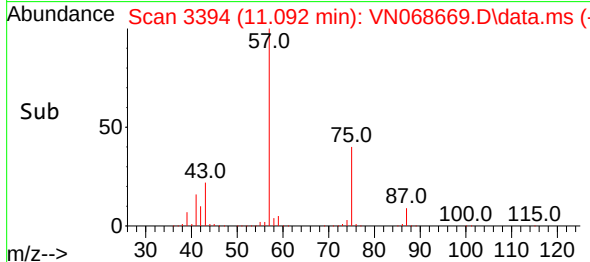

#62
4-Bromofluorobenzene
Concen: 71.149 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.003 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion: 95 Resp: 578483
Ion Ratio Lower Upper
95 100
174 75.3 0.0 122.0
176 71.7 0.0 117.6


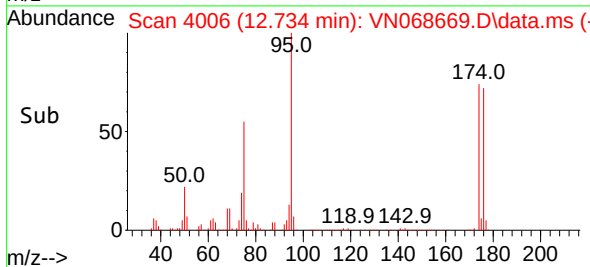

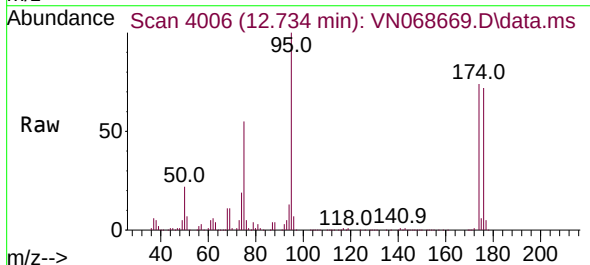




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampleId :
PB139323TB


Tgt Ion:117 Resp: 838306
Ion Ratio Lower Upper
117 100
82 56.5 53.1 79.7
119 31.0 25.5 38.3

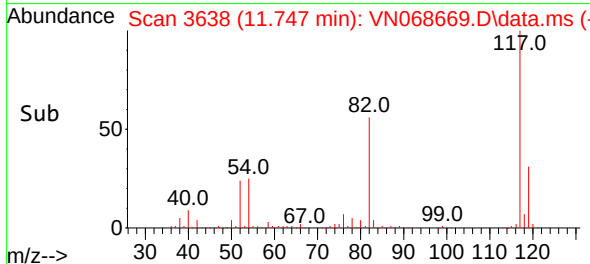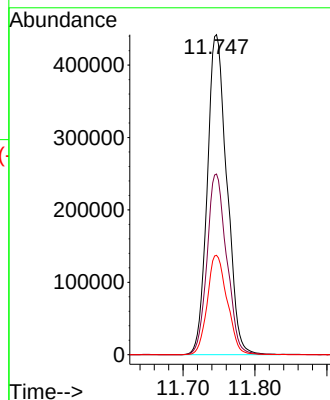

#68
m/p-Xylenes
Concen: 0.239 ug/l
RT: 11.956 min Scan# 3716
Delta R.T. -0.000 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion:106 Resp: 2830
Ion Ratio Lower Upper
106 100
91 220.2 180.6 270.8

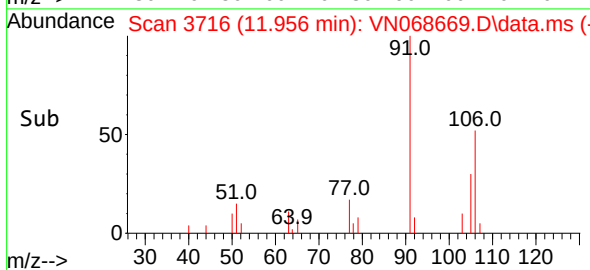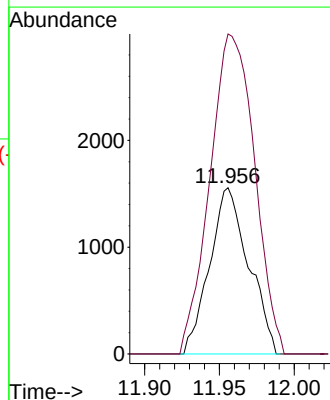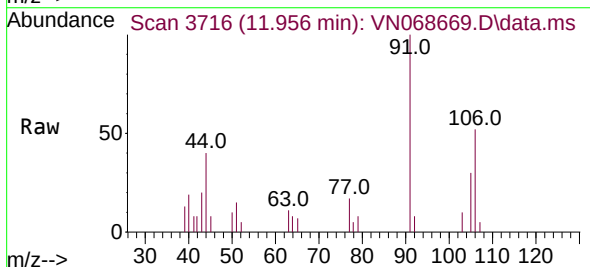

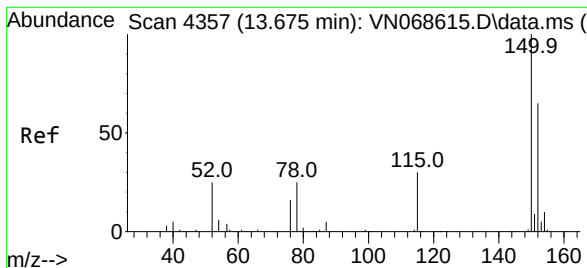

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.678 min Scan# 4358

Delta R.T. 0.003 min

Lab File: VN068669.D

Acq: 25 Sep 2021 15:53

Tgt Ion:152 Resp: 363104

Ion Ratio Lower Upper

152 100

115 61.7 36.1 108.5





150 156.7 0.0 351.8

Instrument :

MSVOA_N

ClientSampleId :

PB139323TB

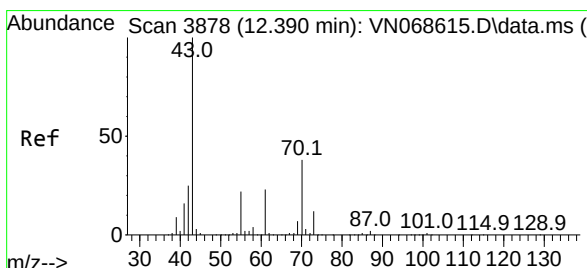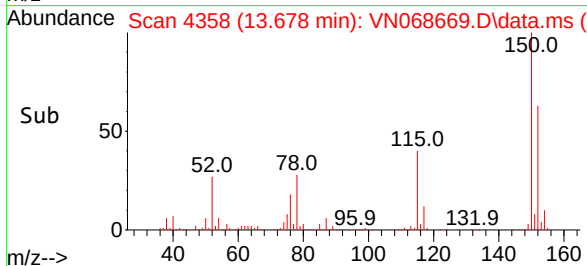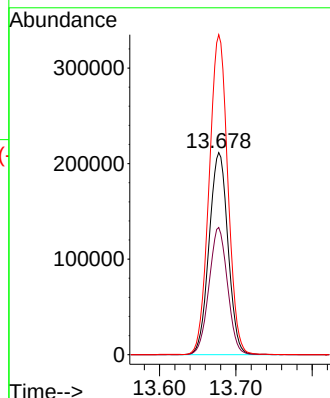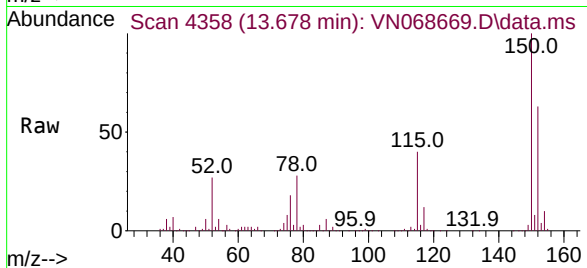

#74

N-ethyl acetate

Concen: 0.385 ug/l

RT: 12.388 min Scan# 3877

Delta R.T. -0.002 min

Lab File: VN068669.D

Acq: 25 Sep 2021 15:53

Tgt Ion: 43 Resp: 5353




Ion Ratio Lower Upper


43 100

70 41.5 29.4 44.2

55 26.4 17.0 25.4#

61 17.0 17.6 26.4#


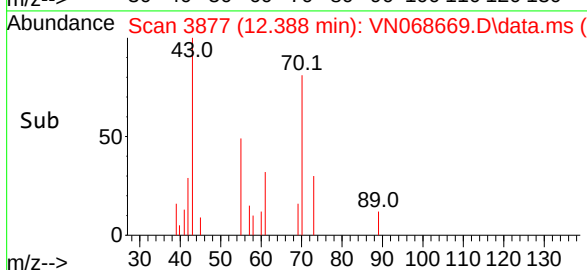
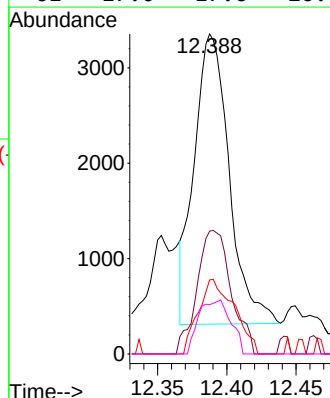
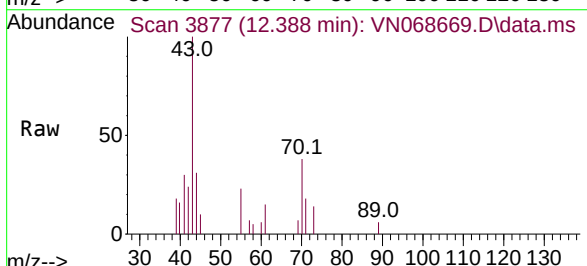


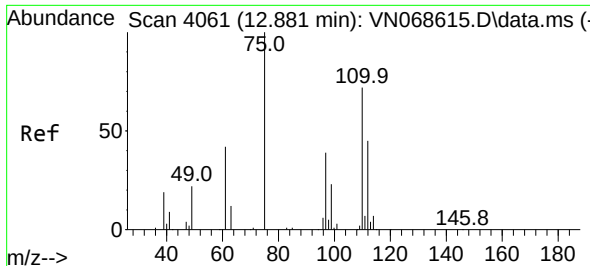

#76
1,2,3-Trichloropropane
Concen: 34.832 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.147 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampleId :
PB139323TB


Tgt Ion: 75 Resp: 312725
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#

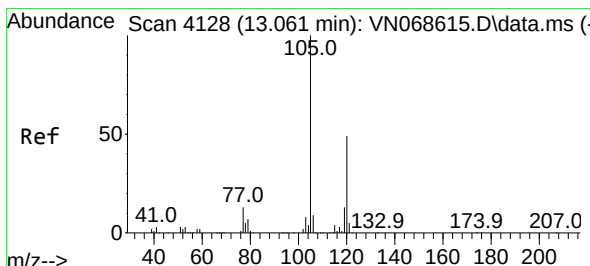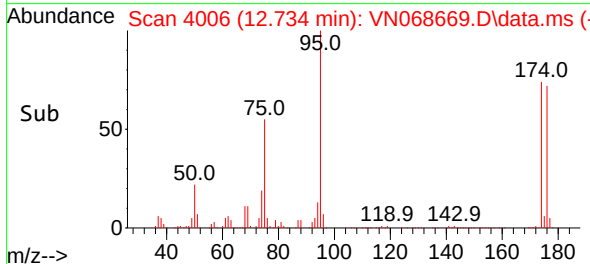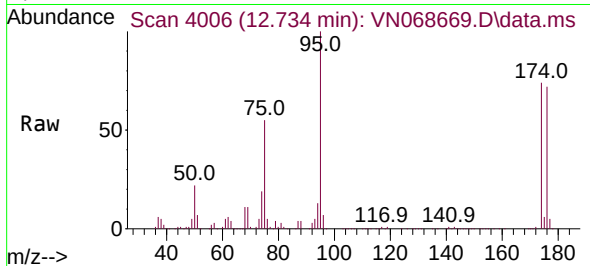

#80
1,3,5-Trimethylbenzene
Concen: 0.216 ug/l
RT: 13.058 min Scan# 4127
Delta R.T. -0.003 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion: 105 Resp: 5528
Ion Ratio Lower Upper
105 100
120 46.6 22.2 66.6


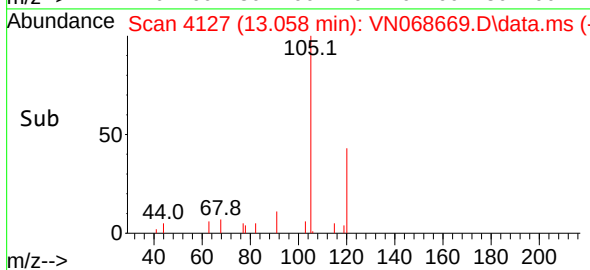

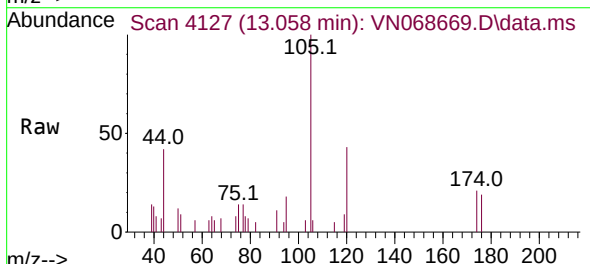




#81
trans-1,4-Dichloro-2-butene
Concen: 98.392 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.108 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53




Instrument :
MSVOA_N
ClientSampleId :
PB139323TB


Tgt Ion: 75 Resp: 312725
Ion Ratio Lower Upper
75 100
53 0.1 87.6 131.4#
89 0.0 37.8 56.8#

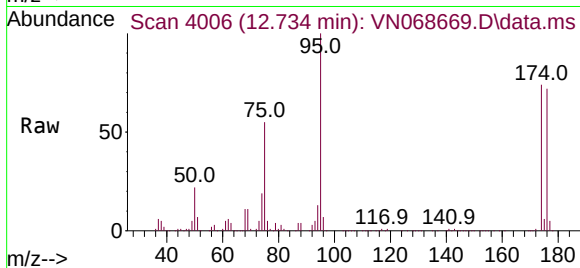

#87
1,3-Dichlorobenzene
Concen: 0.217 ug/l
RT: 13.616 min Scan# 4335
Delta R.T. -0.000 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53


Tgt Ion: 146 Resp: 2744
Ion Ratio Lower Upper
146 100
111 44.0 24.3 72.8
148 58.1 32.0 96.0

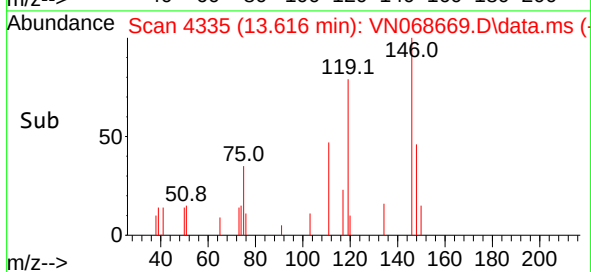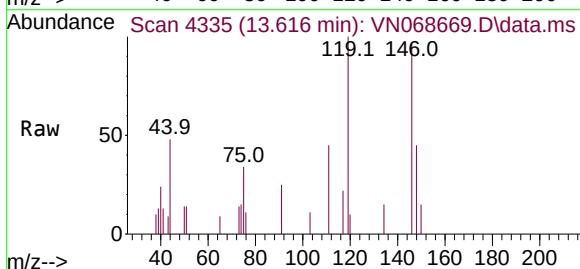



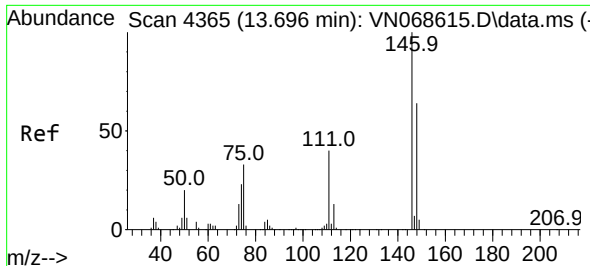


#88
 1,4-Dichlorobenzene
 Concen: 0.213 ug/l
 RT: 13.616 min Scan# 4335
 Delta R.T. -0.080 min
 Lab File: VN068669.D
 Acq: 25 Sep 2021 15:53


Instrument :
 MSVOA_N
 ClientSampled :
 PB139323TB

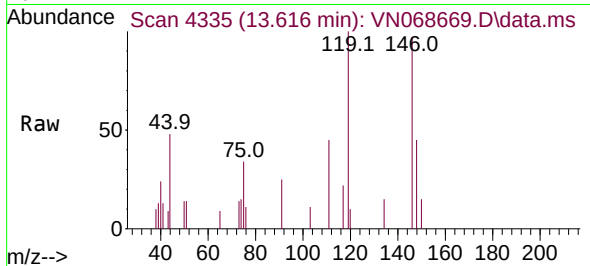



Tgt Ion:	146	Resp:	2744
Ion Ratio	Lower	Upper	
146	100		
111	44.0	23.4	70.2
148	58.1	31.8	95.3

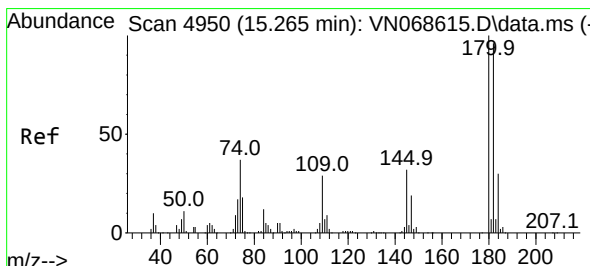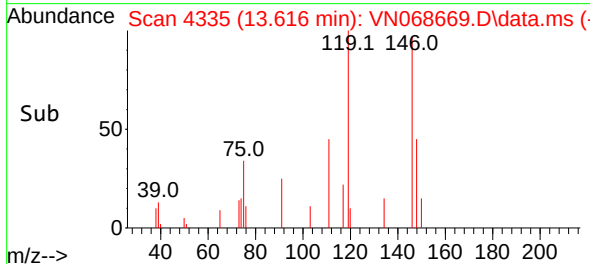


#93
 1,2,4-Trichlorobenzene
 Concen: 0.555 ug/l
 RT: 15.268 min Scan# 4951
 Delta R.T. 0.003 min
 Lab File: VN068669.D
 Acq: 25 Sep 2021 15:53

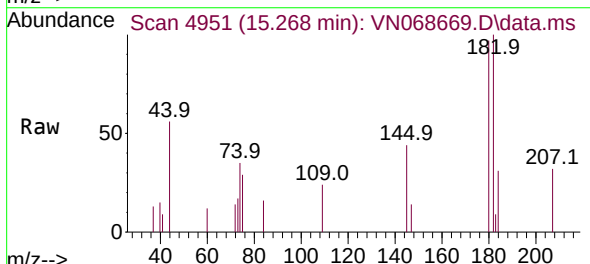

Tgt Ion:	180	Resp:	3379
Ion Ratio	Lower	Upper	
180	100		
182	88.6	47.5	142.5
145	29.2	17.2	51.6



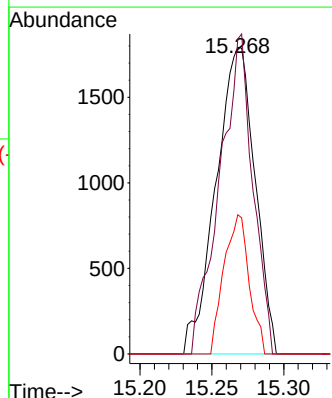



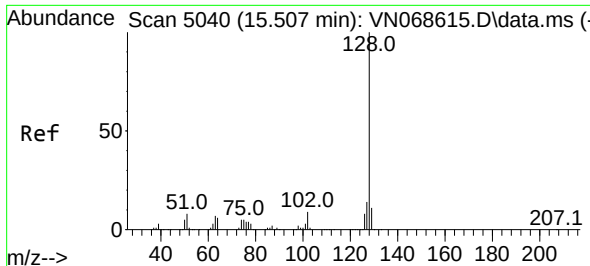

#95
Naphthalene
Concen: 2.318 ug/l
RT: 15.512 min Scan# 5042
Delta R.T. 0.005 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Instrument :
MSVOA_N
ClientSampleId :
PB139323TB

Tgt Ion:128 Resp: 13025
Ion Ratio Lower Upper
128 100
127 11.7 10.6 15.8
129 7.9 8.6 12.8#

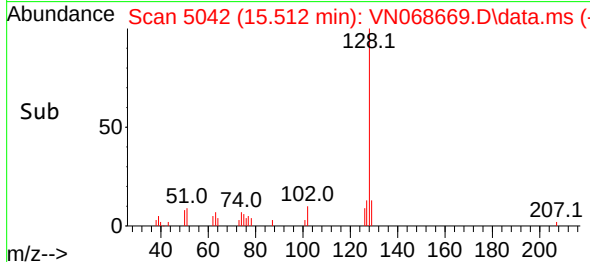

#96
1,2,3-Trichlorobenzene
Concen: 0.582 ug/l
RT: 15.705 min Scan# 5114
Delta R.T. 0.002 min
Lab File: VN068669.D
Acq: 25 Sep 2021 15:53

Tgt Ion:180 Resp: 3465
Ion Ratio Lower Upper
180 100
182 102.9 47.8 143.3
145 34.1 18.2 54.6

