
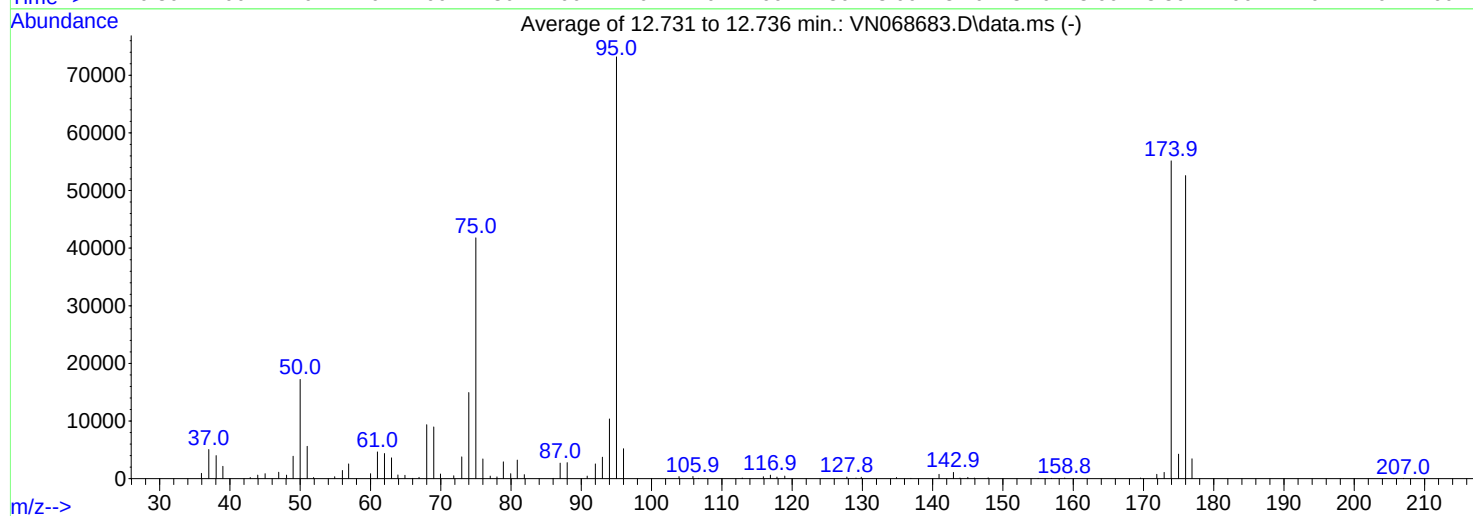


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092521\
 Data File : VN068683.D
 Acq On : 25 Sep 2021 22:12
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N092321W.M
 Title : SW846 8260
 Last Update : Thu Sep 23 13:52:37 2021

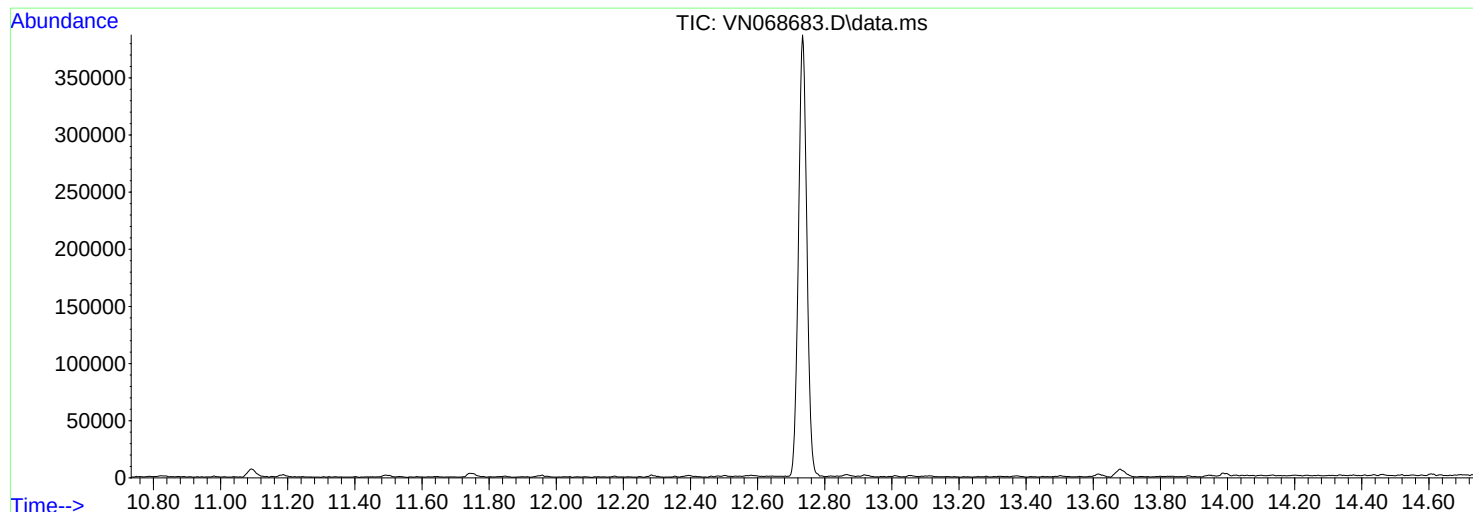

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	17221	PASS
75	95	30	60	57.1	41784	PASS
95	95	100	100	100.0	73200	PASS
96	95	5	9	7.1	5195	PASS
173	174	0.00	2	2.0	1099	PASS
174	95	50	100	75.3	55139	PASS
175	174	5	9	7.7	4241	PASS
176	174	95	101	95.4	52595	PASS
177	176	5	9	6.5	3438	PASS