
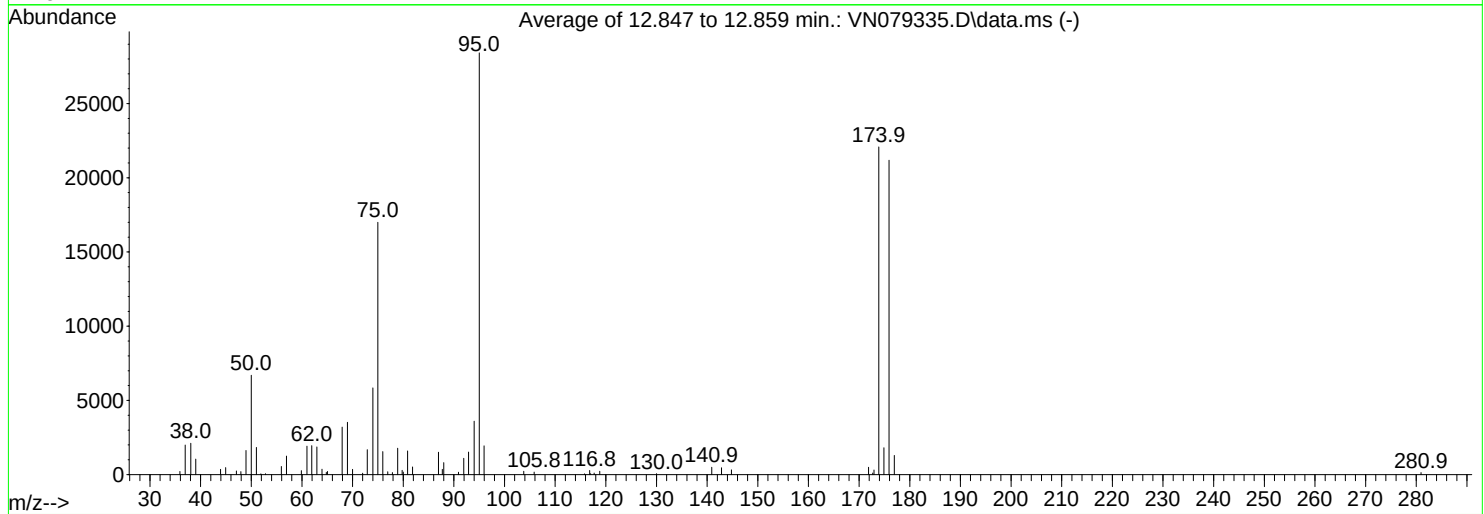


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092523\
Data File : VN079335.D
Acq On : 25 Sep 2023 08:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 05:05:24 2023

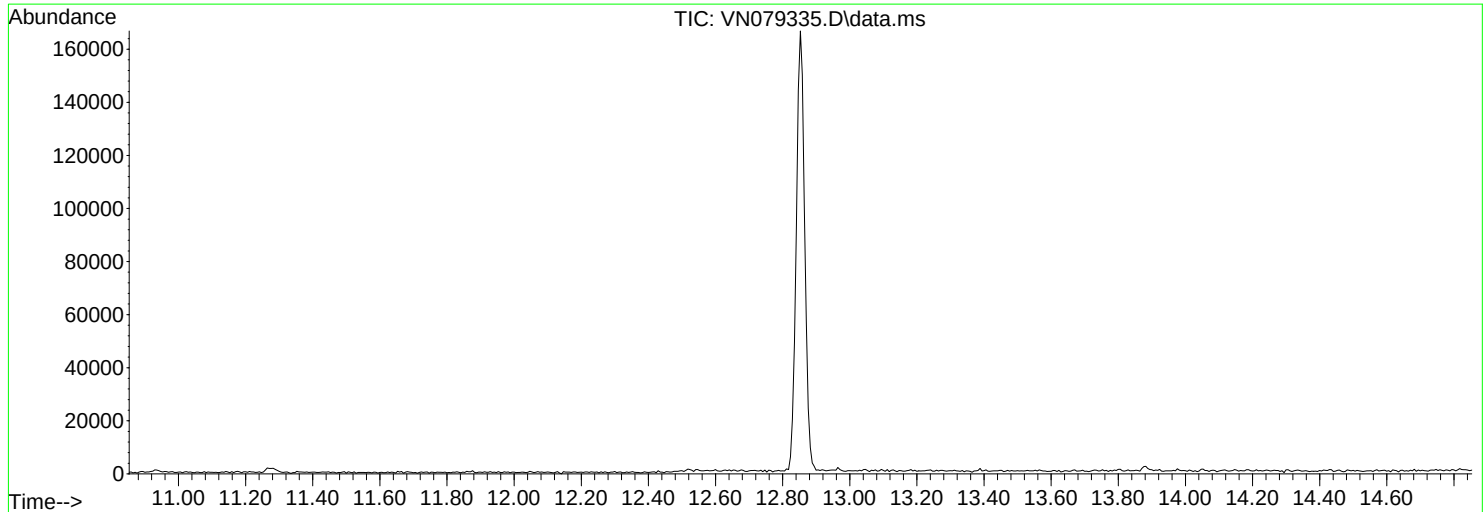

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	6697	PASS
75	95	30	60	59.8	17003	PASS
95	95	100	100	100.0	28416	PASS
96	95	5	9	6.8	1940	PASS
173	174	0.00	2	1.4	314	PASS
174	95	50	100	77.7	22075	PASS
175	174	5	9	8.2	1808	PASS
176	174	95	101	96.0	21184	PASS
177	176	5	9	6.1	1298	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	211	51.90	58	67.95	3200	79.80	281
36.95	1992	52.80	65	69.00	3528	80.00	170
38.05	2108	55.95	549	70.00	360	80.85	159
39.05	1041	56.95	1248	72.00	96	81.85	51
43.95	360	59.90	271	72.90	1684	86.95	1506
44.95	474	61.00	1922	74.00	5847	87.70	353
47.05	249	61.95	1947	75.00	17003	88.00	812
47.95	210	62.95	1863	75.95	1554	90.90	158
48.95	1624	63.95	371	76.95	194	91.95	1102
50.00	6697	64.80	155	77.85	139	92.90	1515
51.00	1834	65.05	221	78.90	1774	94.00	3602

Average of 12.847 to 12.859 min.: VN079335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	28416	142.85	469				
95.95	1940	144.80	323				
103.80	228	171.85	498				
105.85	176	172.70	107				
115.80	52	172.95	314				
116.80	276	173.90	22075				
117.00	63	174.90	1808				
117.70	106	175.90	21184				
118.80	227	176.95	1298				
130.00	63	280.95	142				
140.90	496						

Instrument :

MSVOA_N

ClientSampleId :

BFB