
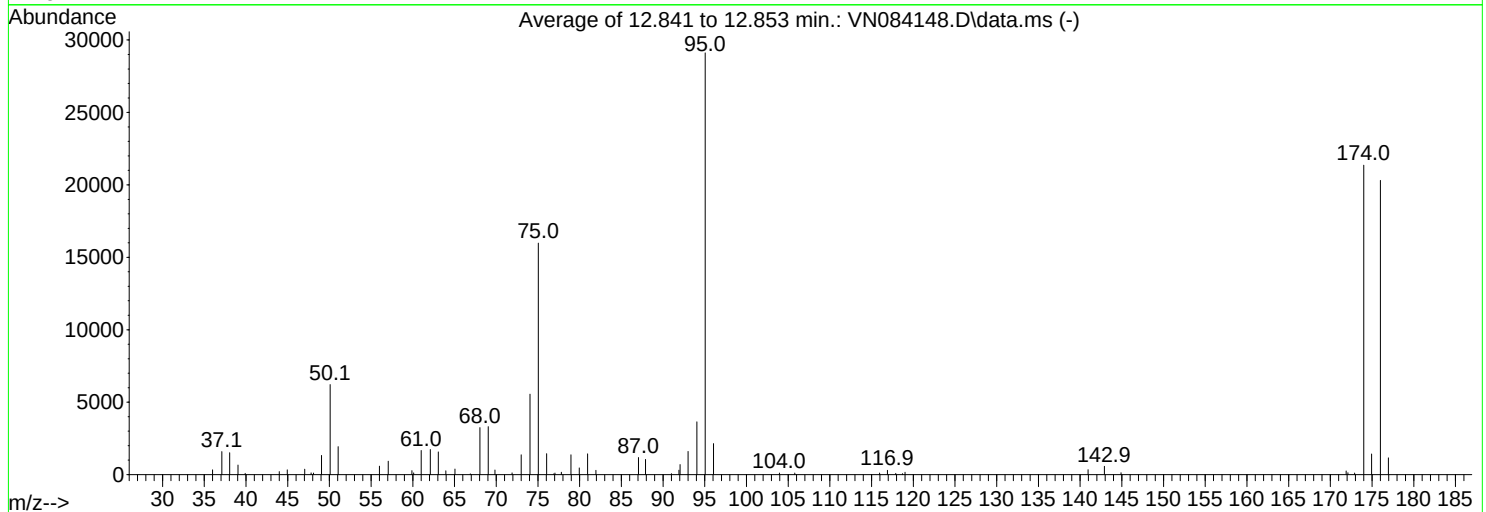


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN092524\
Data File : VN084148.D
Acq On : 25 Sep 2024 08:28
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

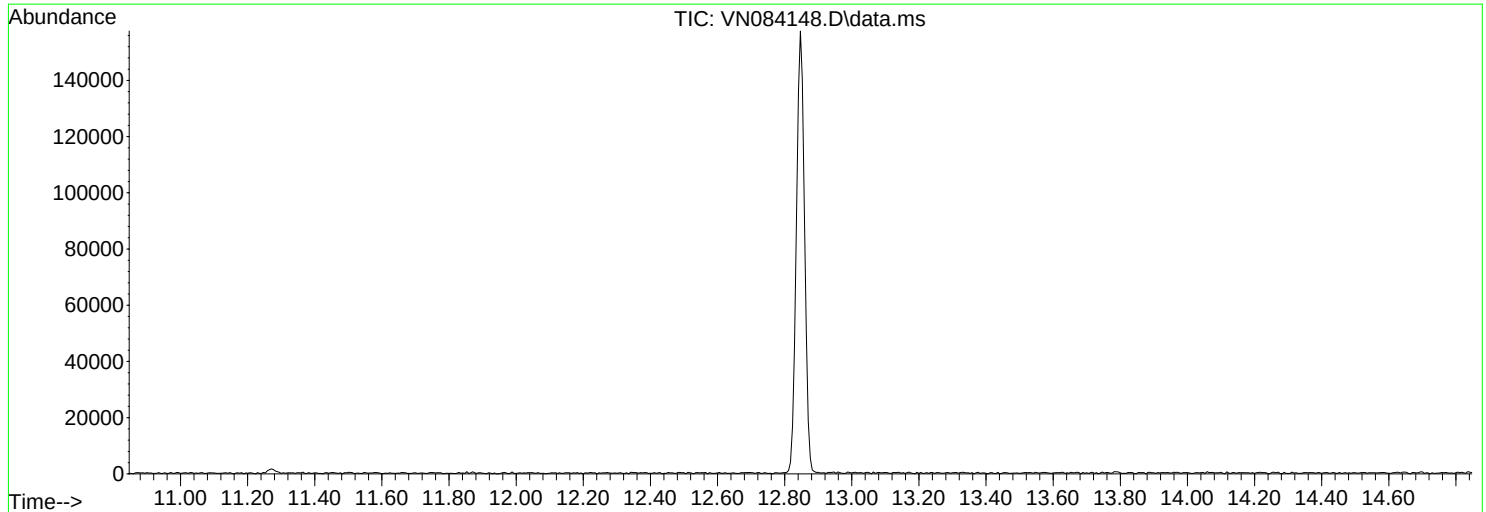

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.3	6213	PASS
75	95	30	60	54.9	15979	PASS
95	95	100	100	100.0	29112	PASS
96	95	5	9	7.4	2141	PASS
173	174	0.00	2	0.5	106	PASS
174	95	50	100	73.4	21357	PASS
175	174	5	9	6.7	1427	PASS
176	174	95	101	95.1	20312	PASS
177	176	5	9	5.7	1155	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	336	50.10	6213	66.90	60	77.80	16
37.10	1589	51.05	1934	68.05	3252	78.95	136
38.05	1518	56.00	582	69.05	3309	79.95	46
39.05	664	57.05	932	69.85	319	80.95	143
39.90	85	59.90	275	71.90	123	81.95	303
44.00	206	60.10	119	73.00	1369	87.05	1187
44.95	333	61.00	1670	74.05	5551	87.90	1052
47.05	376	62.10	1732	75.05	15979	91.00	69
47.80	123	63.05	1573	76.05	1448	91.90	305
48.10	110	63.95	268	76.90	60	92.05	701
49.05	1331	65.05	388	77.05	109	93.00	1607

Average of 12.841 to 12.853 min.: VN084148.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	3645	142.90	572				
95.05	29112	144.90	128				
96.05	2141	171.90	256				
103.95	114	172.10	135				
105.80	107	172.90	106				
115.95	116	174.00	21357				
116.90	299	174.95	1427				
117.90	92	176.00	20312				
118.70	66	176.95	1155				
119.00	167						
140.95	344						

Instrument :

MSVOA_N

ClientSampleId :

BFB